R&S®RTM20xx
Digital Oscilloscope
User Manual

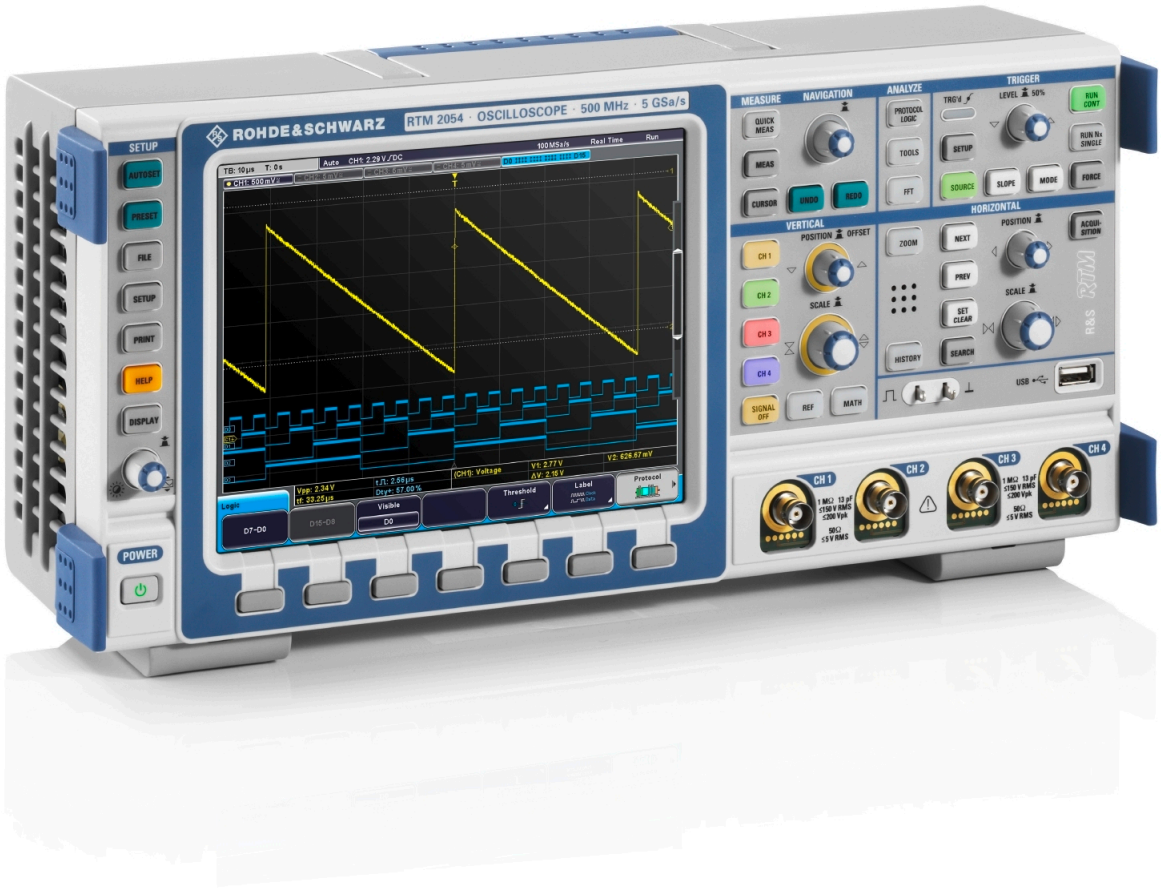

1317.4726.02 ─ 01

Test & Measurement

User Manual

ROHDE&SCHWARZ

This document describes the following R&S®RTM models:

- R&S®RTM2032 (5710.0999K32)
- R&S®RTM2034 (5710.0999K34)
- R&S®RTM2052 (5710.0999K52)
- R&S®RTM2054 (5710.0999K54)

In addition to the base unit, the following options are described:

- R&S®RTM-K1 (1305.0295.02)
- R&S®RTM-K2 (1305.0308.02)
- R&S®RTM-K3 (1317.3065.02)
- R&S®RTM-K5 (5710.0882.02)

The firmware of the instrument makes use of several valuable open source software packages. For information, see the "Open Source Acknowledgement" on the user documentation CD-ROM (included in delivery).
Rohde & Schwarz would like to thank the open source community for their valuable contribution to embedded computing.

© 2013 Rohde & Schwarz GmbH & Co. KG
Mühldorfstr. 15, 81671 München, Germany
Phone: +49 89 41 29 - 0
Fax: +49 89 41 29 12 164
E-mail: info@rohde-schwarz.com
Internet: www.rohde-schwarz.com
Subject to change – Data without tolerance limits is not binding.
R&S® is a registered trademark of Rohde & Schwarz GmbH & Co. KG.
Trade names are trademarks of the owners.

The following abbreviations are used throughout this manual: R&S®RTM is abbreviated as R&S RTM.

Basic Safety Instructions

Always read through and comply with the following safety instructions!

All plants and locations of the Rohde & Schwarz group of companies make every effort to keep the safety standards of our products up to date and to offer our customers the highest possible degree of safety. Our products and the auxiliary equipment they require are designed, built and tested in accordance with the safety standards that apply in each case. Compliance with these standards is continuously monitored by our quality assurance system. The product described here has been designed, built and tested in accordance with the EC Certificate of Conformity and has left the manufacturer's plant in a condition fully complying with safety standards. To maintain this condition and to ensure safe operation, you must observe all instructions and warnings provided in this manual. If you have any questions regarding these safety instructions, the Rohde & Schwarz group of companies will be happy to answer them.

Furthermore, it is your responsibility to use the product in an appropriate manner. This product is designed for use solely in industrial and laboratory environments or, if expressly permitted, also in the field and must not be used in any way that may cause personal injury or property damage. You are responsible if the product is used for any purpose other than its designated purpose or in disregard of the manufacturer's instructions. The manufacturer shall assume no responsibility for such use of the product.

The product is used for its designated purpose if it is used in accordance with its product documentation and within its performance limits (see data sheet, documentation, the following safety instructions). Using the product requires technical skills and, in some cases, a basic knowledge of English. It is therefore essential that only skilled and specialized staff or thoroughly trained personnel with the required skills be allowed to use the product. If personal safety gear is required for using Rohde & Schwarz products, this will be indicated at the appropriate place in the product documentation. Keep the basic safety instructions and the product documentation in a safe place and pass them on to the subsequent users.

Observing the safety instructions will help prevent personal injury or damage of any kind caused by dangerous situations. Therefore, carefully read through and adhere to the following safety instructions before and when using the product. It is also absolutely essential to observe the additional safety instructions on personal safety, for example, that appear in relevant parts of the product documentation. In these safety instructions, the word "product" refers to all merchandise sold and distributed by the Rohde & Schwarz group of companies, including instruments, systems and all accessories. For product-specific information, see the data sheet and the product documentation.

Safety labels on products

The following safety labels are used on products to warn against risks and dangers.

Symbol	Meaning	Symbol	Meaning
	Notice, general danger location Observe product documentation		ON/OFF supply voltage
	Caution when handling heavy equipment		Standby indication
	Danger of electric shock		Direct current (DC)

Symbol	Meaning	Symbol	Meaning
	Warning! Hot surface		Alternating current (AC)
	Protective conductor terminal		Direct/alternating current (DC/AC)
	Ground		Device fully protected by double (reinforced) insulation
	Ground terminal		EU labeling for batteries and accumulators For additional information, see section "Waste disposal/Environmental protection", item 1.
	Be careful when handling electrostatic sensitive devices		EU labeling for separate collection of electrical and electronic devices For additonal information, see section "Waste disposal/Environmental protection", item 2.
	Warning! Laser radiation For additional information, see section "Operation", item 7.		

Signal words and their meaning

The following signal words are used in the product documentation in order to warn the reader about risks and dangers.

DANGER Indicates a hazardous situation which, if not avoided, will result in death or serious injury.

WARNING Indicates a hazardous situation which, if not avoided, could result in death or serious injury.

CAUTION Indicates a hazardous situation which, if not avoided, could result in minor or moderate injury.

NOTICE Indicates information considered important, but not hazard-related, e.g. messages relating to property damage.
In the product documentation, the word ATTENTION is used synonymously.

These signal words are in accordance with the standard definition for civil applications in the European Economic Area. Definitions that deviate from the standard definition may also exist in other economic areas or military applications. It is therefore essential to make sure that the signal words described here are always used only in connection with the related product documentation and the related product. The use of signal words in connection with unrelated products or documentation can result in misinterpretation and in personal injury or material damage.

Operating states and operating positions

The product may be operated only under the operating conditions and in the positions specified by the manufacturer, without the product's ventilation being obstructed. If the manufacturer's specifications are not observed, this can result in electric shock, fire and/or serious personal injury or death. Applicable local or national safety regulations and rules for the prevention of accidents must be observed in all work performed.

1. Unless otherwise specified, the following requirements apply to Rohde & Schwarz products: predefined operating position is always with the housing floor facing down, IP protection 2X, use only indoors, max. operating altitude 2000 m above sea level, max. transport altitude 4500 m above sea level. A tolerance of ±10 % shall apply to the nominal voltage and ±5 % to the nominal frequency, overvoltage category 2, pollution severity 2.
2. Do not place the product on surfaces, vehicles, cabinets or tables that for reasons of weight or stability are unsuitable for this purpose. Always follow the manufacturer's installation instructions when installing the product and fastening it to objects or structures (e.g. walls and shelves). An installation that is not carried out as described in the product documentation could result in personal injury or even death.
3. Do not place the product on heat-generating devices such as radiators or fan heaters. The ambient temperature must not exceed the maximum temperature specified in the product documentation or in the data sheet. Product overheating can cause electric shock, fire and/or serious personal injury or even death.

Electrical safety

If the information on electrical safety is not observed either at all or to the extent necessary, electric shock, fire and/or serious personal injury or death may occur.

1. Prior to switching on the product, always ensure that the nominal voltage setting on the product matches the nominal voltage of the AC supply network. If a different voltage is to be set, the power fuse of the product may have to be changed accordingly.
2. In the case of products of safety class I with movable power cord and connector, operation is permitted only on sockets with a protective conductor contact and protective conductor.
3. Intentionally breaking the protective conductor either in the feed line or in the product itself is not permitted. Doing so can result in the danger of an electric shock from the product. If extension cords or connector strips are implemented, they must be checked on a regular basis to ensure that they are safe to use.
4. If there is no power switch for disconnecting the product from the AC supply network, or if the power switch is not suitable for this purpose, use the plug of the connecting cable to disconnect the product from the AC supply network. In such cases, always ensure that the power plug is easily reachable and accessible at all times. For example, if the power plug is the disconnecting device, the length of the connecting cable must not exceed 3 m. Functional or electronic switches are not suitable for providing disconnection from the AC supply network. If products without power switches are integrated into racks or systems, the disconnecting device must be provided at the system level.
5. Never use the product if the power cable is damaged. Check the power cables on a regular basis to ensure that they are in proper operating condition. By taking appropriate safety measures and carefully laying the power cable, ensure that the cable cannot be damaged and that no one can be hurt by, for example, tripping over the cable or suffering an electric shock.

6. The product may be operated only from TN/TT supply networks fuse-protected with max. 16 A (higher fuse only after consulting with the Rohde & Schwarz group of companies).
7. Do not insert the plug into sockets that are dusty or dirty. Insert the plug firmly and all the way into the socket provided for this purpose. Otherwise, sparks that result in fire and/or injuries may occur.
8. Do not overload any sockets, extension cords or connector strips; doing so can cause fire or electric shocks.
9. For measurements in circuits with voltages V_{rms} > 30 V, suitable measures (e.g. appropriate measuring equipment, fuse protection, current limiting, electrical separation, insulation) should be taken to avoid any hazards.
10. Ensure that the connections with information technology equipment, e.g. PCs or other industrial computers, comply with the IEC60950-1/EN60950-1 or IEC61010-1/EN 61010-1 standards that apply in each case.
11. Unless expressly permitted, never remove the cover or any part of the housing while the product is in operation. Doing so will expose circuits and components and can lead to injuries, fire or damage to the product.
12. If a product is to be permanently installed, the connection between the protective conductor terminal on site and the product's protective conductor must be made first before any other connection is made. The product may be installed and connected only by a licensed electrician.
13. For permanently installed equipment without built-in fuses, circuit breakers or similar protective devices, the supply circuit must be fuse-protected in such a way that anyone who has access to the product, as well as the product itself, is adequately protected from injury or damage.
14. Use suitable overvoltage protection to ensure that no overvoltage (such as that caused by a bolt of lightning) can reach the product. Otherwise, the person operating the product will be exposed to the danger of an electric shock.
15. Any object that is not designed to be placed in the openings of the housing must not be used for this purpose. Doing so can cause short circuits inside the product and/or electric shocks, fire or injuries.
16. Unless specified otherwise, products are not liquid-proof (see also section "Operating states and operating positions", item 1). Therefore, the equipment must be protected against penetration by liquids. If the necessary precautions are not taken, the user may suffer electric shock or the product itself may be damaged, which can also lead to personal injury.
17. Never use the product under conditions in which condensation has formed or can form in or on the product, e.g. if the product has been moved from a cold to a warm environment. Penetration by water increases the risk of electric shock.
18. Prior to cleaning the product, disconnect it completely from the power supply (e.g. AC supply network or battery). Use a soft, non-linting cloth to clean the product. Never use chemical cleaning agents such as alcohol, acetone or diluents for cellulose lacquers.

Operation

1. Operating the products requires special training and intense concentration. Make sure that persons who use the products are physically, mentally and emotionally fit enough to do so; otherwise, injuries or material damage may occur. It is the responsibility of the employer/operator to select suitable personnel for operating the products.

2. Before you move or transport the product, read and observe the section titled "Transport".
3. As with all industrially manufactured goods, the use of substances that induce an allergic reaction (allergens) such as nickel cannot be generally excluded. If you develop an allergic reaction (such as a skin rash, frequent sneezing, red eyes or respiratory difficulties) when using a Rohde & Schwarz product, consult a physician immediately to determine the cause and to prevent health problems or stress.
4. Before you start processing the product mechanically and/or thermally, or before you take it apart, be sure to read and pay special attention to the section titled "Waste disposal/Environmental protection", item 1.
5. Depending on the function, certain products such as RF radio equipment can produce an elevated level of electromagnetic radiation. Considering that unborn babies require increased protection, pregnant women must be protected by appropriate measures. Persons with pacemakers may also be exposed to risks from electromagnetic radiation. The employer/operator must evaluate workplaces where there is a special risk of exposure to radiation and, if necessary, take measures to avert the potential danger.
6. Should a fire occur, the product may release hazardous substances (gases, fluids, etc.) that can cause health problems. Therefore, suitable measures must be taken, e.g. protective masks and protective clothing must be worn.
7. Laser products are given warning labels that are standardized according to their laser class. Lasers can cause biological harm due to the properties of their radiation and due to their extremely concentrated electromagnetic power. If a laser product (e.g. a CD/DVD drive) is integrated into a Rohde & Schwarz product, absolutely no other settings or functions may be used as described in the product documentation. The objective is to prevent personal injury (e.g. due to laser beams).
8. EMC classes (in line with EN 55011/CISPR 11, and analogously with EN 55022/CISPR 22, EN 55032/CISPR 32)
   - Class A equipment:
     Equipment suitable for use in all environments except residential environments and environments that are directly connected to a low-voltage supply network that supplies residential buildings
     Note: Class A equipment is intended for use in an industrial environment. This equipment may cause radio disturbances in residential environments, due to possible conducted as well as radiated disturbances. In this case, the operator may be required to take appropriate measures to eliminate these disturbances.
   - Class B equipment:
     Equipment suitable for use in residential environments and environments that are directly connected to a low-voltage supply network that supplies residential buildings

Repair and service

1. The product may be opened only by authorized, specially trained personnel. Before any work is performed on the product or before the product is opened, it must be disconnected from the AC supply network. Otherwise, personnel will be exposed to the risk of an electric shock.

2. Adjustments, replacement of parts, maintenance and repair may be performed only by electrical experts authorized by Rohde & Schwarz. Only original parts may be used for replacing parts relevant to safety (e.g. power switches, power transformers, fuses). A safety test must always be performed after parts relevant to safety have been replaced (visual inspection, protective conductor test, insulation resistance measurement, leakage current measurement, functional test). This helps ensure the continued safety of the product.

Batteries and rechargeable batteries/cells

If the information regarding batteries and rechargeable batteries/cells is not observed either at all or to the extent necessary, product users may be exposed to the risk of explosions, fire and/or serious personal injury, and, in some cases, death. Batteries and rechargeable batteries with alkaline electrolytes (e.g. lithium cells) must be handled in accordance with the EN 62133 standard.

1. Cells must not be taken apart or crushed.
2. Cells or batteries must not be exposed to heat or fire. Storage in direct sunlight must be avoided. Keep cells and batteries clean and dry. Clean soiled connectors using a dry, clean cloth.
3. Cells or batteries must not be short-circuited. Cells or batteries must not be stored in a box or in a drawer where they can short-circuit each other, or where they can be short-circuited by other conductive materials. Cells and batteries must not be removed from their original packaging until they are ready to be used.
4. Cells and batteries must not be exposed to any mechanical shocks that are stronger than permitted.
5. If a cell develops a leak, the fluid must not be allowed to come into contact with the skin or eyes. If contact occurs, wash the affected area with plenty of water and seek medical aid.
6. Improperly replacing or charging cells or batteries that contain alkaline electrolytes (e.g. lithium cells) can cause explosions. Replace cells or batteries only with the matching Rohde & Schwarz type (see parts list) in order to ensure the safety of the product.
7. Cells and batteries must be recycled and kept separate from residual waste. Rechargeable batteries and normal batteries that contain lead, mercury or cadmium are hazardous waste. Observe the national regulations regarding waste disposal and recycling.

Transport

1. The product may be very heavy. Therefore, the product must be handled with care. In some cases, the user may require a suitable means of lifting or moving the product (e.g. with a lift-truck) to avoid back or other physical injuries.
2. Handles on the products are designed exclusively to enable personnel to transport the product. It is therefore not permissible to use handles to fasten the product to or on transport equipment such as cranes, fork lifts, wagons, etc. The user is responsible for securely fastening the products to or on the means of transport or lifting. Observe the safety regulations of the manufacturer of the means of transport or lifting. Noncompliance can result in personal injury or material damage.
3. If you use the product in a vehicle, it is the sole responsibility of the driver to drive the vehicle safely and properly. The manufacturer assumes no responsibility for accidents or collisions. Never use the product in a moving vehicle if doing so could distract the driver of the vehicle. Adequately secure the product in the vehicle to prevent injuries or other damage in the event of an accident.

Waste disposal/Environmental protection

1. Specially marked equipment has a battery or accumulator that must not be disposed of with unsorted municipal waste, but must be collected separately. It may only be disposed of at a suitable collection point or via a Rohde & Schwarz customer service center.
2. Waste electrical and electronic equipment must not be disposed of with unsorted municipal waste, but must be collected separately.
   Rohde & Schwarz GmbH & Co. KG has developed a disposal concept and takes full responsibility for take-back obligations and disposal obligations for manufacturers within the EU. Contact your Rohde & Schwarz customer service center for environmentally responsible disposal of the product.
3. If products or their components are mechanically and/or thermally processed in a manner that goes beyond their intended use, hazardous substances (heavy-metal dust such as lead, beryllium, nickel) may be released. For this reason, the product may only be disassembled by specially trained personnel. Improper disassembly may be hazardous to your health. National waste disposal regulations must be observed.
4. If handling the product releases hazardous substances or fuels that must be disposed of in a special way, e.g. coolants or engine oils that must be replenished regularly, the safety instructions of the manufacturer of the hazardous substances or fuels and the applicable regional waste disposal regulations must be observed. Also observe the relevant safety instructions in the product documentation. The improper disposal of hazardous substances or fuels can cause health problems and lead to environmental damage.

For additional information about environmental protection, visit the Rohde & Schwarz website.

Instrucciones de seguridad elementales

¡Es imprescindible leer y cumplir las siguientes instrucciones e informaciones de seguridad!

El principio del grupo de empresas Rohde & Schwarz consiste en tener nuestros productos siempre al día con los estándares de seguridad y de ofrecer a nuestros clientes el máximo grado de seguridad. Nuestros productos y todos los equipos adicionales son siempre fabricados y examinados según las normas de seguridad vigentes. Nuestro sistema de garantía de calidad controla constantemente que sean cumplidas estas normas. El presente producto ha sido fabricado y examinado según el certificado de conformidad de la UE y ha salido de nuestra planta en estado impecable según los estándares técnicos de seguridad. Para poder preservar este estado y garantizar un funcionamiento libre de peligros, el usuario deberá atenerse a todas las indicaciones, informaciones de seguridad y notas de alerta. El grupo de empresas Rohde & Schwarz está siempre a su disposición en caso de que tengan preguntas referentes a estas informaciones de seguridad.

Además queda en la responsabilidad del usuario utilizar el producto en la forma debida. Este producto está destinado exclusivamente al uso en la industria y el laboratorio o, si ha sido expresamente autorizado, para aplicaciones de campo y de ninguna manera deberá ser utilizado de modo que alguna persona/cosa pueda sufrir daño. El uso del producto fuera de sus fines definidos o sin tener en cuenta las instrucciones del fabricante queda en la responsabilidad del usuario. El fabricante no se hace en ninguna forma responsable de consecuencias a causa del mal uso del producto.

Se parte del uso correcto del producto para los fines definidos si el producto es utilizado conforme a las indicaciones de la correspondiente documentación del producto y dentro del margen de rendimiento definido (ver hoja de datos, documentación, informaciones de seguridad que siguen). El uso del producto hace necesarios conocimientos técnicos y ciertos conocimientos del idioma inglés. Por eso se debe tener en cuenta que el producto solo pueda ser operado por personal especializado o personas instruidas en profundidad con las capacidades correspondientes. Si fuera necesaria indumentaria de seguridad para el uso de productos de Rohde & Schwarz, encontraría la información debida en la documentación del producto en el capítulo correspondiente. Guarde bien las informaciones de seguridad elementales, así como la documentación del producto, y entréguelas a usuarios posteriores.

Tener en cuenta las informaciones de seguridad sirve para evitar en lo posible lesiones o daños por peligros de toda clase. Por eso es imprescindible leer detalladamente y comprender por completo las siguientes informaciones de seguridad antes de usar el producto, y respetarlas durante el uso del producto. Deberán tenerse en cuenta todas las demás informaciones de seguridad, como p. ej. las referentes a la protección de personas, que encontrarán en el capítulo correspondiente de la documentación del producto y que también son de obligado cumplimiento. En las presentes informaciones de seguridad se recogen todos los objetos que distribuye el grupo de empresas Rohde & Schwarz bajo la denominación de "producto", entre ellos también aparatos, instalaciones así como toda clase de accesorios. Los datos específicos del producto figuran en la hoja de datos y en la documentación del producto.

Señalización de seguridad de los productos

Las siguientes señales de seguridad se utilizan en los productos para advertir sobre riesgos y peligros.

Símbolo	Significado	Símbolo	Significado
	Aviso: punto de peligro general Observar la documentación del producto		Tensión de alimentación de PUESTA EN MARCHA / PARADA
	Atención en el manejo de dispositivos de peso elevado		Indicación de estado de espera (standby)
	Peligro de choque eléctrico		Corriente continua (DC)
	Advertencia: superficie caliente		Corriente alterna (AC)
	Conexión a conductor de protección		Corriente continua / Corriente alterna (DC/AC)
	Conexión a tierra		El aparato está protegido en su totalidad por un aislamiento doble (reforzado)
	Conexión a masa		Distintivo de la UE para baterías y acumuladores Más información en la sección "Eliminación/protección del medio ambiente", punto 1.

Símbolo	Significado	Símbolo	Significado
	Aviso: Cuidado en el manejo de dispositivos sensibles a la electrostática (ESD)		Distintivo de la UE para la eliminación por separado de dispositivos eléctricos y electrónicos Más información en la sección "Eliminación/protección del medio ambiente", punto 2.
	Advertencia: rayo láser Más información en la sección "Funcionamiento", punto 7.		

Palabras de señal y su significado

En la documentación del producto se utilizan las siguientes palabras de señal con el fin de advertir contra riesgos y peligros.

PELIGRO — Indica una situación de peligro que, si no se evita, causa lesiones graves o incluso la muerte.

ADVERTENCIA — Indica una situación de peligro que, si no se evita, puede causar lesiones graves o incluso la muerte.

ATENCIÓN — Indica una situación de peligro que, si no se evita, puede causar lesiones leves o moderadas.

AVISO — Indica información que se considera importante, pero no en relación con situaciones de peligro; p. ej., avisos sobre posibles daños materiales.
En la documentación del producto se emplea de forma sinónima el término CUIDADO.

Las palabras de señal corresponden a la definición habitual para aplicaciones civiles en el área económica europea. Pueden existir definiciones diferentes a esta definición en otras áreas económicas o en aplicaciones militares. Por eso se deberá tener en cuenta que las palabras de señal aquí descritas sean utilizadas siempre solamente en combinación con la correspondiente documentación del producto y solamente en combinación con el producto correspondiente. La utilización de las palabras de señal en combinación con productos o documentaciones que no les correspondan puede llevar a interpretaciones equivocadas y tener por consecuencia daños en personas u objetos.

Estados operativos y posiciones de funcionamiento

El producto solamente debe ser utilizado según lo indicado por el fabricante respecto a los estados operativos y posiciones de funcionamiento sin que se obstruya la ventilación. Si no se siguen las indicaciones del fabricante, pueden producirse choques eléctricos, incendios y/o lesiones graves con posible consecuencia de muerte. En todos los trabajos deberán ser tenidas en cuenta las normas nacionales y locales de seguridad del trabajo y de prevención de accidentes.

1. Si no se convino de otra manera, es para los productos Rohde & Schwarz válido lo que sigue: como posición de funcionamiento se define por principio la posición con el suelo de la caja para abajo, modo de protección IP 2X, uso solamente en estancias interiores, utilización hasta 2000 m sobre el nivel del mar, transporte hasta 4500 m sobre el nivel del mar. Se aplicará una tolerancia de ±10 % sobre el voltaje nominal y de ±5 % sobre la frecuencia nominal. Categoría de sobrecarga eléctrica 2, índice de suciedad 2.
2. No sitúe el producto encima de superficies, vehículos, estantes o mesas, que por sus características de peso o de estabilidad no sean aptos para él. Siga siempre las instrucciones de instalación del fabricante cuando instale y asegure el producto en objetos o estructuras (p. ej. paredes y estantes). Si se realiza la instalación de modo distinto al indicado en la documentación del producto, se pueden causar lesiones o, en determinadas circunstancias, incluso la muerte.
3. No ponga el producto sobre aparatos que generen calor (p. ej. radiadores o calefactores). La temperatura ambiente no debe superar la temperatura máxima especificada en la documentación del producto o en la hoja de datos. En caso de sobrecalentamiento del producto, pueden producirse choques eléctricos, incendios y/o lesiones graves con posible consecuencia de muerte.

Seguridad eléctrica

Si no se siguen (o se siguen de modo insuficiente) las indicaciones del fabricante en cuanto a seguridad eléctrica, pueden producirse choques eléctricos, incendios y/o lesiones graves con posible consecuencia de muerte.

1. Antes de la puesta en marcha del producto se deberá comprobar siempre que la tensión preseleccionada en el producto coincida con la de la red de alimentación eléctrica. Si es necesario modificar el ajuste de tensión, también se deberán cambiar en caso dado los fusibles correspondientes del producto.
2. Los productos de la clase de protección I con alimentación móvil y enchufe individual solamente podrán enchufarse a tomas de corriente con contacto de seguridad y con conductor de protección conectado.
3. Queda prohibida la interrupción intencionada del conductor de protección, tanto en la toma de corriente como en el mismo producto. La interrupción puede tener como consecuencia el riesgo de que el producto sea fuente de choques eléctricos. Si se utilizan cables alargadores o regletas de enchufe, deberá garantizarse la realización de un examen regular de los mismos en cuanto a su estado técnico de seguridad.
4. Si el producto no está equipado con un interruptor para desconectarlo de la red, o bien si el interruptor existente no resulta apropiado para la desconexión de la red, el enchufe del cable de conexión se deberá considerar como un dispositivo de desconexión.
   El dispositivo de desconexión se debe poder alcanzar fácilmente y debe estar siempre bien accesible. Si, p. ej., el enchufe de conexión a la red es el dispositivo de desconexión, la longitud del cable de conexión no debe superar 3 m).
   Los interruptores selectores o electrónicos no son aptos para el corte de la red eléctrica. Si se integran productos sin interruptor en bastidores o instalaciones, se deberá colocar el interruptor en el nivel de la instalación.
5. No utilice nunca el producto si está dañado el cable de conexión a red. Compruebe regularmente el correcto estado de los cables de conexión a red. Asegúrese, mediante las medidas de protección y de instalación adecuadas, de que el cable de conexión a red no pueda ser dañado o de que nadie pueda ser dañado por él, p. ej. al tropezar o por un choque eléctrico.

6. Solamente está permitido el funcionamiento en redes de alimentación TN/TT aseguradas con fusibles de 16 A como máximo (utilización de fusibles de mayor amperaje solo previa consulta con el grupo de empresas Rohde & Schwarz).
7. Nunca conecte el enchufe en tomas de corriente sucias o llenas de polvo. Introduzca el enchufe por completo y fuertemente en la toma de corriente. La no observación de estas medidas puede provocar chispas, fuego y/o lesiones.
8. No sobrecargue las tomas de corriente, los cables alargadores o las regletas de enchufe ya que esto podría causar fuego o choques eléctricos.
9. En las mediciones en circuitos de corriente con una tensión U_{eff} > 30 V se deberán tomar las medidas apropiadas para impedir cualquier peligro (p. ej. medios de medición adecuados, seguros, limitación de tensión, corte protector, aislamiento etc.).
10. Para la conexión con dispositivos informáticos como un PC o un ordenador industrial, debe comprobarse que éstos cumplan los estándares IEC60950-1/EN60950-1 o IEC61010-1/EN 61010-1 válidos en cada caso.
11. A menos que esté permitido expresamente, no retire nunca la tapa ni componentes de la carcasa mientras el producto esté en servicio. Esto pone a descubierto los cables y componentes eléctricos y puede causar lesiones, fuego o daños en el producto.
12. Si un producto se instala en un lugar fijo, se deberá primero conectar el conductor de protección fijo con el conductor de protección del producto antes de hacer cualquier otra conexión. La instalación y la conexión deberán ser efectuadas por un electricista especializado.
13. En el caso de dispositivos fijos que no estén provistos de fusibles, interruptor automático ni otros mecanismos de seguridad similares, el circuito de alimentación debe estar protegido de modo que todas las personas que puedan acceder al producto, así como el producto mismo, estén a salvo de posibles daños.
14. Todo producto debe estar protegido contra sobretensión (debida p. ej. a una caída del rayo) mediante los correspondientes sistemas de protección. Si no, el personal que lo utilice quedará expuesto al peligro de choque eléctrico.
15. No debe introducirse en los orificios de la caja del aparato ningún objeto que no esté destinado a ello. Esto puede producir cortocircuitos en el producto y/o puede causar choques eléctricos, fuego o lesiones.
16. Salvo indicación contraria, los productos no están impermeabilizados (ver también el capítulo "Estados operativos y posiciones de funcionamiento", punto 1). Por eso es necesario tomar las medidas necesarias para evitar la entrada de líquidos. En caso contrario, existe peligro de choque eléctrico para el usuario o de daños en el producto, que también pueden redundar en peligro para las personas.
17. No utilice el producto en condiciones en las que pueda producirse o ya se hayan producido condensaciones sobre el producto o en el interior de éste, como p. ej. al desplazarlo de un lugar frío a otro caliente. La entrada de agua aumenta el riesgo de choque eléctrico.
18. Antes de la limpieza, desconecte por completo el producto de la alimentación de tensión (p. ej. red de alimentación o batería). Realice la limpieza de los aparatos con un paño suave, que no se deshilache. No utilice bajo ningún concepto productos de limpieza químicos como alcohol, acetona o diluyentes para lacas nitrocelulósicas.

Funcionamiento

1. El uso del producto requiere instrucciones especiales y una alta concentración durante el manejo. Debe asegurarse que las personas que manejen el producto estén a la altura de los requerimientos necesarios en cuanto a aptitudes físicas, psíquicas y emocionales, ya que de otra manera no se pueden excluir lesiones o daños de objetos. El empresario u operador es responsable de seleccionar el personal usuario apto para el manejo del producto.
2. Antes de desplazar o transportar el producto, lea y tenga en cuenta el capítulo "Transporte".
3. Como con todo producto de fabricación industrial no puede quedar excluida en general la posibilidad de que se produzcan alergias provocadas por algunos materiales empleados —los llamados alérgenos (p. ej. el níquel)—. Si durante el manejo de productos Rohde & Schwarz se producen reacciones alérgicas, como p. ej. irritaciones cutáneas, estornudos continuos, enrojecimiento de la conjuntiva o dificultades respiratorias, debe avisarse inmediatamente a un médico para investigar las causas y evitar cualquier molestia o daño a la salud.
4. Antes de la manipulación mecánica y/o térmica o el desmontaje del producto, debe tenerse en cuenta imprescindiblemente el capítulo "Eliminación/protección del medio ambiente", punto 1.
5. Ciertos productos, como p. ej. las instalaciones de radiocomunicación RF, pueden a causa de su función natural, emitir una radiación electromagnética aumentada. Deben tomarse todas las medidas necesarias para la protección de las mujeres embarazadas. También las personas con marcapasos pueden correr peligro a causa de la radiación electromagnética. El empresario/operador tiene la obligación de evaluar y señalizar las áreas de trabajo en las que exista un riesgo elevado de exposición a radiaciones.
6. Tenga en cuenta que en caso de incendio pueden desprenderse del producto sustancias tóxicas (gases, líquidos etc.) que pueden generar daños a la salud. Por eso, en caso de incendio deben usarse medidas adecuadas, como p. ej. máscaras antigás e indumentaria de protección.
7. Los productos con láser están provistos de indicaciones de advertencia normalizadas en función de la clase de láser del que se trate. Los rayos láser pueden provocar daños de tipo biológico a causa de las propiedades de su radiación y debido a su concentración extrema de potencia electromagnética. En caso de que un producto Rohde & Schwarz contenga un producto láser (p. ej. un lector de CD/DVD), no debe usarse ninguna otra configuración o función aparte de las descritas en la documentación del producto, a fin de evitar lesiones (p. ej. debidas a irradiación láser).
8. Clases de compatibilidad electromagnética (conforme a EN 55011 / CISPR 11; y en analogía con EN 55022 / CISPR 22, EN 55032 / CISPR 32)
   - Aparato de clase A:
     Aparato adecuado para su uso en todos los entornos excepto en los residenciales y en aquellos conectados directamente a una red de distribución de baja tensión que suministra corriente a edificios residenciales.
     Nota: Los aparatos de clase A están destinados al uso en entornos industriales. Estos aparatos pueden causar perturbaciones radioeléctricas en entornos residenciales debido a posibles perturbaciones guiadas o radiadas. En este caso, se le podrá solicitar al operador que tome las medidas adecuadas para eliminar estas perturbaciones.
   - Aparato de clase B:
     Aparato adecuado para su uso en entornos residenciales, así como en aquellos conectados directamente a una red de distribución de baja tensión que suministra corriente a edificios residenciales.

Reparación y mantenimiento

1. El producto solamente debe ser abierto por personal especializado con autorización para ello. Antes de manipular el producto o abrirlo, es obligatorio desconectarlo de la tensión de alimentación, para evitar toda posibilidad de choque eléctrico.
2. El ajuste, el cambio de partes, el mantenimiento y la reparación deberán ser efectuadas solamente por electricistas autorizados por Rohde & Schwarz. Si se reponen partes con importancia para los aspectos de seguridad (p. ej. el enchufe, los transformadores o los fusibles), solamente podrán ser sustituidos por partes originales. Después de cada cambio de partes relevantes para la seguridad deberá realizarse un control de seguridad (control a primera vista, control del conductor de protección, medición de resistencia de aislamiento, medición de la corriente de fuga, control de funcionamiento). Con esto queda garantizada la seguridad del producto.

Baterías y acumuladores o celdas

Si no se siguen (o se siguen de modo insuficiente) las indicaciones en cuanto a las baterías y acumuladores o celdas, pueden producirse explosiones, incendios y/o lesiones graves con posible consecuencia de muerte. El manejo de baterías y acumuladores con electrolitos alcalinos (p. ej. celdas de litio) debe seguir el estándar EN 62133.

1. No deben desmontarse, abrirse ni triturarse las celdas.
2. Las celdas o baterías no deben someterse a calor ni fuego. Debe evitarse el almacenamiento a la luz directa del sol. Las celdas y baterías deben mantenerse limpias y secas. Limpiar las conexiones sucias con un paño seco y limpio.
3. Las celdas o baterías no deben cortocircuitarse. Es peligroso almacenar las celdas o baterías en estuches o cajones en cuyo interior puedan cortocircuitarse por contacto recíproco o por contacto con otros materiales conductores. No deben extraerse las celdas o baterías de sus embalajes originales hasta el momento en que vayan a utilizarse.
4. Las celdas o baterías no deben someterse a impactos mecánicos fuertes indebidos.
5. En caso de falta de estanqueidad de una celda, el líquido vertido no debe entrar en contacto con la piel ni los ojos. Si se produce contacto, lavar con agua abundante la zona afectada y avisar a un médico.
6. En caso de cambio o recarga inadecuados, las celdas o baterías que contienen electrolitos alcalinos (p. ej. las celdas de litio) pueden explotar. Para garantizar la seguridad del producto, las celdas o baterías solo deben ser sustituidas por el tipo Rohde & Schwarz correspondiente (ver lista de recambios).
7. Las baterías y celdas deben reciclarse y no deben tirarse a la basura doméstica. Las baterías o acumuladores que contienen plomo, mercurio o cadmio deben tratarse como residuos especiales. Respete en esta relación las normas nacionales de eliminación y reciclaje.

Transporte

1. El producto puede tener un peso elevado. Por eso es necesario desplazarlo o transportarlo con precaución y, si es necesario, usando un sistema de elevación adecuado (p. ej. una carretilla elevadora), a fin de evitar lesiones en la espalda u otros daños personales.

2. Las asas instaladas en los productos sirven solamente de ayuda para el transporte del producto por personas. Por eso no está permitido utilizar las asas para la sujeción en o sobre medios de transporte como p. ej. grúas, carretillas elevadoras de horquilla, carros etc. Es responsabilidad suya fijar los productos de manera segura a los medios de transporte o elevación. Para evitar daños personales o daños en el producto, siga las instrucciones de seguridad del fabricante del medio de transporte o elevación utilizado.
3. Si se utiliza el producto dentro de un vehículo, recae de manera exclusiva en el conductor la responsabilidad de conducir el vehículo de manera segura y adecuada. El fabricante no asumirá ninguna responsabilidad por accidentes o colisiones. No utilice nunca el producto dentro de un vehículo en movimiento si esto pudiera distraer al conductor. Asegure el producto dentro del vehículo debidamente para evitar, en caso de un accidente, lesiones u otra clase de daños.

Eliminación/protección del medio ambiente

1. Los dispositivos marcados contienen una batería o un acumulador que no se debe desechar con los residuos domésticos sin clasificar, sino que debe ser recogido por separado. La eliminación se debe efectuar exclusivamente a través de un punto de recogida apropiado o del servicio de atención al cliente de Rohde & Schwarz.
2. Los dispositivos eléctricos usados no se deben desechar con los residuos domésticos sin clasificar, sino que deben ser recogidos por separado.
   Rohde & Schwarz GmbH & Co.KG ha elaborado un concepto de eliminación de residuos y asume plenamente los deberes de recogida y eliminación para los fabricantes dentro de la UE. Para desechar el producto de manera respetuosa con el medio ambiente, diríjase a su servicio de atención al cliente de Rohde & Schwarz.
3. Si se trabaja de manera mecánica y/o térmica cualquier producto o componente más allá del funcionamiento previsto, pueden liberarse sustancias peligrosas (polvos con contenido de metales pesados como p. ej. plomo, berilio o níquel). Por eso el producto solo debe ser desmontado por personal especializado con formación adecuada. Un desmontaje inadecuado puede ocasionar daños para la salud. Se deben tener en cuenta las directivas nacionales referentes a la eliminación de residuos.
4. En caso de que durante el trato del producto se formen sustancias peligrosas o combustibles que deban tratarse como residuos especiales (p. ej. refrigerantes o aceites de motor con intervalos de cambio definidos), deben tenerse en cuenta las indicaciones de seguridad del fabricante de dichas sustancias y las normas regionales de eliminación de residuos. Tenga en cuenta también en caso necesario las indicaciones de seguridad especiales contenidas en la documentación del producto. La eliminación incorrecta de sustancias peligrosas o combustibles puede causar daños a la salud o daños al medio ambiente.

Se puede encontrar más información sobre la protección del medio ambiente en la página web de Rohde & Schwarz.

Customer Support

Technical support – where and when you need it

For quick, expert help with any Rohde & Schwarz equipment, contact one of our Customer Support Centers. A team of highly qualified engineers provides telephone support and will work with you to find a solution to your query on any aspect of the operation, programming or applications of Rohde & Schwarz equipment.

Up-to-date information and upgrades

To keep your instrument up-to-date and to be informed about new application notes related to your instrument, please send an e-mail to the Customer Support Center stating your instrument and your wish. We will take care that you will get the right information.

Europe, Africa, Middle East

Phone +49 89 4129 12345
customersupport@rohde-schwarz.com

North America

Phone 1-888-TEST-RSA (1-888-837-8772)
customer.support@rsa.rohde-schwarz.com

Latin America

Phone +1-410-910-7988
customersupport.la@rohde-schwarz.com

Asia/Pacific

Phone +65 65 13 04 88
customersupport.asia@rohde-schwarz.com

China

Phone +86-800-810-8228 /
+86-400-650-5896
customersupport.china@rohde-schwarz.com

ROHDE&SCHWARZ

1171.0200.22-06.00

Contents

1 Preface....9

1.1 Documentation Overview....9

1.2 Conventions Used in the Documentation....10

1.2.1 Typographical Conventions....10

2 Acquisition and Waveform Setup....11

2.1 Basics....11

2.1.1 Vertical System....11

2.1.2 Sampling and Acquisition....12

2.1.3 Horizontal System....15

2.1.4 Probes....16

2.2 Setting up the Waveform....20

2.2.1 Setting Up the Signal Input with Autoset....20

2.2.2 Adjusting the Signal Input Manually....20

2.2.3 Setting the Acquisition....21

2.2.4 Starting and Stopping Acquisition....21

2.3 Reference for Waveform Setup....22

2.3.1 HORIZONTAL Controls....22

2.3.2 Acquisition Menu....23

2.3.3 Vertical Settings....27

3 Triggers....36

3.1 Basics of Triggering....36

3.2 Setting Up the Trigger....37

3.2.1 Configuring the Trigger Event....37

3.2.2 Positioning the Trigger....38

3.2.3 Setting Up a Trigger Sequence....38

3.3 Reference for Triggers....39

3.3.1 TRIGGER Controls....39

3.3.2 Trigger Settings....40

4 Display....54

4.1 General Display Settings....54

4.1.1 Configuring the Display....55
4.1.2 Display Menu....57
4.2 XY-Diagram....61
4.2.1 Configuring XY-Diagrams....62
4.2.2 XYZ Setup Menu....64
4.3 Zoom....66
4.3.1 Zoom Display....66
4.3.2 Zooming for Details....68
4.3.3 Zoom Menu....69
4.4 Markers....71
4.4.1 Using Timestamp Markers....71
4.4.2 Reference for Markers....73
5 Reference Waveforms....74
5.1 Using References....74
5.1.1 Displaying a Reference Waveform....74
5.1.2 Saving and Loading References....75
5.2 Reference for REF key....76
6 Measurements....78
6.1 Cursor Measurements....78
6.1.1 Cursor Measurements Types and Results....78
6.1.2 Performing Cursor Measurements....81
6.1.3 Cursor Menu....82
6.2 Quick Measurements....85
6.3 Automatic Measurements....87
6.3.1 Measurement Types and Results....87
6.3.2 Configuring and Performing Automatic Measurements....93
6.3.3 Auto Measure Menu (MEAS key)....94
7 Mathematics....98
7.1 Configuring and Using Math Waveforms....98
7.1.1 Displaying Mathematical Waveforms....98
7.1.2 Editing Equations and Equation Sets....99
7.1.3 Saving and Loading Equation Sets....100

7.2 Reference for Mathematics....101

8 FFT....110

8.1 FFT Display....110

8.2 Configuring and Using FFT Calculations....111

8.2.1 Setting Up the FFT Analysis....111

8.2.2 Configuring the Diagrams....112

8.2.3 Measuring on FFT....115

8.3 Reference for FFT key....115

9 Masks....122

9.1 About Masks....122

9.1.1 Masks....122

9.1.2 Mask Testing....122

9.1.3 File Formats for Masks....123

9.2 Working with Masks....124

9.2.1 Creating New Masks....125

9.2.2 Loading Masks....127

9.2.3 Performing a Mask Test....127

9.3 Reference for MASKS key....128

10 Search....132

10.1 Search Conditions and Results....132

10.1.1 Search Results....132

10.2 Configuring and Performing Searches....134

10.3 Reference for Search Menu....135

10.3.1 Main Search Menu....135

10.3.2 Edge Setup....137

10.3.3 Width Setup....138

10.3.4 Peak Setup....139

10.3.5 Rise/Fall Time Setup....139

10.3.6 Runt Setup....141

10.3.7 Data2Clock Search....142

10.3.8 Pattern Search....144

10.3.9 Gate Menu....146

10.3.10 Events Menu....147

11 Protocol Analysis....148

11.1 Basics of Protocol Analysis....148

11.1.1 Configuring Common Protocol Settings....148

11.1.2 Protocol - Common Settings....149

11.1.3 Display Settings....150

11.1.4 Label List....151

11.1.5 Frame Table: Decode Results....154

11.2 SPI/SSPI Bus (Option R&S RTM-K1)....155

11.2.1 The SPI Protocol....155

11.2.2 SPI/SSPI Bus Configuration....156

11.2.3 SPI/SSPI Trigger....159

11.2.4 SPI/SSPI Decode Results....162

11.3 I²C (Option R&S RTM-K1)....165

11.3.1 The I²C Protocol....165

11.3.2 I²C Configuration....167

11.3.3 I²C Trigger....168

11.3.4 I²C Label List....172

11.3.5 I²C Decode Results....173

11.4 UART/RS-232 Interface (Option R&S RTM-K2)....175

11.4.1 The UART / RS232 Interface....175

11.4.2 UART/RS-232 Configuration....176

11.4.3 UART/RS-232 Trigger....179

11.4.4 UART/RS-232 Decode Results....183

11.5 CAN (Option R&S RTM-K3)....185

11.5.1 CAN Configuration....185

11.5.2 CAN Trigger Settings....186

11.5.3 CAN Label List....191

11.5.4 CAN Decode Results....192

11.5.5 Search on Decoded CAN Data....194

11.6 LIN (Option R&S RTM-K3)....197

11.6.1 The LIN Protocol....197

11.6.2 LIN Configuration Settings....198

11.6.3 LIN Trigger Settings....199
11.6.4 LIN Label List....202
11.6.5 LIN Decode Results....203
11.6.6 Search on Decoded LIN Data....205

12 Mixed Signal Option (MSO, R&S RTM-B1)....208
12.1 About MSO....208
12.2 Digital Channels....209
12.2.1 Digital Channels - Configuration Settings....209
12.3 Parallel Buses....211
12.3.1 Analyzing Parallel Buses....211
12.3.2 Parallel Clocked Bus....212
12.3.3 Parallel Bus (Unclocked)....213

13 Data and File Management....215
13.1 Printing....215
13.1.1 Printing a Screenshot....215
13.1.2 Printer Settings....216
13.2 Saving and Loading....217
13.2.1 Storage Locations....217
13.2.2 Quick Access with PRINT key....223
13.2.3 Device Settings....225
13.2.4 Waveforms....227
13.2.5 Screenshots....230
13.2.6 References, Masks, and Equation Sets: Import/Export....232

14 General Instrument Setup....233
14.1 Firmware and Options....233
14.1.1 Updating Firmware....233
14.1.2 Activating Options....234
14.2 Reference for Setup....234

15 Remote Control....241
15.1 Basics....241
15.1.1 Remote Control Interfaces....241
15.1.2 Setting Up a LAN Connection....243

15.1.3 Switching to Remote Control....248
15.1.4 Messages and Command Structure....248
15.1.5 Command Sequence and Synchronization....259
15.1.6 Status Reporting System....261
15.1.7 General Programming Recommendations....272
15.2 Command Reference....273
15.2.1 Conventions used in Remote Command Description....273
15.2.2 Common Commands....274
15.2.3 General Remote Settings and Queries....277
15.2.4 Acquisition and Setup....281
15.2.5 Trigger....301
15.2.6 Display....314
15.2.7 Reference Waveforms....322
15.2.8 Measurements....326
15.2.9 Mathematics....345
15.2.10 FFT....348
15.2.11 Masks....354
15.2.12 Search....358
15.2.13 Protocol Analysis....374
15.2.14 Mixed Signal Option (MSO, R&S RTM-B1)....434
15.2.15 Data and File Management....441
15.2.16 General Instrument Setup....450
15.2.17 Status Reporting....453
15.3 Programming Examples....458
15.3.1 Data Export....458
15.3.2 Search....460
15.3.3 Data and File Management....461
List of Commands....463
Index....476

1 Preface

1.1 Documentation Overview

The user documentation for the R&S RTM consists of the following parts:

- Online Help system on the instrument
- "Getting Started" printed manual in English
- Documentation CD-ROM with:
  - Getting Started
  - User Manual
  - Service Manual
  - Data sheet and product brochure
  - Firmware package including the online help
  - Links to useful sites on the Rohde & Schwarz internet

Online Help

The Online Help is embedded in the instrument's firmware. It offers quick, context-sensitive description of the softkeys and front panel controls at the push of the HELP key.

Getting Started

The English edition of this manual is delivered with the instrument in printed form. The manual is also available in other languages in PDF format on the Documentation CD-ROM. It provides the information needed to set up and start working with the instrument, and describes basic operations and typical measurement examples. The manual includes also safety information.

User Manual

The user manual is available in PDF format on the Documentation CD-ROM. This manual describes all instrument functions in detail. It provides an introduction to remote control and a complete description of the remote control commands with programming examples.

Service Manual

The Service Manual is available in PDF format on the Documentation CD-ROM. It describes how to check compliance with rated specifications, instrument function, repair, troubleshooting and fault elimination. It contains all information required for repairing the instrument by replacing modules.

Documentation updates

You can download the newest version of the "Getting Started" and "User Manual" from the "Downloads > Manuals" section on the Rohde & Schwarz "Scope of the Art" Web page: http://www.scope-of-the-art.com/product/rtm.html.

The online help is included in the firmware update package. The help has to be updated separately to get the information suitable for the firmware version. The firmware and help update package is available in the "Downloads > Firmware" section on the Rohde & Schwarz "Scope of the Art" Web page, and on the Documentation CD-ROM.

1.2 Conventions Used in the Documentation

This chapter describes the conventions used throughout this documentation.

1.2.1 Typographical Conventions

The following text markers are used throughout this documentation:

Convention	Description
"Graphical user interface elements"	All names of graphical user interface elements on the screen, such as dialog boxes, menus, options, buttons, and softkeys are enclosed by quotation marks.
KEYS	Key names are written in capital letters.
`File names, commands, program code`	File names, commands, coding samples and screen output are distinguished by their font.
Input	Input to be entered by the user is displayed in italics.
Links	Links that you can click are displayed in blue font.
"References"	References to other parts of the documentation are enclosed by quotation marks.

2 Acquisition and Waveform Setup

The chapter describes the horizontal and vertical basic settings including the acquisition and probe settings.

2.1 Basics

This chapter provides background information on the essential settings in the vertical and horizontal systems, on acquisition setup and probing.

2.1.1 Vertical System

The controls and parameters of the vertical system are used to scale and position the waveform vertically.

2.1.1.1 Input coupling

The input coupling influences the signal path between input connector and the following internal signal stage. The coupling can be set to DC, AC, or ground.

- DC coupling shows all of an input signal. DC coupling is available with 1 MΩ input impedance to connect standard passive probes. DC coupling is the default for 50 Ω input impedance.
- AC coupling is useful if the DC component of a signal is of no interest. AC coupling blocks the DC component of the signal so that the waveform is centered around zero volts.

2.1.1.2 Vertical scale and position

Vertical scale and vertical position directly affect the resolution of the waveform amplitude. The vertical scale corresponds to the ADC input range. To get the full resolution of the ADC, waveforms should cover most of the height of the diagram.

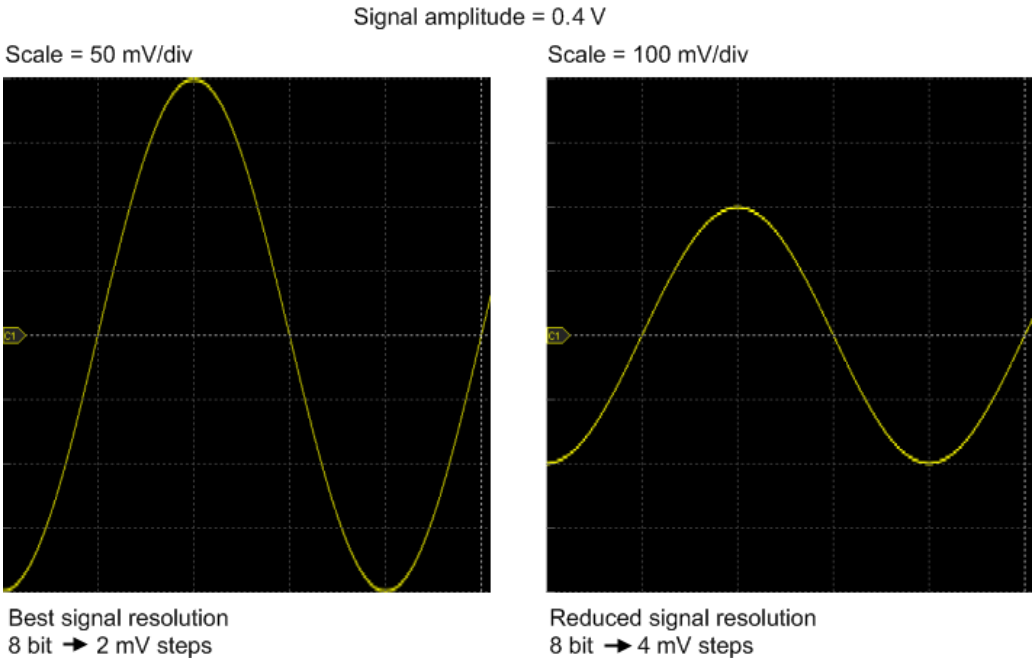

Fig. 2-1: Input range and resolution of the ADC

2.1.1.3 Bandwidth

For analog applications the highest signal frequency determines the required oscilloscope bandwidth. As a rule of thumb, the oscilloscope bandwidth should be 3 times higher than the maximum frequency included in the analog test signal to measure the amplitude with high accuracy.

Most test signals are more complex than a simple sine wave and include several spectral components. A digital signal, for example, is built up of several odd harmonics. As a rule of thumb, for digital signals the oscilloscope bandwidth should be 5 times higher than the clock frequency to be measured.

The oscilloscope is not a stand-alone system. You need a probe to measure the signal of interest, and the probe has a limited bandwidth, too. The combination of oscilloscope and probe creates a *system bandwidth*. To maintain the oscilloscope bandwidth, that is, to reduce the effect of the probe on the system bandwidth, the probe bandwidth should exceed the bandwidth of the oscilloscope, the recommended factor is 1.5 x oscilloscope bandwidth.

See also: chapter 2.1.4.1, "Voltage Probes", on page 16

2.1.2 Sampling and Acquisition

The vertical system of a digital oscilloscope conditions the test signal in a way that the following A/D Converter (ADC) can transform the measured voltage into digital data.

2.1.2.1 Sampling and Processing

The A/D converter samples the continuous signal under test at specific points in time and delivers digital values called **ADC samples**. The rate at which the converter is working is the **ADC sample rate**, a constant value usually specified in GHz: $f_{ADC} = 1 / T_I$

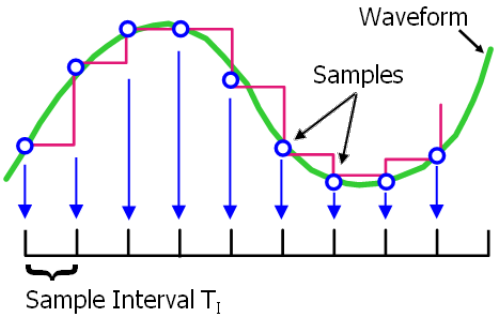

The digital ADC samples are processed according to the acquisition settings. The result is a waveform record that contains **waveform samples** and is stored in the **waveform memory**. The waveform samples are displayed on the screen and build up the waveform.

The number of waveform samples in one waveform record is called **record length**, and the rate of recording waveform samples - the number of waveform samples per second - is the **sample rate**. The higher the sample rate, the better is the resolution and the more details of the waveform are visible.

A sufficient resolution is essential for correct reconstruction of the waveform. If the signal is undersampled, aliasing occurs - a false waveform is displayed. To avoid aliasing and accurately reconstruct a signal, Nyquist theorem postulates that the sample rate must be at least twice as fast as the highest frequency component of the signal. However, the theorem assumes ideal conditions, so the Nyquist sample rate is usually not sufficient.

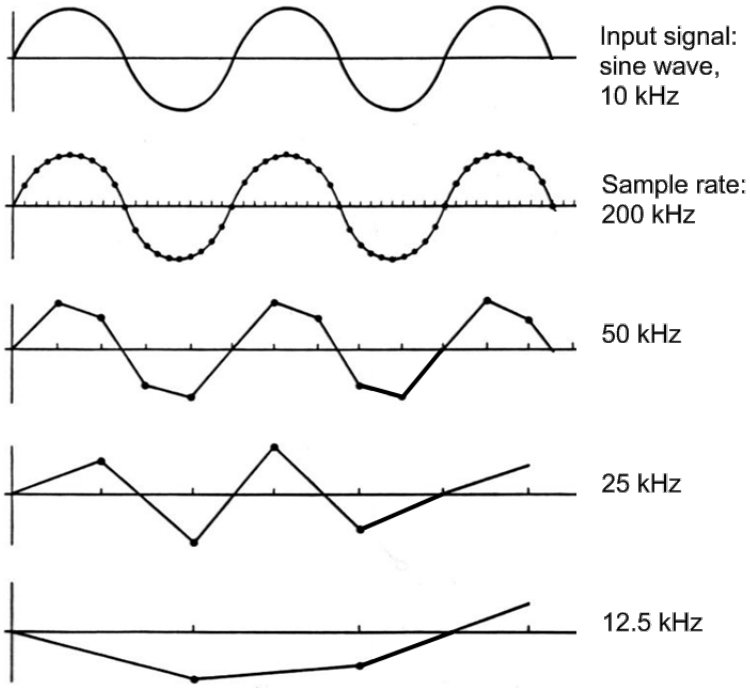

Fig. 2-2: Waveforms acquired with different sample rates

This means that the sample rate must be set to a value 3 to 5 times the fastest frequency component of the signal. A higher sample rate increases signal fidelity, increases the chance to capture glitches and other signal anomalies, and improves the zoom-in capabilities.

2.1.2.2 Acquisition Settings

The resulting sample rate can be the same as the constant ADC sample rate, or higher, or lower.

By default, the **real time sample mode** is used. With fast time base settings, the sample rate becomes higher than the ADC sample rate. The missising waveform samples are added to the ADC samples with sin(x)/x interpolation automatically.

When measuring high-frequency, repetitive signals whose frequency components are even higher than the ADC sample rate, **equivalent-time sampling** is used to capture the waveform. This sample mode captures ADC samples over a number of subsequent repetitions at different points in time, and creates one waveform with higher sample rate from this data.

At lower time base settings, the required sample rate is lower than the ADC sample rate. To reduce the sample rate, **decimation** methods are used: sample and peak detect.

As digital waveform data is stored in the memory, and the memory can save many waveform records, further **waveform arithmetic** processing is possible: average and envelope waveforms are resulting waveforms, created from a composite of sample points taken from multiple acquisitions. Another function called **smoothing** calculates a mean

value of several adjacent sample points of the same waveform and displays it. The result is a moving average that uses the full data and can be used for non-periodic signals.

2.1.2.3 Acquisition Control

You can run the R&S RTM in two ways:

- Continuous: the instrument acquires data until you stop it manually.
- NxSingle: the instrument samples and processes a specified number of acquisitions.

The determining point of an acquisition is the trigger. The instrument acquires continuously and keeps the sample points to fill the pre-trigger part of the waveform record. When the trigger occurs, the instrument continues acquisition until the post-trigger part of the waveform record is filled. Then it stops acquiring and waits for the next trigger. When a trigger is recognized, the instrument will not accept another trigger until the acquisition is complete.

The trigger modes define how the instrument triggers:

- Normal: The instrument acquires a waveform only if a real trigger occurs, that is, if all trigger conditions are fulfilled.
- Auto: The instrument triggers repeatedly after a fixed time interval if the trigger conditions are not fulfilled. If a real trigger occurs, it takes precedence. If the real trigger is faster than the auto trigger, both modes are virtually the same.

In practice, both trigger modes are useful: The auto mode lets you see the signal with very little adjustment, while the normal mode selects the interesting part of the waveform. If you want to acquire a specified number of waveforms with NxSingle, make sure to select the normal trigger mode. Thus you get only the required number of interesting acquisitions.

See also: chapter 3, "Triggers", on page 36

2.1.3 Horizontal System

As described before in chapter 2.1.2.3, "Acquisition Control", on page 15, the trigger is the determining point of the waveform record.

Two parameters set the position of the horizontal acquisition window in relation to the trigger point: **time reference** and **trigger offset**. Using these parameters, you choose the part of the waveform you want to see: around the trigger, before, or after the trigger.

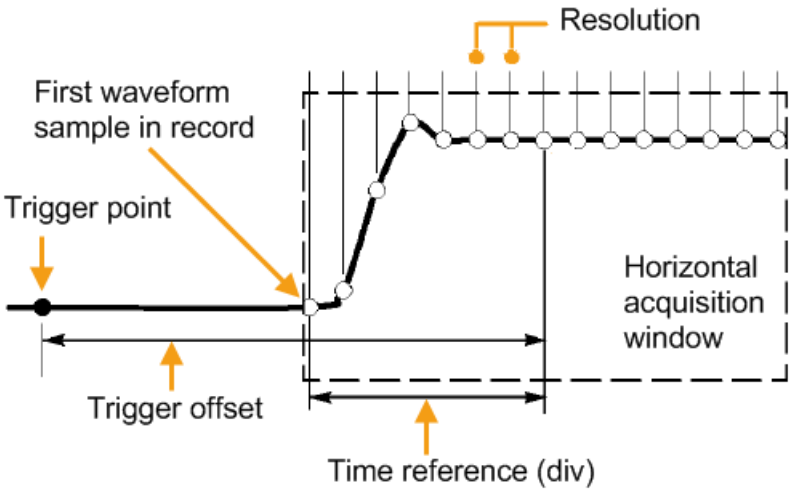

2.1.4 Probes

A probe connects the signal source (DUT) to the oscilloscope, and delivers the signal to be measured. It is the essential first link in the measurement chain.

An ideal probe fulfills the following requirements:

- Safe and reliable contacts
- Infinite bandwidth
- The probe should not load the signal source and thus impact the circuit operation.
- The connection should not introduce or suppress signal components (hum, noise, filter) and thus degrade or distort the transferred signal.

In reality, the probe can never be an ideal one, it always affects the signal transmission and the signal source, and thus the measured signal. It depends on the frequency to be measured and on the signal source to determine the acceptable loading, and to determine which kind of probe delivers good results.

The solution depends on the quantity to be measured with respect to:

- Signal type: voltage, current, power, pressure, optical, etc.
- Signal amplitude: The oscilloscope itself can only display voltages in a limited range. Most probes can adjust the dynamic range to amplitudes from a few mV to 10 V. Smaller or much larger signals require specialized equipment.
- Signal frequency: High frequencies require advanced equipment in order to get correct results.
- Source characteristic: The source impedance is the decisive factor when choosing the suitable connection.

2.1.4.1 Voltage Probes

The following table provides an overview on common voltage probes and their usage.

Table 2-1: Voltage probes overview

Probe type	Attenuation	Typical bandwidth range	Oscilloscope input	Usage
Passive, high impedance	1:1	10 MHz	1 MΩ	Low speed, low level signals
Passive, high impedance	10:1	500 MHz	1 MΩ	General purpose
Passive, low impedance	10:1	up to 10 GHz	50 Ω	High frequency
Active, single-ended	10:1	up to 10 GHz	50 Ω	High speed
Active, differential	10:1		50 Ω	Floating

For a list of recommended probes refer to the R&S RTM product brochure.

Besides the possible input voltage range, two factors are very important when selecting a voltage probe: Bandwidth and impedance over frequency.

- **Bandwidth:**
  The combination of probe and oscilloscope builds up a system. The resulting system bandwidth is approximately determined with:

  $$\frac{1}{BW_{system}} = \sqrt{\left(\frac{1}{BW_{probe}}\right)^2 + \left(\frac{1}{BW_{scope}}\right)^2}$$

  To measure the signal with low measurement error, the system bandwidth should be higher than the highest frequency component of the signal. The probe bandwidth must be even higher than the system bandwidth.
- **Impedance:**
  A minimum impedance is required to keep the circuit loading low. Over frequency, the impedance decreases, in particular with passive probes. The probe impedance should be approximately 10 times the impedance of the circuit test point at the highest signal frequency.

Passive voltage probes

Passive probes have the following qualities:

- No active components inside
- BNC connector for universal use
- Compensation needs to be executed when the probe is connected to a scope input:
  LF compensation matches the probe (mainly cable) capacitance to the oscilloscope input capacitance.
  High frequency adjustment is an option for higher measurement frequencies in the MHz range.
- With high impedance probes, the impedance varies significantly over frequency.
- With low impedance probes, the impedance variation over frequency is low, but the load on the source is high.

If you use passive probes, remember some recommendations:

- Use a probe recommended for your oscilloscope model.
- Use a ground lead as short as possible to minimize the effect of ground lead inductance. The resonance frequency can be much lower than the system bandwidth and thus can affect the measurement results, in particular, if you measure steep edge rise times.
- Select a probe that has a bandwidth of 5 to 10 times the highest frequency being measured. This will preserve the harmonics and thus the waveform integrity.

Active voltage probes - general

Active probes require operating power from the instrument and have a proprietary interface to the instrument. Their main qualities are:

- Low loading on signal source
- The probe is automatically recognized by the instrument, no adjustment is required.
- Adjustable DC offset at probe tip allows for high resolution on small AC signals which are superimposed on DC levels.
- Connections should be as short as possible to keep the usable bandwidth high.
- The operating voltage range has to be observed.
- The probe impedance depends on the signal frequency.

RT-ZS single-ended active probes and RT-ZD differential active probes provide special features for easier use and precise measurements. These special featuers are not available on RT-ZSxxE probes.

- The micro button on the probe head remotely controls important functions on the instrument, like running and stopping the acquisition, autoset, auto zero and setting the offset to mean value.
- The R&S ProbeMeter measures DC voltages between the probe tip and the ground connection with very high precision. The result is displayed on the instrument's screen. So you can check DC voltages with different levels without having to adjust the measurement range of the oscilloscope. The R&S ProbeMeter also measures the zero error of the probe to optimize measurement results at small signal levels.

When you connect an R&S RT-ZSxx active probe to a channel input of the R&S RTM, the oscilloscope recognizes the probe, reads the identification and calibration data from the probe box and shows the result in the "Setup" and "Probe Attributes" tabs. This data together with the deskew time for a given channel is stored and processed by the R&S RTM. If you connect the probe the next time to the same channel, the information is fetched and used.

Differential active probes

Differential active probes are designed to measure signals that are referenced against each other, and voltages that are not references to ground, for example twisted pair signal lines. The R&S RT-ZD probes are differential probes with high input impedance, they can be used to measure voltages between any two test points.

Compared with two-channel measurement setup with single-ended probes, the measurement with differential probes is symmetric due to the same amplification and cable

length on both paths. It is also immune to interference and noise and occupies only one input channel.

A differential probe has three sockets: the positive signal socket (+), the negative signal socket (-), and the ground socket.

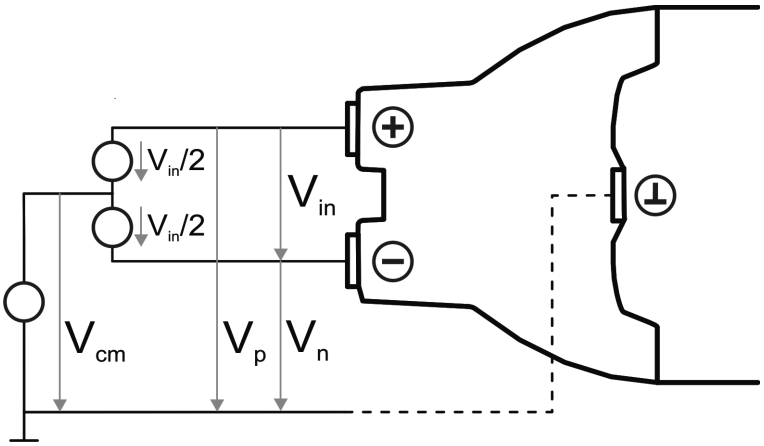

Differential probes provide multiple input voltages:

- Differential mode input voltage (V_{in})
  Voltage between the positive and negative signal sockets
- Positive single-ended input voltage (V_p)
  Voltage between the positive signal socket and the ground socket
- Negative single-ended input voltage (V_n)
  Voltage between the negative signal socket and the ground socket
- Common mode input voltage (V_{cm})
  Mean voltage of positive and negative signal sockets referred to the ground socket, respectively

Two of these voltages are independent values, the other two can be calculated:

$$V_{in} = V_p - V_n$$

$$V_{cm} = \frac{V_p + V_n}{2}$$

R&S RT-ZD probes detect only differential input voltages and provide it to the oscilloscope. Common mode signals are suppressed by the probe. This characteristic is described by the Common Mode Rejection Ratio (CMRR):

$$CMRR = \frac{DifferentialGain}{CommonModeGain}$$

In addition, the R&S ProbeMeter of R&S RT-ZD differential probes can measure differential and common mode DC voltages. The measurement result is displayed on the oscilloscope's screen. The common mode mesurement of the R&S ProbeMeter allows to check the input voltage relative to ground and is a convenient way to detect breaches of the operating voltage window, and the reason of unwanted clippings.

2.2 Setting up the Waveform

This chapter contains the fundamental procedures for setting up the acquisition and adjusting the channel waveforms.

Passive probes

Passive probes require compensation for exact signal display and measurement. The compensation procedure is described in the "Getting Started" manual.

2.2.1 Setting Up the Signal Input with Autoset

Autoset is the solution for the major part of routine test-setup. It is also a good start if you need to use more complex trigger settings. Autoset finds appropriate horizontal and vertical scales and trigger conditions to present a stable waveform.

1. Connect the probe to the input connector CH N.

   The instrument recognizes the probe and turns the channel on.
2. Press the AUTOSET button on the left of the display.

2.2.2 Adjusting the Signal Input Manually

The settings mentioned here are described in detail in:

- chapter 2.3.1, "HORIZONTAL Controls", on page 22
- chapter 2.3.3.2, "Channel Menu", on page 29
- chapter 2.3.3.1, "VERTICAL Controls", on page 27

1. Connect the probe to the input connector CH N.

   The instrument recognizes the probe and turns the channel on.
2. Use the SCALE rotary knob in the HORIZONTAL area of the front panel to set up the time base.
3. Use the POSITION rotary knob to set up the trigger position. Press the knob to reset the trigger offset to 0 s.
4. Press the channel key corresponding to the input channel. It is lighted with the color of the channel waveform.
5. In the softkey menu, press the "Coupling" softkey repeatedly to select the correct coupling.
6. Select the "Bandwidth" limit.
7. If you use a passive probe, adjust the probe settings:
   a) Select the "Termination" (input impedance).
   b) Select "More" to switch the menu page.

c) Press the "Probe" softkey and select the attenuation.

8. Use the SCALE rotary knob in the VERTICAL area of the front panel to adjust the vertical scale of the waveform. Press the knob to toggle between fine and rough adjustment.
9. Use the POSITION rotary knob to adjust the vertical position of the waveform. Vertical position is defined by the position of the waveform's zero line and the offset between the zero line and the waveform axis. Pressing the knob toggles between these parameters.
   By default, offset is disabled. Press the "Offset" softkey in the "Channel" menu to enable the offset. Use the NAVIGATION knob or the POSITION / OFFSET knob to adjust. Turn clockwise to move the waveform down.
10. Proceed with: chapter 2.2.3, "Setting the Acquisition", on page 21.

2.2.3 Setting the Acquisition

Prerequisites:

- Probes are connected.
- Vertical and horizontal settings are adjusted.

For details on acquisition settings, see chapter 2.3.2, "Acquisition Menu", on page 23.

1. Press the ACQUISITION key in the HORIZONTAL area of the front panel.
2. Select the "Sample Mode" - Real time or Equivalent time.
   This defines the behavior of the oscilloscope if the sample rate is higher than the ADC sample rate.
   Use Equivalent time to capture fast repetitive signals whose frequency components may be much higher than the sample rate of the ADC.
3. Select the "Decimation Mode" - for example, Peak detect.
   This defines the behavior of the instrument if the oscilloscope captures more samples than the waveform memory can save.
4. Select the "Wavef. Arithmetic" - for example, Average or Envelope.
   This defines how the resulting waveform is built from several consecutive acquisitions of the signal.
5. If "Average" is selected, enter the "Number of Averages", that is the number of waveforms used for average calculation.
6. Select the "Waveform Rate".

2.2.4 Starting and Stopping Acquisition

You can control the acquisition in two ways:

- Running continuous acquisition until you stop it

- Running one acquisition or a given number of acquisitions

Prerequisites:

- Probes are connected.
- Vertical and horizontal settings are adjusted.
- Triggering is set.
- Channels to be acquired are turned on.

To start and stop continuous acquisition

1. Check if the trigger mode is set to "Normal". The trigger mode is shown in the top information bar.
   If not, press the MODE key on the front panel to toggle the setting.
2. Press the RUN CONT key to start acquisition.
   The acquisition starts if a trigger occurs.
3. To stop, press the RUN CONT key again.
   The acquisition stops immediately.

To acquire a limited number of acquisitions

1. Press the ACQUISITION key in the HORIZONTAL area of the front panel.
2. Select "Nx Single" and enter the number of acquisitions.
3. Press the RUN N× SINGLE key on the front panel.
   You can stop the acquisition before it is finished by pressing the key again.

2.3 Reference for Waveform Setup

2.3.1 HORIZONTAL Controls

Time base settings adjust the display in horizontal direction. Use the rotary knobs in the HORIZONTAL functional block for setting.

POSITION.....23
SCALE.....23

POSITION
The rotary knob changes the trigger offset. This is the horizontal position of the trigger point in relation to the reference point - the zero point of the grid. Thus, you can set the trigger point even outside the diagram and analyze the signal some time before or after the trigger.

The reference point is set with SETUP >"Time Reference".

Turn clockwise to move the trigger point to the right. At zero-crossing, the knob shortly snaps in and the setting is kept constant to simplify the zero-setting. The current trigger position is shown in the top information bar, denoted by "T". Press the knob to reset the trigger offset to 0.

Note: If a zoom or FFT window is displayed, the knob can adjust other values depending on the selection of the SCALE rotary knob.

See also: "Time Reference" on page 235

Remote command:
`TIMebase:POSition` on page 284

SCALE
The rotary knob adjusts the time scale of the horizontal axis for all signals, also known as time base. The current scale value is shown in the top information bar, denoted by "TB". Turn clockwise to stretch the waveforms - the scale value time/div decreases.

If a Zoom or FFT window is displayed, press the knob to switch between the settings, then turn to adjust the selected value.

Remote command:
`TIMebase:SCALe` on page 283

2.3.2 Acquisition Menu

The ACQUISITION key in the HORIZONTAL functional block opens the "Acquisition" menu, where you select the acquisition mode. Acquisition modes control the data processing - how the waveform is built from the captured ADC samples. The current acquisition mode is shown in the top information bar, the second value from right.

The settings are placed on two menu pages.

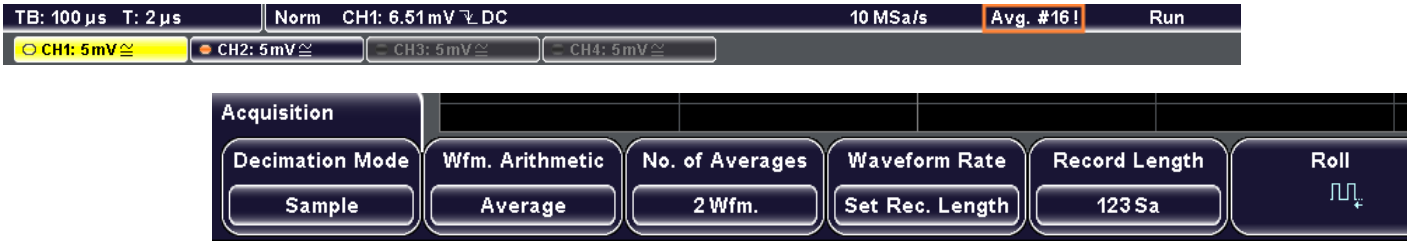

Decimation Mode....24
Wavef. Arithmetic....24
Nx Single....25
No. of Averages....25
Limit Freq....25
Waveform Rate....25
Record Length....26
Roll....26
Sample Mode....26
Interpolation....27

Decimation Mode
Decimation reduces the data stream of the ADC to a stream of waveform points with lower sample rate and a less precise resolution if the oscilloscope captures more samples than the waveform memory can save.

"Sample" The oscilloscope acquires the input data with a sample rate which is aligned to the time base (horizontal scale) and the memory depth. Usually, most signals are displayed optimally with this acquisition mode if all trigger conditions are met.

"Peak Detect" The minimum and the maximum of n samples are recorded as waveform points, the other samples are discarded. Thus the instrument can detect fast signal peaks at slow time scale settings that would be missed with other acquisition modes.

"High Resolution" The average of n captured sample points is recorded as one waveform sample. Averaging reduces the noise, the result is a more precise waveform with higher vertical resolution.

Remote command:
`CHANnel<m>:TYPE` on page 286

Wavef. Arithmetic
Waveform arithmetic builds the resulting waveform from several consecutive acquisitions of the signal (envelope and average) or by other operations on the captured data. The arithmetic works with all sample modes and decimated waveforms.

"Off" No arithmetic is applied.

"Envelope" The minimum and maximum values are saved in addition to the normal waveform samples. The resulting diagram shows two envelope waveforms below and above the normal waveform: the minimums (floor) and maximums (roof) representing the borders in which the signal occurs. The envelope is refreshed with each acquisition and it is reset each time the waveform parameters are changed.

"Average" The average is calculated from the data of the current acquisition and a number of acquisitions before. The method reduces random noise and other heterodyne signals. It requires a stable, triggered and repetitive signal.
The number of acquisitions for average calculation is defined with No. of Averages.

"Smooth" Smoothing calculates a mean value of several adjacent sample points and displays it. The result is a smoothed waveform. Thus, smoothing is a moving average that uses the full data and can be used for non-periodic signals. It works like a low-pass, and increases the vertical resolution at the expense of bandwidth reduction.

"Filter" Filter is a low-pass with 3 db attenuation at a configurable limit frequency set with "Limit Freq.". The filter removes higher frequencies from the channel signals.

Remote command:
`CHANnel<m>:ARIThmetics` on page 287

Nx Single
Sets the number of waveforms acquired with RUN N× SINGLE.

Remote command:
`ACQuire:NSINgle:COUNt` on page 282

No. of Averages
Defines the number of waveforms used to calculate the average waveform with "Wfm. Arithmetics" = "Average". Only numbers from the 2^n progression are available. The higher the number, the better the noise is reduced.

Remote command:
`ACQuire:AVERage:COUNt` on page 285

Limit Freq.
Sets the limit frequency for "Wfm. Arithmetics" = "Filter". The low pass filter has 3 dB attenuation at the given limit frequency.

Remote command:
`ACQuire:FILTer:FREQuency` on page 287

Waveform Rate
Defines the mode to set the sample rate (samples per second saved in the memory) and the waveform acquisition rate (waveforms per second).

"Max. Wfm. Rate" The instrument combines sample rate and memory depth to acquire at maximum waveform acquisition rate. In connection with persistence, the mode can display rare signal anomalies.
Note: Due to less memory depth, aliasing effects may occur.

"Max. Sa. Rate" The instrument acquires the signal at maximum sample rate and uses the full memory depth. The result is a waveform with maximum number of waveform samples, high degree of accuracy, and low risk of aliasing. However, the waveform acquisition rate is low.

"Automatic" Default mode: To display the best waveform, the instrument selects the optimum combination of waveform acquisition rate and sample rate using the full memory depth (maximum record length).

"Set Rec. Length" The instrument acquires the signals at a sample rate that fills up an user-defined record length, which is defined using "Record Length".

Remote command:
`ACQuire:WRATe` on page 286

Record Length
Sets the record length, the number of recorded waveform points that build the waveform across the acquisition time. The value is used if "Waveform Rate" is set to "Set Rec. Length".

Remote command:
ACQuire:POINts[:VALue]

Roll
Enables the roll mode.

The roll mode moves the captured input data on the display from the right to the left. The instrument shows the waveform immediately, without waiting for the complete acquisition of the waveform record. The roll mode displays the untriggered signal. Use the roll mode for slow, non-repetitive signals with 200 kHz or slower.

Remote command:
`TIMebase:ROLL:ENABle` on page 287

Sample Mode
Defines how the waveform is created from the sample points which are acquired by the ADC.

"Real Time" At slow time base settings the oscilloscope can acquire enough points to create an accurate waveform, so the sampled points of the input signal are used directly to build the waveform.
With fast time base settings, the sample rate is higher than the ADC sample rate. Waveform samples are added to the ADC samples according to the selected interpolation method.
See also: "Interpolation" on page 27
Real-time sampling is used to capture fast, single-shot, transient signals.

"Equivalent Time" Random equivalent-time sampling: This mode requires repetitive, stable signals. It is used to capture fast signals whose frequency components may be much higher than the sample rate of the ADC. The waveform points are taken from several acquisitions at a different time in relation to the trigger point. The time difference between the sample and the trigger is random. Then, all the sampled points are put together into one composite waveform.

Remote command:
`ACQuire:MODE` on page 285

Interpolation
Selects the interpolation method if the real time sample mode needs interpolation.

"Sin (x)/x"	Two adjacent ADC sample points are connected by a sin(x)/x curve, and also the adjoining sample points are considered by this curve. The interpolated points are located on the resulting curve. This interpolation method is the default method. It is very precise and shows the best signal curve.
"Linear"	Two adjacent ADC sample points are connected by a straight line, the interpolated points are located on the line. You see a polygonal waveform similar to the real signal, and also the ADC sample points as vertexes.
"Sample & Hold"	The ADC sample points are displayed like a histogram. For each sample interval, the voltage is taken from the sample point and considered as constant, and the intervals are connected with vertical lines. Thus, you see the discrete values of the ADC.

Remote command:
`ACQuire:INTerpolate` on page 285

2.3.3 Vertical Settings

To adjust the vertical settings, you use the keys and rotary knobs in the VERTICAL functional block of the front panel and the channel-specific softkey menu.

2.3.3.1 VERTICAL Controls

REF functions are described in chapter 5, "Reference Waveforms", on page 74. MATH functions are described in chapter 7, "Mathematics", on page 98.

CH N....28
SIGNAL OFF....28
POSITION / OFFSET....28

└ POSITION....28
└ OFFSET....28
SCALE, Y-Scale....29

CH N
Each channel key turns on an analog channel, selects it, and opens the "Channel" menu with the vertical settings of the selected channel. The key is illuminated in the channel color, if the channel is active.

The effect of the keypress depends on state of the channel:

- If channel is off: Pressing the key turns the channel on and selects it. The rotary knobs alongside light up in the channel color.
- If the channel is on: Pressing the key selects the channel waveform and open its channel setup menu.

Remote command:
`CHANnel<m>:STATe` on page 288

SIGNAL OFF
Turns the selected signal off and selects the next channel, math or reference waveform.

The key lights up in the color of the selected signal and changes the light according to the new selection.

Remote command:
`CHANnel<m>:STATe` on page 288

POSITION / OFFSET
The rotary knob adjusts the vertical position or the DC offset (if enabled). It lights up in the color of the selected waveform. Pressing the key toggles the parameter, the current parameter and its value are shown in a temporary label marked with the channel color.

Note: By default, offset is disabled. Press "Offset" in the "Channel" menu to enable the offset.

POSITION ← POSITION / OFFSET
Position changes the vertical location of the selected channel, math, or reference waveform, or of the decoded bus signal. Turn clockwise to move the waveform up. At zero-crossing, the knob shortly snaps in and the setting is kept constant to simplify the zero-setting.

Remote command:
`CHANnel<m>:POSition` on page 290
`CALCulate:MATH<m>:POSition` on page 346
`BUS<b>:POSition` on page 376

OFFSET ← POSITION / OFFSET
The offset voltage is subtracted to correct an offset-affected signal. The vertical center of the selected channel is shifted by the offset value and the signal is re-positioned within the diagram area.

Use the offset to measure small AC voltages that are overlaid by higher DC voltages. Unlike AC coupling, the DC part of the signal is not lost with offset setting. The device under test is not affected. The offset always has to be set manually, it is not included in the autoset process.

Turn clockwise to move the waveform down. At zero-crossing, the knob shortly snaps in and the setting is kept constant to simplify the zero-setting.

If an active probe is connected, the offset limit is defined by the probe. Refer to the documentation of the probe for allowed values.

Remote command:
`CHANnel<m>:OFFSet` on page 290
`PROBe<m>:SETup:UOFFset` on page 300

SCALE, Y-Scale
Sets the vertical scale in Volts per division to change the amplitude of the selected channel, math, or reference waveform, or of the decoded bus signal. The current value is shown in the waveform label above the grid. The knob lights up in the color of the selected waveform.

Turn SCALE clockwise to stretch the waveform. Doing so, the scale value V/div decreases. Press the knob to toggle between fine and rough adjustment.

To set the vertical sclae for a channel waveform numerically, press the "Y-Scale" softkey in the channel menu and then use the NAVIGATION knob.

Remote command:
`CHANnel<m>:SCALe` on page 289
`CALCulate:MATH<m>:SCALe` on page 346
`BUS<b>:DSIZe` on page 375

2.3.3.2 Channel Menu

The softkeys of the "Channel <n>" menu are placed on two menu pages. Each channel has its own menu.

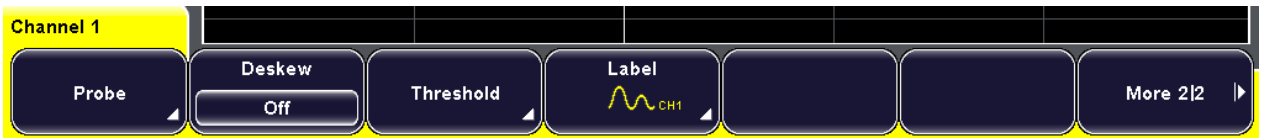

The channel label shows the basic vertical settings: vertical scale (in the figure below, channel 1: 5 mV/div), coupling (DC), termination (50 Ω, and bandwidth (limited). The label of the active channel is highlighted with the channel color (channel 1).

Coupling....30
Termination....30
Bandwidth....30
Offset....31
Invert....31
Y-Scale....31
Probe....31
Deskew....31
Threshold....31
Label....32

Coupling
Selects the connection of the input signal. The current coupling of each channel is shown in the waveform labels above the grid.

"AC" A 2 Hz high-pass filter is placed into the signal path that removes the DC offset voltage from the input signal. AC coupling is labeled with ≈.

"DC" DC coupling passes the input signal unchanged. It is labeled with ≅.

"GND" Connects the input virtually to the ground. All channel data is set to a constant ground value. Ground connection is labeled with ⏚.

Remote command:
`CHANnel<m>:COUPling` on page 289

Termination
Adjusts the input impedance of the instrument to the impedance of the DUT. By default, the oscilloscope has an input impedance of 1 MΩ || 13 pF. If an active probe is used, the termination is read out from the probe - usually it is 50 Ω.

"50Ω" In measurement systems that are dimensioned for a characteristic impedance of 50 Ω, reflections along the signal path are minimized by setting the input resistor of the oscilloscope also to 50 Ω. This increases the accuracy of measurement results. 50 Ω termination is identified for each channel by the icon Ω in the waveform label.

"1 MΩ" The high input resistor minimizes the loading effect on the device under test. This value is set automatically if a passive probe is connected and cannot be changed.

Remote command:
`CHANnel<m>:COUPling` on page 289

Bandwidth
Selects the bandwidth limit. The specified full bandwidth indicates the range of frequencies that the instrument can acquire and display accurately with less than 3dB attenuation. The probe has also a limited bandwidth and thus affects the resulting system bandwidth.

See also: chapter 2.1.1.3, "Bandwidth", on page 12

"Full" At full bandwidth, all frequencies in the specified range are acquired and displayed. Full bandwidth is used for most applications.

"400 MHz, 200MHz, 20MHz"	Frequency limit. Frequencies above the selected limit are removed to reduce noise at different levels. These bandwidth limits are indicated by the icon $B_{\sqcup}$ in the waveform label. The 400 MHz filter is not available for 350 MHz instruments (R&S RTM203x).

Remote command:
`CHANnel<m>:BANDwidth` on page 290

Offset
See "OFFSET" on page 28.

Invert
Turns the inversion of the signal amplitude on or off. To invert means to reflect the voltage values of all signal components against the ground level. Inversion affects only the display of the signal but not the trigger. For example: if the oscilloscope triggers on the rising edge, the trigger is not changed by inversion, but the actually rising edge is displayed as falling edge.

Inversion is indicated by a line above the channel name in the waveform label.

Remote command:
`CHANnel<m>:POLarity` on page 291

Y-Scale
See "SCALE, Y-Scale" on page 29

Probe
Opens the Probe menu. The menu is different for active and passive probes.

- chapter 2.3.3.3, "Probe Menu (Passive Probe)", on page 32
- chapter 2.3.3.4, "Probe Menu (Active Probe)", on page 33

Deskew
Deskew compensates delay differences between channels caused by the different length of cables, probes, and other sources. Correct deskew values are important for accurate triggering.

Signals which are routed over lines with different lengths have a different propagation delay. If high speed signals are measured, this delay may lead to a non-synchronous waveform display. For example, a coax cable with a length of one meter has a propagation delay of typically 5.3 ns.

Remote command:
`CHANnel<m>:SKEW` on page 291

Threshold
Access: CH N > "More" (page 2) > "Threshold"

Threshold value for digitization of analog signals. If the signal value is higher than the threshold, the signal state is high (1 or true for the boolean logic). Otherwise, the signal state is considered low (0 or false) if the signal value is below the threshold.

You can:

- Select one of the default values for TTL, ECL, or CMOS
  - TTL: 1,4 V
  - ECL: -1,3 V
  - CMOS: 2,5 V
- Set the "User" value individually
- Let the instrument analyze the signal and find an appropriate level

The threshold is applied to the selected channel.

Remote command:
`CHANnel<m>:THReshold` on page 292

Label
Opens the "Label" menu to define an additional name label for the selected waveform.

See: chapter 2.3.3.5, "Label Menu", on page 34

2.3.3.3 Probe Menu (Passive Probe)

In the probe menu for passive probes, the probe attenuation for the selected channel is set. If the probe is known to the instrument, the attenuation factor is set automatically. For unknown probes, you can select a default factor or enter a user-defined value.

Access: CH N > "More > Probe"

x1, x10, x100, x1000: attenuation factor
The keys select a default attenuation factor of the connected probe. The vertical scaling and measured values are multiplied by this factor so that the displayed values are equal to the undivided measured signal values.

To set an arbitrary attenuation factor, press the "User" softkey.

User: user-defined attenuation factor
You can enter an arbitrary attenuation factor in the range between x0.001 and x1000. The vertical scaling and measured values are multiplied by this factor so that the displayed values are equal to the undivided measured signal values.

Remote command:
`PROBe<m>:SETup:ATTenuation:MANual` on page 297

Unit
Selects the unit that the probe can measure.

- V - for voltage measurements
- A - for current measurements

Remote command:
PROBe<m>:SETup:ATTenuation:UNIT on page 297

2.3.3.4 Probe Menu (Active Probe)

In the probe menu for active probes, you can also adjust the offset value for the selected channel. Termination and attenuation are read out from the probe and do not need any adjustment.

Access: CH N > "More > Probe"

Offset
See "OFFSET" on page 28.

ProbeMeter
Activates the integrated R&S ProbeMeter of active R&S probes and selects the probe type. This voltmeter measures DC voltages between the probe tip and ground connection with very high precision and enables ground-referenced measurements of voltages. The DC measurement is performed continuously and in parallel to the measurements of the oscilloscope. If activated, the DC offset measured on the probe tip is shown in a colored label below the channel label.

"Inactive" ProbeMeter is disabled.

"Single Ended" ProbeMeter of a single-ended active probe is enabled.

Remote command:
PROBe<m>:SETup:OFFSwitch on page 299
PROBe<m>:SETup:DCOFfset? on page 298

Micro Button
Active R&S probes have a configurable Micro Button on the probe head. Pressing this button, you can perform an action on the instrument directly from the probe. During internal automatic processes the button is disabled, for example, during self alignment, autoset, and find level.

Select the action that you want to start from the probe.

"Continuous" Pressing the Micro Button starts continuous acquisition like the RUN key. The acquisition is running as long as you press the Micro Button again.

"Single" Starts one acquisition.

"Autoset" Starts the autoset procedure.

"None" Select this option to prevent unwanted actions due to unintended usage of the Micro Button.

Remote command:
`PROBe<m>:SETup:MODE` on page 299

Info
Shows general information on the connected probe, for example, type, serial number, and production date, as well as electrical characteristics like bandwidth, attenuation, input capacitance and impedance, voltage and DC offset range.

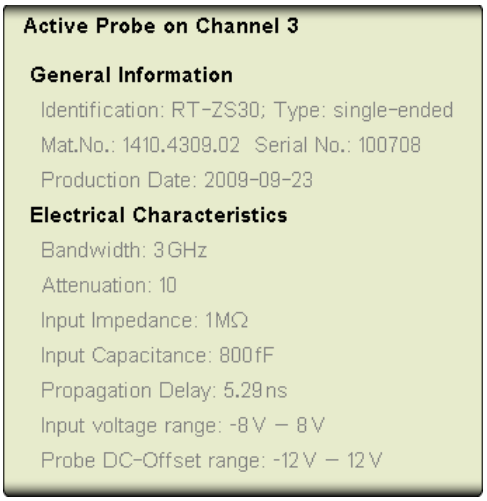
Active Probe on Channel 3
General Information
Identification: RT-ZS30; Type: single-ended
Mat.No.: 1410.4309.02 Serial No.: 100708
Production Date: 2009-09-23
Electrical Characteristics
Bandwidth: 3 GHz
Attenuation: 10
Input Impedance: 1MΩ
Input Capacitance: 800 fF
Propagation Delay: 5.29 ns
Input voltage range: -8 V – 8 V
Probe DC-Offset range: -12 V – 12 V

2.3.3.5 Label Menu

Access: CH N > "More > Label"

In the "Label" menu, you can define an additional name label for the selected waveform.

Label
Shows or hides the channel name. The name label is shown at the vertical center of the channel on the right edge of the display.

Remote command:
`CHANnel<m>:LABel:STATe` on page 292

Library
Selects a predefined label text and assigns it. The text can be edited with "Edit Label".

Edit Label
Opens on-screen keyboard to enter a label text. If you previously have selected a text from the library, it is already written in the entry line, and you can modify it.

The maximum name length is 8 characters, and only ASCII characters provided on the on-screen keyboard can be used.

Remote command:
`CHANnel<m>:LABel` on page 292

3 Triggers

3.1 Basics of Triggering

Triggering means to capture the interesting part of the relevant waveforms. Choosing the right trigger type and configuring all trigger settings correctly allows you to detect various incidents in analog, digital, and logic signals.

Trigger

A trigger occurs if the complete set of trigger conditions is satisfied simultaneously. It establishes the time-zero point in the waveform record. The instrument acquires continuously and keeps the sample points to fill the pretrigger part of the waveform record. When the trigger occurs, the instrument continues acquisition until the posttrigger part of the waveform record is filled. Then it stops acquiring and displays the waveform. When a trigger is recognized, the the instrument will not accept another trigger until the acquisition is complete.

Trigger conditions

A simple set of trigger conditions includes:

- Source of the trigger signal
- Trigger type and and its setup
- Horizontal position of the trigger: trigger position and reference point
- Trigger mode

The R&S RTM provides various trigger types for troubleshooting and signal analysis, for example, edge trigger, width trigger, pattern trigger, and specific triggers like video and bus triggers.

More complex trigger conditions are also available: you can setup a trigger sequence to join two edge triggers with an optional delay time or event count. Similar setups are also known as multi-step trigger or A/B trigger.

Furthermore, hysteresis avoids unwanted trigger events caused by noise.

Trigger event

In particular for the A/B trigger sequence, it is important to distinguish between the trigger and the event. An event is the fulfillment of the event conditions, but an event may not be the trigger. The trigger occurs only if the conditions of all events - the A event and the B event - in a trigger sequence and all further trigger conditions are all fulfilled.

Trigger information

Information on the most important trigger settings are shown in the information bar. The label shows:

- Trigger source and level
- Trigger coupling and filters

- Trigger slope or other conditions specific for the selected trigger type

Fig. 3-1: Trigger information: Normal trigger mode, trigger source is channel 1, width trigger to find negative pulses shorter than a given pulse width, trigger level = 1.71 mV

Fig. 3-2: Trigger information: Normal trigger mode, trigger sequence; A-event has source channel 1, edge trigger on rising edge with DC coupling and HF reject, trigger level 1.71 mV; B-event has source channel 2, edge trigger on rising edge and trigger level 0 V; instrument triggers on the second B-event

3.2 Setting Up the Trigger

This chapter provides step-by-step procedures for the important stages of trigger setup. The settings mentioned here are described in detail in chapter 3.3, "Reference for Triggers", on page 39.

3.2.1 Configuring the Trigger Event

Prerequisites:

- Horizontal and vertical settings are set appropriately to the signals.
- The acquisition is running, the RUN CONT key lights green.

1. Press the SETUP key in the TRIGGER functional block.

   The "Trigger" menu opens.
2. Press the "Source" softkey and select the trigger source.
3. Press "Setup" to return to the "Trigger" menu.
4. Press the "Type" softkey repeatedly until the required trigger type is selected.
5. Select "Setup".
6. Configure the settings for the selected trigger type.

   For details, see:

   - chapter 3.3.2.3, "Edge", on page 43
   - chapter 3.3.2.4, "Width", on page 45
   - chapter 3.3.2.5, "Video", on page 46
   - chapter 3.3.2.6, "Pattern", on page 48
   - chapter 3.3.2.7, "Rise Time / Fall Time", on page 50
   - chapter 3.3.2.8, "Protocol", on page 52

7. Set the "Normal" trigger mode: Press the AUTO/NORMAL key on the front panel until "Norm" is shown in the information bar.

3.2.2 Positioning the Trigger

By positioning the trigger, you define which part of the waveform is displayed: mainly the pretrigger part, or the posttrigger part, or the part around the trigger point. Therefore, you set the time reference (also known as reference point) and the trigger position in relation to the time reference.

1. To set the time reference point:
   a) Press the SETUP key on the left of the display.
   b) Select "Time Reference".
   c) Turn the navigation knob to move the reference point.
2. To set the trigger position, turn the POSITION rotary knob in the HORIZONTAL functional block.

3.2.3 Setting Up a Trigger Sequence

An A/B trigger sequence consists of two edge triggers connected by a time delay or event count.

1. Press the SETUP key in the TRIGGER functional block.
2. Press the "Trigger Type" softkey and select "Edge" trigger.
3. Select "Setup", configure the A trigger and select "Back".
4. Press the "B-Trigger" softkey to enable the B-trigger.

   The LEVEL knob and SLOPE key on the front panel are automatically assigned to the B-trigger. You can change the assignment with the "Trigger Level" softkey in the "Trigger" menu.
5. Press the "B-Setup" softkey.
6. Configure the B-trigger: Select "B-Source" and "Slope", and turn the LEVEL rotary knob to adjust the B-trigger level.
7. Define the connection between the A and B triggers by doing one of the following:
   - Press "Time" and adjust the delay time with the navigation knob.
   - Press "Events" and enter the number of B-trigger events that have to be fulfilled until the instrument triggers.

3.3 Reference for Triggers

The trigger settings are located in the TRIGGER functional block on the front panel and in the "Trigger" softkey menu.

3.3.1 TRIGGER Controls

The keys and the rotary knob in the TRIGGER functional block adjust the trigger and start or stop acquisition.

RUN CONT
Starts and stops the continuous acquisition. A green light indicates a running acquisition. A red light shows that acquisition is stopped.

The status is also shown at the right end of the information bar: "Run" or "Complete".

Remote command:
`RUN` on page 281
`RUNContinous` on page 282
`STOP` on page 282

RUN Nx SINGLE
Starts a defined number of acquisitions. Press the key again to stop running acquisitions.

To set the number of acquisitions, press the ACQUISITION key and enter "Nx Single".

Remote command:
`SINGle` on page 282
`RUNSingle` on page 282

FORCE
If the acquisition is running in normal mode and no valid trigger occurs, forcing the trigger provokes an immediate single acquisition. Thus you can confirm that a signal is available and use the waveform display to determine how to trigger on it.

MODE
Toggles the trigger mode between Auto and Normal. The trigger mode determines the behaviour of the instrument if no trigger occurs. The current setting is shown in the information bar.

"Auto" The instrument triggers repeatedly after a time interval if the trigger conditions are not fulfilled. If a real trigger occurs, it takes precedence. This mode helps to see the waveform even before the trigger is set. The waveform on the screen is not synchronized, and successive waveforms are not triggered at the same point of the waveform.

"Normal" The instrument acquires a waveform only if a trigger occurs, that is, if all trigger conditions are fulfilled. If no trigger occurs, no waveform is acquired and the last acquired waveform is displayed. If no waveform was captured before, nothing is displayed.

Remote command:
`TRIGger:A:MODE` on page 302

LEVEL
The rotary knob changes the trigger treshold voltage for all trigger types that require one trigger level. Some trigger types require two trigger levels, for example, the rise time/fall time trigger. These levels can be set in the trigger setup menu.

Turn clockwise to move the trigger level up. Press the knob to set the level to 50% of the signal amplitude.

If a B-trigger is enabled, the knob can set the level for both the A- and B-trigger. To assign the level to the A- or B-trigger, use "Trigger Level" in the "Trigger" menu.

Remote command:
`TRIGger:A:LEVel<n>[:VALue]` on page 302
`TRIGger:A:FINDlevel` on page 302
`TRIGger:B:FINDlevel` on page 313

SETUP
Opens the "Trigger" menu.

SOURCE
Opens the "Trigger Source" menu for the A-trigger. Press the key repeatedly until the required source is selected. The key lights up in the color of the selected trigger channel. The selected source is shown in the information bar.

SLOPE
If you have selected "Edge" trigger as trigger type with an analog trigger source, the SLOPE key toggles the trigger slope. The current setting is shown by an icon in the information bar.

If a B-trigger is enabled, the key can set the slope for both the A- and B-trigger. To assign the slope to the A- or B-trigger, use "Trigger Level" in the "Trigger" menu.

3.3.2 Trigger Settings

Trigger settings consist of general settings in the "Trigger" menu and the trigger type-specific setup. For B-trigger setup, a separate menu is provided.

- Common Trigger Settings....41
- Trigger Source Settings....42
- Edge....43
- Width....45
- Video....46
- Pattern....48
- Rise Time / Fall Time....50
- Protocol....52
- B-Setup....52

3.3.2.1 Common Trigger Settings

The "Trigger" menu is general menu for all trigger types and leads to the type-specific menus.

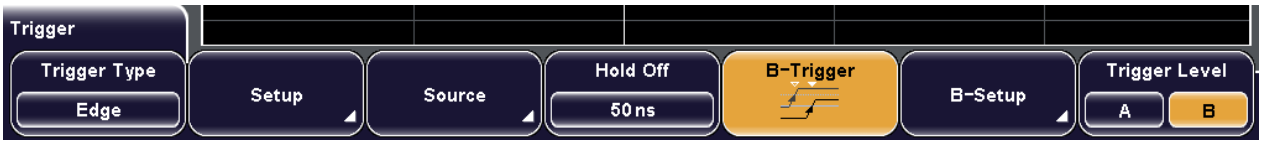

To set the trigger offset, use the horizontal POSITION rotary knob, see "POSITION" on page 23.

Trigger Type....41
Setup....41
Source....41
Hold Off....42
B-Trigger....42
B-Setup....42
Trigger Level....42

Trigger Type
Selects the trigger type.

For details, see:
- chapter 3.3.2.3, "Edge", on page 43
- chapter 3.3.2.4, "Width", on page 45
- chapter 3.3.2.5, "Video", on page 46
- chapter 3.3.2.6, "Pattern", on page 48
- chapter 3.3.2.7, "Rise Time / Fall Time", on page 50
- chapter 3.3.2.8, "Protocol", on page 52

Remote command:
`TRIGger:A:TYPE` on page 303

Setup
Opens the setup menu for the selected trigger type.

Source
Opens the "Trigger Source" menu for the selected trigger type.

See: chapter 3.3.2.2, "Trigger Source Settings", on page 42

Remote command:
TRIGger:A:SOURce on page 303

Hold Off
Enables the holdoff and defines the holdoff time. The next trigger occurs only after the holdoff time has passed.

The trigger holdoff defines when the next trigger after the current will be recognized. Thus, it affects the next trigger to occur after the current one. Holdoff helps to obtain stable triggering when the oscilloscope is triggering on undesired events.

Remote command:
TRIGger:A:HOLDoff:MODE on page 304
TRIGger:A:HOLDoff:TIME on page 304

B-Trigger
Activates or deactivates the second edge trigger event that follows a first edge trigger event in a trigger sequence. The instrument triggers if both trigger event conditions (A and B) are fulfilled.

If the B-trigger is activated, the LEVEL rotary knob and the SLOPE key are automatically assigned to the B-event. You can toggle the assignment of these controls with the "Trigger Level" setting in the "Trigger" menu.

Remote command:
TRIGger:B:ENABle on page 312

B-Setup
Opens the menu for B-trigger configuration. The B-trigger is a second edge trigger event that can be combined with a preceeding edge trigger event. The trigger conditions of this second event are considered when the conditions of the main event (A-trigger) are met.

For a description of the menu, see chapter 3.3.2.9, "B-Setup", on page 52.

Trigger Level
Assigns the SLOPE key and the LEVEL rotary knob on the front panel to the A- or B-event. The function is only relevant if the B-trigger is enabled. The SOURCE key sets always the A-trigger source.

3.3.2.2 Trigger Source Settings

Access: Trigger SETUP > "Source"

The content of the "Trigger Source" menu depends on the trigger type.

The figure below shows the trigger source menu for the width trigger with MSO option R&S RTM-B1 installed.

Remote Command: TRIGger:A:SOURce on page 303

Channel N
Selects one of the analog input channels as trigger source.

Logic Channels
Selects one of the digital channels as trigger source if MSO option R&S RTM-B1 is installed.

Logic channels are available for edge and width triggers but they are not selectable if the B-trigger is enabled.

AC Line
Selects the mains supply of the oscilloscope as trigger input for the edge trigger. The instrument extracts the trigger signal from the power supply.

Extern
Sets the External Trigger Input on the rear panel as trigger source. Select the signal type that is connected: AC or DC.

Remote command:
TRIGger:EXTern:COUPling on page 303

3.3.2.3 Edge

The edge trigger is the simpliest and most common trigger type. It is well-known from analog oscilloscopes; and you can use it for analog and digital signals. The trigger event occurs when the signal from the trigger source passes the specified treshold voltage - the trigger level - in the specified direction (slope).

The edge trigger is also selected with the AUTOSET function.

Slope....43
Coupling....44
LF Reject....44
HF Reject....44
Low-pass....44
Hysteresis A / B....44

Slope
Sets the edge for the trigger.

"Rising" Selects the rising edge, that is a positive voltage change.

"Falling" Selects the falling edge, that is a negative voltage change.

"Both" Selets the rising as well as the falling edge.

Remote command:
TRIGger:A:EDGE:SLOPe on page 304

Coupling
Sets the coupling for the trigger source.

"AC" Alternating Current coupling. A 5 Hz high pass filter is connected into the trigger path and removes the DC offset voltage from the trigger signal.

"DC" Direct Current coupling. The trigger signal remains unchanged.

Remote command:
TRIGger:A:EDGE:COUPling on page 305

LF Reject
Sets the trigger coupling to high frequency. A 15 kHz high-pass filter is connected into the trigger path and removes lower frequencies from the trigger signal. Use this mode only with very high frequency signals.

Remote command:
TRIGger:A:EDGE:COUPling on page 305

HF Reject
Turns an additional 5 kHz low-pass filter in the trigger path on or off. This filter removes higher frequencies and is available with AC and DC coupling.

Remote command:
TRIGger:A:EDGE:FILTer:LPASs on page 305

Low-pass
Turns an additional 100 MHz low-pass filter in the trigger path on or off. This filter removes higher frequencies and is available with AC and DC coupling.

Remote command:
TRIGger:A:EDGE:FILTer:NREJect on page 305

Hysteresis A / B
Sets a hysteresis range around the trigger level. If the signal jitters inside this range and crosses the trigger level thereby, no trigger event occurs. Thus, hysteresis avoids unwanted trigger events caused by noise oscillation around the trigger level.

Hysteresis is available for the edge trigger (A-event and B-event) and for the width trigger.

To see the hysteresis on the display, activate "Trigger Hyst." in the "Display > Auxillary Cursors" menu.

The hysteresis value depends on the vertical scale.

Remote command:
TRIGger:A:HYSTeresis on page 304
TRIGger:B:HYSTeresis on page 314

3.3.2.4 Width

The width trigger compares the pulse width (duration) with a given time limit. It detects pulses with an exact pulse width, pulses shorter or longer than a given time, as well as pulses inside or outside the allowable time range.

The instrument triggers if the pulse does not cross the specified voltage treshold twice. The pulse width is measured at the trigger level.

Comparison....45
Polarity....45
Time t....46
Variation....46
Time t1, Time t2....46
Find level....46

Comparison
Sets how the measured pulse width is compared with the given limit(s).

"ti<t, ti>t"	Triggers on pulse width shorter or longer than the reference "Time t".
"ti=t"	Triggers on pulse width equal to the reference "Time t" if "Variation" Δt = 0. If "Variation" ≠ 0: this setting triggers on pulses within the range t±Δt.
"ti≠t"	Triggers on pulses unequal to the reference "Time t", if "Variation" Δt = 0. If "Variation" ≠ 0: this setting triggers on pulses outside a range t±Δt.
"Inside, Outside"	Triggers on pulses inside or outside a range specified with "Time t1" and "Time t2". This method is an alternative setting to the range definition with "Time t" and "Variation". The values are interdependent. "Variation" and "Time t" are adjusted If you change t1 and t2, and vice versa.

Remote command:
`TRIGger:A:WIDTh:RANGe` on page 306

Polarity
Sets the polarity of the pulse.

"Pos."	Positive going pulse, the width is defined from the rising to the falling slopes.
"Neg."	Negative going pulse, the width is defined from the falling to the rising slopes.

Remote command:
`TRIGger:A:WIDTh:POLarity` on page 305

Time t
Sets the reference time, the nominal value for comparisons ti<t, ti>t, ti=t, ti≠t.

Remote command:
`TRIGger:A:WIDTh:WIDTh` on page 306

Variation
Sets a range Δt to the reference "Time t", if comparison is set to "ti=t" or "ti≠t". The instrument triggers on pulses inside or outside the range ti±Δt.

Remote command:
`TRIGger:A:WIDTh:DELTa` on page 306

Time t1, Time t2
Set the lower and upper time limits defining the time range if "Inside" or "Outside" is set for comparison. "Time t" and "Variation" are adjusted accordingly.

Find level
Sets the trigger level automatically to *0.5 * (MaxPeak – MinPeak)*.

3.3.2.5 Video

The video or TV trigger is used to analyze analog baseband video signals. You can trigger on baseband video signals from standard definition and high definition standards.

The trigger level is determined and set automatically by the instrument.

First select the standard and the signal polarity, then decide to trigger on lines or fields and enter the specific settings.

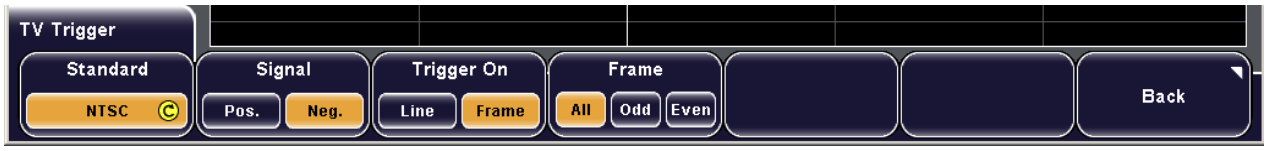

Most video signals have an output impedance of 75 Ω. The channel inputs of the R&S RTM have an input impedance of 50 Ω or 1 MΩ. Make sure to provide the adequate matching to ensure amplitude fidelity. A simple 75 Ω feed-through termination combined with 1 MΩ oscilloscope inputs is suitable for most applications.

Standard....46
Signal....47
Trigger On....47
Line....47
All Lines....47
Frame....48

Standard
Selects the color television standard.

You can trigger on various SDTV signals like PAL, PAL-M, SECAM, NTSC and SDTV 576i (PAL and SECAM).

HDTV standards are indicated by the number of active lines and the scanning system (p for progressive scanning, i for interlaced scanning.

Remote command:
`TRIGger:A:TV:STANdard` on page 307

Signal
Selects the polarity of the signal. Note that the sync pulse has the opposite polarity. If the video modulation is positve, the sync pulses are negative. If the modulation is negative, sync pulses are positive. The edges of the sync pulses are used for triggering, therefore incorrect polarity setting causes a sporadic triggering by the video information.

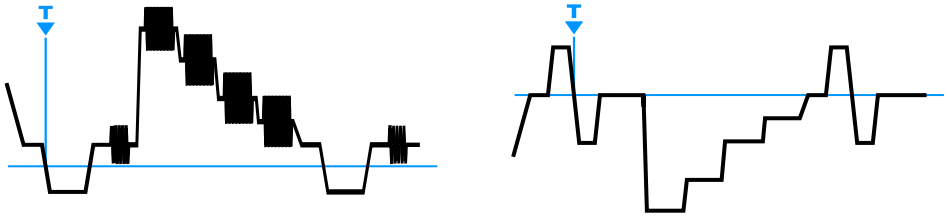

Fig. 3-3: Positive video signal with negative bi-level sync pulse (SDTV, left) and negative signal with positive tri-level sync pulse (HDTV, right)

Remote command:
`TRIGger:A:TV:POLarity` on page 307

Trigger On
Toggles between triggering on line starts or frame starts.

Line aloows to trigger on "All Lines" or on one specified "Line".

"Frame" has different effect depending on the selected signal standard:
- For standards using progressive scanning (HDTV 720/1080i), the instrument triggers on the frame start.
- All other available standards use interlaced scanning, and the instrument triggers on the field start. You can select the field type to be triggered on using "Frame".

Remote command:
`TRIGger:A:TV:FIELd` on page 307

Line
Sets an exact line number if "Trigger on" is "Line". If the other trigger conditions are also met, the oscilloscope triggers exactly on the beginning of the selected line in any field.

Remote command:
`TRIGger:A:TV:LINE` on page 308

All Lines
The oscilloscope triggers on the beginning of all video signal lines if "Trigger on" is "Line".

Remote command:
`TRIGger:A:TV:FIELd` on page 307

Frame
The oscilloscope triggers on the beginning of the video signal fields if the other trigger conditions are fulfilled. The setting is available for video signals using interlaced scanning.

"All" Triggers on all fields

"Odd" Triggers only on odd fields.

"Even" Triggers only on even fields.

Remote command:
`TRIGger:A:TV:FIELd` on page 307

3.3.2.6 Pattern

The Pattern trigger is is a logic trigger. It provides any logical combination of the input channels and supports you in verifying the operation of digital logic.Thus you can also trigger on bus patterns of parallel buses.

The channel pattern is configured in the "Source" menu. Additionally, you can set a time limitation to the pattern in the "Setup" menu.

Pattern

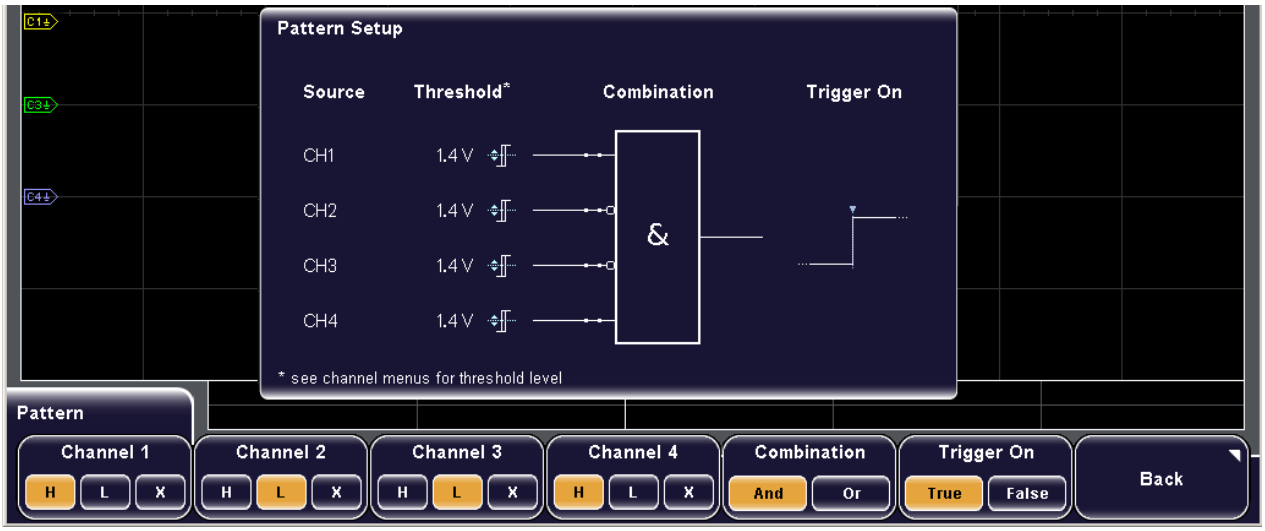

Channel N....48
Combination....49
Trigger On....49

Channel N
Select the state for each channel. The states are:

"H" High: the signal voltage is higher than the trigger level.

"L" Low: the signal voltage is lower than the trigger level.

"X" Don't care: the channel does not affect the trigger.
If MSO option R&S RTM-B1 is installed, the digital channels D0 to D15 are available in addition to analog channels.
If X is set for all channels, the oscilloscope triggers only in automatic trigger mode.

Remote command:
`TRIGger:A:PATTern:SOURce` on page 308

Combination
Sets the logical combination of the trigger states of the channels.

"And" The required states of all channels must appear in the input signal at the same time.

"Or" At least one of the channels must have the required state.

Remote command:
`TRIGger:A:PATTern:FUNCtion` on page 309

Trigger On
Sets the trigger point depending on the result of the logical combination of the channel states.

Remote command:
`TRIGger:A:PATTern:CONDition` on page 309

Time Limitation

In addition to the pattern and the trigger levels, you can define a timing condition - how long the result of the pattern condition must be true or false.

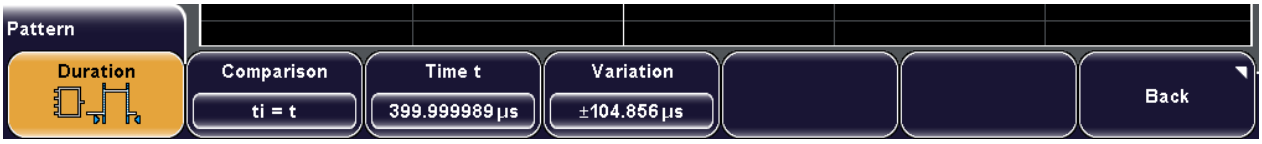

Duration
Enables or disables the time limitation to the pattern state.

Remote command:
`TRIGger:A:PATTern:MODE` on page 309

Comparison
Sets how the duration time of the resulting patten state is compared with the given time limit(s).

"ti<t, ti>t" Triggers if the pattern state changes before or after the "Time t" has expired.

"ti=t" Triggers if the pattern state changes exactly at "Time t" if "Variation" $\Delta t = 0$.
If "Variation" $\neq 0$: this setting triggers within the range $t \pm \Delta t$.

"ti≠t" Triggers on pattern state durations unequal to the "Time t", if "Variation" Δt = 0.
If "Variation" ≠ 0: this setting triggers outside a range t±Δt.

"Inside, Outside" Triggers on pattern state durations inside or outside a range specified with "Time t1" and "Time t2".
This method is an alternative setting to the range definition with "Time t" and "Variation". The values are interdependent. "Variation" and "Time t" are adjusted If you change t1 and t2, and vice versa.

"Timeout" Defines how long the result of the pattern condition must be true. The instrument triggers at "Time t".

Remote command:
`TRIGger:A:PATTern:WIDTh:RANGe` on page 310
`TRIGger:A:PATTern:MODE` on page 309

Time t
Sets the reference time, the nominal value for comparisons ti<t, ti>t, ti=t, ti≠t and timeout

Remote command:
`TRIGger:A:PATTern:WIDTh[:WIDTh]` on page 310

Time t1, Time t2
Set the lower and upper time limits defining the time range if "Inside" or "Outside" is set for comparison. "Time t" and "Variation" are adjusted accordingly.

Variation
Sets a range Δt to the reference "Time t", if comparison is set to "ti=t" or "ti≠t". The instrument triggers on pulses inside or outside the range ti±Δt.

Remote command:
`TRIGger:A:PATTern:WIDTh:DELTa` on page 310

3.3.2.7 Rise Time / Fall Time

The rise time trigger, also known as slew rate or transition trigger, can detect fast or slow rising or falling edges selectively. It triggers on edges, if the rise or fall time from the lower to higher voltage level (or vice versa) is shorter or longer as defined, or inside or outside a specified time range. The trigger finds slew rates that are faster than expected or permissible to avoid overshooting and other interfering effects. It also detects very slow edges violating the timing in pulse series.

Polarity
Sets the edge, the transition time of which is to be analyzed:

"Rising" Rise time trigger

"Falling" Fall time trigger

Remote command:
TRIGger:A:RISetime:SLOPe on page 311

Upper Level
Sets the upper voltage threshold. When the signal crosses this level, the slew rate measurement starts or stops depending on the selected polarity.

To set the value using the Level 50% rotary knob, press the knob to toggle upper and lower level and then turn the knob.

Remote command:
TRIGger:A:LEVel<n>:RISetime:UPPer on page 311

Lower Level
Sets the lower voltage threshold. When the signal crosses this level, the slew rate measurement starts or stops depending on the selected slope.

Remote command:
TRIGger:A:LEVel<n>:RISetime:LOWer on page 311

Comparison
Selects how the time limit for the slew rate is defined. The time measurement starts when the signal crosses the first trigger level - the upper or lower level depending on the selected slope - and stops when the signal crosses the second level.

"Greater than" Triggers on transition times longer than the given "Rise Time".

"Lower than" Triggers on transition times shorter than the given "Rise Time".

"Equal" Triggers on transition times inside the time range *Rise Time ± Variation*.

"Not equal" Triggers on transition times outside the time range *Rise Time ± Variation*.

Remote command:
TRIGger:A:RISetime:RANGe on page 311

Rise Time
For the comparisons "Greater than" and "Lower than", the setting defines the minimum and maximum transition time limits, respectively.

For the comparisons "Equal" and "Not equal", the setting defines the center of a range, which is defined by "Variation"

Remote command:
TRIGger:A:RISetime:TIME on page 311

Variation
Defines a time range around the given "Rise Time" value.

Remote command:
TRIGger:A:RISetime:DELTa on page 312

3.3.2.8 Protocol

The "Protocol" trigger menu contains the trigger settings for the serial bus or interface that is configured with PROTOCOL. Protocol analysis requires additional options.

For protocol setup and trigger settings, see chapter 11, "Protocol Analysis", on page 148.

To trigger on parallel buses, use the pattern trigger. See: chapter 3.3.2.6, "Pattern", on page 48.

3.3.2.9 B-Setup

The B-trigger is a second edge trigger event that can be combined with a preceeding edge trigger event. The conditions of this second event are considered when the conditions of the main event (A-trigger) are met.

B-Source....52
Slope....52
Level....52
Trigger On....53
Time....53
Events....53
Hysteresis A / B....53

B-Source
Selects one of the input channels as B-trigger source. Press the softkey repeatedly until the required source is selected.

Remote command:
`TRIGger:B:SOURce` on page 312

Slope
Sets the edge for the B-trigger event.

"Positive" Selects the rising edge, that is a positive voltage change.

"Negative" Selects the falling edge, that is a negative voltage change.

"Both" Selets the rising as well as the falling edge.

Remote command:
`TRIGger:B:EDGE:SLOPe` on page 312

Level
Sets the trigger level for the B-trigger event.

Remote command:
`TRIGger:B:LEVel` on page 312

Trigger On
Sets an additional delay condition for the B-event: time delay or event delay. According to this selection, set also "Time" or "Events" to define the condition completely.

Remote command:
`TRIGger:B:MODE` on page 313

Time
Sets the time the instrument waits after an A-event until it recognizes B-events.

Remote command:
`TRIGger:B:DELay` on page 313

Events
Sets a number of B-trigger events that fulfill all B-trigger conditions but do not cause the trigger. The oscilloscope triggers on the n-th event (the last of the specified number of events).

Remote command:
`TRIGger:B:EVENt:COUNt` on page 313

Hysteresis A / B
Sets a hysteresis range around the trigger level. If the signal jitters inside this range and crosses the trigger level thereby, no trigger event occurs. Thus, hysteresis avoids unwanted trigger events caused by noise oscillation around the trigger level.

Hysteresis is available for the edge trigger (A-event and B-event) and for the width trigger.

To see the hysteresis on the display, activate "Trigger Hyst." in the "Display > Auxillary Cursors" menu.

The hysteresis value depends on the vertical scale.

Remote command:
`TRIGger:A:HYSTeresis` on page 304
`TRIGger:B:HYSTeresis` on page 314

4 Display

This chapter provides information on display configuration and display modes.

The default display is a waveform diagram with a time axis in x-direction and the signal amplitudes displayed in y-direction - the Y(t) or time diagram. You can adjust the visibility of diagram elements and waveform to your needs. See chapter 4.1, "General Display Settings", on page 54 for details.

You can also display and configure XY-diagrams to combine the voltage levels of two waveforms in one diagram. This display mode is described in chapter 4.2, "XY-Diagram", on page 61.

Furthermore, you can zoom into waveforms to analyze the results in more detail. The zoom display mode is described in chapter 4.3, "Zoom", on page 66.

In a Y(t)-diagram and in zoom mode, you can set markers to mark positions of interest in the waveform. See chapter 4.4, "Markers", on page 71 for details.

In addition to zoom and XY-diagram modes, the following functional modes are available:

- FFT analysis, see chapter 8.2, "Configuring and Using FFT Calculations", on page 111
- Mask testing, see chapter 9.2, "Working with Masks", on page 124

4.1 General Display Settings

General display settings adjust the visibility of diagram elements and waveforms.

The individual diagram elements can be shown or hidden:

- Basic diagram elements: grid and crosshairs
- Point of the trigger event
- Channel cursors to mark the ground level and the DC offset

You can also adjust how the waveforms are displayed. The intensity and brightness of the individual screen elements can influence the readability of the results. Depending on which type of result you are interested in, e.g. frequency of occurance, time of occurance, or amplitude of a specific value, different settings may be necessary to highlight that aspect in the display.

The waveform display depends on the following criteria:

- Waveform style: dots or line
- Intensity: adjusts the optimal contrast of the display
  Three settings can be changed to improve the contrast for the relevant display elements.
  - The intensity of the waveform determines the strength of the signal in the diagram.
  - The intensity of the background lighting determines the contrast of the signal.
  - The intensity of the grid has an influence on the readability of the signal.

- Persistence defines how long a data point is displayed in the diagram. Each new data point remains on the screen for the defined persistence time, or infinitely until the persistence time is changed or the persistence is cleared.
- Signal colors or brightness depend on on the cumulative frequency of the values. By default, values that occur frequently are displayed brighter than rare values. Alternatively, the brightness level can be converted to a color range, i.e. the color changes gradually with increasing cumulative occurance.
  It is also possible to invert the brightness display so that rare values are brighter than frequent values. This setting is useful in combination with persistence to detect rare values within the waveform.

4.1.1 Configuring the Display

4.1.1.1 Configuring the Diagram Elements

To display the grid or crosshairs

1. Press "DISPLAY > Grid > Lines" to display a grid.
2. Press "DISPLAY > Grid > Reticle" to display crosshairs.
3. Press "DISPLAY > Grid > Off" to remove both the grid and the crosshairs.

To display the trigger event or the channel cursors

The marker of trigger event and the channel cursors are auxiliary cursors. By default, both auxiliary cursors are displayed. They help to evaluate specific results more easily.

1. Press "DISPLAY > Aux. Cursor > Trigger Event" to display a trigger cursor.

   A rhombus marks the point where the trigger event happened.
2. Press "DISPLAY > Aux. Cursor > Channel Cursors" to display a channel cursor.

   A dashed line is displayed that marks the ground level of the displayed channel. If a DC offset is defined, a second auxiliary line is displayed. The distance between those two lines is the DC offset.
3. Press "DISPLAY > Aux. Cursor > Defaults" to restore the default setting (both cursors displayed).

4.1.1.2 Configuring the Waveform Display

The waveform display depends on the following criteria:

- Intensities adjust the optimal contrast of the display. See "To configure intensity" on page 56.
- Persistence defines how long a data point is displayed in the diagram. See "To configure persistence" on page 56.

- Brightness and signal colors depend on the cumulative frequency of the value. See: "To configure brightness" on page 56
- Waveform as line or points: see "To set the waveform style" on page 57.

To configure intensity

For optimal contrast, you can change the intensity of the waveform, of the grid, and of the backlight.

1. Press "DISPLAY > Intensities".
2. To set the intensity of the waveform:
   a) Press "Waveform".
   b) Enter a percentage between 0 (not visible) and 100% (very strong). The default value is 50%. You can also use the "INTENSITY" knob on the left side of the screen to adjust the waveform intensity directly.
3. To set the intensity of the grid:
   a) Press "Grid".
   b) Enter a percentage between 0 and 100%. The default value is 34%.
4. To set the intensity of the backlight:
   a) Press "Backlight".
   b) Enter a percentage between 10 and 100%. The default value is 50%.

To configure persistence

1. To display only the current signal at any time, press "DISPLAY > Intensities > Persistence" until "Off" is highlighted.
2. To have the instrument define the optimal persistence automatically, press "DISPLAY > Intensities > Persistence" until "Automatic" is highlighted.
3. To configure the persistence manually:
   a) Press "DISPLAY > Intensities > Persistence" until "Manual" is highlighted.
   b) Press "DISPLAY > Intensities > Persist. Time" to define the persistence time.
   c) Enter a value between 50 ms and 9.6 s or "Infinite".

   Each new data point in the diagram area remains on the screen for the defined duration. If "Infinite" is selected, each new data point in the diagram area remains on the screen infinitely until this setting is changed or the persistence is cleared.
4. To update the waveform, press "DISPLAY > Intensities > Clear Persist.".

To configure brightness

For better distinction of rare and frequent values, you can apply a color range to the value frequency. With this color range, rare values are displayed in blue, while more frequent values are red and very frequent values are displayed in yellow or white, with various colors inbetween.

It is also possible to invert the brightness display so that rare values are brighter than frequent values.

1. To convert the brightness level to a color range, press "DISPLAY > Temperature Colors".
2. To invert the brightness level of the signals, press "DISPLAY > Inverse Brightn.".

To set the waveform style

By default, the individual data points are connected by a line. Alternatively, only the individual data points can be displayed.

You can change the strength of the line using the "INTENSITY" knob on the left side of the screen.

► Press "DISPLAY > Dots Only" to display the data points only.

4.1.2 Display Menu

The DISPLAY key provides functions for configuring the display.

Display Mode....58
XYZ Setup....58
Intensities....58
└ Waveform....58
└ Backlight....58
└ Grid....59
└ Persistence....59
└ Persist. Time....59
└ Clear Persist....59
Dots Only....59
Inverse Brightn....59
Temper. Colors....60
Aux. Cursors....60
└ Trigger Event....60
└ Channel Cursors....60
└ Trigger Hyst....61

└ Defaults....61
Grid....61
VirtualScreen....61

Display Mode
Toggles the diagram mode.

"Y(t)" Default time diagram with a time axis in x-direction and the signal amplitudes displayed in y-direction.

"XY-diagram" XY-diagrams combine the voltage levels of two waveforms in one diagram. They use the voltage level of a second waveform as the x-axis, rather then a time base. This allows you to perform phase shift measurements, for example.You can also define the intensity of the XY-diagram according to a further signal source Z.
Together with the XY-diagram, the Y(t)-diagrams of the source signals are displayed in separate windows.
With R&S RTM1054, it is also possible to define two source signals in y-direction for comparison.

Remote command:
`DISPlay:MODE` on page 314

XYZ Setup
See chapter 4.2.2, "XYZ Setup Menu", on page 64.

Intensities
Provides functions to define the intensity of various display elements.

Waveform ← Intensities
Waveform intensity determines the strength of the waveform lines in the diagram. Enter a percentage between 0 (barely visible) and 100% (very strong), or press and turn the "INTENSITY" knob on the left side of the screen to adjust the waveform intensity directly. The default value is 50%.

Remote command:
`DISPlay:INTensity:WAVeform` on page 317

Backlight ← Intensities
Defines the intensity of the background lighting of the display in percent. Enter a percentage between 10% and 100%. The default value is 50%.

Remote command:
`DISPlay:INTensity:BACKlight` on page 317

Grid ← Intensities
Defines the intensity of the grid on the screen in percent. Enter a percentage between 0%and 100%. The default value is 34%.

Remote command:
DISPlay:INTensity:GRID on page 317

Persistence ← Intensities
Defines the persistence of the waveform on the screen.

"Off"	Deactivates persistence
"Automatic"	The optimal persistence time is determined automatically by the instrument
"Manual"	User-defined persistence according to "Persist. Time" setting.

Remote command:
DISPlay:PERSistence:STATe on page 318
DISPlay:PERSistence:TIME:AUTO on page 318

Persist. Time ← Intensities
User-defined persistence time if "Manual" persistence is selected. Each new data point remains on the screen for the duration defined here. Possible values are from 50 ms to 9.6 s or "Infinite". If "Infinite" is selected, each new data point remains on the screen infinitely until this setting is changed or the persistence is cleared.

Remote command:
DISPlay:PERSistence:TIME on page 318
DISPlay:PERSistence:INFinite on page 318

Clear Persist. ← Intensities
Clears the displayed persistence on the screen.

Remote command:
DISPlay:PERSistence:CLEar on page 319

Dots Only
If activated, only the individual data points are displayed. If deactivated, the individual data points are connected by a line. Define the strength of the line using the "INTENSITY" knob on the left side of the screen.

Remote command:
DISPlay:STYLe on page 319

Inverse Brightn.
Inverts the brightness level of the signals. Normally, values that occur frequently are brighter than rare values. This setting inverts this behavior: Rare values are brighter than frequent values. Use this setting in combination with persistence to detect rare values within the waveform.

Remote command:
DISPlay:PALette on page 314 (INVerse, IFColor)

Temper. Colors
Temperature Colors: Converts the brightness level of the displayed signals into a color range, i.e. the color changes gradually in a wide color spectrum with increasing cumulative occurance.

By default, rare values are displayed in blue, while more frequent values are red and very frequent values are displayed in yellow or white, with various colors inbetween. This results in a higher contrast, which provides a better perception of details in the waveforms.

Note: The colors change if you invert the brightness display.

Remote command:
`DISPlay:PALette` on page 314 (NORMal, FColor)

Aux. Cursors
Provides functions to display auxiliary cursors. Highlighted functions are active.

Trigger Event ← Aux. Cursors
Show or hides the point of the trigger. A small rhombus markes the intersection of the trigger level and the trigger offset T.



The offset is related to the reference point and is displayed in the header of the display. If you change the trigger level or the trigger position, a line appears temporarily to highlight the changed value.

If the B-trigger is activated, the trigger is the result of an A-event followed by an B-event. The trigger point has the color of the B-trigger source.

Channel Cursors ← Aux. Cursors
Activates or deactivates the channel cursor of the active channel. A channel cursor is a line that marks the ground level of a channel. This line is displayed temporarily if the y-scaling is modified and fades out automatically.



If a DC offset is defined, a second auxiliary line is displayed. The distance between those two lines is the DC offset.

Trigger Hyst. ← Aux. Cursors
Shows or hides the hysteresis range around the trigger level when the trigger level or the hysteresis are changed. Hysteresis avoids unwanted trigger events caused by noise oscillation around the trigger level.

See also: "Hysteresis A / B" on page 44

Defaults ← Aux. Cursors
Restores the default cursor settings, i.e. both auxiliary cursors are displayed.

Grid
Defines how the grid is displayed.

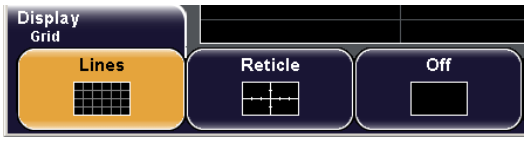

"Lines" Displays the grid as horizontal and vertical lines.

"Reticle" Displays crosshairs instead of a grid.

"Off" Removes the grid from the display.

Remote command:
`DISPlay:GRID:STYLe` on page 319

VirtualScreen
Enables or disables the virtual screen.

If enabled, the virtual screen has 20 divisions, 8 of them are displayed. To select the divisions to be displayed, press and turn the "Intensity / Virtual screen" knob at the left of the screen.

If disabled, only 8 divisions are available, and all divisions are displayed.

Remote command:
`DISPlay:VSCReen:ENABle` on page 319
`DISPlay:VSCReen:POSition` on page 320

4.2 XY-Diagram

XY-diagrams combine the voltage levels of two waveforms in one diagram. They use the amplitude of a second waveform as the x-axis, rather then a time base. This allows you to perform phase shift measurements, for example. With harmonically related signals the resulting XY-diagrams are Lissajous patterns. XY-diagrams can also be used to display the IQ representation of a signal.

It is also possible to define two source signals in y-direction for comparison.

The intensity of the XY-waveform can be set to a defined level, or be modulated dynamically using a further source signal. In the latter case, the amplitudes of additional source signal determine the intensity of the displayed waveform. For details, see chapter 4.2.1.2, "Configuring the Intensity of an XY-Waveform", on page 63.

Together with the XY-diagram, the time diagrams of the source signals are displayed in separate windows.

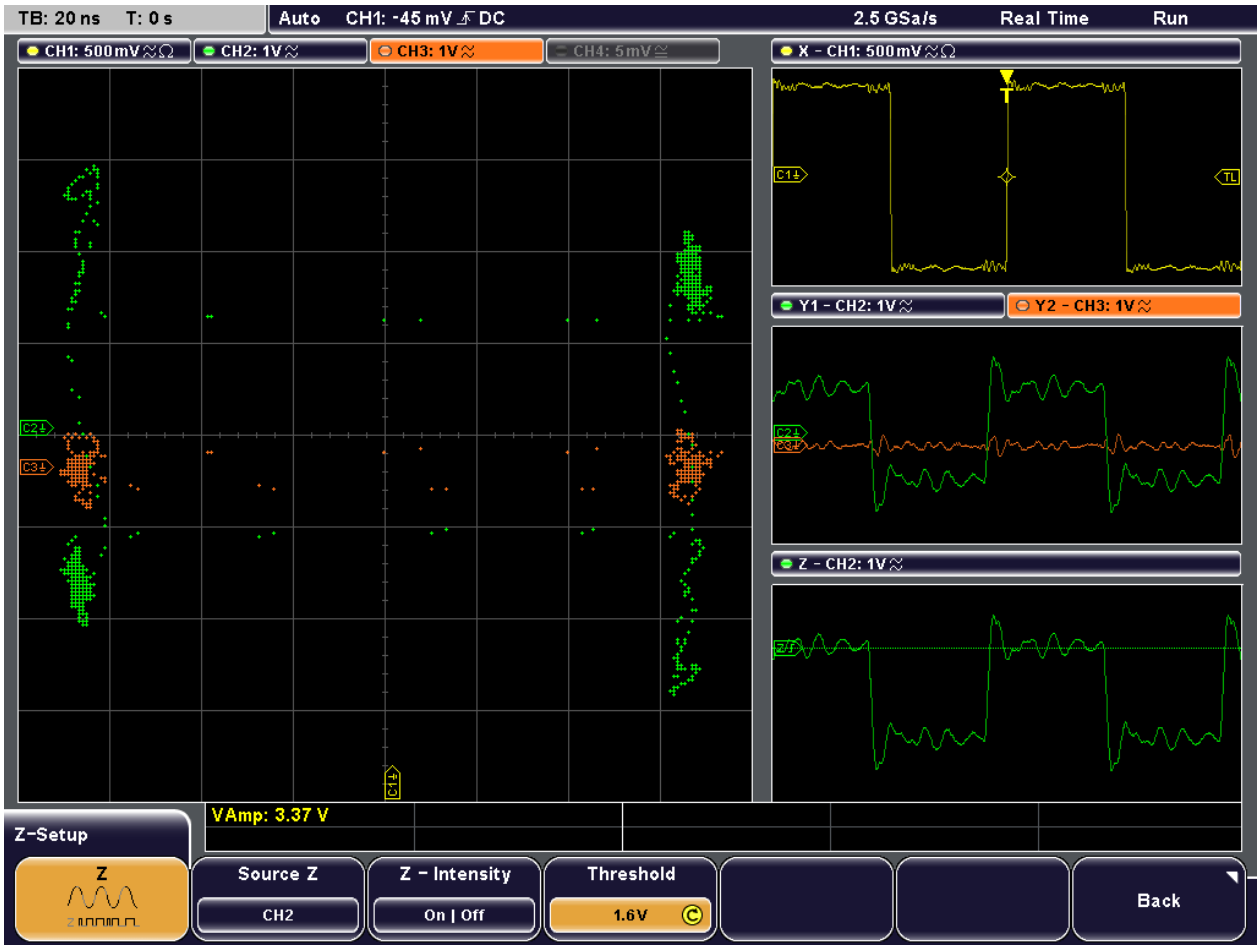

Fig. 4-1: XYZ-display

4.2.1 Configuring XY-Diagrams

XY-diagrams combine the voltage levels of two waveforms in one diagram. A further signal source can be used to determine the intensity of the XY-waveform.

4.2.1.1 Setting Up the XY-Diagram

To switch the display to XY-diagram and vice versa

► Press "DISPLAY > Display Mode" until the "XY" mode is selected.

To configure an XY-diagram

Prerequisite: The "Display Mode" is set to "XY".

1. Select "DISPLAY > XYZ Setup > Source X" to define the signal to be used as the x-axis source. Press "Source X" repeatedly until the required channel is highlighted.
2. Select "DISPLAY > XYZ Setup > Source Y1" to define the signal to be used as the (first) y-axis source. Press "Source Y1" repeatedly until the required channel is highlighted.
3. Optionally, select "DISPLAY > XYZ Setup > Source Y2" to define the signal to be used as a second y-axis source. Press "Source Y2" repeatedly until the required channel is highlighted.

   The XY-diagram is displayed in the main window, and additional windows are opened to display the X, Y1, Y2, and Z time diagrams, if the source is defined.

4.2.1.2 Configuring the Intensity of an XY-Waveform

You can define the intensity of the XY-diagram as a constant value or according to the amplitude of a further signal source Z.

- Constant intensity: To configure the intensity of an XY-waveform at a defined level
- The waveform intensity is modulated dynamically according to the signal source Z. The higher the signal level Z is, the stronger the waveform is displayed: To configure the intensity of an XY-waveform modulated by a signal amplitude.
- The waveform intensity is defined by a threshold value: If the Z signal value is below the selected threshold, the corresponding x/y point is not displayed. If the Z signal value is above the threshold, the x/y point is displayed with the defined intensity level: To configure the intensity of an XY-waveform using a threshold value

To configure the intensity of an XY-waveform at a defined level

Prerequisite: The "Display Mode" is set to "XY", and the XY-diagram is configured.

1. Press "DISPLAY > XYZ Setup > Z Setup".
2. Press the left "Source Z" softkey until "OFF" is highlighted to deactivate intensity control by the Z source.
3. Press "DISPLAY > Intensities > Trace" to define the intensity level of the waveform.
4. Enter a percentage between 0 (not visible) and 100% (very strong). The default value is 50%.

Regardless of which menu is currently displayed, you can use the "INTENSITY" knob on the left side of the screen to adjust the waveform intensity directly.

To configure the intensity of an XY-waveform modulated by a signal amplitude

Prerequisite: The "Display Mode" is set to "XY", and the XY-diagram is configured.

1. Press "DISPLAY > XYZ Setup > Z Setup".
2. Press the left "Source Z" softkey until "ON" is highlighted to activate intensity control by the Z source.
3. Press the second "Source Z" softkey repeatedly until the required channel for intensity control is selected.
4. Press "Z-Intensity" until "Modulation" is highlighted to select intensity control via modulation.

To configure the intensity of an XY-waveform using a threshold value

Prerequisite: The "Display Mode" is set to "XY", and the XY-diagram is configured.

1. Press "DISPLAY > XYZ Setup > Z Setup".
2. Press the left "Source Z" softkey until "ON" is highlighted to activate intensity control by the Z source.
3. Press the second "Source Z" softkey repeatedly until the required channel for intensity control is selected.
4. Press "Z-Intensity" until "ON | OFF" is highlighted to select intensity control via a threshold value.
5. Press "Threshold" and enter the required value to define the threshold value.

4.2.2 XYZ Setup Menu

The setup of XY-diagrams is a submenu of the "Display" menu.

Access: DISPLAY > "XYZ Setup"

Source X
Defines the source to be displayed in x direction in an XY-diagram, replacing the usual time base. The source can be selected from any of the analog channels.

The function is available in R&S RTM1054.

Remote command:
`DISPlay:XY:XSOurce` on page 315

Source Y1
Defines the (first) source to be displayed in y direction in an XY-diagram. The source can be selected from any of the analog channels.

The function is available in R&S RTM1054.

Remote command:
DISPlay:XY:Y1Source on page 315

Source Y2
Defines an optional second source to be displayed in y direction in an XY-diagram. The source can be selected from any of the analog channels.

The function is available in R&S RTM1054.

Remote command:
DISPlay:XY:Y2Source on page 316

X-CH1 Y-CH2
Defines channel 1 to be displayed in x direction in an XY-diagram, replacing the usual time base, and sets channel 2 to the y-axis.

The function is available in R&S RTM1052.

X-CH2 Y-CH1
Defines channel 2 to be displayed in x direction in an XY-diagram, replacing the usual time base, and sets channel 1 to the y-axis.

The function is available in R&S RTM1052.

Z Setup
The intensity of the waveform displayed in an XY-diagram can be set to a defined level, or be modulated dynamically using a further source signal Z. In the latter case, the amplitudes of the source signal determine the intensity of the displayed waveform.

Z ← Z Setup
Activates or deactivates the intensity control of the waveform via an additional signal source. If deactivated, the intensity is defined by the general "Intensity" setting for the trace.

Remote command:
DISPlay:XY:ZMODe on page 316

Source Z ← Z Setup
Defines the source to be used to determine the intensity of the waveform. The source can be selected from any of the analog channels. Pressing the softkey repeatedly scrolls through the list of available source channels.

Remote command:
DISPlay:XY:ZSOurce on page 316

Z-Intensity ← Z Setup
Toggles between intensity modes.

"Modulation" Modulated intensity; Intensity is modulated continuously according to the selected "Source Z".

"On | Off" Intensity is determined by a "Threshold" value. If the Z signal value is below the selected threshold, the corresponding x/y point is displayed with lowest intensity. If the Z signal value is above the threshold, the x/y point is displayed with the defined intensity level.

Remote command:
`DISPlay:XY:ZMODe` on page 316

Threshold ← Z Setup
Defines the threshold for intensity with a two-state modulation, if "Z-Intensity" is set to "ON | OFF".

Remote command:
`DISPlay:XY:ZTHReshold` on page 316

4.3 Zoom

You can zoom into waveforms to analyze the results in more detail. The zoomed area and its position can be configured numerically or using the rotary knobs.

Using Markers
You can use markers to quickly zoom into a place of interest in the display, see "To zoom into a marker position" on page 72.

4.3.1 Zoom Display

When you activate zoom display, two windows are displayed: the original waveform diagram at the top (Y(t)-window), and the zoom window at the bottom. The *zoom area* defines the part of the original waveform to be zoomed. It is indicated by white lines in the original Y(t)-window.

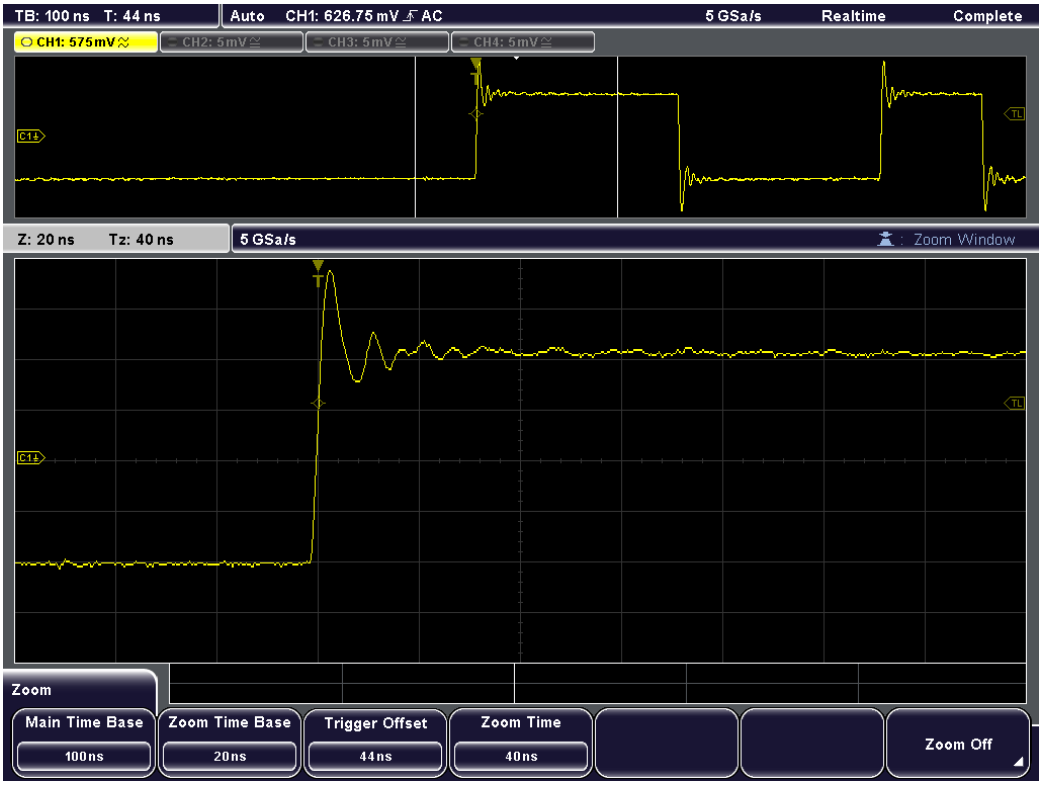

The usual channel parameters are displayed in the information bar above the original Y(t)-window (see the general display information described in the "Getting Started" manual).

In addition, the zoom area parameters are indicated in the information bar above the zoom window. The following information is given there:

Z	Zoom Time Base, i.e. scaling for the time base in the zoom window in seconds per division; determines the width of the zoom area that is displayed in the zoom window (10 divisions * scaling per division)
Tz	Zoom Time, i.e. the offset of the trigger point to the reference point 0s in the zoom window; determines the position of the zoom area
	Sample rate for zoom window

Pressing the horizontal SCALE rotary knob moves the focus between the Y(t)-window (Time Control), the zoom area (Zoom Control) and the zoom window. The currently selected screen area is highlighted and displayed in the information bar of the zoom window. Depending on the selection, the functions of the SCALE and POSITION rotary knobs may change.

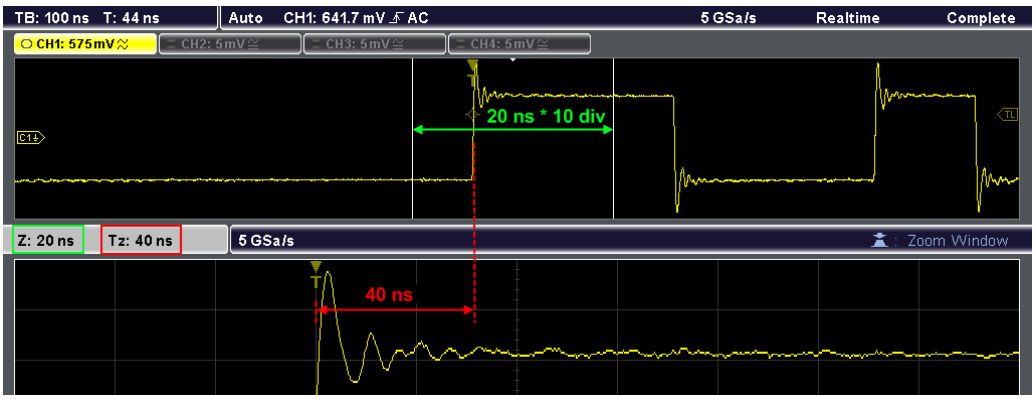

Fig. 4-2: Zoom area width and position

When you deactivate the zoom display, the previous display is restored.

4.3.2 Zooming for Details

The zoomed area and its position can be configured numerically or using the rotary knobs.

To display a zoom diagram

► Press the ZOOM key.

The key lights up and two windows are displayed: the original signal vs. time at the top, the zoom at the bottom.

To deactivate the zoom display

► Press the ZOOM key again, or press the "Zoom Off" softkey in the "Zoom" menu to close the zoom window.

The ZOOM key is no longer illuminated and the previous display is restored.

To configure the zoom area numerically

1. Press the "Zoom Time Base" softkey to define the scaling for the time base in the zoom diagram in seconds per division. The scaling is indicated by "Z" in the information bar above the zoom diagram and determines the width of the zoom area that is displayed in the zoom diagram (10 divisions * scaling per division).
2. Press the "Zoom Time" softkey to define the offset of the trigger point to the reference point 0s in the zoom diagram. The offset is indicated by "Tz" in the information bar above the zoom window and determines the position of the zoom area.

   The zoom area is indicated by white lines in the original Y(t)-window. The zoom window displays the data in the defined zoom area from the main time base in greater detail.

To configure the zoom area via the rotary knobs

Pressing the horizontal SCALE rotary knob moves the focus between the Y(t)-window (Time Control), the zoom area (Zoom Control) and the zoom window. The currently selected screen area is highlighted and displayed in the information bar of the zoom window. Depending on the selection, the functions of the SCALE and POSITION rotary knobs may change.

1. Press the horizontal SCALE rotary knob to select "Zoom Control" or "Zoom Window". The functions for the rotary knobs are the same for both elements; for very high zoom factors, however, it may be faster to scroll through with the "Zoom Window" focus.
2. Turn the horizontal SCALE rotary knob counter-clockwise to enlarge the zoom area, or clockwise to decrease it.

   The zoom diagram and the "Z" parameter (Zoom Time Base) in the information bar above it are adapted.
3. Turn the horizontal POSITION rotary knob counter-clockwise to move the zoom area to the left, or clockwise to move it to the right.

   The zoom diagram and the "Tz" parameter (Zoom Time) in the information bar above it are adapted.

   The zoom window displays the data in the defined zoom area from the main time base in greater detail.

To configure the original Y(t)-diagram

1. Press the horizontal SCALE rotary knob to select "Time Control", the original Y(t)-window.
2. Press "Main Time Base" to define the scaling for the time base in the original Y(t)-window in seconds per division. Alternatively, turn the horizontal SCALE rotary knob.
3. Press "Trigger Offset" to define the offset of the trigger point to the reference point for 0s in the original Y(t)-window. Alternatively, turn the horizontal POSITION rotary knob.
   Note that changing the offset in the original window also changes the offset for the zoom window (Zoom Time).

4.3.3 Zoom Menu

The ZOOM key provides functions for configuring the zoom display.

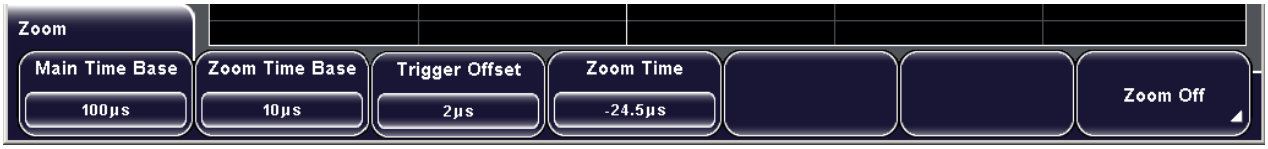

Main Time Base....70
Zoom Time Base....70
Trigger Offset....70
Zoom Time....70
Zoom Off....71

Main Time Base
Defines the scaling for the time base in the (original) Y(t)-window in seconds per division. The scaling is indicated by "TB" in the information bar above the window.

Note: If "Time Control" is selected, the main time base can be adjusted using the horizontal SCALE rotary knob.

See also "SCALE" on page 23, "To configure the original Y(t)-diagram" on page 69 and figure 8-2.

Remote command:
`TIMebase:SCALe` on page 283

Zoom Time Base
Defines the scaling for the time base in the zoom window in seconds per division. The scaling determines the width of the zoom area that is displayed in the zoom window (10 divisions * scaling per division).

The zoom area is indicated by white lines in the original Y(t)-window.

Remote command:
`TIMebase:ZOOM:SCALe` on page 320

Trigger Offset
Defines the horizontal position of the trigger point in relation to the reference point - to the zero point of the grid. The value is indicated by "T" in the information bar above the window.

The reference point is set with SETUP >"Time Reference".

Note: If a zoom or FFT window is displayed and "Time Control" is selected, the trigger offset can be adjusted using the horizontal POSITION rotary knob.
See also:
- "POSITION" on page 23
- "Time Reference" on page 235
- "To configure the original Y(t)-diagram" on page 69

Remote command:
`TIMebase:POSition` on page 284

Zoom Time
Defines the offset of the trigger point to the reference point 0s in the zoom window. The offset determines the position of the zoom area that is displayed in the zoom window.

Remote command:
`TIMebase:ZOOM:TIME` on page 320

Zoom Off
Closes the zoom window and returns to the previous display.

Remote command:
`TIMebase:ZOOM:STATe` on page 320

4.4 Markers

Markers allow you to mark certain positions on the screen, e.g. a rising or falling edge, or an unexpected signal value, or a search result. You can then use the markers to identify areas of interest you want to zoom into, and quickly move through the data.

Two marker types are available:

- Timestamp markers can be used if no search is enabled. They can be set manually at any position of the waveform. These markers are indicated by blue vertical lines. You can set up to 8 timestamp markers. Timestamp markers are descibed in this chapter.
- If a search is active, you can set search markers to selected search results. These markers are indicated by magenta search result flags. Search result markers are described in chapter 10.1, "Search Conditions and Results", on page 132

4.4.1 Using Timestamp Markers

Timestamp markers are displayed as colored lines on the screen. If more markers are available but currently not visible on the screen (e.g. in a zoomed display), this is indicated by a small arrow at the right or left edge of the display.

See also: "To use markers on search results" on page 135.

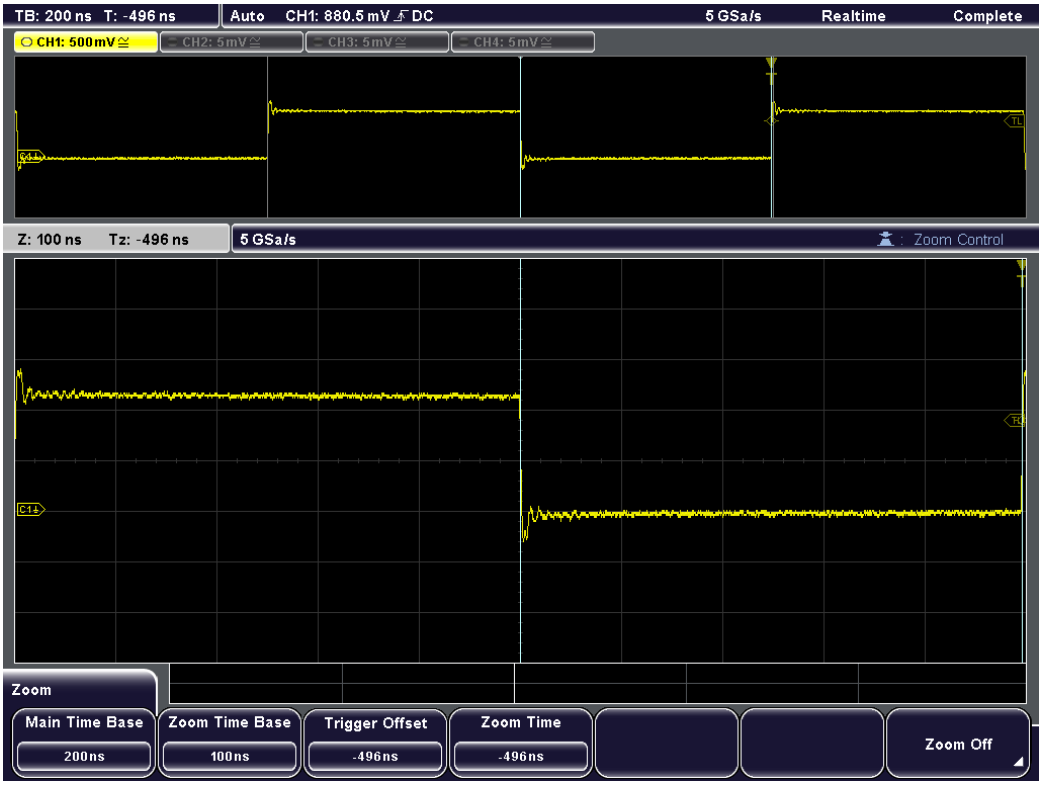

Fig. 4-3: Zoomed display using markers

To set a marker

1. Turn the horizontal "Position" rotary knob and move the position to be marked to the reference point, usually in the middle of the display.
2. Press the SET CLEAR key to insert a new marker at the reference position.

To select a marker

When you select a marker it is automatically moved to the reference point of the display.

1. Press the NEXT key to move the next (right) marker to the reference point of the display or zoom area.
2. Press the PREV key to move the previous (left) marker to the reference point of the display or zoom area.

To remove a marker

1. Select the marker to be deleted using the NEXT or PREV key.
2. Press the SET CLEAR key to remove the marker at the reference position.

To zoom into a marker position

1. Set a marker in the display as described above.

2. If not yet active, activate the zoom function by pressing the ZOOM key.

   The marker lines are displayed both in the original window and in the zoom window.

3. Select the marker that indicates the area you want to zoom into using the NEXT or PREV key.

   The center of the zoom area is moved to the marker (see figure 4-3).

4. If necessary, fine-tune the position of the zoom area around the marker as described in "To configure the zoom area via the rotary knobs" on page 69.

4.4.2 Reference for Markers

The marker keys are used for both marker types, timestamp markers and search result markers.

For details on setting and moving markers; see

- chapter 4.4.1, "Using Timestamp Markers", on page 71
- "To use markers on search results" on page 135

NEXT....73
PREV....73
SET CLEAR....73

NEXT
Moves the next (right) marker to the reference point of the display or zoom area. If a search is enabled, the key navigates the search result markers.

Note: If another marker is available at the right, but currently not visible on the screen, a small red arrow is displayed at the right edge of the display.

Remote command:
`TSTamp:NEXT` on page 321 (for timestamp markers only)

PREV
Moves the previous (left) marker to the reference point of the display or zoom area. If a search is enabled, the key navigates the search result markers.

Note: If another marker is available at the left, but currently not visible on the screen, a small red arrow is displayed at the left edge of the display.

Remote command:
`TSTamp:PREVious` on page 321 (for timestamp markers only)

SET CLEAR
Sets a new marker at the reference point of the display, or deletes an existing marker at this point. Use the NEXT and PREV keys to move the markers to the reference point.

In the display of search results, the marker is set to or removed from the search result that is selected in the "Event Table".

5 Reference Waveforms

Reference waveforms are waveform data stored in in the internal reference storages. Four internal reference storages are available: RE1 - RE4. These four reference waveforms can be displayed.

Reference waveforms can be saved to and loaded from any storage device - internal memory or external USB flash device. The file format is `.TRF`, and the file size is about 12.4 Byte. The file content depends on the storage device:

- Internal storage of the R&S RTM: TRF files contain also the instrument settings, so you can restore also the settings when you load a reference waveform.
- External USB flash drive: TRF files contain only the waveform data, the instrument settings are not saved and cannot be restored.

See chapter 13.2.4.1, "Waveform File Formats", on page 227 for details on file formats.

You can copy the stored references to another storage device with usual export/import functions. With export/import, you can also change the target file format and convert the data. If you export a TRF file to a USB flash drive, the instrument settings get lost and cannot be loaded with the waveform data anymore. To copy a stored reference, use FILE >"Import/Export References". See also: chapter 13.2.1.2, "Importing and Exporting Data", on page 218.

Furthermore, you can save waveforms directly to a USB flash drive with FILE > "Waveforms", without creating a reference waveform before. See: chapter 13.2.4, "Waveforms", on page 227.

5.1 Using References

You can store any of the active waveforms as reference waveform - channel, math, and other reference waveforms - or load a previously saved reference.

If MSO option R&S RTM-B1 is installed, you can store also the pods of digital channels as references.

For each selected reference waveform, you can adjust the vertical position and scale as usual, and, unlike for other waveform types, you can also adjust the horizontal position and scale individually.

The current scale values are shown in the waveform label of the reference waveform.

5.1.1 Displaying a Reference Waveform

A reference waveform is displayed as soon as data is written to its storage, either from an active waveform, or loaded from a reference file. You can hide it and display it again by using the "Visible" key.

1. Press the REF key to display the "Reference" menu.

2. Press "Reference" and select the reference storage position.
   If a reference was already loaded to the selected reference position before, the stored reference waveform is displayed.
3. Select the data that will be used as reference by doing one of the following:
   - Press "Source" and select one of the active waveforms, then press "Update".
   - Load a previously saved reference.
     See also: "To load references and reference settings" on page 75.

   The selected data is written to the selected reference storage and displayed.
4. Press "Visible" to hide and show the reference waveform.

5.1.2 Saving and Loading References

If you need more than four references, or you want to keep a reference for other measurements, you can save it and load it back to the instrument when needed. Import and export is also possible.

The instrument settings are saved together with the reference waveform only in the internal storage. They are removed from the reference file when you save or export the file to an external storage (USB flash device).

To save references

1. Press REF to display the "Reference" menu
2. Press "Save".
3. Press "Source" and select the waveform whose data you want to save as a reference.
   All active waveforms can be saved.
4. Press "Storage" and define the storage settings.
   See: "To select the storage directory" on page 218.
5. Press "File Name" and enter the name of the target file.
   See: "To define a new file or directory name" on page 218.
6. Press "Save".

To copy a stored reference, use FILE > "Import/Export References". For import/export procedure, see chapter 13.2.1.2, "Importing and Exporting Data", on page 218.

To load references and reference settings

1. Press REF.
2. Press "Load".
3. Press "Reference" and select the reference number you want to load the reference to.

4. Press "Load".

   A file explorer is displayed.

5. Select the storage device and the file that contains the reference. Use the "Navigation" knob to scroll through the directories. To change the directory, scroll to the name of the directory and press the knob, or press "Change Directory".

6. Press "Load".

   The saved reference is loaded to the R&S RTM.

7. If you also want to load the settings that were used to create the reference waveform:

   a) In the "Reference" or "Load" menu, press "Reference" and select the reference number you want to load the settings to.
   b) Press "Load Settings".
   "Load Settings" is only available if the waveform was loaded to the reference storage before, you cannot laod the setting first.

5.2 Reference for REF key

The REF key provides functions for working with reference waveforms on the instrument.

For details on working with these functions, see chapter 5.1, "Using References", on page 74.

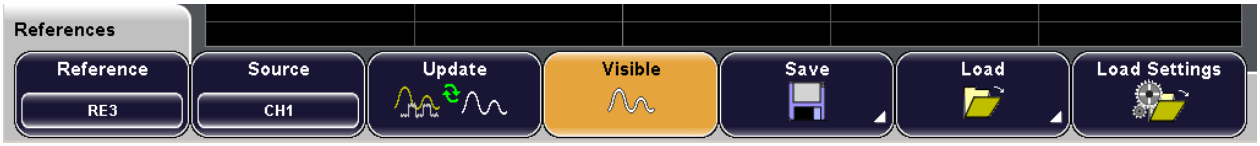

Reference....76
Source....76
Update....77
Visible....77
Save....77
Load....77
└ Reference....77
└ Load....77
Load Settings....77

Reference
Selects one of the four possible internal reference storages.

See also: chapter 5.1, "Using References", on page 74.

Source
Defines the source of the reference waveform. Any active channel, math or reference waveform can be selected.

If MSO option R&S RTM-B1 is installed, you can store also the pods of digital channels as references.

Remote command:
REFCurve<m>:SOURce on page 322
REFCurve<m>:SOURce:CATalog? on page 323

Update
Stores the waveform defined as the "Source" to the selected reference waveform. The reference waveform is kept until you update or load another waveform to the reference.

See also: chapter 5.1.1, "Displaying a Reference Waveform", on page 74.

Remote command:
REFCurve<m>:UPDate on page 323

Visible
Displays or hides the selected reference waveform.

Remote command:
REFCurve<m>:STATe on page 322

Save
Opens the "Save" menu with basic functions to save the equation set.

See "Save Menu" on page 220 .

Remote command:
REFCurve<m>:SAVE on page 323

Load
Provides functions to load reference data.

Reference ← Load
Selects one of the four possible internal reference storages.

See also: chapter 5.1, "Using References", on page 74.

Load ← Load
Opens the "Load" menu and a file explorer to select the reference waveform file for loading.

See "Load Menu" on page 221.

Remote command:
REFCurve<m>:LOAD on page 324

Load Settings
Loads the device settings that were used to obtain the stored reference waveform. The settings are only available if the file was stored to the internal storage `/INT/REFERENCE` and never written to an external storage (USB stick).

Remote command:
REFCurve<m>:LOAD:STATe on page 324

6 Measurements

The following measurement methods are available:

- CURSOR: Cursor measurements determine specific measurement results at the current cursor positions of an active waveform; the results are displayed in a result table.
- QUICK MEAS: performs basic automatic measurements for the selected channel immediately; the results are displayed directly at the waveform and in a result table.
- MEAS: With automatic measurements, up to four amplitude and time measurements or pulse counts can be configured and performed simultaneously; based on an active channel, reference, or math waveforms. The results are displayed in a result table, the color of the results corresponds with the source waveform color. These measurements can be performed together with the "Quick Meas" measurements.

Use the full height of the screen for waveform display to get best vertical resolution and measurement results.

6.1 Cursor Measurements

Using the CURSOR key you can determine specific measurement results at the current cursor positions for various waveforms. The cursors can be set to the required position with the Navigation rotary knob, or set to typical positions on a keypress.

You can measure on any active channel, math, or reference waveform, and also on the resulting waveform of an FFT analysis and on XY-waveforms.

If MSO option R&S RTM-B1 is installed, active digital channels are available as measurement sources for time and count cursor measurements, and the bit values of the pods can be determined.

6.1.1 Cursor Measurements Types and Results

Cursor measurements are based on automatic measurements. The cursor measurement is limited to the cursor positions or the part of the waveform between the cursors while automatic measurements considers the complete display of the waveform. Thus you can focus the measurement to the interesting part of the waveform by using cursors. The results are displayed in the right part of the result table.

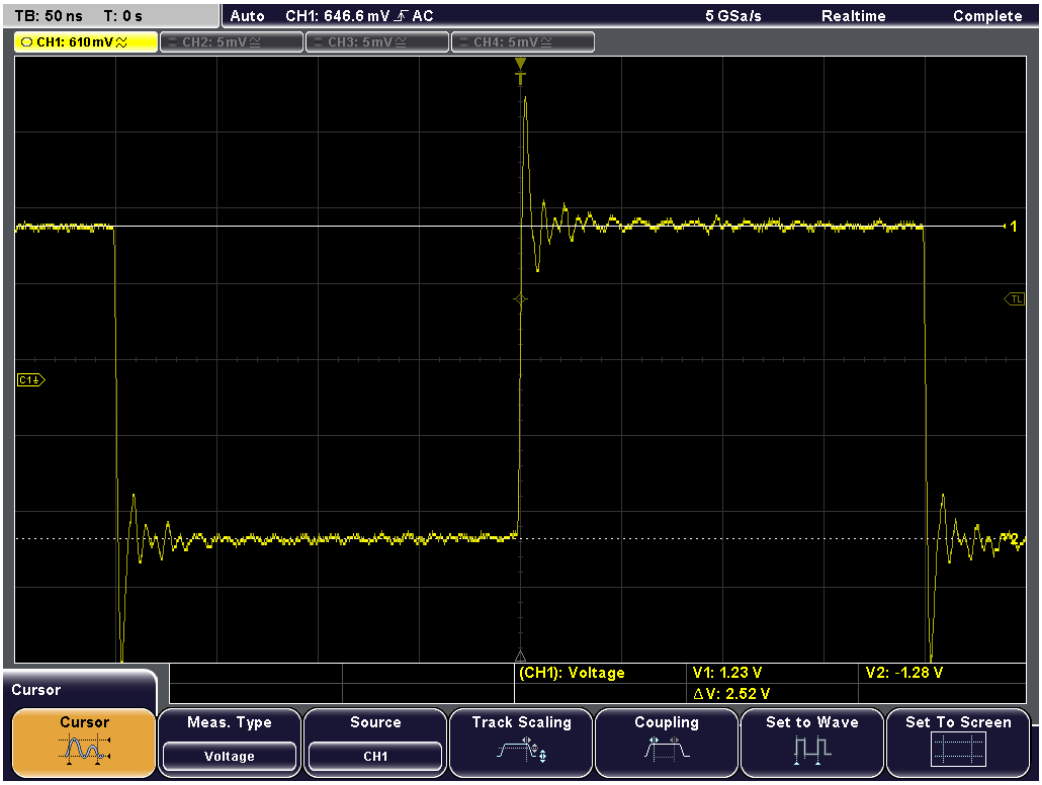

For cursor measurements on channel, math, and reference waveforms, various measurement types are available, for example, Peak, RMS, Mean und Count. Cursor measurement is also possible on the results of an FFT analysis. It measures the frequencies and levels at the cursor positions and their differences.

If MSO option R&S RTM-B1 is installed, time and count measurements can be performed on active digital channels, and the bit values of the pods can be determined.

Available cursor measurements are:

Voltage....79
Time....80
Voltage & Time....80
Ratio X....80
Ratio Y....80
Count....80
Peak Values....80
RMS, Mean, σ....80
Duty Ratio....81
Burst Width....81
Rise Time....81
V-Marker....81
Crest factor....81

Voltage
Sets two horizontal cursor lines and measures the voltages at the two cursor positions and the delta of the two values.

Results: V1, V2, ΔV

Time
Sets two vertical cursor lines and measures the time from the trigger point to each cursor point, the time between the two cursors and the frequency calculated from that time.

Results: t1, t2, Δt, 1/t

Voltage & Time
Combines the "Voltage" cursor and "Time" cursor measurements. Two horizontal and two vertical cursor lines are set and the voltages and time from the trigger point are measured at the cursor positions, as well as the delta of the voltage and time values.

Results: t1, t2, Δt, V1, V2, ΔV

Ratio X
Provides three cursors and measures the ratio of the x-values (e.g. a duty cycle) between the first and second cursors and the first and third cursors:

(x2-x1)/(x3-x1)

The ratio is displayed as a floating value, in percent, in degrees and as a radian.

Results: abs, %, °, π

Ratio Y
Provides three cursors and measures the ratio of the y-values (e.g. overshooting) between the first and second cursors and the first and third cursors:

(y2-y1)/(y3-y1)

The ratio is displayed as a floating value and in percent.

Results: abs, %

Count
Provides three cursors to count signal transitions. The time base is defined by the first two cursors, the third cursor defines the threshold value. As a result, the number of rising and falling edges as well as the number of positive and negative impulses is counted.

Results: ⎍, ⎏, ⎎, ⎐

Peak Values
Measures the positive and negative peak values between the two cursors, as well as the absolute difference between the two peak values (peak-to-peak value):

Vpp = |(Vp+) - (Vp-)|

Results: Vp+, Vp-, Vpp

RMS, Mean, σ
Measures the root mean square (RMS), the mean value, and the standard deviation of measurement results between the two cursors.

Results: Mean, RMS, σ

Duty Ratio
Measures the positive and negative duty cycles. The duty cycle is the ratio between the duration of a positve pulse (high active) or a negative pulse (low-active) and the period of a rectangular waveform. The measurement requires at least one complete period of the signal between cursor 1 and cursor 2. Pulse duration and period are measured at cursor 3.

Results: Dty+, Dty- (in %)

Burst Width
Measures the duration of a burst. Two vertical cursors mark the beginning and the end of the burst. The horizontal cursor sets the threshold value, and the time between the first and the last edge of the burst is returned.

Result: BstW

Rise Time
Measures the rise and fall times of the left-most edge in the display between the upper and lower reference levels. The reference levels are set in the Auto Measure menu: MEAS > "Reference Level".

See also: Reference Level: Upper, Middle, Lower Levels.

Results: tr, tf

V-Marker
Two vertical markers are provided and the values of the waveform at the marker positions are measured. Additionally, the differences of the two values in x- and y-direction are displayed.

Results: V1, V2, Δt, ΔV

Crest factor
The crest factor is also known as peak-to-average ratio. It is calculated from the maximum value divided by the RMS value of the waveform. The measurement value is displayed as "Crest" in the result table.

$$Crest = \frac{V_{P+}}{RMS}$$

6.1.2 Performing Cursor Measurements

The cursors are activated according to the latest setting as soon as you press the CURSOR key.

To configure cursor measurements

1. Press the CURSOR key.

   The cursors are activated according to the latest setting.

2. Press "Meas. Type" to select the type of measurement to perform. The type determines which results are displayed in the result table.
   See also: "Meas.Type" on page 83.

3. Press "Source" to select the waveform for which the measurement is to be performed. The source can be any active waveform depending on the selected measurement type.
4. Move the cursors to obtain the required results.
   See also: "To change the position of the cursors" on page 82.

   The cursor measurement is performed and the results are displayed in the result table.

To change the position of the cursors

The cursor measurement displays the results depending on the current position of the cursors. Move the cursors to obtain the results for a specific time range or at specific signal points.

1. Press the NAVIGATION rotary knob to select the first cursor. If a selection menu is open, it is closed.

   Tip: If the cursors have disappeared from the screen or must be moved extensively within the screen, press "Set To Screen" in the "Cursor" menu to reset the cursors to their default positions.
2. Turn the NAVIGATION knob to change the position of the selected cursor line.
3. Press the knob again to select the next cursor line, and turn to adjust position.
4. To simplify the cursor positioning, the following functions are helpful:
   - "Track Scaling" to adjust the cursor position when the vertical or horizontal scaling are changed
   - "Coupling" to keep the distance between two cursor lines constant while one of the cursors is moved
   - "Set to Wave" to set the cursor lines to typical points of the waveform based on automatic measurements in the background

   See also: chapter 6.1.3, "Cursor Menu", on page 82.

   The results of the cursor measurement in the result table are updated.

To deactivate cursor measurements

1. Press the CURSOR key.
2. Press the "Cursor" softkey.

   The "Cursor" softkey is no longer highlighted, no more measurements are performed, the cursor lines disappear and the results are removed from the result table.

6.1.3 Cursor Menu

The CURSOR key opens the "Cursor" menu to configure manual measurements.

See also: chapter 6.1.2, "Performing Cursor Measurements", on page 81.

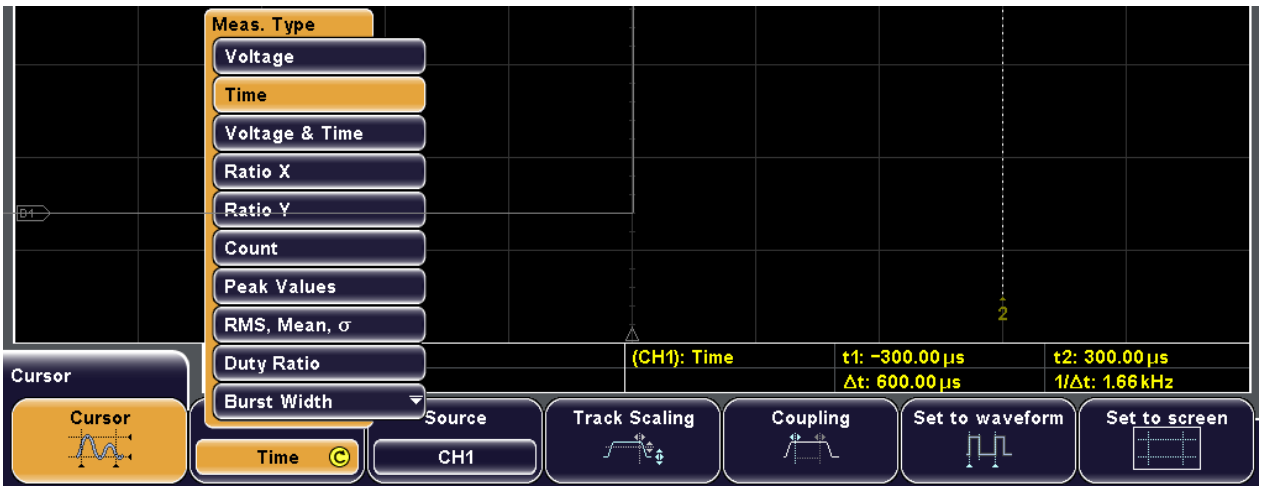

Cursor....83
Meas.Type....83
Source....83
Track Scaling....84
Coupling....84
Set to Wave....84
Set To Screen....84
Prev. peak....84
Next peak....85
NAVIGATION....85

Cursor
Activates or deactivates the selected cursor measurement.

Remote command:
`CURSor<m>:STATe` on page 327

Meas.Type
Selects the cursor measurement type. Depending on the type, different results are displayed in the result table.

For a list of all cursor measurement types and their description, see chapter 6.3.1.1, "Measurement Types", on page 87.

Depending on the measurement type, two or three cursors are provided which can be set to the required position using the "Navigation" rotary knob. See also: "To change the position of the cursors" on page 82.

The measurement type setting is not available for cursor measurments on FFT analysis.

Remote command:
`CURSor<m>:FUNCtion` on page 328

Source
Defines the source of the cursor measurement as one of the active channel, math, or reference waveforms.

If MSO option R&S RTM-B1 is installed, also digital channels D0 to D15 are available for time, ratio X, count, duty ratio, and burst width measurements, and the pods D0...D7 and D8...D15 are available for V-marker measurements. Available sources depend on the selected measurement type.

The source setting is not available for cursor measurements on FFT analysis and in XY mode.

Remote command:
`CURSor<m>:SOURce` on page 327

Track Scaling
If enabled, "Track Scaling" adjusts the cursor lines if the vertical or horizontal scales are changed. The cursor lines keep their relative position to the waveform.

If disabled, the cursor lines remain on their position on the display if the scaling is changed.

Remote command:
`CURSor<m>:TRACking:SCALe[:STATe]` on page 331

Coupling
If enabled, the cursors of a can be coupled and moved together. Press the NAVIGATION key to select both corsors or one cursor to be moved.

If disabled, the NAVIGATION key toggles the single cursor lines.

Remote command:
`CURSor<m>:XCOupling` on page 330
`CURSor<m>:YCOupling` on page 330

Set to Wave
Autoset for cursor lines, sets the cursor lines to typical points of the waveform depending on the selected measurement type. For example, for voltage measurement, the cursor lines are set to the upper and lower peaks of the waveform. For time measurement, the cursor lines are set to the edges of two consecutive positive or two consecutive negative pulses.

Remote command:
`CURSor<m>:SWAVe` on page 331

Set To Screen
Resets the cursors to their initial positions. This is helpful if the cursors have disappeared from the display or need to be moved for a larger distance.

Remote command:
`CURSor<m>:SSCReen` on page 331

Prev. peak
For FFT analysis only: sets the selected cursor to the previous (left) level peak.

To select the cursor, press the NAVIGATION knob.

Remote command:
`CURSor<m>:SPPeak` on page 331

Next peak
For FFT analysis only: sets the selected cursor to the next (right) level peak.

To select the cursor, press the NAVIGATION knob.

Remote command:
`CURSor<m>:SNPeak` on page 331

NAVIGATION
Select cursor: Press the NAVIGATION rotary knob to select a cursor line. If a menu is open, it is closed. Press the knob repeatedly to select the required cursor line or - if Coupling is enabled - a pair of coupled cursor lines.

Move selected cursor: Turn the rotary knob to change the position of the selected cursor line.

Remote command:
`CURSor<m>:X1Position` on page 330
`CURSor<m>:X2Position` on page 330
`CURSor<m>:X3Position` on page 330
`CURSor<m>:Y1Position` on page 330
`CURSor<m>:Y2Position` on page 330
`CURSor<m>:Y3Position` on page 330

6.2 Quick Measurements

Quick measurement performs all currently available automatic measurements for the selected channel. The measurements cannot be configured. The results are displayed either directly at the waveform (WF) or in the right part of the result table (T) and are updated continuously.

► Press the QUICK MEAS key to activate quick measurement.

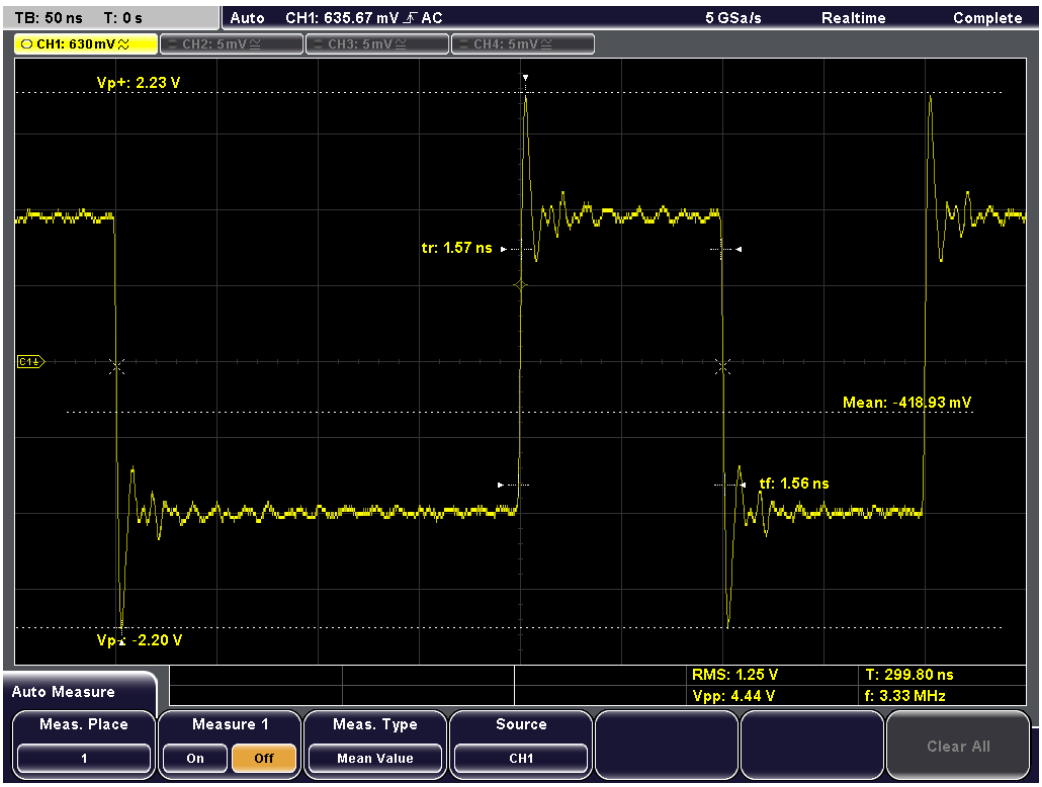

The following measurement results are determined for the displayed section of the waveform:

Label	Description	Display
Vp+	Positive peak value	WF
Vp-	Negative peak value	WF
tr	Rising time of the first rising edge	WF
Mean	Mean value	WF
tf	Falling time of the first falling edge	WF
RMS	RMS	T
Vpp	Peak to peak value	T
T	Period length	T
f	Frequency	T

When you activate quick measurements, cursor measurements are automatically deactivated, as well as the reference and math menus. Deactivate quick measurements before selecting these functions. Channels other than the selected one are switched off in quick measurement mode.

► Press the QUICK MEAS key again to deactivate the quick measurement and remove the results.

Remote command:

- MEASurement<m>:ALL[:STATe] on page 335
- MEASurement<m>:AON on page 335
- MEASurement<m>:AOFF on page 335
- MEASurement<m>:ARESult? on page 335

6.3 Automatic Measurements

Using the MEAS key you can configure up to four amplitude and time measurements or pulse counts on one of the active channel, reference or math waveforms.

If MSO option R&S RTM-B1 is installed, active digital channels are available as measurement sources for time and count measurements.

- Measurement Types and Results....87
- Configuring and Performing Automatic Measurements....93
- Auto Measure Menu (MEAS key)....94

6.3.1 Measurement Types and Results

- Measurement Types....87
- Measurement Results....92
- Statistics....93

6.3.1.1 Measurement Types

The R&S RTM provides a varity of automatic measurements:

Mean Value....88
RMS Value....88
Mean Cycle....88
RMS Cycle....88
Peak Peak....88
Peak +....88
Peak -....88
Frequency....88
Period....89
Amplitude....89
Crest factor....89
Top Level....89
Base Level....89
Pulse Width (positive pulse)....89
Pos. Overshoot....89
Neg. Overshoot....89
Pulse Width (negative pulse)....90
Duty Cycle +....90

Duty Cycle -....90
Rise Time....90
Fall Time....90
σ-Std. Dev. Wave....90
σ-Std. Dev. Cycle....90
Delay....91
Phase....91
Burst Width....91
Count positive pulses....91
Count negative pulses....91
Count rising edges....91
Count falling edges....91
Trigger Freq....91
Trigger Period....92
Trigger B Freq....92
Trigger B Period....92

Mean Value
Determines the mean value of the complete displayed waveform. The measurement value is displayed as "Mean" in the result table.

RMS Value
Measures the RMS (Root Mean Square) value of the voltage of the complete displayed waveform. The measurement value is displayed as "RMS" in the result table.

Mean Cycle
Measures the mean value of the left-most signal period. The measurement value is displayed as "MnCy" in the result table.

RMS Cycle
Measures the RMS (Root Mean Square) value of the voltage of the left-most signal period. The measurement value is displayed as "RMSCy" in the result table.

Peak Peak
Measures the peak-to-peak value within the displayed section of the waveform. The measurement value is displayed as "Vpp" in the result table.

Peak +
Measures the maximum value within the displayed section of the waveform. The measured value is displayed as "Vp+" in the result table.

Peak -
Measures the minimum value within the displayed section of the waveform. The measured value is displayed as "Vp-" in the result table.

Frequency
Measures the frequency of the signal. The result is based on the length of the left-most signal period within the displayed section of the waveform. The measurement value is displayed as "f" in the result table.

Period
Measures the length of the left-most signal period within the displayed section of the waveform. The measurement value is displayed as "T" in the result table.

Amplitude
Measures the amplitude of a square wave. To do so, the potential difference between high and low level ("Vbase" and "Vtop") is calculated. The measurement requires at least one complete period of a triggered signal. The measured value is displayed as "VAmp" in the result table.

Crest factor
The crest factor is also known as peak-to-average ratio. It is calculated from the maximum value divided by the RMS value of the waveform. The measurement value is displayed as "Crest" in the result table.

$$Crest = \frac{V_{P+}}{RMS}$$

Top Level
Measures the mean value of the high level of a square wave. To do so, the mean value of the tilt is calculated (without the overshoot). The measurement and requires at least one complete period of a triggered signal. The measured value is displayed as "Vtop" in the result table.

Base Level
Measures the mean value of the low level of a square wave. To do so, the mean value of the tilt is calculated (without the overshoot). The measurement requires at least one complete period of a triggered signal. The measured value is displayed as "Vbase" in the result table.

Pulse Width (positive pulse)
⎍: Measures the width of a positive pulse. A positive pulse consists of a rising edge followed by a falling edge. The measurement and requires at least one complete period of a triggered signal. The measured value is displayed as "t⎍" in the result table.

Pos. Overshoot
Positive overshoot of a square wave, calculated from measurement values Top Level, Peak +, and Amplitude. The measured value is displayed as "+Ovr" in the result table.

$$+Ovr = \frac{V_{top} - V_{P+}}{V_{Amp}} \cdot 100\%$$

Neg. Overshoot
Negative overshoot of a square wave, calculated from measurement values Min, Low, and Amplitude. The measured value is displayed as "-Ovr" in the result table.

$$-Ovr = \frac{V_{base} - V_{P-}}{V_{Amp}} \cdot 100\%$$

Pulse Width (negative pulse)
⊔: Measures the width of a negative pulse. A negative pulse consists of a falling edge followed by a rising edge. The measurement requires at least one complete period of a triggered signal. The measured value is displayed as "t⊔" in the result table.

Duty Cycle +
Measures the positive duty cycle. The duty cycle is the ratio between the duration of a positve pulse (high active) and the period of a rectangular waveform. The measurement requires at least one complete period of a triggered signal.

The result is the measured value as a percentage of the signal period and is displayed as "Dty+" in the result table.

Duty Cycle -
Measures the positive duty cycle. The duty cycle is the ratio between the duration of a negative pulse (low active) and the period of a rectangular waveform. The measurement requires at least one complete period of a triggered signal.

The result is the measured value as a percentage of the signal period and is displayed as "Dty-" in the result table.

Rise Time
Measures the rise time of the left-most rising edge within the displayed section of the waveform. The rise time is determined as the time it takes the signal to rise from the lower reference level to the upper reference level which are set with "Upper Level" and "Lower Level" in the "Reference Level" menu. The measurement result is displayed as "tr" in the result table.

See also: "Reference Level: Upper, Middle, Lower Levels" on page 97.

Fall Time
Measures the falling time of the left-most falling edge within the displayed section of the waveform. The fall time is determined as the time it takes the signal to fall from the upper reference level to the lower reference level which are set with "Upper Level" and "Lower Level" in the "Reference Level" menu. The measurement result is displayed as "tf" in the result table.

σ-Std. Dev. Wave
Measures the standard deviation of the complete waveform.

$$\sigma_X = \sqrt{\frac{1}{N_{Eval} - 1} \sum_{i=1}^{N_{Eval}} (x(i) - X_{Mean})^2}$$

X_{Mean} = Mean Value
X(i) = Value of the measured waveform sample
N_{Eval} = Number of waveform samples

σ-Std. Dev. Cycle
Measures the standard deviation of one cycle, usually of the first, left-most signal period.

Delay
Measures the time difference on the middle reference level between two slopes of the same or different waveforms. The measurement value is displayed as "Delay" in the result table.

Select the sources and slopes in the Delay Setup menu.

Set the middle reference level in the Reference Level menu.

Phase
Phase difference between two waveforms (time difference/period * 360) on the middle reference level. The measurement value is displayed as "Phase" in the result table.

Select the waveforms in the Phase Setup menu.

Set the middle reference level in the Reference Level menu.

Burst Width
Duration of one burst, measured from the first edge to the last edge that cross the middle reference level. The measurement value is displayed as "Bst" in the result table.

Set the middle reference level in the Reference Level menu.

Count positive pulses
Count ⎍: Counts positive pulses within the displayed section of the waveform. A positive pulse consists of a rising edge followed by a falling edge. The mean value of the signal is determined. If the signal passes the mean value, an edge is counted. The pulse is counted if a rising edge and a falling edge are detected. The number of positive pulses is displayed as "Cnt ⎍" in the result table.

Count negative pulses
Count ⏔: Counts negative pulses within the displayed section of the waveform. A negative pulse consists of a falling edge followed by a rising edge. The mean value of the signal is determined. If the signal passes the mean value, an edge is counted. The pulse is counted if a falling edge and a rising edge are detected. The number of negative pulses is displayed as "Cnt ⏔" in the result table.

Count rising edges
Count ⎍: Counts transitions of the signal from low level to high level within the displayed section of the waveform. To do so, the mean value of the signal is determined. If the signal passes the mean value, a rising edge is counted. The number of rising edges is displayed as "Cnt ⎍" in the result table.

Count falling edges
Count ⏌: Counts transitions of the signal from high level to low level within the displayed section of the waveform. To do so, the mean value of the signal is determined. If the signal passes the mean value, a falling edge is counted. The number of falling edges is displayed as "Cnt ⏌" in the result table.

Trigger Freq.
Measures the frequency of the A-trigger signal based on the length of its period. The measurement value is displayed as "f(Tr)" in the result table.

Trigger Period
Measures the length of the A-trigger signal periods (hardware counter). The measurement value is displayed as "T(Tr)" in the result table.

Trigger B Freq.
Measures the frequency of the B-trigger signal based on the length of its period. The measurement value is displayed as "f(TrB)" in the result table.

Trigger B Period
Measures the length of the B-trigger signal periods. The measurement value is displayed as "T(TrB)" in the result table.

6.3.1.2 Measurement Results

The results of an automatic measurement are displayed in the result table below the diagram. The color of the results in the left part of the result table corresponds with the source waveform color. If the result for the selected measurement type cannot be determined, e.g. because a complete period of a signal is required but not available, a "?" is displayed.

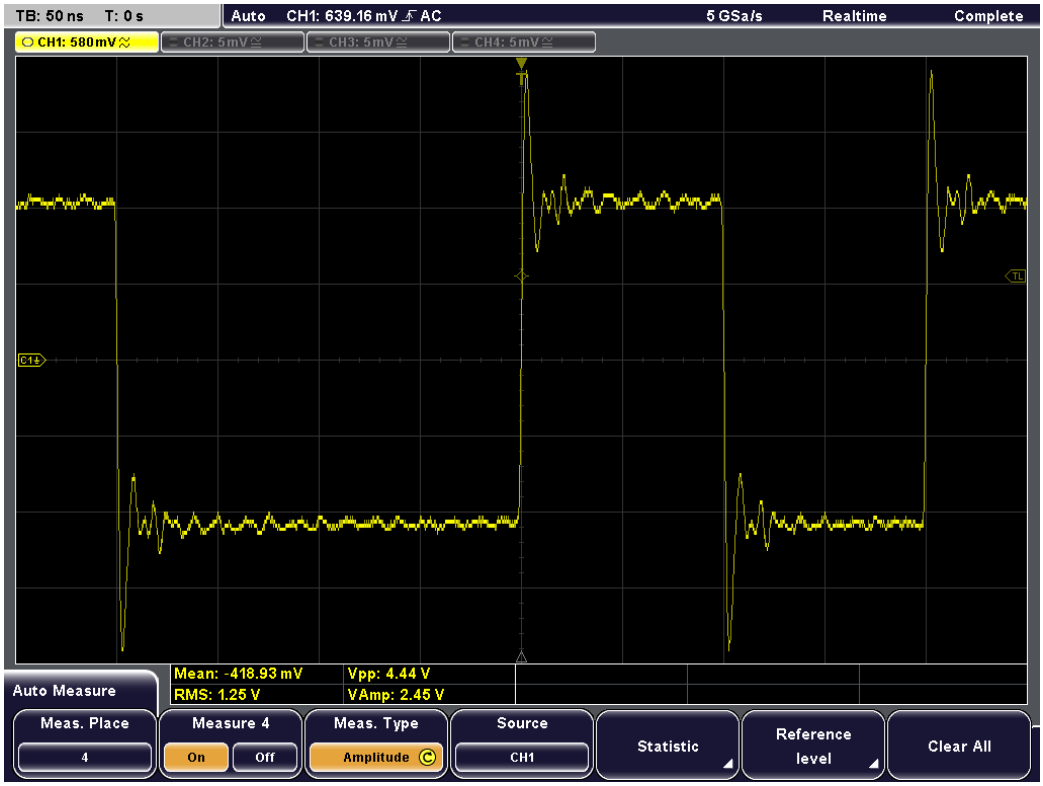

Remote command:

MEASurement<m>:RESult[:ACTual]? on page 340

6.3.1.3 Statistics

For each active measurement, you can enable a statistic evaluation of the measurement results. It returns the current, minimum and maximum measurement values, the average and standard deviation, and the number of measured waveforms.

For configuration settings, see "Statistic" on page 96.

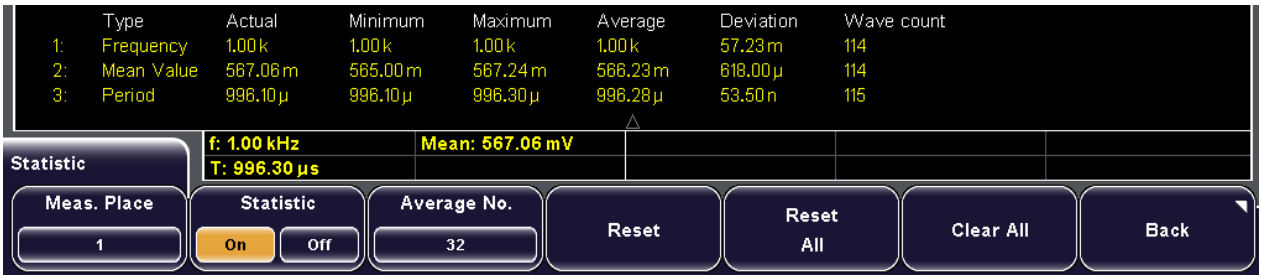

Remote command:

- `MEASurement<m>:RESult[:ACTual]?` on page 340
- `MEASurement<m>:RESult:AVG?` on page 343
- `MEASurement<m>:RESult:STDDev?` on page 343
- `MEASurement<m>:RESult:NPEak?` on page 344
- `MEASurement<m>:RESult:PPEak?` on page 344
- `MEASurement<m>:RESult:WFMCount?` on page 344
- `MEASurement<m>:STATistics:VALue:ALL?` on page 344
- `MEASurement<m>:STATistics:VALue<n>?` on page 345

6.3.2 Configuring and Performing Automatic Measurements

To configure and activate automatic measurements

1. Press the MEAS key.
2. Press "Meas. Place" to select one of the four measurement positions.
3. Press "Meas. Type" to select the type of measurement to perform. The type determines which results are displayed in the result table.
   See also: "Meas. Type" on page 95.
4. Press "Source" to select the waveform for which the measurement is to be performed. The source can be any active waveform depending on the selected measurement type.
5. For rise time, fall time, delay and phase measurements, press "Reference Level" and set the reference levels as percentages of the high signal level.
   See also: "Reference Level: Upper, Middle, Lower Levels" on page 97

6. Press "Measure 1-4" until "On" is highlighted to activate the measurement.

   The selected measurement is activated and the results are displayed in the result table.

To activate configured automatic measurements

1. Press the MEAS key.
2. Press "Meas. Place" to select one of the four measurement positions.
3. Press "Measure 1-4" until "On" is highlighted.

To deactivate automatic measurements

1. Press the MEAS key.
2. Press "Meas. Place" to select the measurement you want to deactivate.
3. Press "Measure 1-4" until "Off" is highlighted.
4. If you want to reset and deactivate all automatic measurements at once, press "Clear All" in the "Auto measure" menu.

   No more measurements are performed, the results are removed from the result table.

To use statistics

1. Press the MEAS key.
2. Configure at least one mesurement as described in "To configure and activate automatic measurements" on page 93.
3. Press "Statistic".
4. Press "Meas. Place" to select the measurement for which you need statistical results.
5. Press "Statistic" until "On" is highlighted.
6. Press Average No. and enter the number of measured waveforms to be used for calculation of average and standard deviation.

6.3.3 Auto Measure Menu (MEAS key)

The MEAS key opens the "Auto Measure" menu to configure automatic measurements.

For details, see chapter 6.3, "Automatic Measurements", on page 87.

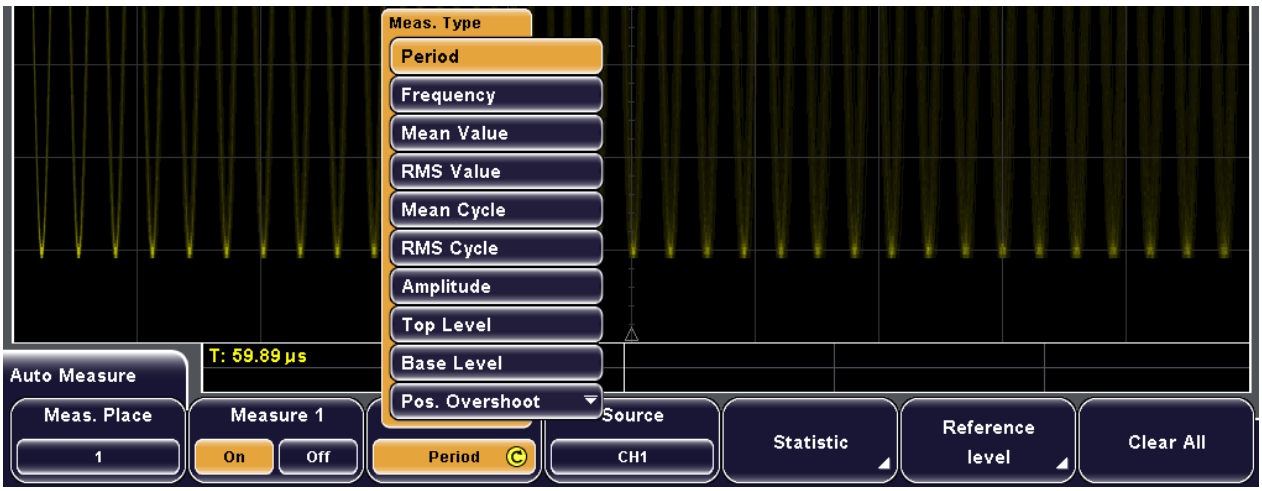

Meas. Place....95
Measure 1-4....95
Meas. Type....95
Source....96
Statistic....96
└ Meas. Place....96
└ Statistic....96
└ No. of Averages....96
└ Reset, Reset All....96
└ Clear All....96
Reference Level: Upper, Middle, Lower Levels....97
Clear All....97
Delay Setup....97
Phase Setup....97

Meas. Place
Selects one of the four available measurements to be configured or activated.

Measure 1-4
Activates or deactivates the selected measurement (1-4).

Remote command:
`MEASurement<m>[:ENABle]` on page 336

Meas. Type
Defines the measurement type to be performed on the selected source. Depending on the type, different results are displayed in the result table.

For a list of all automatic measurement types and their description, see chapter 6.3.1, "Measurement Types and Results", on page 87.

Remote command:
`MEASurement<m>:MAIN` on page 336
`MEASurement<m>:RESult[:ACTual]?` on page 340

Source
Selects one of the active signal, reference or math waveforms as the source of the selected measurement. Available sources depend on the selected measurement type.

If MSO option R&S RTM-B1 is installed, active digital channels are available as measurement sources for time and count measurements.

Remote command:
`MEASurement<m>:SOURce` on page 338

Statistic
Opens a submenu to enable and configure up to four statistics.

Meas. Place ← Statistic
Selects the measurement for which statistical evaluation is configured.

Statistic ← Statistic
Activates or deactivates the statistical evaluation for the selected measurement (1-4).

Remote command:
`MEASurement<m>:STATistics[:ENABle]` on page 342

No. of Averages ← Statistic
Sets the number of measured waveforms used for calculation of average and standard deviation. The maximum number is 1000.

Remote command:
`MEASurement<m>:STATistics:WEIGht` on page 342

Reset, Reset All ← Statistic
Deletes the statistical results for the current measurement or all measurements, respectivley, and starts a new statistical evaluation if the acquisition is running.

Remote command:
`MEASurement<m>:STATistics:RESet` on page 343

Clear All ← Statistic
Resets and deactivates all active statistic measurements.

Reference Level: Upper, Middle, Lower Levels
Set the lower and upper reference levels for rise and fall time mesurements (cursor and automatic mesurements) as well as the middle reference level used for phase and delay measurements. The levels are defined as percentages of the high signal level. The settings are valid for all measurement places.

Remote command:
`REFLevel:RELative:MODE` on page 341
`REFLevel:RELative:LOWer` on page 341
`REFLevel:RELative:MIDDle` on page 342
`REFLevel:RELative:UPPer` on page 341

Clear All
Resets and deactivates all four measurements.

Remote command:
`MEASurement<m>:AOFF` on page 335

Delay Setup
Configures the delay measurement that measures the time difference between two edges of the same or different waveforms.

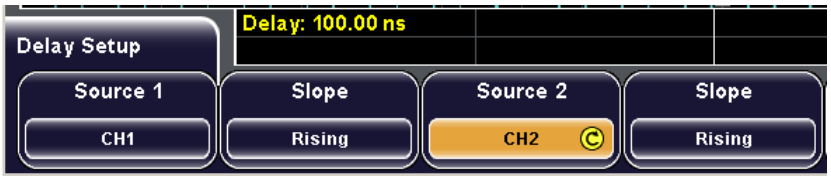

"Source 1, Source 2" Select one of the active channel, math or reference waveforms for each measurement source.

"Slope" Select the rising or falling slope for each measurement source.

Remote command:
`MEASurement<m>:SOURce` on page 338
`MEASurement<m>:DELay:SLOPe` on page 339

Phase Setup
Configures the phase measurement that measures the pahse difference between two waveforms.

"Source 1, Source 2" Select one of the active channel, math or reference waveforms for each measurement source.

Remote command:
`MEASurement<m>:SOURce` on page 338

7 Mathematics

Mathematical (math) waveforms are calculated data. Each math waveform is defined by an equation. You can configure and save up to five equations (MA1 – MA5), four of these equation can be displayed (MA1 – MA4).

Each equation consists of one or two operands and a operator. An operand can be an input channel, a constant value, or a math waveform with lower number than the operand's number. For example, the MA3 equation can use the results of MA2 and MA1 as operands.

Each equation and also the set of all defined equations can get a label.

An equation set can be saved to and loaded from any storage device - internal memory or external USB flash device. The file format is always `.FML`, and the file size is 526 Byte. It is also possible to copy the stored equation sets to another storage device with FILE > "Import/Export Equation Sets". See also: chapter 13.2.1.2, "Importing and Exporting Data", on page 218.

7.1 Configuring and Using Math Waveforms

Math waveforms are configured using the "Equation Set Editor". Each equation for a math waveform is configured and displayed individually, and you can save and load the configuration of all five math waveforms as an "Equation Set".

7.1.1 Displaying Mathematical Waveforms

For each of the math waveforms MA1 - MA4 you can define whether it is displayed or not and which equation is performed in each one. MA5 is always invisible.

1. Press MATH to display the "Mathematics" menu.
2. Press "Equation" and select the mathematical waveform that contains the equation you want to display.
   To check which equation is configured for which channel:
   a) Press "Edit Equations". The "Equation Set Editor" is displayed, where you can see the configuration for each math waveform. Currently displayed waveforms are indicated by the symbol.
   b) Press "Back" to exit the editor.
3. Press "Visible" until "On" is highlighted.

   The selected equation is calculated and the results are displayed as an additional (mathematical) waveform on the screen. If necessary, change the vertical scaling of the math waveform to improve the display using the vertical SCALE rotary knob.

If the required equation is not included, edit the current equation set, or load an appropriate equation set that was saved before. See also: "To configure an equation" on page 99 and "To load an equation set" on page 101.

7.1.2 Editing Equations and Equation Sets

To each math waveform an equation is assigned. The mathematical operation is defined by the operator and is performed on the operands. Operands are one or two of the active channel or math waveforms, or a constant value.

All five math waveforms together build an equation set that can be stored and loaded.

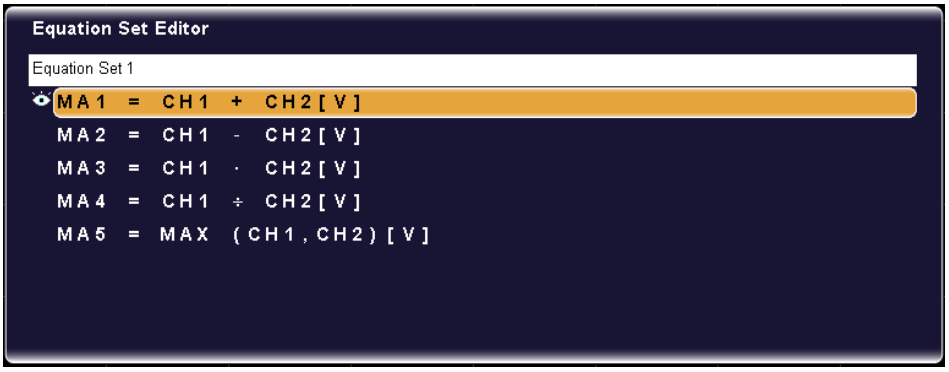

To configure an equation

1. Press "MATH > Edit Equations" to display the "Equation Set Editor" with the current equation set configuration.
2. Press "Equation" and select the equation to be configured.
3. Press "Operator" to select the operator of the equation.
   See also: "Operator" on page 103.
4. Press "Operand1".
   See also: "Operand 1" on page 107.
5. If the equation requires a second operand, press "Operand2" and define the second operand.
6. If one of the operands is defined as a constant, define its value:
   a) Press "Operand1" or "Operand2" to select the constant for the corresponding operand.
   b) Press "Edit Constant" to define its value.
   c) Press "Constant" and select either a pre-defined constant, or one of 10 available user-defined constants.

d) If you selected a user-defined constant, define its value:
   - Press "Value" and enter the numeric value.
   - Press "Decimal Point" to move the decimal point within the numeric value.
   - Press "Prefix" to define an SI-prefix to the unit. See also: "Prefix" on page 108.
   - Press "Unit" to define the unit of the value. See also: "Unit" on page 109.

e) Press "Save" to store the user-defined constant.

7. Press "Unit" to define the unit of the equation results. See also: "Unit" on page 102.
8. Optionally, press "Equation Label" to define a name for the equation. This label is displayed on the "Equation" softkey and in the "Equation Set Editor".

To edit an equation set

1. Press "MATH > Edit Equations" to display the "Equation Set Editor".
2. Press "Equation" to select the first equation to be configured. This equation is assigned to the first math waveform (MA1).
3. Configure the equation.
   See: "To configure an equation" on page 99.
4. Repeat steps 3 and 4 to configure all 5 equations in the equation set.
5. Press "Back" to exit the editor and return to the main "Mathematics" menu.
6. For each equation MA1 to MA4, define whether it is to be displayed or not:
   a) Press "Equation" to select the equation.
   b) Press "Visible" to switch the display of the math waveform on or off.
7. Optionally, press "Eq. Set Label" to define a name for the equation set. This label is displayed in the "Equation Set Editor".

7.1.3 Saving and Loading Equation Sets

If you want to keep math configurations for specific measurement purposes for later use, you can save equations sets in the instrument or on external storage device.

To copy a stored equation sets to another storage device, use FILE > "Equation Sets". For import/export procedure, see chapter 13.2.1.2, "Importing and Exporting Data", on page 218.

To save the current equation set

1. Press MATH to display the "Mathematics" menu.
2. Press "Save".
3. Define the storage location using the "Storage" softkey, and the file name using the "File name" softkey.

See: chapter 13.2.1.1, "Configuring Storage Locations", on page 218.

4. Optionally, define a comment to be added to the equation set using the "Comment" softkey.
5. Press "Save".

   The equation set is saved as configured.

To load an equation set

1. Press "MATH > Load".

   A file explorer is displayed.
2. If necessary, switch to the storage location that contains the file by pressing "Storage".
3. Select the file that contains the equation set. Use the "Navigation" knob to scroll through the directories. To change the directory, scroll to the name of the directory and press the knob, or press "Change dir.".
4. Press "Load".

   The equation set is loaded to the R&S RTM.

7.2 Reference for Mathematics

The MATH key provides functions to configure and display calculated data.

For details on working with these functions, see chapter 7.1, "Configuring and Using Math Waveforms", on page 98.

Equation....102
Visible....102
Unit....102
Edit Equations....103
└ Equation....103
└ Operator....103
└ Operand 1....107
└ Operand 2....108
└ Edit Constant....108
└ Constant....108
└ Value....108
└ Decimal Point....108
└ Prefix....108
└ Unit....109
└ Save....109

└ Equation Label....109
Eq. Set Label....109
Save....109
Load....109

Equation
Selects one of five possible mathematical channels.

Visible
Defines whether the selected mathematical waveform is displayed on the display or not.

Note: MA5 cannot be displayed, it is always invisible.

Remote command:
`CALCulate:MATH<m>:STATe` on page 345

Unit
Defines the unit of the equation results. The selected unit only has an effect on the displayed unit, not on the size of the values.

The following units are available:
- V (Volts)
- A (Amperes)
- Ω (Ohms)
- S (Siemens)
- V/A (Volts per Ampere)
- W (Watts, active power)
- VA (Voltamps, apparent power)
- VAr (Voltamps, reactive power)
- Vs (Volt-seconds = Weber, unit of magnetic flux)
- V/s (Volts per second)
- dB (decibels)
- dBm (dB referred to 1 mW)
- dBV (dB referred to 1 V)
- dBµV (dB referred to 1 µV)
- s (Second)
- 1/s, Hz (Hertz)
- s/DIV
- F (Farad)
- H (Henry)
- % (Percent)
- ° (Degree)
- π (Pi)
- Pa (Pascal)
- m (Meter)
- g (Acceleration)
- °C (Degrees Celsius)
- K (Kelvin)
- °F (Degrees Fahrenheit)
- N (Newton)
- J (Joule)
- C (Coulomb)

- Wb (Weber)
- T (Tesla)
- (dez) (dezimal)
- (bin) (binary)
- (hex) (hexadezimal)
- (oct) (octal)
- DIV (Division, graticule)
- px (pixel)
- Bit
- Bit/s
- Byte
- Bd (Baud)
- Sa (Samples)
- Sa/sec. (Samples per second)
- cyc (cycles)
- Trc. (Traces)
- Sa/X
- ⎍ Rising edge
- ⎏ Falling edge
- ⎍⎍ Positive impulse
- ⎏⎏ Negative impulse
- Ev. (Events)
- Symb. (symbols)
- Sy./s (symbols per second)
- Wfm. (waveforms)

Edit Equations
Provides functions to configure the calculations for the mathematical channels.

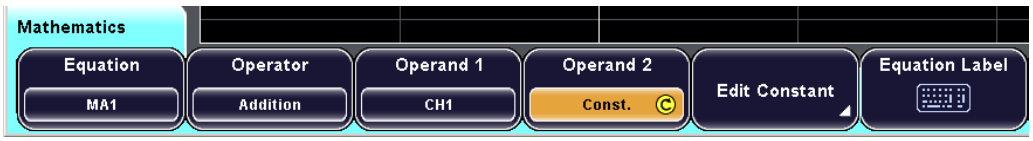

Remote command:
`CALCulate:MATH<m>[:EXPRession][:DEFine]` on page 346

Equation ← Edit Equations
Selects one of five possible mathematical channels.

Operator ← Edit Equations
Defines the operation to be performed on the specified operands in the mathematical channel.

"Addition" Op1 + Op2
Adds the two operands.

"Subtraction" Op1 - Op2
Subtracts the second operand from the first operand.

"Multiplication" Op1 * Op2
Multiplies the two operands.



"Division" Op1 / Op2
Divides the first operand by the second operand.
For small amplitudes of the second operand, the result increases quickly. If the second operand crosses zero, the result would be a range of +∞ to -∞. In this case, instead of 0V, the calculation function uses the value that the Least Significant Bit (LSB) of the second operand represents. (For an 8-bit value, for example, 1/256).
You can limit the zero-crossings of the operand by using the "Maximum" operator. This limitation results in a smaller result range and a finer resolution.



"Maximum" Maximum (Op1, Op2)
Compares the amplitudes of both operands and displays the maximum amplitude. The sign of the result is taken from Operand1. Use this operation in combination with the "Reciprocal" or "Division" operation to limit the minimal amplitudes of an operand.
Example: Operand1 is a homopolar sine signal with V_{pp}=3V. Operand2 is a constant value of 1V. The result is always larger than 1V or smaller than -1V.



"Minimum" Minimum (Op1, Op2)
Compares the amplitudes of both operands and displays the minimum amplitude. The sign of the result is taken from Operand1. Use this operation in combination with the "Reciprocal" or "Division" operation to limit the maximal amplitudes of an operand.
Example: Operand1 is a MATH waveform within the range of +/-10V. Operand2 is a constant value of 1V. The result is always smaller than 1V or larger than -1V.



"Square" Op1 * Op1
Squares the operand. If the operand contains negative values that have been clipped, then the result contains positive clipping.



"Square Root" Square Root (Op1)
Calculates the square root of the operand. Note that the square root of a negative number is undefined and the result is clipped.



"Abs. Value" |Op1|
Calculates the absolute value of the operand. All negative values are inverted to positive values. The positive values remain unmodified. If the operand has negative values that have been clipped, the result contains positive clipping.



"Pos. Wave" Max (Op1, 0)
Extracts the positive data points from the operand. For all negative values the result is zero. The positive values remain unmodified.



"Neg. Wave" Min (Op1, 0)
Extracts the negative data points from the operand. For all positive values the result is zero. The negative values remain unmodified.



"Reciprocal" 1V / Op1
Divides 1V by the operand values.
For small operand amplitudes the result increases quickly. If the operand crosses zero, the result would be a range of +∞ to -∞. In this case, instead of 0V, the calculation function uses the value that the Least Significant Bit (LSB) of the operand represents. (For an 8-bit value, for example, 1/256).
You can limit the zero-crossings of the operand by using the "Maximum" operator. This limitation results in a smaller result range and a finer resolution.



"Inverse" Inverts all voltage values of the operand, i.e. all values are mirrored at the ground level. Thus, a positive voltage offset becomes negative. If the amplitude of the operand is clipped, the result is the inverted limitation.



"Common Log." log (Op1)
Calculates the logarithm to the basis 10 of the operand. Note that the logarithm of a negative number is undefined and the result is clipped.



"Natural Log." ln (Op1)
Calculates the logarithm to the basis e (Euler number) of the operand. Note that the logarithm of a negative number is undefined and the result is clipped.



"Derivative" f'(Op1)
The derivative corresponds to the rise of the tangent through a function point and indicates the dimension of the change in quantity of the operand in time. The larger the quantity change of the operand per time becomes, the larger the result of the derivative is.
The calculation is approximated using the secant based on the current calculated value and a value with a distance of 0.1 DIV. Due to this, the time axis has a finitely small resolution. Therefore, scale the input signal to display the required area appropriately.

"Integral" Calculates the definite integral of the operand.
The calculation is displayed in the illustration. The integration starts at point "a" and adds the area beneath the waveform. Point "b" indicates the currently calculated value. At the end of the positive alternation, the integral function reaches its maximum. Due to the homopolar operand used in this example, the waveform of the area reaches zero after the negative alternation.
Use a V-Marker to measure the area for an extract of the waveform.
See also: "Meas.Type" on page 83.

"IIR low pass" IIR ⅃ (Op1,fg=Op2)
Calculates a low-pass filtered waveform of "Operand 1". The cut-off frequency is set with constant "Operand 2". Signal components with frequencies higher than the cut-off frequency are attenuated significantly.

"IIR high pass" IIR ⅂ (Op1,fg=Op2)
Calculates a high-pass filtered waveform of "Operand 1". The cut-off frequency is set with constant "Operand 2". Signal components with frequencies below the cut-off frequency are attenuated significantly.

Remote command:
`CALCulate:MATH<m>[:EXPRession][:DEFine]` on page 346

Operand 1 ← Edit Equations
Defines the first operand for the mathematical operation. The source can be any active channel signal, a constant value, or a mathematical waveform with lower number than the one to be defined.

"CH1 | CH2 | CH3 | CH4" An active channel waveform

"Const." A constant value

"MA1 | MA2 | MA3 | MA4" A mathematical waveform. Only math waveforms with lower number are available.

Operand 2 ← Edit Equations
Defines the second operand for the mathematical operation, if required. The source can be any active channel signal, a constant value, or a mathematical waveform with lower number than the one to be defined.

"CH1 | CH2 | CH3 | CH4" An active channel waveform

"Const." A constant value

"MA1 | MA2 | MA3 | MA4" A mathematical waveform. Only math waveforms with lower number are available.

Edit Constant ← Edit Equations
Provides functions to define a constant value to be used in a mathematical operation. In addition to the value, a decimal point, the unit and an SI-prefix can be defined.

This softkey is only available if "Constant" is selected as one of the operands.

Constant ← Edit Constant ← Edit Equations
Specifies a pre-defined constant or a user-defined constant for a mathematical operation. Either one of the following pre-defined constants can be selected, or one of 10 user-defined constants.

- Pi
- 2*Pi
- 1/2*Pi
- e

Value ← Edit Constant ← Edit Equations
Specifies the value for a user-defined constant. This function is only available if one of the user-defined constants is selected by the "Constant" softkey.

Decimal Point ← Edit Constant ← Edit Equations
Moves the decimal point within the user-defined constant value.

Prefix ← Edit Constant ← Edit Equations
Defines an SI-prefix for the unit of a user-defined constant value. The following prefixes are available:

- None
- m (Milli, 10^{-3})
- µ (Mikro, 10^{-6})
- n (Nano, 10^{-9})
- p (Piko, 10^{-12})
- f (Femto, 10^{-15})

- a (Atto, 10^{-18})
- z (Zepto, 10^{-21})
- y (Yokto, 10^{-24})
- K (Kilo, 10^{3})
- M (Mega, 10^{6})
- G (Giga, 10^{9})
- T (Tera, 10^{12})
- P (Peta, 10^{15})
- E (Exa, 10^{18})
- Z (Zetta, 10^{21})
- Y (Yotta, 10^{24})

Unit ← Edit Constant ← Edit Equations
Defines the unit of the user-defined constant value. The selected unit only has an effect on the displayed unit, not on the size of the values.

For a list of available units, see "Unit" on page 102.

Save ← Edit Constant ← Edit Equations
Saves the defined constant to the equation of the math waveform.

Equation Label ← Edit Equations
Defines a label for the current equation.

Eq. Set Label
Defines a label for the equation set.

Save
Opens the "Save" menu with basic functions to save the equation set.

See "Save Menu" on page 220.

Load
Displays the "Load" menu and a file explorer to select an equation set file.

See "Load Menu" on page 221.

8 FFT

In addition to signal vs. time and signal vs. signal displays, the frequencies of a signal as determined by FFT analysis can be displayed. FFT analysis is configured and activated using the FFT key. Analysis is always performed on the signal channel that was most recently activated, however you can change the channel source.

Various parameters concerning the time base, scaling and the waveform arithmetic can be configured for the FFT display. You can configure FFT either numerically using the softkeys, or graphically using the rotary knobs.

On the FFT display, you can perform frequency and level measurements by means of a cursor measurement. Automatic measurements are not available.

8.1 FFT Display

When you activate FFT display, two windows are displayed: the signal vs. time at the top, the result of the FFT analysis at the bottom.

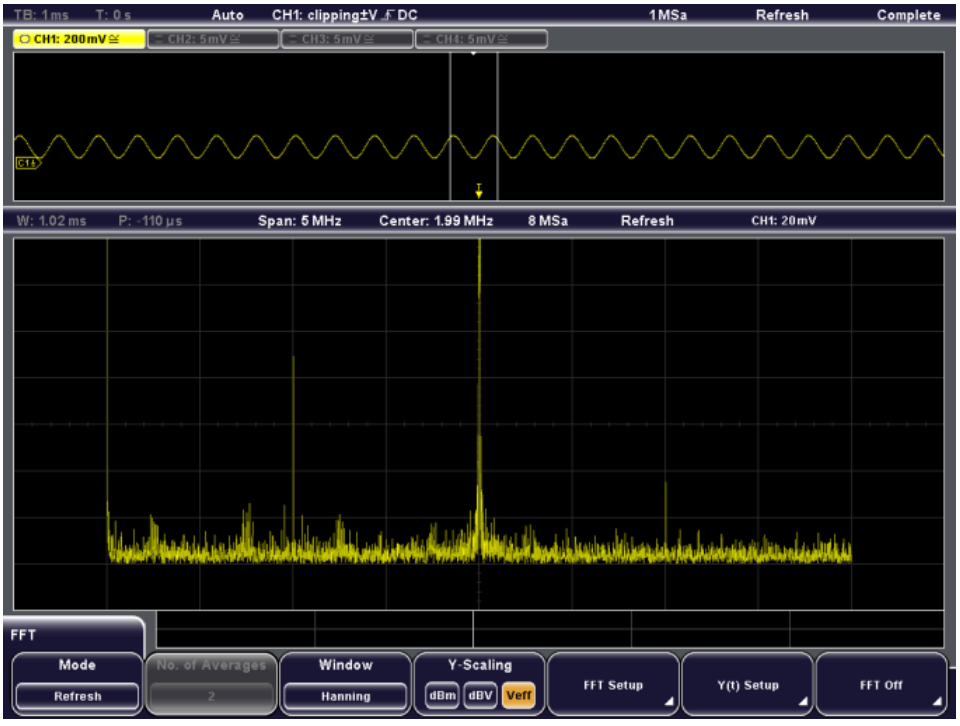

The display can be restricted to the results for a certain time base extract and to a specified frequency range. The time range is indicated by white lines in the Y(t)-diagram (see also figure 8-1).

Move the focus between the Y(t)-window (Time Control), the FFT time base extract (Time Section) and the FFT frequency range (FFT Control) by pressing the horizontal SCALE rotary knob. The currently selected screen element is highlighted and displayed in the information bar. Depending on the selection, the functions of the SCALE and POSITION rotary knobs may change.

The usual channel parameters are displayed in the information bar above the Y(t)-window (see the general display information described in the "Getting Started" manual).

In addition, FFT-specific parameters are indicated in the information bar above the FFT window. The following information is given there:

	Description	Setting
1	Width of the time base extract for which FFT is calculated	YT-Window
2	Position of time base extract	Position
3	Width of the displayed frequency range	Span
4	Center of the displayed frequency range	Center
5	Sample rate for FFT calculation	
6	FFT result mode	Waveform Arithmetic
7	Signal source and vertical scaling factor per division	CH1...CH4 / Y-Scale / Y-Scaling
8	Focus of the horizontal SCALE knob	Press SCALE

When you deactivate the FFT display, the previous display is restored.

8.2 Configuring and Using FFT Calculations

- Setting Up the FFT Analysis....111
- Configuring the Diagrams....112
- Measuring on FFT....115

8.2.1 Setting Up the FFT Analysis

To display an FFT diagram

► Press the FFT key.

The key lights up and two windows are displayed: the signal vs. time at the top, the result of the FFT analysis at the bottom.

To deactivate the FFT display

► Press the FFT key again, or press the "FFT off" softkey in the "FFT" menu to deactivate the FFT display.

The FFT key is no longer illuminated and the previous display is restored.

To configure the general FFT display

1. Press the FFT key to activate the FFT display and open the "FFT" menu.
2. If necessary, press one of the CH1...CH4 keys to change the signal source of the FFT calculation.
3. Press "Waveform Arithmetic" to define the mode for FFT calculation and display. The waveform arithmetic defines whether the values are updated regularly, or whether values from previous spectra are included in the calculation and display.
   For details see "Wfm. Arithmetic" on page 116.
4. If "Average" mode is selected, press "No. of Averages" to define how many spectra are considered for the calculation.
5. Press "Window" to define which type of function is laid over the input values. If the input values are to be used unaltered, use the "Rectangle" window. To reduce noise, use a bell-shaped window.
   For details see "Window" on page 117.
6. Press "Y-Scaling" to select logarithmic or linear scaling of the y-axis in the FFT window (see "Y-Scaling" on page 118).
7. Define the settings for the FFT window as described in "To configure the FFT diagram numerically" on page 112.
8. Define the settings of the signal vs. time window as described in "To configure the Y(t)-window numerically" on page 114. These settings are identical to the general trigger and scaling settings defined for the channel (see also chapter 2.2.2, "Adjusting the Signal Input Manually", on page 20).

8.2.2 Configuring the Diagrams

To configure the FFT diagram numerically

Alternatively to configuring the FFT window numerically via the softkeys, you can use the rotary knobs to change the settings graphically, see "To configure the FFT diagram graphically" on page 113.

1. Press "FFT-Setup" in the "FFT" menu.
2. Define the time base extract for which the FFT is to be calculated and displayed. The extract is defined by its width and position (see figure 8-1).
   a) Press "YT-Window" to define the width of the time base extract.

b) Press "Position" to define the position of the time base extract. The position is defined as an offset of the center of the extract range to the 0s reference point.

The time base extract is indicated by a white frame in the Y(t)-window. The width (W) and position (P) are indicated in the information bar beneath the Y(t)-window.

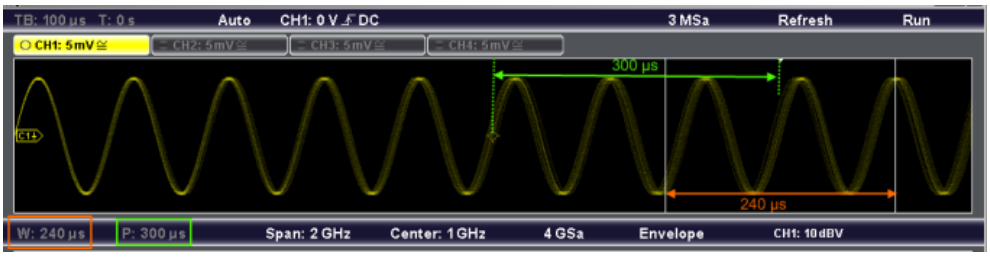

Fig. 8-1: Width and position of the time base extract for FFT calculation

3. Press "Y-Scale" to define the scaling of the FFT amplitudes.
4. Define the frequency range to be displayed in the FFT window. The range is defined as (Center - Span/2) to (Center + Span/2). For details see "Span" on page 119 and "Center" on page 119.
   a) Press "Span" to define the width of the frequency range.
   b) Press "Center" to define the center frequency of the range.

To configure the FFT diagram graphically

1. Define the time base extract for which the FFT is to be calculated and displayed. The extract is defined by its width and position (see figure 8-1).
   a) Press the horizontal SCALE rotary knob to select the FFT time base extract ("W"/"P" settings are highlighted).
   b) Turn the horizontal SCALE rotary knob to define the width of the time base extract. Turn the knob counter-clockwise to enlarge the extract, or clockwise to decrease it.
   c) Turn the horizontal POSITION rotary knob to define the position of the time base extract. Turn the knob counter-clockwise to move the extract to the left, or clockwise to move it to the right.
2. Define the frequency range to be displayed in the FFT diagram. The range is defined as (Center - Span/2) to (Center + Span/2). For details see "Span" on page 119 and "Center" on page 119.
   a) Press the horizontal SCALE rotary knob to select the FFT frequency range ("Span"/"Center" settings are highlighted).
   b) Turn the horizontal SCALE rotary knob to define the span of the frequency range. Turn the knob counter-clockwise to enlarge the span, or clockwise to decrease it.
   c) Turn the horizontal POSITION rotary knob to define the center of the frequency range. Turn the knob counter-clockwise to move the center to the left, or clockwise to move it to the right.

d) Turn the vertical SCALE rotary knob to define the scaling of the FFT amplitudes. Turn the knob counter-clockwise to decrease the amplitudes, or clockwise to enlarge them.

To configure the Y(t)-window numerically

Alternatively to configuring the Y(t)-window numerically via the softkeys, you can use the rotary knobs to change the settings graphically, see "To configure the Y(t)-window graphically" on page 114.

1. Press "Y(t)-Setup" in the "FFT" menu.
2. Press "Y-Scale" to define the scaling of the signal amplitudes in the Y(t)-window.
3. Press "Y-Position" to define the vertical position of the time axis in the Y(t)-window, in divisions.
4. Press "Main Time Base" to define the scaling for the time base in the Y(t)-window in seconds per division.
   Note that when you change the scaling for the main time base, the width of the FFT time base extract is also changed.
5. Press "Trigger Offset" to define the offset of the trigger point to the reference point for 0s.
   Note that when you change the trigger offset, the position of the FFT time base extract is also changed.

   The scaling factor for the time base (TB) and the trigger offset (T) are indicated in the information bar above the Y(t)-window.

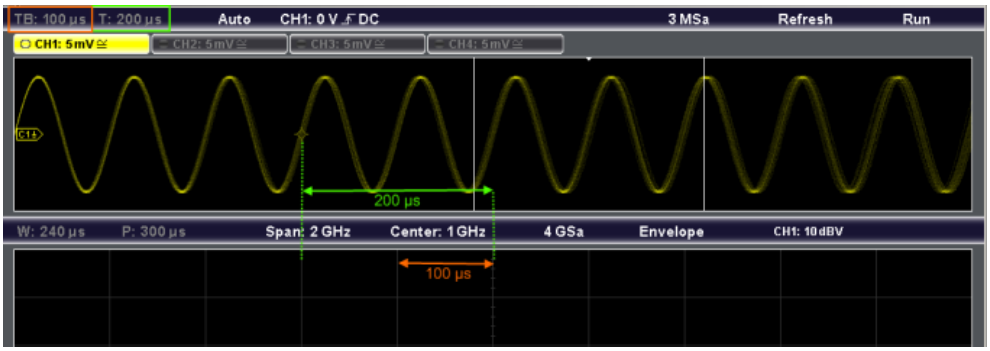

Fig. 8-2: Time base (per division) and trigger offset in Y(t)-window

To configure the Y(t)-window graphically

1. Press the horizontal SCALE rotary knob to select the Y(t)-window ("TB"/"T" settings are highlighted).
2. Turn the vertical SCALE rotary knob to define the scaling of the signal amplitudes in the Y(t)-window. Turn the knob counter-clockwise to decrease the amplitudes, or clockwise to enlarge them.

3. Turn the vertical POSITION rotary knob to define the vertical position of the time axis in the Y(t)-window. Turn the knob counter-clockwise to move the time axis down, or clockwise to move it up.
4. Turn the horizontal SCALE rotary knob to define the scaling for the time base in the Y(t)-window. Turn the knob counter-clockwise to increase the scaling, or clockwise to decrease it (and thus spread the waveform).
   Note that when you change the scaling for the main time base, the width of the FFT time base extract is also changed.
5. Turn the horizontal POSITION rotary knob to define the offset of the trigger point to the reference point for 0s. Turn the knob counter-clockwise to move the trigger point to the left, or clockwise to move it to the right.
   Note that when you change the trigger offset, the position of the FFT time base extract is also changed.

8.2.3 Measuring on FFT

You can perform cursor measurements in FFT mode. Automatic measurements are not available.

1. Press FFT, then set up and configure the FFT diagram.
2. Press CURSOR.
3. In the "Cursor" menu, set the cursor lines to the required positions. Use "Prev. Peak" and "Next Peak" to set the selected cursor line to the level peaks.
   See also: chapter 6.1.3, "Cursor Menu", on page 82.

   The frequency and level results are shown in the results table.

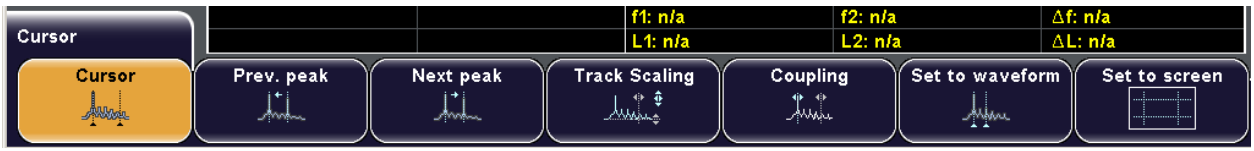

8.3 Reference for FFT key

The FFT key enables the FFT mode and opens the FFT menu.

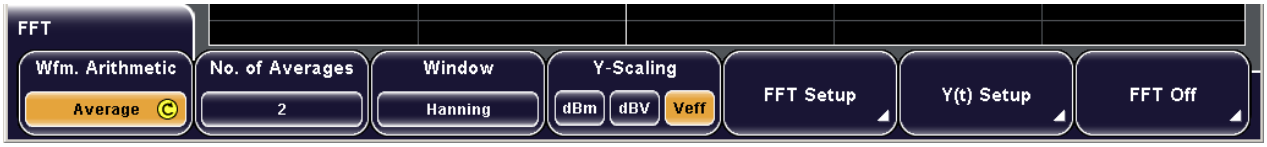

See also:

- chapter 8.2, "Configuring and Using FFT Calculations", on page 111
- chapter 8.1, "FFT Display", on page 110

FFT....116
Wfm. Arithmetic....116
No. of Averages....117
Window....117
Y-Scaling....118
FFT-Setup....118
└ Span....119
└ Center....119
└ Y-Scale....119
└ YT-Window....119
└ Position....120
└ Points....120
Y(t)-Setup....120
└ Y-Scale....120
└ Y-Position....120
└ Main Time Base....120
└ Trigger Offset....121
└ Show Channels....121
FFT Off....121

FFT

The FFT key activates and deactivates a Fast Fourier Transformation (FFT) for the most recently selected channel and provides functions to configure and display FFTs.

If activated, the FFT key lights up. Two windows are displayed: the signal vs. time window at the top, and the result window of the FFT analysis at the bottom.

When deactivated, the previous display is restored.

To display the FFT for a different channel, press the corresponding channel key.

Remote command:

`CALC:MATH:EXPR "FFTMAG(CHx)"`; see also `CALCulate:MATH<m>[:EXPRession][:DEFine]` on page 346.

Wfm. Arithmetic

Defines the arithmetic mode for FFT calculation and display.

"None" The FFT is performed without any additional weighting or postprocessing of the acquired data. The new input data is acquired and displayed, and thus overwrites the previously saved and displayed data.



"Envelope" In addition to the normal spectrum, the maximal oscillations are saved separately and updated for each new spectrum. The maximum values are displayed together with the newly acquired values and form an envelope. This envelope indicates the range of all FFT trace values that occurred.
If any signal parameters are changed, the envelope is reset.

"Average" The average of several spectrums is calculated. The number of spectrums used for the averaging is defined using the knob or the "No. of Averages" softkey. This mode is useful for noise rejection.

Remote command:
`CALCulate:MATH<m>:ARIThmetics` on page 349

No. of Averages
Defines the number of spectrums used for averaging.

This function is only available if "Average" mode is selected.

Remote command:
`CALCulate:MATH<m>:FFT:AVERage:COUNt` on page 350

Window
Window functions are multiplied with the input values and thus can improve the FFT display.

If discontinuities occur at the borders of the measurement interval, the algorithm interprets such discontinuities as a sudden edge, which can distort the result. For bell-shaped functions, the border values are multiplied with smaller values and thus have less influence on the result.

"Hanning" The Hanning window is bell shaped. Unlike the Hamming window, its value is zero at the borders of the measuring interval. Thus, the noise level within the spectrum is reduced and the width of the spectral lines enlarges. Use this window to measure amplitudes of a periodical signal precisely.



"Hamming" The Hamming window is bell shaped. Its value is not zero at the borders of the measuring interval. Thus, the noise level inside the spectrum is higher than Hanning or Blackman, but smaller than the rectangular window. The width of the spectral lines is thinner than the other bell-shaped functions. Use this window to measure amplitudes of a periodical signal precisely.



"Blackman" The Blackman window is bell shaped and has the steepest fall in its wave shape of all other available functions. Its value is zero at both borders of the measuring interval. In the Blackman window the amplitudes can be measured very precisely. However, determining the frequency is more difficult. Use this window to measure amplitudes of a periodical signal precisely.



"Rectangle" The rectangular window multiplies all points by one. The result is a high frequency accuracy with thin spectral lines, but also with increased noise. Use this function preferably with pulse response tests where start and end values are zero.

Remote command:
`CALCulate:MATH<m>:FFT:WINDow:TYPE` on page 349

Y-Scaling
Defines the scaling unit for the y-axis. The display values are valid for 50Ω termination impendance. To achieve this, the existing internal terminating resistor can be used, or an external terminating resistor can be connected parallel to the high impedance input.

To set the scale value, use "FFT Setup" > "Y-Scale".

"dBm" logarithmic scaling; related to 1 mW

"dBV" logarithmic scaling; related to 1 Veff

"Veff" linear scaling; displays the RMS value of the voltage

Remote command:
`CALCulate:MATH<m>:FFT:MAGNitude:SCALe` on page 350

FFT-Setup
Defines the settings for the FFT window. The display can be restricted to the results for a certain time base extract and to a specified frequency range.

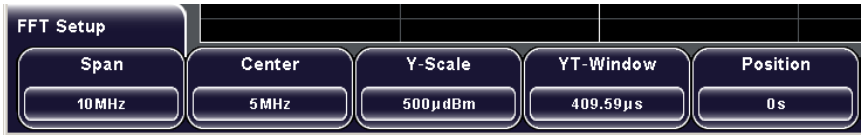

Span ← FFT-Setup
The span is specified in Hertz and defines the width of the displayed frequency range, which is (Center - Span/2) to (Center + Span/2). The position of the span is defined using the "Center" function.



Note: If the FFT frequency range is selected ("Span"/"Center" is highlighted), the width of the span can be adjusted using the horizontal SCALE rotary knob.

Remote command:
`CALCulate:MATH<m>:FFT:SPAN` on page 352
`CALCulate:MATH<m>:FFT:FULLspan` on page 352
`CALCulate:MATH<m>:FFT:STARt` on page 353
`CALCulate:MATH<m>:FFT:STOP` on page 353

Center ← FFT-Setup
Defines the position of the displayed frequency domain, which is (Center - Span/2) to (Center + Span/2). The width of the domain is defined using the "Span" function.



Note: If the FFT frequency range is selected ("Span"/"Center" is highlighted), the width of the span can be adjusted using the horizontal POSITION rotary knob.

Remote command:
`CALCulate:MATH<m>:FFT:CFRequency` on page 352
`CALCulate:MATH<m>:FFT:STARt` on page 353
`CALCulate:MATH<m>:FFT:STOP` on page 353

Y-Scale ← FFT-Setup
Changes the vertical scaling of the FFT display (in V/dBm) per division.

Note: If the FFT frequency range is selected ("Span"/"Center" is highlighted), the Y-Scale can be defined using the vertical SCALE rotary knob.

See also "SCALE, Y-Scale" on page 29.

Remote command:
`CALCulate:MATH<m>:SCALe` on page 346

YT-Window ← FFT-Setup
Defines the width of the time base extract from the Y(t)-window for which the FFT is calculated. The extract is indicated by white lines in the Y(t)-window. The value is indicated by "W" in the information bar above the FFT window.

Note: If the FFT time base extract is selected ("W"/"P" is highlighted), the width can be adjusted using the horizontal SCALE rotary knob.

See also figure 8-1.

Remote command:
CALCulate:MATH<m>:FFT:TIME:RANGe on page 353

Position ← FFT-Setup
Defines the position of the time base extract in the Y(t)-window for which the FFT is calculated. The value is indicated by "P" in the information bar above the FFT window.

Note: If the FFT time base extract is selected ("W"/"P" is highlighted), the position can be adjusted using the horizontal POSITION rotary knob.

See also figure 8-1.

Remote command:
CALCulate:MATH<m>:FFT:TIME:POSition on page 354

Points ← FFT-Setup
Defines how many samples are used for FFT calculation

The value is changed in 2^n steps from 2048 (2^{11}) to 65536 (2^{16}).

Remote command:
CALCulate:MATH<m>:FFT:BANDwidth[:RESolution]:RATio on page 351

Y(t)-Setup
Defines the settings for the signal vs. time window.

Y-Scale ← Y(t)-Setup
Changes the vertical scaling of the Y(t)-window (channel scaling).

Note: If the Y(t)-window is selected (indicated by a white border), the Y-Scale can be adjusted using the vertical SCALE rotary knob.

See "SCALE, Y-Scale" on page 29.

Remote command:
CHANnel<m>:SCALe on page 289

Y-Position ← Y(t)-Setup
Defines the vertical position of the time axis in the Y(t)-window, in divisions.

Note: If the Y(t)-window is selected (indicated by a white border), the Y-Position can be adjusted using the vertical POSITION rotary knob.

Remote command:
CHANnel<m>:POSition on page 290

Main Time Base ← Y(t)-Setup
Defines the scaling for the time base in the (original) Y(t)-window in seconds per division. The scaling is indicated by "TB" in the information bar above the window.

Note: If "Time Control" is selected, the main time base can be adjusted using the horizontal SCALE rotary knob.

See also "SCALE" on page 23, "To configure the original Y(t)-diagram" on page 69 and figure 8-2.

Remote command:
`TIMebase:SCALe` on page 283

Trigger Offset ← Y(t)-Setup
Defines the horizontal position of the trigger point in relation to the reference point - to the zero point of the grid. The value is indicated by "T" in the information bar above the window.

The reference point is set with SETUP >"Time Reference".

Note: If a zoom or FFT window is displayed and "Time Control" is selected, the trigger offset can be adjusted using the horizontal POSITION rotary knob.
See also:

- "POSITION" on page 23
- "Time Reference" on page 235
- "To configure the original Y(t)-diagram" on page 69

Remote command:
`TIMebase:POSition` on page 284

Show Channels ← Y(t)-Setup
Displays all active channels in the Y(t)-window. By default, only the selected channel is visible, the channel used for FFT calculation.

FFT Off
Closes the FFT display and returns to the previous display.

9 Masks

Masks are used to determine whether the amplitude of a signal remains within specified limits, e.g. to detect errors or test compliance of digital signals.

9.1 About Masks

9.1.1 Masks

A mask is specified by an upper and a lower limit line. The signal must run inside these limit lines, otherwise a mask violation occurs.

A new mask is created from an existing signal: Mask limits are created by copying the waveform, and the limits are moved and stretched. The result is a tolerance tube around the signal that is used as mask.

Once a mask has been defined, the copied waveform envelope is kept in the instrument until the next mask is defined or loaded. The settings for stretch and move are not kept. If you want to keep the complete mask definition, or you need more than one mask, you can save the mask to and load from any storage device - internal memory or external USB flash device.

It is also possible to copy the saved masks to another storage device with "Export/Import Masks". In an export/import operation, the name of the target file can be changed, so you can copy and rename the file in one operation. You can also change the target file format and convert the data during export/import. To copy a mask, use FILE >"Import/Export Masks".

See also:

- chapter 9.1.3, "File Formats for Masks", on page 123
- chapter 13.2.1.2, "Importing and Exporting Data", on page 218

9.1.2 Mask Testing

The mask test analyzes whether tested signal runs inside the mask. The overall test result is shown in the results table:

Total: 2785	2746	Passed: 98.59 %
2s	39	Failed: 1.4 %

left column = number of tested acquisitions and test duration
middle column = number of passed acquisitions (green) and number of failed acquisitions (red)
right column = percentage share of passed and failed acquisitions

During a mask test, various actions can be executed when mask violations occur: notification by a sound, stop of acquisition, printout or saving a screenshot, saving the waveform data.

Remote commands for mask test results:

- `MASK:COUNt?` on page 357
- `MASK:VCOunt?` on page 357
- `MASK:RESet:COUNter` on page 357

9.1.3 File Formats for Masks

Data of masks is always saved as a succession of pairs of values - lower and upper limit - and the pairs are written as two consecutive single values. Depending on the file format, only amplitude values are stored, or the amplitude values are stored together with their sample index.

Amplitude values are not saved as voltage values but as division values. The minimum value for evaluation is -5.12 DIV, the maximum is +5.12 DIV. The internal vertical range of the instrument exceeds the visible vertical range of ±4 DIV.

With export, you can convert the MSK file to CSV, TXT, or BIN formats. Import is possible for MSK and CSV files.

MSK Format

MSK is the specific binary format for masks of the R&S RTM. It contains pairs of amplitude values (in divisions) , their sample indexes and current instrument settings. Thus, the amplitude values are not related to time and voltage. The data can be loaded back to the instrument for further use. The format is not intended for analysis outside the R&S RTM.

CSV Format

In a Comma Separated Values text file, the waveform is stored in a two-columned table. Columns are separated by a comma, and the lines are separated by line breaks `\r\n` (`0x0D 0x0A`).

The first column contains the sample indexes, and the second column contains the associated amplitude values in divisions. The first line indicates the units of the values in each column, and the name of the waveform. For each sample index, two values (minimum and maximum) are written. The range of amplitude values is -5.12 to +5.12 divisions.

The data can be loaded back to the instrument for further use.

Example: CSV file

```
[Sa],MSK1[DIV]
0.000E+00,-3.273E+00
0.000E+00,-7.831E-01
1.000E+00,-3.313E+00
1.000E+00,-8.232E-01
2.000E+00,-3.273E+00
2.000E+00,-8.232E-01
3.000E+00,-3.273E+00
3.000E+00,-7.831E-01
4.000E+00,-3.273E+00
```

```
4.000E+00,-7.831E-01
5.000E+00,-3.313E+00
5.000E+00,-8.232E-01
6.000E+00,-3.273E+00
6.000E+00,-8.232E-01
7.000E+00,-3.273E+00
7.000E+00,-7.831E-01
8.000E+00,-3.313E+00
8.000E+00,-7.831E-01
9.000E+00,-3.273E+00
9.000E+00,-7.831E-01
1.000E+01,-3.273E+00
1.000E+01,-8.232E-01
...
```

At export, the sample indexes are written in scientific notification.

If you create a mask manually in a CSV file, you can write the indexes simply as intergers. The file should contain 1000 pairs of min-max values.

TXT Format

TXT files are ASCII files that contain only amplitude values in divisions but no time values. Amplitude values are separated by commas. Pairs of values are listed as two subsequent single values, without any identification. There is no comma at the end of the file.

Example: TXT file

```
4.00,4.20,4.05,4.25,4.08,4.28,....., -4.05,-4.25,-4.00,-4.20
```

BIN Format

BIN files contain binary amplitude values only but no time values. Each value has a word size of 8, or 16, or 32 bit, the word size is the same throughout the file.

Words are given in Big Endian order - beginning with the MSB (Most Significant Byte) and ending with the LSB (Least Significant Byte). Pairs of values are listed as two subsequent single values, without any identification.

9.2 Working with Masks

Masks define a frame with which you can compare the signal values. You can load preconfigured masks or define your own masks based on existing waveforms. When you perform a test, you can define which actions are to be taken upon violation of the mask limits.

Masks are displayed in the color used for reference waveforms.

9.2.1 Creating New Masks

You create a new mask based on a channel waveform, then optimize it by changing its position and proportions, and save it.

1. Select and adjust the channel waveform that will be used as basis for the mask, and run continuous acquisition.
2. Press TOOLS.
3. Press "Masks Tests"

   The selected waveform is displayed with its envelope, other waveforms are switched off in masks mode.
4. Press "New Mask".
5. Press "Copy Channel" to create the new mask.
   The mask is created from the envelope and displayed in the color used for reference waveforms.

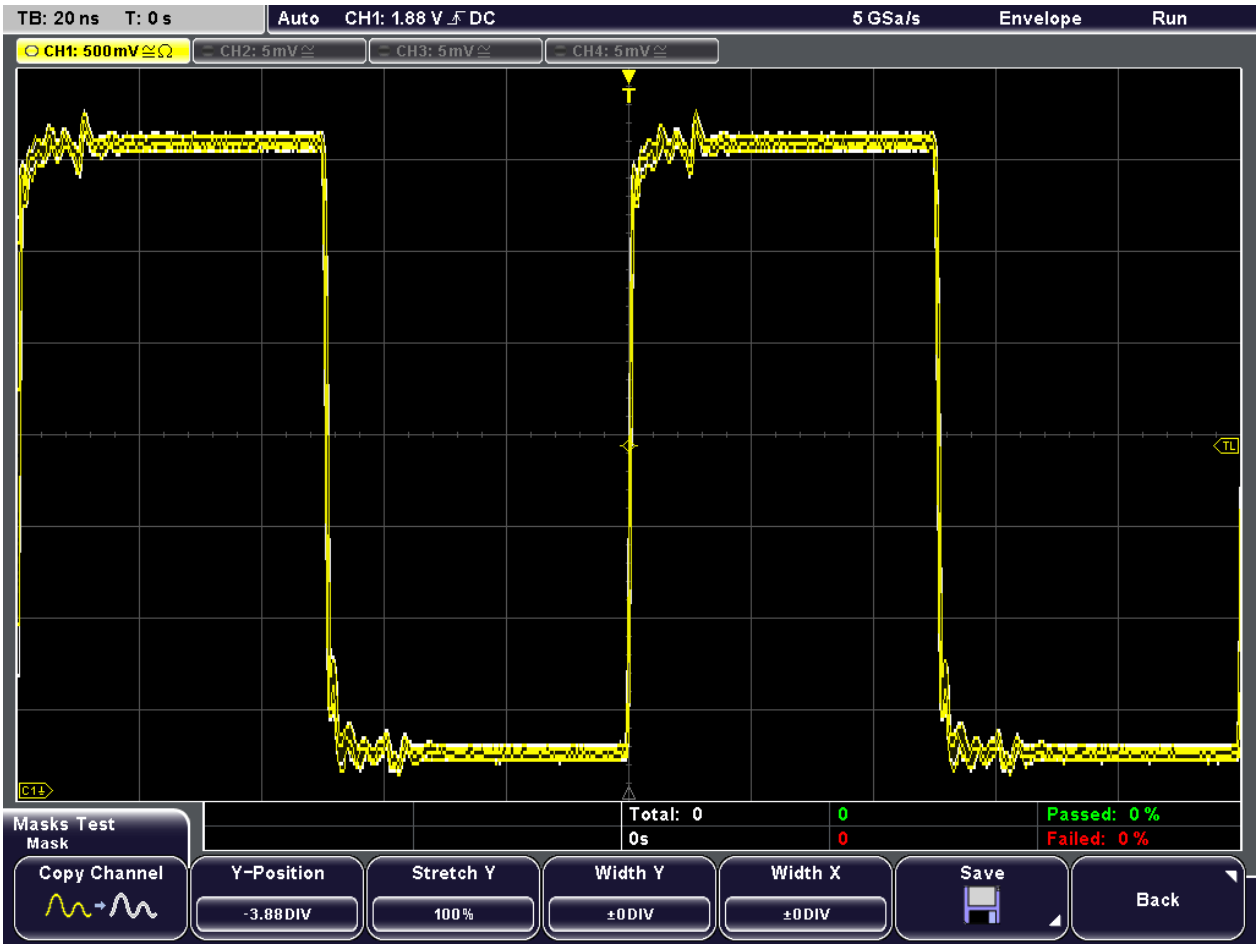

6. To change the width of the waveform in vertical direction, press "Width Y" and turn the "Navigation" rotary knob.

The specified factor in divisions is added to the y-values of the upper mask limit and subtracted from the y-values of the lower mask limit. Thus, the upper half of the mask is pulled upwards, the lower half is pulled down.

7. Similarly, to change the width of the waveform in horizontal direction, press "Width X" and turn the "Navigation" rotary knob.
The left half of the mask is pulled to the left, the right half is pulled to the right.

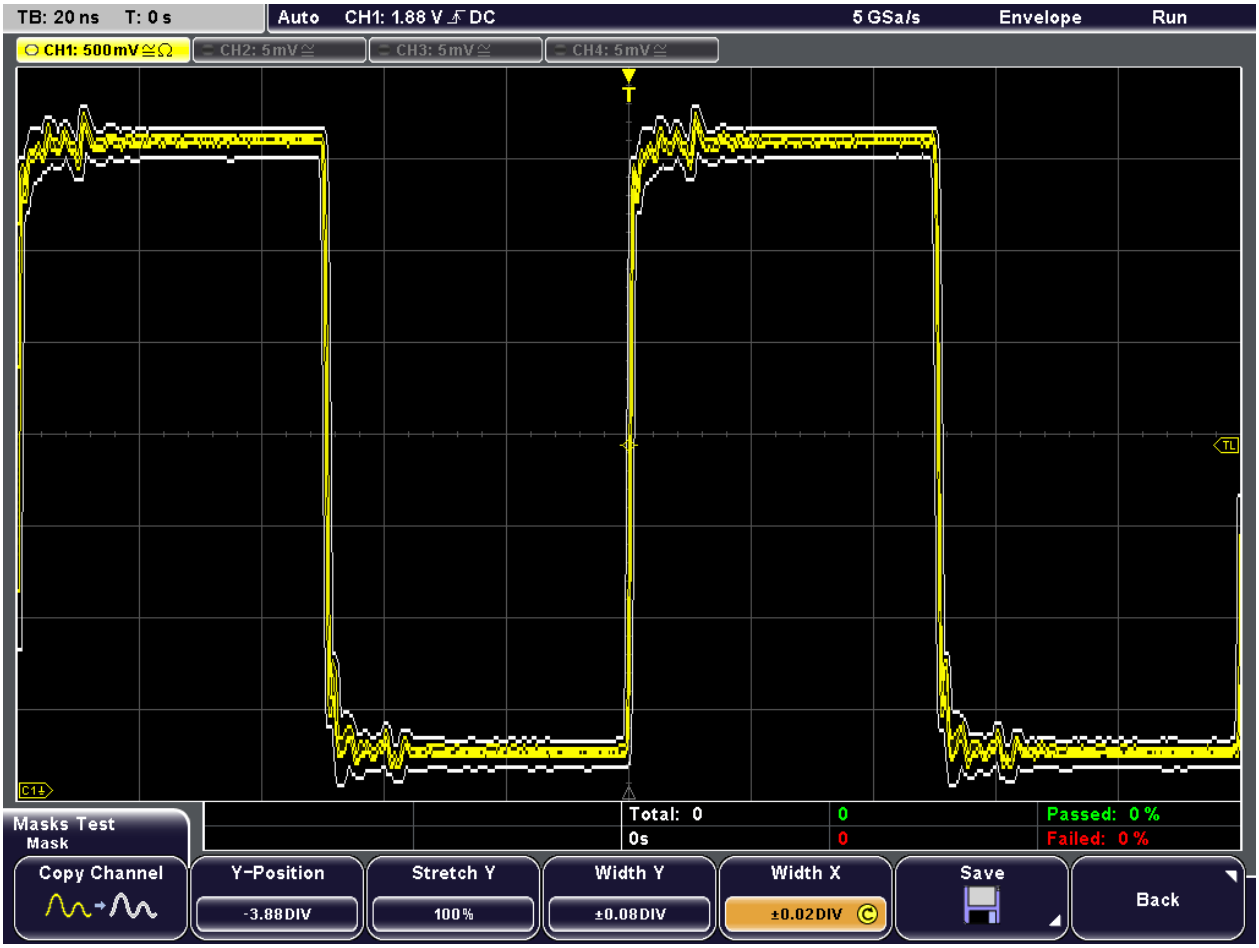

8. To move the mask vertically on the screen, press "Y-Position" and turn the "Navigation" rotary knob to change the y-position.
The current position is indicated as an offset from the center in divisions; a positive value indicates the waveform was moved upwards; a negative value indicates the waveform was moved down.

9. To change the scaling of the mask in y-direction, press "Stretch Y" and turn the "Navigation" rotary knob.
Turn the knob clockwise to increase the factor, or counterclockwise to decrease the factor. A value over 100% stretches the amplitudes; a value less than 100% compresses the amplitudes.

10. Save the new mask:

    a) Press "Save".

b) Define the storage settings as described for waveforms in chapter 13.2.1.1, "Configuring Storage Locations", on page 218.
c) Press "Save".

9.2.2 Loading Masks

You can load mask data from MSK or CSV files from any storage device.

To copy a mask, use FILE >"Import/Export Masks". For import/export procedure, see chapter 13.2.1.2, "Importing and Exporting Data", on page 218.

1. Press TOOLS > "Masks Tests" to display the "Mask Test" menu.
2. Press "Load Mask".

   The "Load" menu and a file explorer is displayed.
3. Press "Storage" and select the storage device (internal directory or USB flash drive connected to front or rear panel).
4. Select the directory and then the file that contains the mask. Use the "Navigation" knob to scroll through the directories. To change the directory, scroll to the name of the directory and press the knob, or press "Change dir.".
5. Press "Load".

   The selected mask is displayed on the screen.

9.2.3 Performing a Mask Test

Using a mask test you can detect limit violations of the measured signal compared to a pre-defined mask.

To perform a mask test

1. Seet up the waveform as usual.
2. Press TOOLS > "Masks Tests" to display the "Mask Test" menu.
3. Create a mask, or load an existing mask.

   See:
   - chapter 9.2.1, "Creating New Masks", on page 125
   - chapter 9.2.2, "Loading Masks", on page 127
4. Press "Actions" to define what happens when a violation occurs. Select one or more of the available actions by pressing the corresponding softkey and define when the action will be executed.
   See: "Actions" on page 130.
5. Press "Test" to start the mask test.

The mask test is performed, i.e. the data from the active channel is compared to the mask.
If the mask limits are exceeded, the specified action is taken. The overall result is shown in the results table:

6. Press "Pause" to stop testing temporarily without closing the "Masks" menu. Press "Pause" again to continue the test.
7. Press "Masks Test Off" to turn off the mask test and exit the "Mask" menu.

9.3 Reference for MASKS key

Masks are used for error detection and compliance tests of digital signals.

You can:

- run mask tests.
- configure actions triggered by mask violation.
- configure new masks based on channel signals.

To start a mask configuration and test, press the TOOLS key and "Masks Test".

Test....128
Pause....129
New Mask....129
└ Copy Channel....129
└ Y-Position....129
└ Stretch Y....129
└ Width Y....129
└ Width X....130
└ Save....130
Load Mask....130
Actions....130
└ Sound, Stop, Screenshot, Print, Waveform....131
Masks Test Off....131

Test
Performs a mask test for the selected signal, i.e. the signal's amplitudes are compared with the specified mask. If the amplitude exceeds the limits of the mask, a violation is detected.

Which action is to be taken when a violation is detected is defined using the Actions softkey. See also: chapter 9.2.3, "Performing a Mask Test", on page 127.

Remote command:
MASK:TEST on page 355

Pause
Temporarily stops the mask test without closing the "Masks" menu. Counts are not deleted, and the actions cannot be changed during a pause.

Remote command:
MASK:TEST on page 355

New Mask
Opens a submenu to define a new mask for testing.

See also: chapter 9.2.1, "Creating New Masks", on page 125

Copy Channel ← New Mask
Creates a new mask from the envelope waveform of the selected channel and stores it in the instrument.

Remote command:
MASK:CHCopy on page 355

Y-Position ← New Mask
Moves the mask vertically within the display. Turn the "Navigation" rotary knob to change the y-position.

The current position is indicated as an offset from the center in divisions; a positive value indicates the waveform was moved upwards; a negative value indicates the waveform was moved down.

Remote command:
MASK:YPOSition on page 356

Stretch Y ← New Mask
Changes the vertical scaling to stretch the mask in y-direction.

Turn the "Navigation" rotary knob clockwise to increase the factor, or counterclockwise to decrease the factor. A value over 100% stretches the amplitudes; a value less than 100% compresses the amplitudes.

Remote command:
MASK:YSCale on page 356

Width Y ← New Mask
Changes the width of the mask in vertical direction.

The specified number of divisions is added to the y-values of the upper mask limit and subtracted from the y-values of the lower mask limit. Thus, the upper half of the mask is pulled upwards, the lower half is pulled down, and the overall height of the mask is twice the "Width Y".

Remote command:
MASK:YWIDth on page 356

Width X ← New Mask
Changes the width of the mask in horizontal direction.

The specified factor in divisions is added to the positive x-values and subtracted from the negative x-values of the mask limits in relation to the mask center. Thus, the left half of the mask is pulled to the left, the right half is pulled to the right.

Remote command:
MASK:XWIDth on page 356

Save ← New Mask
Opens a menu to save the mask in an instrument-specific format. The complete mask definition - envelope waveform with width, stretch and position settings - is stored.

See "Save Menu" on page 220.

Remote command:
MASK:SAVE on page 355

Load Mask
Opens a file explorer to select a previously stored mask. The selected mask is loaded and can be used for a subsequent test.

Remote command:
MASK:LOAD on page 355

Actions
Opens a submenu to select the actions to be taken when a violation against the mask limits occurs. For each action, you can define when and how often the action will be executed.

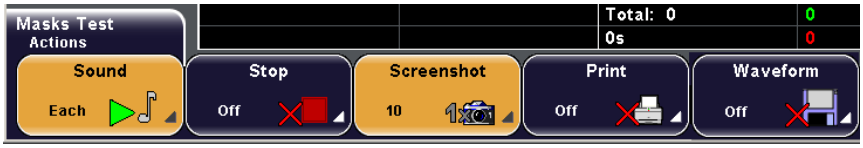

"Sound"	Generates a beep sound.
"Stop"	Stops the waveform acquisition.
"Screenshot"	Saves a screenshot according to the settings in FILE > "Screenshots".
"Print"	Prints a screenshot to a printer connected to the USB connector on the front or rear panel.

"Waveform" Saves the waveform data according to the settings in FILE > "Waveform".

Remote command:
MASK:ACTion:SOUNd:EVENt:MODE on page 357
MASK:ACTion:STOP:EVENt:MODE on page 357
MASK:ACTion:SCRSave:EVENt:MODE on page 357
MASK:ACTion:PRINt:EVENt:MODE on page 357
MASK:ACTion:WFMSave:EVENt:MODE on page 357

Sound, Stop, Screenshot, Print, Waveform ← Actions
For each action, you can define when and how often the action will be executed.

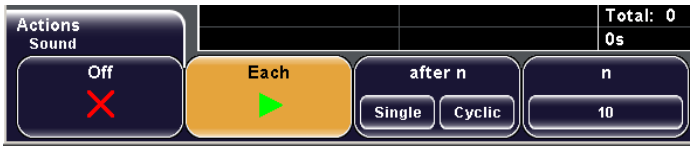

"Off" No action is executed.

"Each" The selected action is executed on each violation of the mask.

"After n / n" "Single": The selected action is executed once after the n-th violation.
"Cyclic": The selected action is executed repeatedly after each n-th violation.
Set the execution interval with softkey "n".

Remote command:
MASK:ACTion:SOUNd:EVENt:COUNt on page 358
MASK:ACTion:STOP:EVENt:COUNt on page 358
MASK:ACTion:SCRSave:EVENt:COUNt on page 358
MASK:ACTion:PRINt:EVENt:COUNt on page 358
MASK:ACTion:WFMSave:EVENt:COUNt on page 358

Masks Test Off
Turns off the mask test and exits the "Mask" menu.

Remote command:
MASK:STATe on page 355

10 Search

10.1 Search Conditions and Results

The search functions of R&S RTM allow to find all edges, pulse widths, peaks, or other events in an acquisition that match the search conditions. For each search type, specific settings are available. Searches can be performed on any channel, math or reference waveform.

Searches can be performed online, that is repeatedly for each new data acquisition in a running acquisition series, or only once after the acquisition has been stopped. In an online search, only the displayed data is searched while the search on a stopped acquisition analyzes the contents of the memory.

The searched time base range can be restricted by defining a gate.

10.1.1 Search Results

Search results are marked in the diagram and listed in a results table with their specific measurement values. In the table, five results are shown. To navigate the search results, turn the NAVIGATION knob. See also: "To analyze search results" on page 134.

Search result markers

For further analysis, for example, for cursor measurements, you can set up to 20 markers to selected search results. Search result markers are different from usual timestamp markers but they are set, navigated and deleted by means of the marker keys, too. As long as a search is enabled, the search result markers are active. If search is off, usual markers can be used.

See also:

- "To use markers on search results" on page 135
- chapter 4.4, "Markers", on page 71

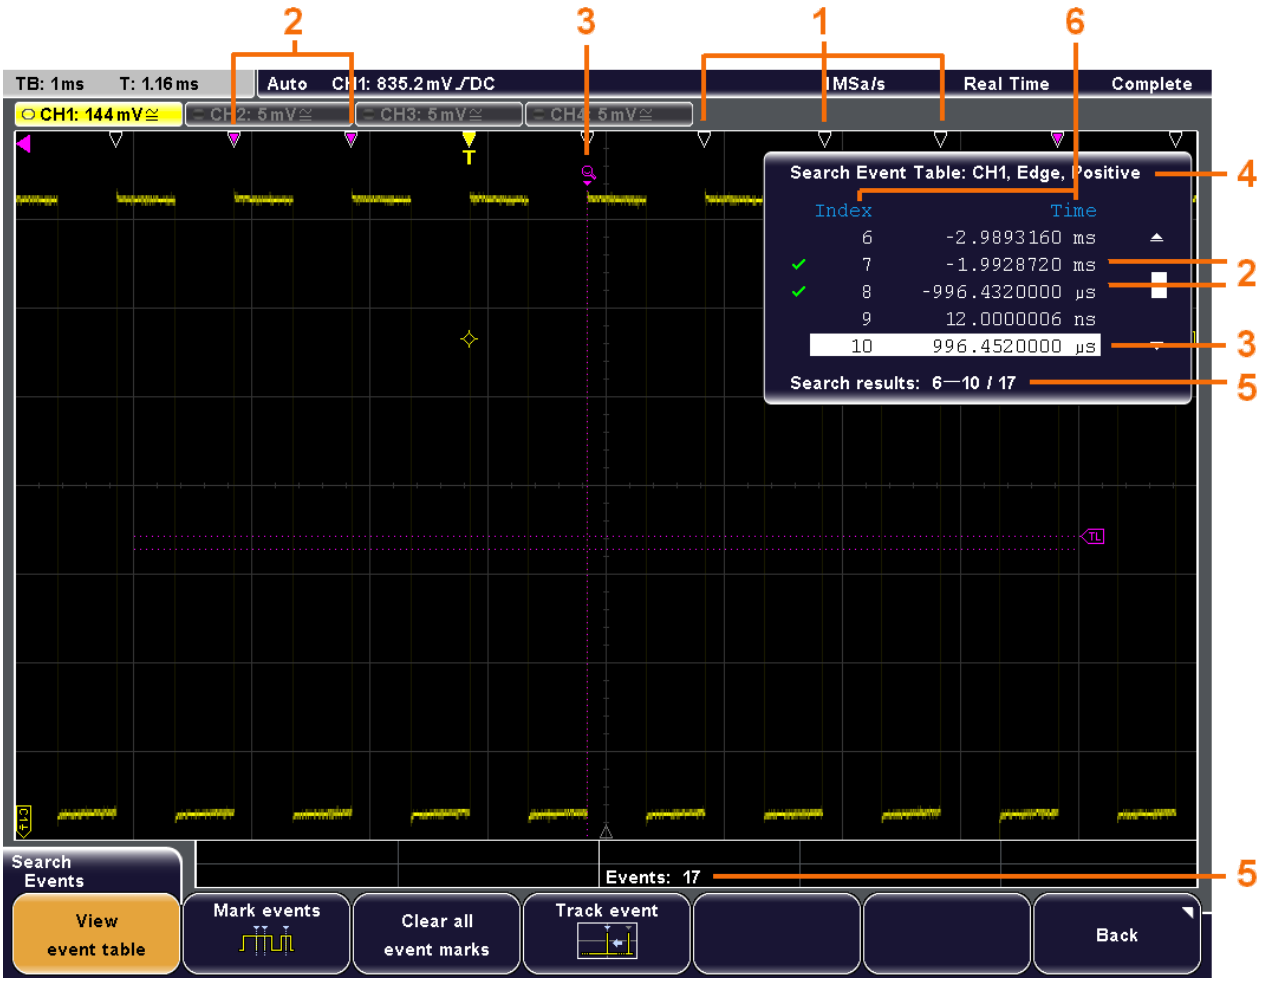

Fig. 10-1: Results of an edge search with R&S RTM

1 = Search results
2 = Marked search results
3 = Selected search result
4 = Search conditions
5 = Number of results, scope of results displayed in the results table
6 = Result values: result number, time value, optional value depending on the search type (voltage, width)

Remote commands:

- `SEARch:RCOunt?` on page 374
- `SEARch:RESult:ALL?` on page 373
- `SEARch:RESult<n>?` on page 373

10.2 Configuring and Performing Searches

To configure and start a search

Prerequisite: Signal acquisition, reference or math waveform is configured.

1. Press the SEARCH key.

   The "Search" menu opens, and the search is enabled.

2. Press "Source" and select the waveform for analysis. All active channel, math, and reference waveforms are available for selection.

3. Press "Search type" and select the event you want to search for: edge, width, peaks, runts, specified rise/fall time, setup/hold time, pattern, or protocol-specific events.

4. Press "Setup" and configure the selected search type.

   Details:

   - chapter 10.3.2, "Edge Setup", on page 137
   - chapter 10.3.3, "Width Setup", on page 138
   - chapter 10.3.4, "Peak Setup", on page 139
   - chapter 10.3.5, "Rise/Fall Time Setup", on page 139
   - chapter 10.3.6, "Runt Setup", on page 141
   - chapter 10.3.7, "Data2Clock Search", on page 142
   - chapter 10.3.8, "Pattern Search", on page 144
   - chapter 11.5.5.1, "CAN Search Setup", on page 194, requires option R&S RTM-K3
   - chapter 11.6.6.1, "LIN Search Setup", on page 205, requires option R&S RTM-K3

5. To restrict the time base range of the source waveform to be searched, press "Gate" and define the search area.

6. Start continuous acquisition with RUN CONT.

   The online search is performed on the displayed data. Search results are updated permanently and indicated at the top of the diagram.
   Stop the acquisition to search the memory data of the latest acquisition.

To analyze search results

1. Stop the running continuous acquisition, or acquire one waveform with RUN N× SINGLE.

2. Press "Events".

3. Press "View event table" in the "Events" menu.

   The first five search results are listed in a table.

4. To select a search result, turn the NAVIGATION knob.

The selected result is highlighted in the table and indicated in the diagram with a magnifier symbol.

5. To see the selected event even if it is outside the display, press "Track event".

   The waveform is moved on the display, and the selected result is shown at the time reference point.

To use markers on search results

1. If the search results table is not visible, press "View event table".
2. To set markers to all results, press "Mark events". If more then 20 results are found, the first 20 results are marked.
3. To set a marker to a selected result:
   a) Select the result in the "Search Event Table" by turning the NAVIGATION knob.
   b) Press the SET CLEAR key.
4. To select a marker:
   - Press the NEXT key to move to next marker to the right.
   - Press the PREV key to move to previous marker to the left.
5. To delete a single marker, select it an press the SET CLEAR key.
6. To delete all markers, press "Clear all event markers".

To finish a search

1. To close the results table, press "View event table".
2. To stop the search, press "Search".

10.3 Reference for Search Menu

10.3.1 Main Search Menu

The SEARCH MENU key opens the same-named menu where you can search various events, for example:

- edges
- peaks
- pulses with defined pulse width
- rise time or fall time
- ... and more

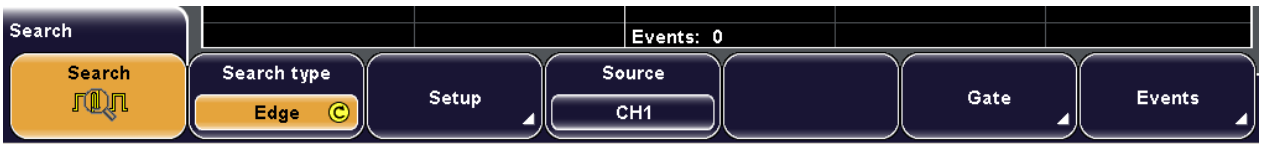

Search
Enables and disables the search mode.

Remote command:
`SEARch:STATe` on page 359

Search type
Selects the event you want to search for.

"Edge" Similar to the edge trigger, an edge search result is found when the waveform passes the given level in the specified direction.
For settings, see chapter 10.3.2, "Edge Setup", on page 137.

"Width" Similar to the width trigger, a width search finds pulses with an exact pulse width, or pulses shorter or longer than a given time, or pulses inside or outside the allowable time range.
For settings, see chapter 10.3.3, "Width Setup", on page 138

"Peak" The peak search finds pulses exceeding a given amplitude.
For settings, see chapter 10.3.4, "Peak Setup", on page 139

"Rise/Fall time" The rise or fall time search finds slopes with an exact rise or fall time, or rise/fall times shorter or longer than a given limit, or rise/fall times inside or outside the allowable time range.
For settings, see chapter 10.3.5, "Rise/Fall Time Setup", on page 139

"Runt" The runt search finds pulses lower than normal in amplitude. The amplitude crosses the first threshold twice without crossing the second one. In addition to the threshold amplitudes, you can define a time limit for the runt in the same way as for width search: runts with exact width, shorter or longer than a given time, or runts inside or outside the allowable time range.
For settings, see chapter 10.3.6, "Runt Setup", on page 141

"Data2Clock" The Data2Clock search - also known as setup/hold - finds violation of setup and hold times. It analyzes the relative timing between two signals: a data signal and the synchronous clock signal.
Many systems require, that the data signal must be steady for some time before and after the clock edge. Setup time is the time that the data signal is steady before clock edge. Hold time is the time that the data signal is steady after clock edge.
For settings, see chapter 10.3.7, "Data2Clock Search", on page 142.

"Pattern" The pattern search finds logical combinations of channel states inside or outside a specified time range. For each channel, its state and threshold level is defined. The states are combined logically, and the time of true pattern results is compared with a specified time range.
For settings, see chapter 10.3.8, "Pattern Search", on page 144.

"Protocol" The protocol search finds various events in decoded data of CAN and LIN signals, for example, a specified frame type, identifier, data, and errors.The protocol search requires option R&S RTM-K3.

For information on protocol search, see

- chapter 11.5.5, "Search on Decoded CAN Data", on page 194
- chapter 11.6.6, "Search on Decoded LIN Data", on page 205

Remote command:
`SEARch:CONDition` on page 359

Setup
Opens a menu to define the specific search parameters.

Source
Selects the waveform to be analyzed with edge, width, peak, rise/fall time, or runt search. All active channel, math, and reference waveforms are available for selection.

Remote command:
`SEARch:SOURce` on page 361

Source Setup
Opens a menu to define the source parameters for Data2Clock and Pattern search: waveform, level, and hysteresis.

Gate
Opens a menu to restrict the time base range of the source waveform for search.

See chapter 10.3.9, "Gate Menu", on page 146

Events
Opens a menu with functions for result display and marker usage.

See: chapter 10.3.10, "Events Menu", on page 147

Remote command:
`SEARch:RESDiagram:SHOW` on page 372

10.3.2 Edge Setup

Access: SEARCH MENU > "Search type = Edge" > "Setup"

Edge
Sets the slope to be found:

"Rising" Rising edge, a positive voltage change

"Falling" Falling edge, a negative voltage change

"Both" Rising edge and falling edge

Remote command:
SEARch:TRIGger:EDGE:SLOPe on page 362

Level
Sets the voltage level for the search.

Remote command:
SEARch:TRIGger:EDGE:LEVel on page 362

Hysteresis
Sets a hysteresis range to the search level in order to avoid unwanted search results caused by noise oscillation around the level. For a rising edge, the hysteresis is below the search level. Otherwise, for a falling edge the hysteresis is above the level.

Remote command:
SEARch:TRIGger:EDGE:LEVel:DELTa on page 362

10.3.3 Width Setup

Access: SEARCH MENU > "Search type = Width" > "Setup"

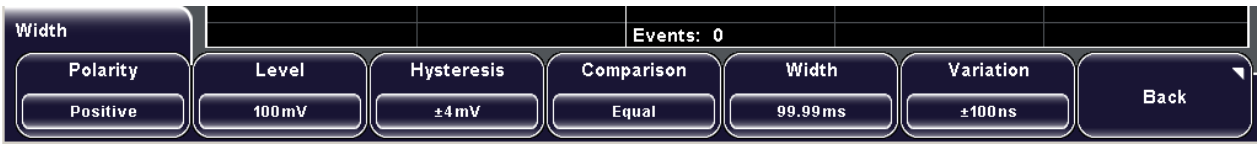

Polarity
Indicates the polarity of the pulse to be searched for.

Remote command:
SEARch:TRIGger:WIDTh:POLarity on page 362

Level
Sets the voltage level on which the pulse width is measured.

Remote command:
SEARch:TRIGger:WIDTh:LEVel on page 363

Hysteresis
Sets a hysteresis range to the search level in order to avoid unwanted search results caused by noise oscillation around the level. For a rising edge, the hysteresis is below the search level. Otherwise, for a falling edge the hysteresis is above the level.

Remote command:
SEARch:TRIGger:WIDTh:LEVel:DELTa on page 363

Comparison
Sets the condition how the measured pulse width is compared with the given limit(s).

"Greater than" Finds pulses longer than the given "Width".
See also: Width

"Lower than"	Finds pulses shorter than the given "Width".
"Equal"	Finds pulses equal to the reference "Width" if "Variation" Δt = 0. If "Variation" ≠ 0, the setting finds pulses within the range width ± Δt. See also: Variation
"Not equal"	Finds pulses unequal to the reference "Width" if "Variation" Δt = 0. If "Variation" ≠ 0, the setting finds pulses outside the range width ± Δt.

Remote command:
`SEARch:TRIGger:WIDTh:RANGe` on page 363

Width
Sets the reference pulse width, the nominal value for comparisons.

Remote command:
`SEARch:TRIGger:WIDTh:WIDTh` on page 364

Variation
Sets a range Δt to the reference "Width" if comparison is set to "Equal" or "Not equal". The instrument finds pulses inside or outside the range width ± Δt.

Remote command:
`SEARch:TRIGger:WIDTh:DELTa` on page 364

10.3.4 Peak Setup

Access: SEARCH MENU > "Search type = Peak" > "Setup"

Polarity
Indicates the polarity of the pulse to be searched for.

Remote command:
`SEARch:MEASure:PEAK:POLarity` on page 364

Magnitude
Sets the amplitude limit.

Remote command:
`SEARch:MEASure:LEVel:PEAK:MAGNitude` on page 364

10.3.5 Rise/Fall Time Setup

Access: SEARCH MENU > "Search type = Rise/Fall time" > "Setup"

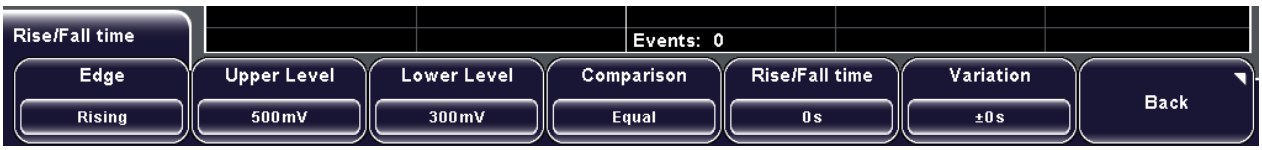

Edge
Sets the slope to be found:
- "Rising" to search for rise time
- "Falling" to search for fall time
- "Both" to search for rise and fall time

Remote command:
`SEARch:TRIGger:RISetime:SLOPe` on page 365

Upper level
Sets the upper voltage threshold. When the signal crosses this level, the rise/fall time measurement starts or stops depending on the selected slope.

Remote command:
`SEARch:TRIGger:LEVel:RISetime:UPPer` on page 365

Lower level
Sets the lower voltage threshold. When the signal crosses this level, the rise time measurement starts or stops depending on the selected slope.

Remote command:
`SEARch:TRIGger:LEVel:RISetime:LOWer` on page 365

Comparison
Sets how the measured rise or fall time is compared with the given limit(s).

"Greater than"	Finds rise/fall times longer than the given "Rise/Fall time".
"Lower than"	Finds rise/fall times shorter than the given "Rise/Fall time".
"Equal"	Finds rise/fall times equal to the reference "Rise/Fall time" if "Variation" $\Delta t = 0$. If "Variation" $\neq 0$, the setting finds rise/fall times within the range time $\pm \Delta t$. See also: Variation.
"Not equal"	Finds rise/fall times unequal to the reference value if "Variation" $\Delta t = 0$. If "Variation" $\neq 0$, the setting finds rise/fall times outside the range time $\pm \Delta t$.

Remote command:
`SEARch:TRIGger:RISetime:RANGe` on page 365

Rise/Fall time
Sets the reference rise or fall time, the nominal value for comparisons.

Remote command:
`SEARch:TRIGger:RISetime:TIME` on page 366

Variation
Sets a range Δt to the reference "Rise/Fall time" if comparison is set to "Equal" or "Not equal". The instrument finds rise/fall times inside or outside the range width ± Δt.

Remote command:
SEARch:TRIGger:RISetime:DELTa on page 366

10.3.6 Runt Setup

Access: SEARCH MENU > "Search type = Runt" > "Setup"

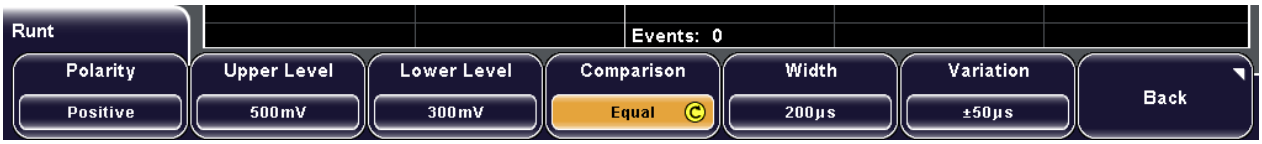

Polarity
Indicates the polarity of the pulse to be searched for.

Remote command:
SEARch:TRIGger:RUNT:POLarity on page 367

Upper level
Sets the upper voltage threshold for runt detection. A negative runt crosses the upper level twice without crossing the lower level.

Remote command:
SEARch:TRIGger:LEVel:RUNT:UPPer on page 367

Lower level
Sets the lower voltage threshold for runt detection. A positive runt crosses the lower level twice without crossing the upper level.

Remote command:
SEARch:TRIGger:LEVel:RUNT:LOWer on page 367

Comparison
Sets the condition how the measured runt width is compared with the given limit(s).

The same conditions as with width search are used, see "Comparison" on page 138.

Remote command:
SEARch:TRIGger:RUNT:RANGe on page 367

Width
Sets the reference runt pulse width, the nominal value for comparisons.

Remote command:
SEARch:TRIGger:RUNT:WIDTh on page 368

Variation
Sets a range Δt to the reference "Width" if comparison is set to "Equal" or "Not equal". The instrument finds pulses inside or outside the range width ± Δt.

Remote command:
SEARch:TRIGger:RUNT:DELTa on page 368

10.3.7 Data2Clock Search

The settings for Data2Clock search are provided in two menus: in the "Setup" menu you define the clock polarity, setup and hold times; and in the "Source Setup" menu you define the waveforms to be used, and the levels and hysteresis for each source.

10.3.7.1 Data2Clock Source Setup

Access: SEARCH MENU > "Search type = Data2Clock" > "Source Setup"

For Data2Clock search, two sources have to be defined: a clock and a data waveform. For each waveform, the level and the hysteresis can be set individually.

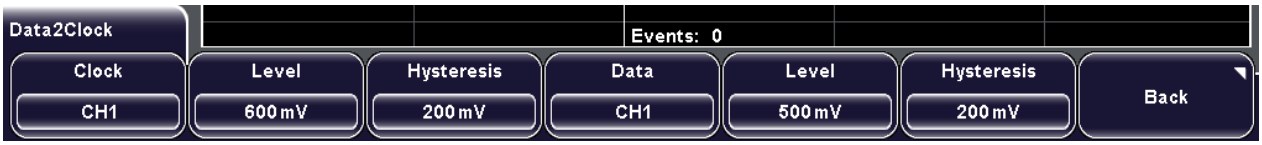

Clock
Selects the input channel of the clock signal.

Remote command:
SEARch:TRIGger:DATatoclock:CSOurce on page 368

Data
Selects the input channel of the data signal.

Remote command:
SEARch:SOURce on page 361

Level
Set the voltage levels for clock and data signals. Clock level and clock edge define the reference point for setup and hold time. The data lavel defines the point of data transition.

Remote command:
SEARch:TRIGger:DATatoclock:CLEVel on page 369
SEARch:TRIGger:DATatoclock:DLEVel on page 369

Hysteresis
Sets a hysteresis range to the search level of the selected signal in order to avoid unwanted search results caused by noise oscillation around the level. For a rising edge, the hysteresis is below the search level. Otherwise, for a falling edge the hysteresis is above the level.

Remote command:
SEARch:TRIGger:DATatoclock:CLEVel:DELTa on page 369
SEARch:TRIGger:DATatoclock:DLEVel:DELTa on page 369

10.3.7.2 Data2Clock Setup

Access: SEARCH MENU > "Search type = Data2Clock" > "Setup"

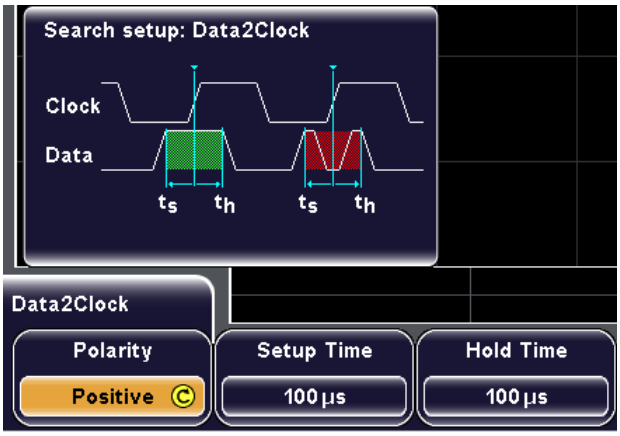

Polarity
Sets the edge of the clock signal to define the time reference point for the setup and hold time.

"Rising" Only positive clock edges are considered.

"Falling" Only negative clock edges are considered.

"Either" The clock edges next to the data edge are considered regardless of the clock slope.

Remote command:
SEARch:TRIGger:DATatoclock:CEDGe on page 369

Setup Time
Sets the minimum time **before** the clock edge while the data signal must stay steady above or below the data level. The setup time can be negative. In this case, the setup interval starts after the clock edge, and the hold time must be positive and longer than the absolute value of the setup time.

Remote command:
SEARch:TRIGger:DATatoclock:STIMe on page 370

Hold Time
Sets the minimum time **after** the clock edge while the data signal must stay steady above or below the data level. The hold time can be negative. In this case, the hold time ends before the clock edge, and the setup time must be positive and longer than the absolute value of the hold time.

Remote command:
`SEARch:TRIGger:DATatoclock:HTIMe` on page 369

10.3.8 Pattern Search

The settings for pattern search are provided in two menus: in the "Setup" menu you define the channel states, their logical combination and the time range for keeping up the true result of the state pattern condition; and in the "Source Setup" menu you define the threshold levels and hysteresis for each channel.

10.3.8.1 Pattern Source Setup

Access: SEARCH MENU > "Search type = Pattern" > "Source Setup"

For pattern search, up to four channels can be used as source. For each channel, the threshold level and the hysteresis can be set individually.

Source
Selects the channel for which the pattern search is defined.

Level
Sets the threshold value for the selected source channel. If the signal value is higher than the trigger level, the signal state is high (1 or true for the boolean logic). Otherwise, the signal state is considered low (0 or false) if the signal value is below the trigger level.

Remote command:
`SEARch:TRIGger:PATTern:LEVel<n>` on page 371

Hysteresis
Sets a hysteresis range to the level of the selected source channel in order to avoid unwanted search results caused by noise oscillation around the level. For a rising edge, the hysteresis is below the search level. Otherwise, for a falling edge the hysteresis is above the level.

Remote command:
`SEARch:TRIGger:PATTern:LEVel<n>:DELTa` on page 371

10.3.8.2 Pattern Setup

Access: SEARCH MENU > "Search type = Pattern" > "Setup"

For pattern search, up to four channels can be used as source. For each channel, you define the state. The states are combined logically, and the time of true pattern results is compared with a specified time range. Thus you can find state transitions inside or outside this time range.

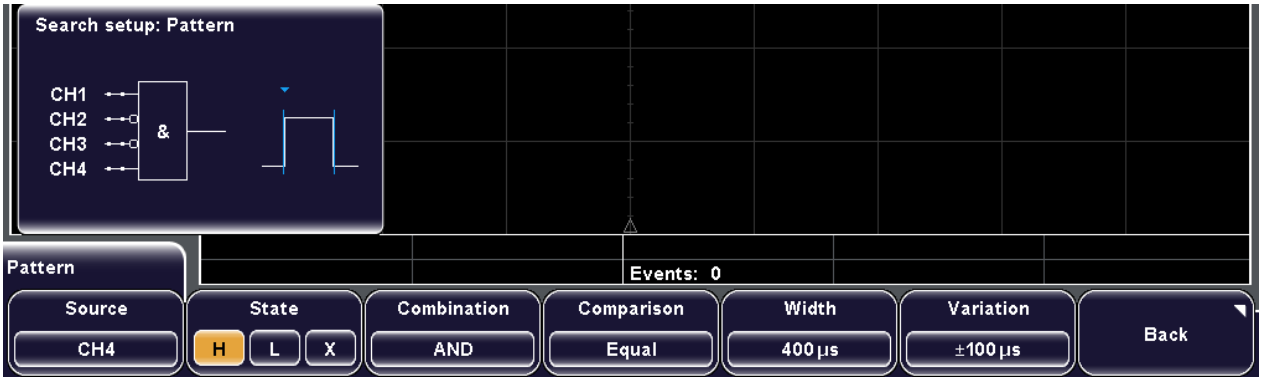

Source
Selects the channel for which the pattern search is defined.

Remote command:
`SEARch:TRIGger:PATTern:SOURce` on page 370

State
Sets the state of the selected source channel. The states are:

"H" High: the signal voltage is higher than the threshold level.

"L" Low: the signal voltage is lower than the threshold level.

"X" Don't care: the channel does not affect the search.

Remote command:
`SEARch:TRIGger:PATTern:SOURce` on page 370

Combination
Sets the logical combination of the channel states.

"AND" The required states of all channels must appear in the input signal at the same time.

"Or" At least one of the channels must have the required state.

"NAND" "Not and" operator, at least one of the channels does not have the required state.

"NOR" "Not or" operator, none of the channels has the required state.

Remote command:
`SEARch:TRIGger:PATTern:FUNCtion` on page 370

Comparison
Sets the condition how the duration of a steady pattern is compared with the given limit(s). The three settings "Width" "Variation" and "Comparison" define the time range for keeping up the true result of the state pattern.

The same conditions as with width search are used, see "Comparison" on page 138.

Remote command:
`SEARch:TRIGger:PATTern:WIDTh:RANGe` on page 371

Width
Sets the limit time of a steady pattern, the nominal value for comparisons.

Remote command:
`SEARch:TRIGger:PATTern:WIDTh[:WIDTh]` on page 372

Variation
Sets a range Δt to the reference "Width" if comparison is set to "Equal" or "Not equal". The instrument finds true results of the state pattern inside or outside the range width ± Δt.

Remote command:
`SEARch:TRIGger:PATTern:WIDTh:DELTa` on page 372

10.3.9 Gate Menu

Access: SEARCH MENU > "Gate"

The gate restricts the time base of the source waveform to be searched.

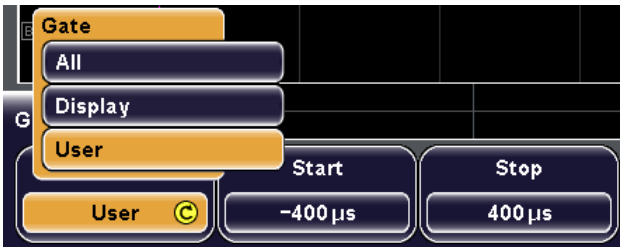

Gate
Defines the search area. If the search is performed on a running acquisition series, the instrument analyzes the displayed data. The search on a stopped acquisition analyzes the contents of the memory.

"All"	Running acquisition: all waveform samples that are displayed on the screen. Stopped acquisition: all data samples that are stored in the memory.
"Display"	Search is restricted to the time range of the display.
"User"	Search is restricted to the time range defined by "Start" and "Stop" values.

Remote command:
`SEARch:GATE:MODE` on page 361

Start
Sets the start time of the search area in relation to the trigger point.

Remote command:
SEARch:GATE:ABSolute:START on page 361

Stop
Sets the end time of the search area in relation to the trigger point.

Remote command:
SEARch:GATE:ABSolute:STOP on page 361

10.3.10 Events Menu

Access: SEARCH MENU > "Events"

Events are the search results which are marked in the waveform diagram and listed in the event table. See also: chapter 10.1.1, "Search Results", on page 132.

View event table
Shows or hides the table of search results.

Remote command:
SEARch:RESDiagram:SHOW on page 372

Mark events
Sets markers to the first search results. Up to 20 markers can be set at once.

Clear all event marks
Removes all markers from search results.

Track event
If enables, the selected result is moved to the reference point. Thus you can always see the selected event in the diagram.

11 Protocol Analysis

With the R&S RTM and some additional options, you can analyze the following parallel and serial protocols:

- SPI (Serial Peripheral Interface with 3 lines) and SSPI (Serial Peripheral Interface with 2 lines) - requires option R&S RTM-K1
- I²C (Inter-Integrated circuit bus) - requires option R&S RTM-K1
- UART/RS232 (EIA-232 serial interface) - requires option R&S RTM-K2
- CAN (Controller Area Network) - requires option R&S RTM-K3
- LIN (Local Interconnect Network) - requires option R&S RTM-K3
- Audio (I2S, LJ, RJ,TDM) - requires option R&S RTM-K5

11.1 Basics of Protocol Analysis

The analysis of serial data consists of three main steps:

- Protocol configuration: Select the protocol type, and configure the input line as well as the protocol-specific settings
- Decoding: Configure the display of the decoded data and enable decoding. As a result, the digitized signal data is displayed on the screen together with the decoded content of the messages.
  You can scale the signal display and zoom into it to see it in more detail.
  You can create and apply label lists for easier identification of the bus nodes on the display.
- Triggering: You can trigger on various events that are typical for the configured bus type, for example, on start and stop of messages, on specific addresses, or on serial patterns.

Analysis can be performed on analog input channels, and - if MSO option R&S RTM-K1 is installed - on digital channels.

11.1.1 Configuring Common Protocol Settings

Common settings for all bus types are the logic threshold and the decoding and display settings.

If the MSO option R&S RTM-B1 is installed, and the digital channels are used for protocol analysis, the thresholds are set in the "Logic" menu.

To set the logic threshold for analog channels

Before you start configuration and analysis, check and set the logic thresholds for all used channels - the voltage values for digitization of analog signals. If the signal value is higher than the threshold, the signal state is 1. Otherwise, the signal state is considered 0 if the signal value is below the threshold.

If you want the instrument to set the thresholds based on the analysis of the signals, press "Find level" in the protocol's "Configuration" menu.

1. Press the CH N key of the required channel.
2. Press the "More" softkey.
3. Press "Threshold" and enter the voltage value.
4. Repeat step 1 to 3 for all channels that are used for protocol analysis.

To configure decoding and data display

1. Press the PROTOCOL LOGIC key on the front panel.
2. If the "Logic" menu is displayed, press "Protocol".
3. Press "Decode" to display the content of the messages in an easily readable and comprehensible form.
4. Press "Display".
5. Press "Bits" to display the individual bit lines above the decoded data.
6. Press "Data format" to select the decoding format: Binary, Hexadecimal, Decimal or ASCII.
7. To attach a descriptive label to the decoded bus, enable "Label" and select a predefined text from the "Library", or enter a user-defined text using "Edit Label".
8. To adjust the position and size of decoded information on the screen, use the vertical POSITION and SCALE rotary knobs.

11.1.2 Protocol - Common Settings

The common settings in the "Protocol" menu define the bus type and open further menus to adjust the display of the decoded bus signal.

Access: PROTOCOL LOGIC > if "Logic" menu is displayed: "Protocol"

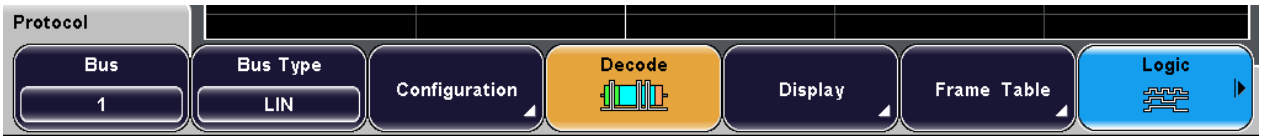

Bus
Selects the bus to be configured.

SPI/SSPI and UART protocols occupy two bus lines (bus 1 and 2 or bus 3 and 4). If one of these buses is configured, the number of buses (suffix <b>) is reduced. Bus 2 and/or bus 4 is not available.

Bus Type
Defines the bus or protocol type for analysis. For most types, a special option to the instrument is required.

Remote command:
`BUS<b>:TYPE` on page 375

Configuration
Opens the configuration menu for the selected bus type.

Decode
Decodes the signal according to the protocol configuration and displays the decoded signal - the content of every message. The decoding format is set with "Display".

Remote command:
`BUS<b>:STATe` on page 374

Display
Opens the "Display" menu, where you can:
- Display the bit lines
- Set the decoding format
- Define labels for the bus and its lines

See: chapter 11.1.3, "Display Settings", on page 150

Frame Table
Opens the "Frame table" menu to configure and display the frame table with detailed decoded data for each frame of the acquisition.

See: chapter 11.1.5, "Frame Table: Decode Results", on page 154

11.1.3 Display Settings

Access: PROTOCOL LOGIC > if "Logic" menu is displayed: "Protocol" > "Display"

Bits
Displays the individual bit lines above the decoded bus line.

Remote command:
`BUS<b>:DSIGnals` on page 375

Data format
Sets the decoding format of the data: Binary, Hexadecimal, Decimal or ASCII.

Remote command:
`BUS<b>:FORMat` on page 375

Label
Opens the "Label" menu to define an additional name label for the selected bus.

Label ← Label
Displays or hides the bus label. The bus label is shown on the the right side of the display. You can enter a label text in several ways:

- Select a predefined string from the "Library".
- Enter a user-defined text using "Edit Label".

Library ← Label
Selects a label text from a list of frequently used terms.

Edit Label ← Label
Opens the on-screen keyboard to enter any label text.

The maximum name length is 8 characters, and only ASCII characters provided on the on-screen keyboard can be used.

Label List
Opens the "Label list" menu to load, sort, and display a name for each bus node instead of the address or ID on the decoded results display. So it is easy to identify the messages of the different bus nodes.

See: chapter 11.1.4, "Label List", on page 151

11.1.4 Label List

For all protocols using ID or address identification, it is possible to create label lists containing addresses or IDs, a symbolic name for each node (symbolic label), and some protocol-specific information. You can load label lists, and activate its usage for decoding. As a result, an additional "Label" column appears in the "Frame Table", containing the symbolic label. The frame captions of the decoded signal show the symbolic label instead of the ID or address values so it is easy to identify the messages of the different bus nodes.

- Content and Format of the PTT File.....151
- Label List Menu.....153

11.1.4.1 Content and Format of the PTT File

Label lists are stored as PTT (protocol translation table) files. The PTT file format is an extension of the CSV format (comma separated values). You can edit it with standard editors, for example, with MS Excel or a text editor.

The PTT file has three types of lines:

- Comment lines begin with a hash character #. A hash character at any other position in the line is treated like a standard character.
- Command lines begin with a commercial at character @. An @ character at any other position in the line is treated like a standard character.
- Standard lines are the lines that not qualify as comment or command lines. They build the core of the label list.

Command lines

Command lines define the version of the PTT file and the protocol name:

- @FILE_VERSION: must appear exactly once in the file
- @PROTOCOL_NAME: must appear at least once in the file. Thus, one file can contain several label lists for different protocols.

```
# --- Start of PTT file
@FILE_VERSION  = 1.0
@PROTOCOL_NAME = i2c
[... Label list for I2C]
@PROTOCOL_NAME = can
[... Label list for CAN]
# --- End of PTT file
```

Standard lines

Standard lines define the contents of the label list. The rules for standard lines follow the csv convention, they are:

- Values are separated by commas
- Space characters following a delimiter are ignored
- Values with a special character (comma, newline, or double quote) must be enclosed in double quotes
- Text in double quotes must be escaped by double quote characters

Additionally, numeric values may be decimal integer (default) or hexadecimal integer (with prefix "0x")

```
# --- Start of PTT file
@FILE_VERSION  = 1.0
@PROTOCOL_NAME = i2c
#    Following two lines are equal:
7,0x01,Temperature
7,0x01, Temperature
#    A comma must be enclosed in double quotes:
7,0x01,"Temperature, Pressure, and Volume"
#    A double quote must also be enclosed in double quotes:
7,0x7F,"Highspeed ""Master"" 01"
#    Following lines yield the same result:
7,0x11,Pressure
0x7,0x11,Pressure
0x7,17,Pressure
```

```
1,17,Pressure
```

Label lists are protocol-specific. Their contents are described in the corresponding protocol chapters:

- chapter 11.3.4, "I²C Label List", on page 172
- chapter 11.5.3, "CAN Label List", on page 191
- chapter 11.6.4, "LIN Label List", on page 202

11.1.4.2 Label List Menu

Access: PROTOCOL > "Bus Type" = "I2C | CAN | LIN" > "Label List"

Apply....153
Load....153
Show....153
Sort....153
Remove....153

Apply
Shows the labels from the label list in the display of decode results instead of the ID or address.

Load
Opens a menu to select and load a PTT file from an USB flash drive. The PTT file contains one or more label lists.

The function is only available if an USB flash drive is connected to the instrument.

Alternatively, you can load a label list together with the device settings, if both were saved with FILE > "Device Settings > Save > Setup & Label".

See also: "Setup & Label" on page 226

Show
Diplays the label list for the selected protocol type. Before, the label list must be loaded from a PTT file.

Sort
Displays the label list in alphanumerical order or sorted by ID or address.

Remove
Deletes the label list from the instrument.

11.1.5 Frame Table: Decode Results

Access: PROTOCOL > "Frame Table"

The frame table shows the detailed decoded data for each frame of the acquisition. The table content is protocol-specific, and the display of the table can be enabled for each individual bus type.

Decode results shown in the frame table can be saved in a CSV file.

To navigate in the frame table

1. Stop the acquisition.
2. Turn the NAVIGATION knob to select a frame.
3. Press the NAVIGATION knob to display the selected frame in the center of the waveform display.

If a search on decoded data was performed, the search results are marked in the frame table.

Frame Table
Displays or hides the table of decode results.

Remote command:
`BUS<b>:RESult` on page 376

Track frame
Defines the automatic synchronization of the selected frame in the frame table and the waveform display.

The function is only available if the acquisition has been stopped.

"Off" Frame table and waveform display are not synchronized.

"Frame Index" The waveform display is connected to the frame that is selected in the frame table. The selected frame is shown in the center of the display. If you select another frame, the waveform display is adjusted automatically.

"Hori. Position" The frame selection in the frame table is connected to the waveform display. The frame in the center of the display is selected in the frame table. When you change the horizontal position of the waveform, the selection in the frame table is adjusted automatically.

Frame time difference
If selected, the time shown in the frame table is the time difference to the previous frame. The column is indicated with "Time diff.". If the setting is disabled, the absolute time in releation to the trigger point is shown in the "Start time" column.

Position
Defines the position of the frame table on the screen: top right, bottom right, or full screen. With full screen setting, the frame table covers nearly the complete righthand half of the screen.

Save
Opens the "Save" menu to save the decoded data in a CSV file (comma-separated list).

Remote command:
`BUS<b>:LIST?` on page 376
`BUS<b>:LIST:SAVE` on page 376

11.2 SPI/SSPI Bus (Option R&S RTM-K1)

11.2.1 The SPI Protocol

A 4-channel instrument is required for full support of the SPI protocol.

The Serial Peripheral Interface SPI is used for communication with slow peripheral devices, in particular, for transmission of data streams.

Main characteristics of SPI are:

- Master-slave communication
- No device addressing; The slave is accessed by a chip select, or slave select line.
- No acknowledgement mechanism to confirm receipt of data
- Duplex capability

Most SPI buses have four lines, two data and two control lines:

- Clock line to all slaves (SCLK)
- Slave Select or Chip Select line (SS or CS)
- Master data output, slave data input (MOSI or SDI)
- Master data input, slave data output (MISO or SDO)

When the master generates a clock and selects a slave device, data may be transferred in either or both directions simultaneously.

As SPI is very simple and efficient for single master - single slave applications, the R&S RTM provides also an SSPI (simple SPI) configuration that does not have a chip select line.

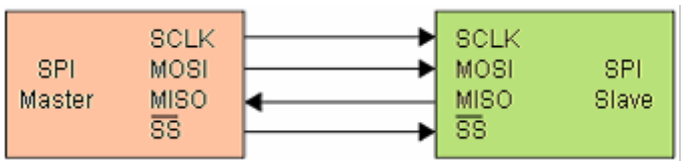

Fig. 11-1: Simple configuration of SPI bus

The data bits of a message are grouped by following criteria:

- A word contains a number of successive bits. The word length is defined in the protocol configuration.
- A frame contains a number of successive words, at least one word.

For SPI buses, the R&S RTM provides the following trigger possibilities:

- On frame start or frame end
- On a specified bit in the message
- On a serial pattern

11.2.2 SPI/SSPI Bus Configuration

- Configuring SPI Buses....156
- SPI/SSPI Configuration Settings....157

11.2.2.1 Configuring SPI Buses

You define the input channels for the lines and some bit information on the message.

1. Press the PROTOCOL LOGIC key on the front panel.
2. If the "Logic" menu is displayed, press "Protocol".
3. Press the "Bus Type" softkey and select "SPI" or "SSPI".
4. Press "Configuration".
5. Press "Source" and select "Clk".
6. Press "Clock" and select the input channel of the clock. Select the "Slope".
7. Press "Source" and select "MOSI".
8. Press "MOSI" and select the input channel. With "Active", select the active state of the data - high or low.
9. If required, repeat steps 6 and 7 for the optional MISO line.
10. For SPI, press "Source" and select "CS". Enter the input channel with "Chip Select" and set the "Active" state.
11. For SSPI, press "Source" and select "Time". Enter the "Idle Time".
12. Set the "First Bit" and the "Symbol Size".

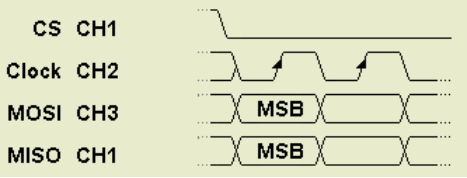

13. Press "Find level", or set the threshold manually for each channel.

See: "To set the logic threshold for analog channels" on page 148

Now you can disply the decoded signal and the frame table with results.

The display of the decoded data is described in "To configure decoding and data display" on page 149.

11.2.2.2 SPI/SSPI Configuration Settings

Access: PROTOCOL > "Bus type" = "SPI or SSPI" "Configuration"

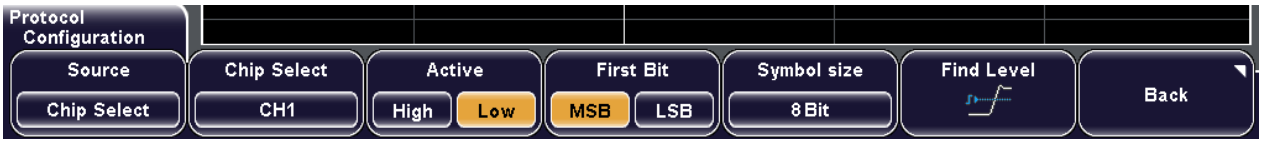

Source....157
Chip Select, Clock, Data....157
Active....157
Slope....158
Time Out....158
First Bit....158
Symbol Size....158
Find Level....158

Source
Toggles the lines of the SPI bus. Each line has to be configured. Select a line and adjust the settings:

- CS (Chip Select, SPI only): Select the input channel and the "Active" state.
- Time (SSPI only): Set the "Time Out" (instead if chip select).
- Clk (Clock): Select the input channel and the "Slope".
- Data: Select the input channel and the "Active" state.

Chip Select, Clock, Data
Select the input channels of the corresponding line. Make sure to select the "Source" before you assign the channel.

If the MSO option R&S RTM-B1 is installed, digital channels can also be used as source.

Remote command:
`BUS<b>:SPI:CS:SOURce` on page 377
`BUS<b>:SPI:CLOCk:SOURce` on page 378
`BUS<b>:SPI:DATA:SOURce` on page 0
`BUS<b>:SSPI:CLOCk:SOURce` on page 386
`BUS<b>:SSPI:DATA:SOURce` on page 0

Active
Selects whether transmitted data or the chip select signal is high active (high = 1) or low active (low = 1).

For CS, the default is low active.

For data, the default is high active.

Remote command:
BUS<b>:SPI:CS:POLarity on page 377
BUS<b>:SPI:DATA:POLarity on page 0
BUS<b>:SSPI:DATA:POLarity on page 0

Slope
Selects if data is sampled on the rising or falling slope of the clock. The clock slope marks the begin of a new bit.

Remote command:
BUS<b>:SPI:CLOCk:POLarity on page 378
BUS<b>:SSPI:CLOCk:POLarity on page 386

Time Out
Sets the minimum idle time between two data packets. If the time interval between the data packets is shorter, the packets are part of the same frame. Within the time out, the data and clock lines are low. A new frame begins when the time out has expired.

Time out is only relevant for SSPI that has no chip select.

Remote command:
BUS<b>:SSPI:BITime on page 387

First Bit
Defines if the data of the messages starts with MSB (most significant bit) or LSB (least significant bit).

Remote command:
BUS<b>:SPI:BORDer on page 379
BUS<b>:SSPI:BORDer on page 387

Symbol Size
Sets the word length, the number of bits in a message.

Remote command:
BUS<b>:SPI:SSIZe on page 379
BUS<b>:SSPI:SSIZe on page 388

Find Level
The instrument analyzes all lines that are configured for the selected bus and sets the threshold for digitization of analog signals for each channel. If no level can be found, the existing value remains unchanged, and you can set the thresholds manually in the channel menu: CH N > "More" (page 2) > "Threshold".

See: "Threshold" on page 31

"Find Level" is not relevant for digital channels (MSO option R&S RTM-B1). Thresholds for digital channels are set in the "Logic > Threshold" menu.

Remote command:
CHANnel<m>:THReshold:FINDlevel on page 379

11.2.3 SPI/SSPI Trigger

- Triggering on SPI Buses.....159
- SPI/SSPI Trigger Settings.....160

11.2.3.1 Triggering on SPI Buses

Prerequisites: The SPI or SSPI bus is configured. After configuration, the trigger type "Protocol (SPI)" or "Protocol (SSPI)" is available. See: chapter 11.2.2.1, "Configuring SPI Buses", on page 156.

Triggers are only available if "Decode" is enabled.

1. Press the SETUP key in the trigger area of the front panel.
2. Select the "Trigger Type": "Protocol (SPI)" or "Protocol (SSPI)"
3. Press "Setup".
4. Press the softkey of the required trigger condition:
   - "Frame Start": begin of the message
   - "Frame End": message end
   - "Bit<x>": a specified bit inside the message
   - "Ser. Pattern": a bit pattern in the message
5. If "Bit<x>" is selected, enter the bit number.
6. If "Ser. Pattern" is selected, press the softkey again and define the pattern:
   a) Set the "Bit Offset", the number of bits before the pattern starts.
   b) Set the "Number of Bits" contained in the pattern.
   c) Enter the pattern, either as binary input, or as hexadecimal input:
      - For binary input, press "Select Bit" and enter the bit number to be set. The bits are counted from the message start, the selected bit is highlighted in the pattern bit line. Then enter the "State" of this bit: 0, 1, or X (don't care). Repeat these settings until all bit states are defined.
      - For hexadecimal input, press "Select Nibble" and select the four bits (half byte) to be set. The selected nibble is highlighted in the lower pattern line. Then press "Value" and turn the navigation knob to change the bits. Repeat these settings until all nibbles are defined.

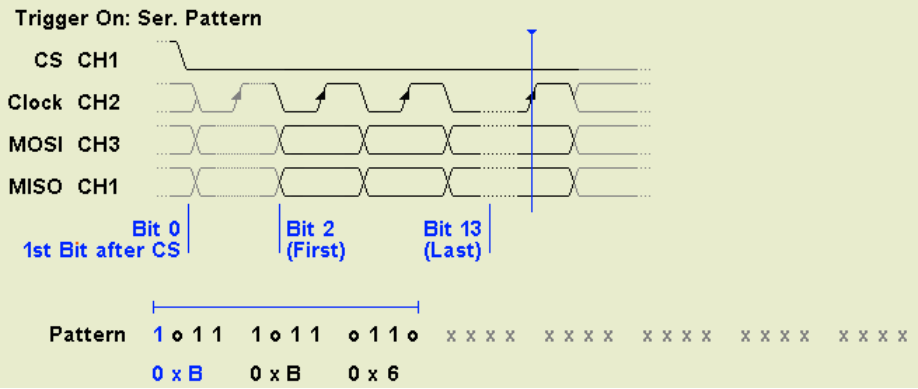
Trigger On: Ser. Pattern
CS CH1
Clock CH2
MOSI CH3
MISO CH1
Bit 0
1st Bit after CS
Bit 2
(First)
Bit 13
(Last)
Pattern
1 o 1 1 1 o 1 1 o 1 1 o x x x x x x x x x x x x x x x x x x x x
0 x B 0 x B 0 x 6

11.2.3.2 SPI/SSPI Trigger Settings

The complete SPI/SSPI trigger is configured in the "Source" and "Setup" menus.

Triggers are only available if "Decode" is enabled.

- SPI/SSPI Trigger Source.....160
- SPI/SSPI Trigger Setup.....160

SPI/SSPI Trigger Source

Access: TRIGGER SETUP > "Trigger Type" = "Protocol (SPI or SSPI)" > "Source"

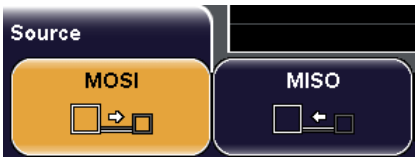

B1, B2, B3, B4
Select one of the configured and decoded buses as trigger source.

SPI/SSPI Trigger Setup

Access: TRIGGER SETUP > "Trigger Type" = "Protocol (SPI or SSPI)" > "Setup"

Frame Start....161
Frame End....161
Bit<x>....161
Ser. Pattern....161
└ Bit Offset....161
└ Number of Bits....162
└ Select Bit....162
└ State....162
└ Select Nibble....162
└ Value....162

Frame Start
Sets the trigger to the start of the message. For SPI, the frame starts when the chip select signal CS changes to the active state. For SSPI, the frame starts when the idle time has expired.

Remote command:
`TRIGger:A:SPI:MODE` on page 380 (`BSTart`)

Frame End
Sets the trigger to the end of the message. For SPI, the frame ends when the chip select signal CS changes to the inactive state. For SSPI, the frame ends when the idle time has expired after the last clock and no new clock appeared during that time.

Remote command:
`TRIGger:A:SPI:MODE` on page 380 (`BEND`)

Bit<x>
Sets the trigger to the specified bit number.

Remote command:
`TRIGger:A:SPI:MODE` on page 380 (`NTHBit`)

Ser. Pattern
Sets the trigger to a specified bit pattern that is configured in the submenu.

Remote command:
`TRIGger:A:SPI:MODE` on page 380 (`PATTern`)
`TRIGger:A:SPI:PATTern` on page 380

Bit Offset ← Ser. Pattern
Sets the number of bits before the first bit of the pattern. These bits are ignored. The first bit after CS is Bit 0.

For example, with bit offset = 2, Bit 0 and Bit 1 after CS are ignored, and the pattern starts with Bit 2.

Remote command:
`TRIGger:A:SPI:POFFset` on page 381

Number of Bits ← Ser. Pattern
Defines the length of the serial pattern in bit.

Remote command:
`TRIGger:A:SPI:PLENgth` on page 381

Select Bit ← Ser. Pattern
Selects the bit number for binary pattern setting. For the selected bit, "State" is to be set. The bits are counted from the message start, the selected bit is highlighted in the pattern bit line.

State ← Ser. Pattern
Toggles the logic state of the selected bit: 0 (low), 1 (high), or X (don't care).

Select Nibble ← Ser. Pattern
Selects four bits (half byte) for hexadecimal entry with "Value". The selected nibble is highlighted in the lower pattern line.

Value ← Ser. Pattern
Sets the hexadecimal value for the selected nibble.

11.2.4 SPI/SSPI Decode Results

You can enable the decoding in the "Protocol" main menu. "Decode" shows the decoded values below the waveforms in the format selected with "Display". Additionally, you can display the binary signal with "Bits".

See also: chapter 11.1.2, "Protocol - Common Settings", on page 149

Fig. 11-2: Decoded SPI signal

C1 = Clock (Clk)
C2 = Data
C3 = Chip Select (Cs)
blue results = completely decoded words
grey brackets = start and end of complete frame
red results = Incomplete word that is not completely contained in the acquisition. Change the horizontal scale, or move the"Time Reference" to get a longer acquisition.

Additionally, you can display and save a "Frame Table" containing decoded data: frame number, start time of the frame, source (line), data and state of the frame.

See also: chapter 11.1.5, "Frame Table: Decode Results", on page 154

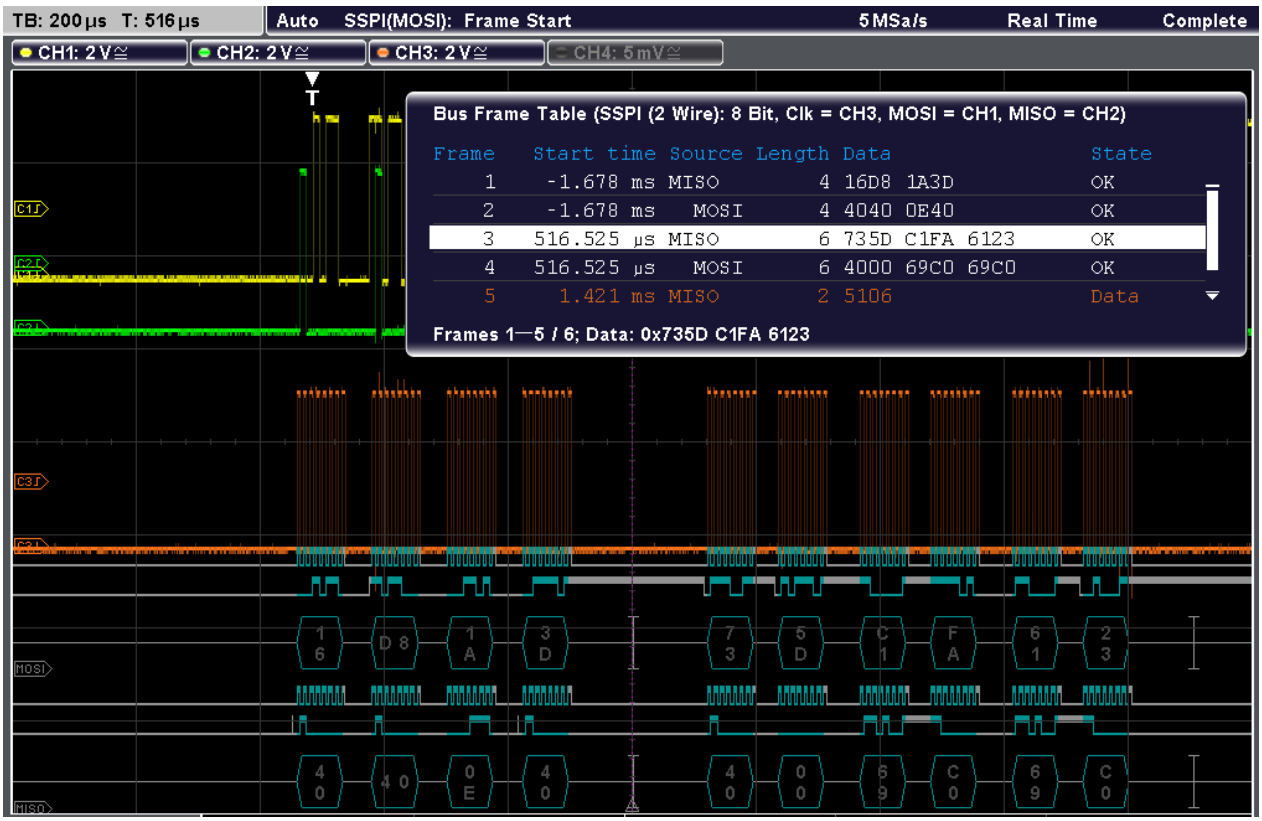
TB: 200 µs T: 516 µs
Auto SSPI(MOSI): Frame Start
5 MSa/s
Real Time
Complete
CH1: 2 V
CH2: 2 V
CH3: 2 V
CH4: 5 mV
Bus Frame Table (SSPI (2 Wire): 8 Bit, Clk = CH3, MOSI = CH1, MISO = CH2)
Frame Start time Source Length Data State
1 -1.678 ms MISO 4 16D8 1A3D OK
2 -1.678 ms MOSI 4 4040 0E40 OK
3 516.525 µs MISO 6 735D C1FA 6123 OK
4 516.525 µs MOSI 6 4000 69C0 69C0 OK
5 1.421 ms MISO 2 5106 Data
Frames 1—5 / 6; Data: 0x735D C1FA 6123
MOSI
MISO

Fig. 11-3: Decoded SSPI signal with frame table

Table 11-1: Content of the SPI/SSPI frame table

Column	Description
Start time	Time of the frame start in relation to the trigger point
Source	MISO or MOSI line
Length	Number of words in the frame
Data	Hexadecimal values of the data words
State	Overall state of the frame

Example:

In the figure above, the first two frames have four words each, the following two frames contain 6 words each. The fifth frame is incomplete.

Remote commands:

- `BUS<b>:SPI:FCOunt?` on page 381
  `BUS<b>:SPI:FRAME<n>:STATus?` on page 382
  `BUS<b>:SPI:FRAME<n>:STARt?` on page 382
  `BUS<b>:SPI:FRAME<n>:STOP?` on page 382
  `BUS<b>:SPI:FRAME<n>:DATA:MOSI?` on page 383
  `BUS<b>:SPI:FRAME<n>:DATA:MISO?` on page 383
  `BUS<b>:SPI:FRAME<n>:WCOunt?` on page 383

BUS<b>:SPI:FRAME<n>:WORD<o>:STARt? on page 384
BUS<b>:SPI:FRAME<n>:WORD<o>:STOP? on page 384
BUS<b>:SPI:FRAME<n>:WORD<o>:MOSI? on page 385
BUS<b>:SPI:FRAME<n>:WORD<o>:MISO? on page 385

11.3 I²C (Option R&S RTM-K1)

The Inter-Integrated Circuit is a simple, lowbandwidth, low-speed protocol used for communication between on-board devices, for example, in LCD and LED drivers, RAM, EEPROM, and others.

11.3.1 The I²C Protocol

This chapter provides an overview of protocol characteristics, data format, address types and trigger possibilities. For detailed information, read the "I2C-bus specification and user manual" available on the NXP manuals web page at http://www.nxp.com/.

I²C characteristics

Main characteristics of I²C are:

- Two-wire design: serial clock (SCL) and serial data (SDA) lines
- Master-slave communication: the master generates the clock and addresses the slaves. Slaves receive the address and the clock. Both master and slaves can transmit and receive data.
- Addressing scheme: each slave device is addressable by a unique address. Multiple slave devices can be linked together and can be addressed by the same master.
- Read/write bit: specifies if the master will read (=1) or write (=0) the data.
- Acknowledge: takes place after every byte. The receiver of the address or data sends the acknowledge bit to the transmitter.

The R&S RTM supports all operating speed modes: high-speed, fast mode plus, fast mode, and standard mode.

Data transfer

The format of a simple I²C message (frame) with 7 bit addressing consists of the following parts:

- Start condition: a falling slope on SDA while SCL is high
- 7-bit address of the slave device that either will be written to or read from
- R/W bit: specifies if the data will be written to or read from the slave
- ACKnowledge bits: is issued by the receiver of the previous byte if the transfer was successful
  Exception: At read access, the master terminates the data transmission with a NACK bit after the last byte.
- Data: a number of data bytes with an ACK bit after every byte

- Stop condition: a rising slope on SDA while SCL is high

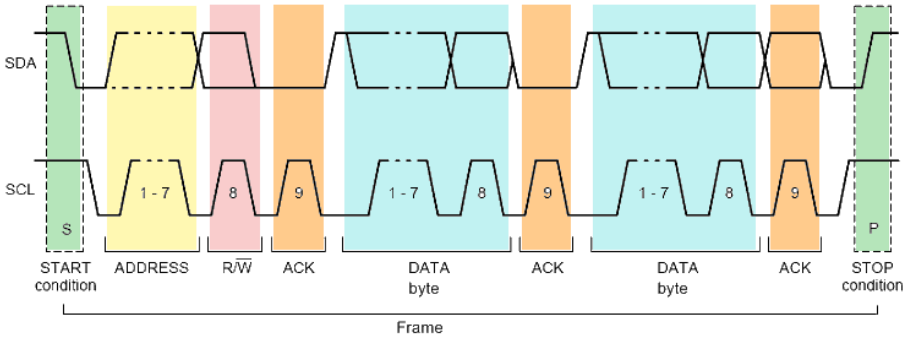

Fig. 11-4: I2C write access with 7-bit address

Address types: 7-bit and 10-bit

Slave addresses can be 7 or 10 bits long. A 7-bit address requires one byte, 7 bits for the address followed by the R/W bit.

A 10-bit address for write access requires two bytes: the first byte starts with the reserved sequence 11110, followed by the two MSB of the address and the write bit. The second byte contains the remaining 8 LSB of the address. The slave acknowledges each address byte.

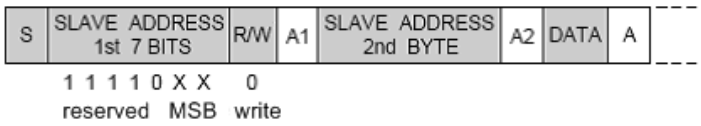

Fig. 11-5: 10-bit address, write access

A 10-bit address for read access requires three bytes. The first two bytes are identical to the write access address. The third byte repeats the address bits of the first byte and sets the read bit.

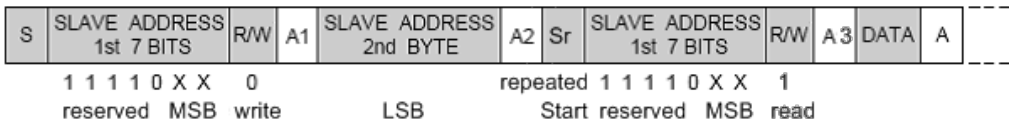

Fig. 11-6: 10-bit address, read access

Trigger

The R&S RTM can trigger on various parts of I²C messages. The data and clock lines must be connected to the input channels, triggering on math and reference waveforms is not possible.

You can trigger on:

- Start or stop condition
- Repeated start condition
- Transfer direction (read or write)

- Bytes with missing acknowledge bit
- Specific slave address
- Specific data pattern in the message

11.3.2 I²C Configuration

11.3.2.1 Configuring I²C

The configuration of the I²C is simple - only assign the two lines to input channels.

1. Press the PROTOCOL LOGIC key on the front panel.
2. If the "Logic" menu is displayed, press "Protocol".
3. Press the "Bus Type" softkey and select "I2C".
4. Press "Configuration".
5. Press "Clock SCL" and select the channel connected to the clock line.
6. Press "Data SDA" and select the channel connected to the data line.
7. Press "Find level", or set the threshold manually for each channel.
   See: "To set the logic threshold for analog channels" on page 148

   Now you can disply the decoded signal and the frame table with results.

The display of the decoded data is described in "To configure decoding and data display" on page 149.

11.3.2.2 I²C Configuration Settings

Clock SCL....167
Data SDA....167
Find Level....168

Clock SCL
Sets the input channel to which the clock line is connected.

If the MSO option R&S RTM-B1 is installed, digital channels can also be used as source.

Remote command:
`BUS<b>:I2C:CLOCk:SOURce` on page 389

Data SDA
Sets the input channel to which the data line is connected.

If the MSO option R&S RTM-B1 is installed, digital channels can also be used as source.

Remote command:
`BUS<b>:I2C:DATA:SOURce` on page 389

Find Level
The instrument analyzes all lines that are configured for the selected bus and sets the threshold for digitization of analog signals for each channel. If no level can be found, the existing value remains unchanged, and you can set the thresholds manually in the channel menu: CH N > "More" (page 2) > "Threshold".

See: "Threshold" on page 31

"Find Level" is not relevant for digital channels (MSO option R&S RTM-B1). Thresholds for digital channels are set in the "Logic > Threshold" menu.

Remote command:
`CHANnel<m>:THReshold:FINDlevel` on page 379

11.3.3 I²C Trigger

- Triggering on I²C 168
- I²C Trigger Settings.....169

11.3.3.1 Triggering on I²C

Prerequisites: The I²C interface is configured. After configuration, the trigger type "Protocol (I2C)" is available. See: chapter 11.3.2.1, "Configuring I²C ", on page 167.

Triggers are only available if "Decode" is enabled.

1. Press the SETUP key in the trigger area of the front panel.
2. Select the "Trigger Type": "Protocol (I2C)".
3. Press "Setup".
4. Press the softkey of the required trigger condition:
   - "Start": begin of the message
   - "Stop": end of the message
   - "Restart": repeated start condition
   - "Acknowledge": transfer of a data byte is not acknowledged
   - "Read/Write": complex trigger condition containing read or write access of the master, slave address, or/and a bit pattern in the message
5. If "Read/Write" is selected, press the softkey again and define the condition:
   a) Press "Master" and select read or write access of the master.
   b) Configure the "Address" of the slave:
      - Select the "Address Length", 7 bit or 10 bit.
      - Press "Slave Address" and turn the navigation knob to set the address.

      If the address is not relevant for your trigger condition, set it to "0xX" (any address).

c) Press "Data Setup" to specify data bytes of the message, and/or to a serial pattern.
d) Set the "Byte Offset", the number of bytes to be ignored before the first byte of interes.t
e) Set the "Number of Bytes" contained in the pattern.
f) Enter the pattern, either as binary input, or as hexadecimal input:

- For binary input, press "Bit" and enter the bit number to be set. The bits are counted inside the selected bytes, the selected bit is highlighted in the pattern bit line. Then enter the "State" of this bit: 0, 1, or X (don't care).
  Repeat these settings until all bit states are defined.
- For hexadecimal input, press "Byte" and select the byte to be set. The selected byte is highlighted in the lower pattern line. Then press "Value" and turn the navigation knob to change the bits.
  Repeat these settings until all bytes are defined.

If the data is not relevant for your trigger condition, set all data bytes to "0xXX".

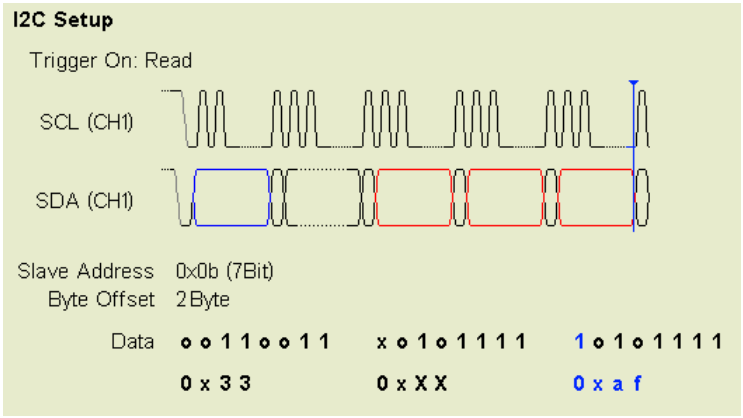
I2C Setup
Trigger On: Read
SCL (CH1)
SDA (CH1)
Slave Address 0x0b (7Bit)
Byte Offset 2Byte
Data
0 0 1 1 0 0 1 1
x 0 1 0 1 1 1 1
1 0 1 0 1 1 1 1
0 x 3 3
0 x X X
0 x a f

11.3.3.2 I²C Trigger Settings

Triggers are only available if "Decode" is enabled.

Start....170
Stop....170
Restart....170
~Acknowledge....170
Read/Write....170
└ Master....171
└ Symbolic ID....171

└ Address Length....171
└ Slave Address....171
└ Data Setup....171
└ Byte Offset....172
└ Number of Bytes....172
└ Bit....172
└ State....172
└ Byte....172
└ Value....172

Start
Sets the trigger to the start of the message. The start condition is a falling slope on SDA while SCL is high.

Remote command:
`TRIGger:A:I2C:PATTern` on page 391 (`STARt`)

Stop
Sets the trigger to the end of the message. The stop condition is a rising slope on SDA while SCL is high.

Remote command:
`TRIGger:A:I2C:PATTern` on page 391 (`STOP`)

Restart
Sets the trigger to a repeated start - when the start condition occurs without previous stop condition. This can happen when a master sends multiple messages without releasing the bus.

Remote command:
`TRIGger:A:I2C:PATTern` on page 391 (`RESTart`)

~Acknowledge
Missing acknowledge: the instrument triggers if the slave does not send the acknowledge bit. Acknowledging takes place after every byte. If the transfer failed, at the moment of the acknowledge bit the SDA line is on high level during the high period of the clock pulse.

Remote command:
`TRIGger:A:I2C:PATTern` on page 391 (`MACKnowledge`)

Read/Write
Sets the trigger to a read or write access of the master, to an address, or/and to a bit pattern in the message. The trigger condition is specified in the submenus. All submenu settings together create the trigger condition. If you want to trigger on a specific parameter, make sure to set all other settings to "any".

If a label list with node names was loaded and applied in the bus configuration, you can select simply the "Symbolic ID" from the list instead of entering the numeric identifier.

Remote command:
TRIGger:A:I2C:PATTern on page 391 (PATTern)

Master ← Read/Write
Toggles the trigger condition between Read and Write access of the master. The R/W bit is 8th bit of the first address byte of a frame. The selected condition is displayed in the I2C Settings: "Trigger On".

Remote command:
TRIGger:A:I2C:ACCess on page 390

Symbolic ID ← Read/Write
If a label list with node names was loaded and applied in the bus configuration, you can select simply the node name from the list instead of entering the numeric identifier.

The instrument trriggers on the identifier of the selected node.

Address Length ← Read/Write
Toggles the lenght of the slave address: 7 bit or 10 bit.

Remote command:
TRIGger:A:I2C:AMODe on page 390

Slave Address ← Read/Write
Sets the address of the slave device in hex. You can set a precise address, or trigger on any address with "0xXX" (7Bit address) or "0xXXX" (10Bit address). X cannot be assigned to a specified bit

Remote command:
TRIGger:A:I2C:ADDRess on page 391

Data Setup ← Read/Write
Opens a submenu to set the trigger on specified data bytes of the message, and/or to a serial pattern.

Remote command:
TRIGger:A:I2C:PATTern on page 391

Byte Offset ← Data Setup ← Read/Write
Sets the number of bytes before the first byte of interest, relating to the end of the address bytes. These offset bytes are ignored.

Remote command:
`TRIGger:A:I2C:POFFset` on page 392

Number of Bytes ← Data Setup ← Read/Write
Sets the number of bytes you want to trigger on. Maximum 3 bytes are possible.

Remote command:
`TRIGger:A:I2C:PLENgth` on page 391

Bit ← Data Setup ← Read/Write
Selects the bit number inside the selected bytes for binary pattern input. For the selected bit, "State" is to be set. the selected bit is highlighted in the "Data" bit line.

State ← Data Setup ← Read/Write
Toggles the logic state of the selected bit: 0 (low), 1 (high), or X (don't care).

Byte ← Data Setup ← Read/Write
Selects a byte for hex input with "Value". The selected byte is highlighted in the "Data" hex line.

Value ← Data Setup ← Read/Write
Sets the hexadecimal value for the selected byte.

If the data is not relevant for your trigger condition, set all data bytes to "0xXX".

11.3.4 I²C Label List

Label lists are protocol-specific. An I²C PTT file contains three values for each address:

- "Type": address type, 7-bit or 10-bit long
- "ID / Addr": hexadecimal address value
- "Symbolic label": name of the address, specifiing its function in the bus network.

Example: I²C PTT file

```
# ------------------------------------------------------------------------------
@FILE_VERSION  = 1.00
@PROTOCOL_NAME = i2c
# ------------------------------------------------------------------------------
# Labels for I2C protocol
#   Column order: Identifier type, Identifier value, Label
# ------------------------------------------------------------------------------
7,0x1E,Voltage
7,0x38,Pressure
7,0x2A,Temperature
7,0x16,Speed
7,0x76,Acceleration
7,0x07,HighSpeed_Master_0x3
```

```
7,0x51,EEPROM
10,0x3A2,DeviceSetup
10,0x1A3,GatewayStatus
10,0x06E,LeftSensor
# ------------------------------------------------------------------------------
```

Label list: I2C (Imported on: 2012-04-05; 12:31)

Symbolic label	ID / Addr
Acceleration	0x76
DeviceSetup	0x3A2
EEPROM	0x51
GatewayStatus	0x1A3
HighSpeed_Master_0x3	0x07
LeftSensor	0x06E
Pressure	0x38
Speed	0x16
Temperature	0x2A
Voltage	0x1E

Fig. 11-7: Label list for I²C

For general information, see chapter 11.1.4, "Label List", on page 151.

11.3.5 I²C Decode Results

You can enable the decoding in the "Protocol" main menu. "Decode" shows the decoded values below the waveforms in the format selected with "Display". Additionally, you can display the binary signal with "Bits".

See also: chapter 11.1.2, "Protocol - Common Settings", on page 149

Additionally, you can display and save a "Frame Table" containing decoded data: frame number, start time of the frame, access type. ID, data and state of the frame.

See also: chapter 11.1.5, "Frame Table: Decode Results", on page 154

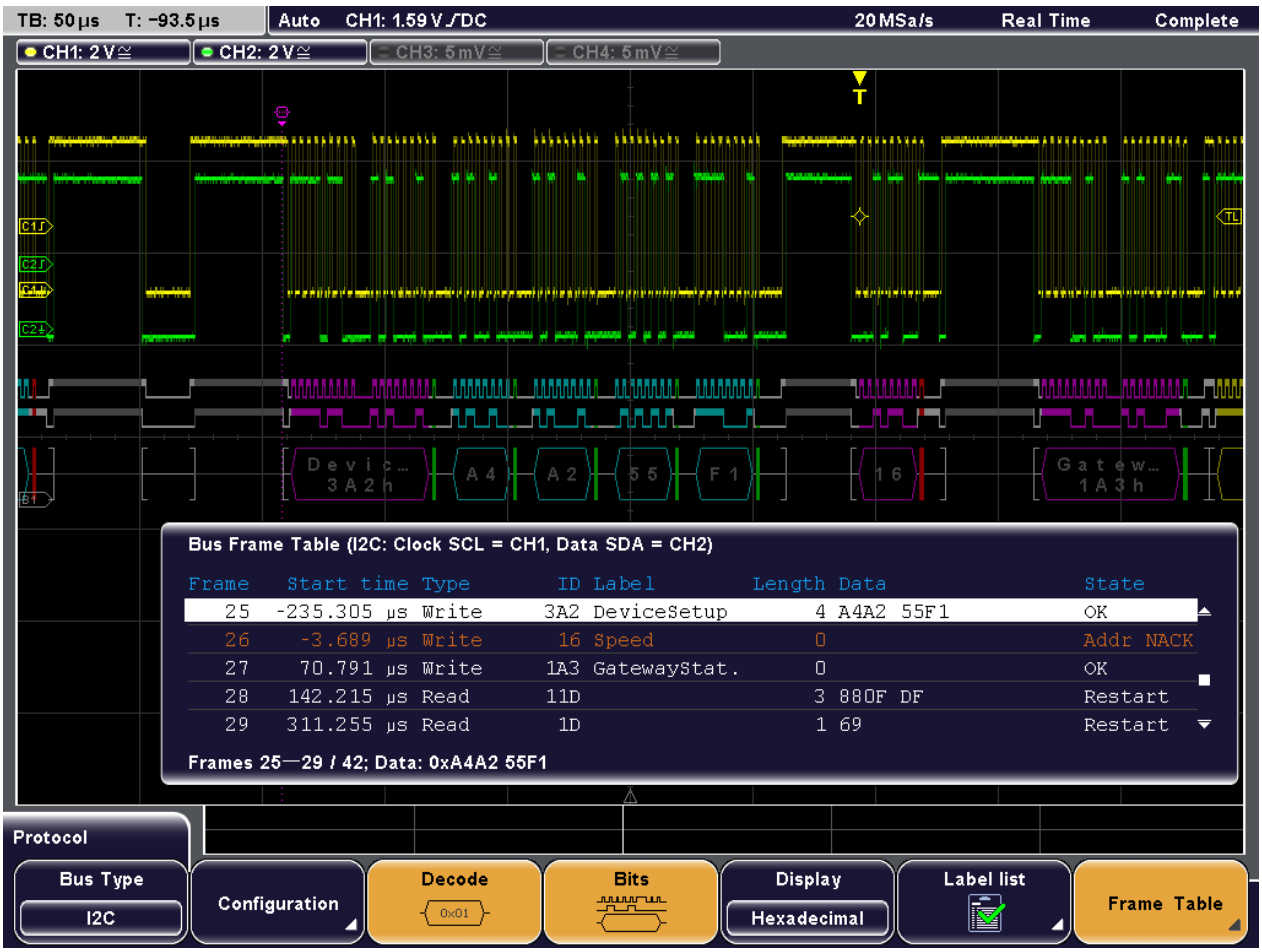
TB: 50 µs T: -93.5 µs
Auto CH1: 1.59 V ⎍DC
20 MSa/s Real Time Complete
CH1: 2 V
CH2: 2 V
CH3: 5 mV
CH4: 5 mV
Bus Frame Table (I2C: Clock SCL = CH1, Data SDA = CH2)
Frame Start time Type ID Label Length Data State
25 -235.305 µs Write 3A2 DeviceSetup 4 A4A2 55F1 OK
26 -3.689 µs Write 16 Speed 0 Addr NACK
27 70.791 µs Write 1A3 GatewayStat. 0 OK
28 142.215 µs Read 11D 3 880F DF Restart
29 311.255 µs Read 1D 1 69 Restart
Frames 25—29 / 42; Data: 0xA4A2 55F1
Protocol
Bus Type
I2C
Configuration
Decode
Bits
Display
Hexadecimal
Label list
Frame Table

Fig. 11-8: Decoded and binary I2C signal, and frame table with decode results

gray brackets = start and end of the frame
violet = address
blue = correct data words
green = acknowledge bit, ok
red = missing acknowledge bit, or other error

Table 11-2: Content of the I²C frame table

Column	Description
Start time	Time of the frame start in relation to the trigger point
Type	Value of the R/W bit, read or write access
ID	Hexadecimal value of the address
Label	Symbolic label, available if a label list was loaded and applied
Length	Number of words in the frame
Data	Hexadecimal values of the data words
State	Overall state of the frame

Remote commands:

- BUS<b>:I2C:FCOunt? on page 392
  BUS<b>:I2C:FRAMe<n>:DATA? on page 392
  BUS<b>:I2C:FRAMe<n>:STATus? on page 393
  BUS<b>:I2C:FRAMe<n>:STARt? on page 393
  BUS<b>:I2C:FRAMe<n>:STOP? on page 394
  BUS<b>:I2C:FRAMe<n>:AACCess? on page 394
  BUS<b>:I2C:FRAMe<n>:ACCess? on page 394
  BUS<b>:I2C:FRAMe<n>:ACOMplete? on page 395
  BUS<b>:I2C:FRAMe<n>:ADBStart? on page 395
  BUS<b>:I2C:FRAMe<n>:ADDRess? on page 395
  BUS<b>:I2C:FRAMe<n>:ADEVice? on page 396
  BUS<b>:I2C:FRAMe<n>:AMODe? on page 396
  BUS<b>:I2C:FRAMe<n>:ASTart? on page 396
  BUS<b>:I2C:FRAMe<n>:BCOunt? on page 397
  BUS<b>:I2C:FRAMe<n>:BYTE<o>:ACCess? on page 397
  BUS<b>:I2C:FRAMe<n>:BYTE<o>:ACKStart? on page 397
  BUS<b>:I2C:FRAMe<n>:BYTE<o>:COMPlete? on page 398
  BUS<b>:I2C:FRAMe<n>:BYTE<o>:STARt? on page 398
  BUS<b>:I2C:FRAMe<n>:BYTE<o>:VALue? on page 398

11.4 UART/RS-232 Interface (Option R&S RTM-K2)

11.4.1 The UART / RS232 Interface

The Universal Asynchronous Receiver/Transmitter UART converts a word of data into serial data, and vice versa. It is the base of many serial protocols like of RS-232. The UART uses only one line, or two lines for transmitter and receiver.

Data transfer

The data is transmitted in symbols, also referred to as words or characters. Each symbol consists of a start bit, several data bits, an optional parity bit, and one or more stop bits. Several symbols can form a frame, or package. The end of a frame is marked by a pause between two symbols.

Start	Data0	Data1	Data2	Data3	Data4	[Data5]	[Data6]	[Data7]	[Data8]	[Parity]	Stop

Fig. 11-9: Bit order in a UART word (symbol)

- The start bit is a logic 0.
- The stop bits and the idle state are always logic 1.

The UART protocol has no clock for synchronization. The receiver synchronizes by means of the start and stop bits, and the bit rate that must be known to the receiver.

Trigger

The R&S RTM can trigger on specified parts of UART serial signals:

- Start bit
- Frame start
- A specified symbol
- Parity errors, and breaks
- Frame errors
- A serial pattern at any or a specified position

11.4.2 UART/RS-232 Configuration

11.4.2.1 Configuring UART/RS-232 Interfaces

To configure the UART interface, you assign the channels to the RX an (optionally) TX lines, set the active state for each line and set some protocol-specific parameters.

1. Press the PROTOCOL LOGIC key on the front panel.
2. If the "Logic" menu is displayed, press "Protocol".
3. Press the "Bus Type" softkey and select "UART".
4. Press "Configuration".
5. Press "RX" and select the channel connected to the receiver line.
6. Press "TX" and select the channel connected to the transmitter line.
7. Set the "Active" state, "Parity" bit and the number of "Stop Bits".
8. Press "More".
9. Enter the "Symbol size".
10. Enter the bit rate:
    - For a standard bit rate, select the "Defined Bit Rate".
    - For a user-defined bit rate, press "User Bit Rate" and enter the value
11. Set the "Idle Time" between two frames.

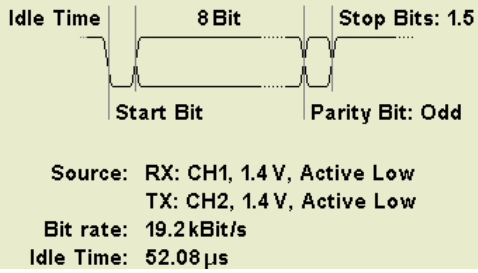

12. Press "Find level", or set the threshold manually for each channel.
    See: "To set the logic threshold for analog channels" on page 148

    Now you can disply the decoded signal and the frame table with results.

The display of the decoded data is described in "To configure decoding and data display" on page 149.

11.4.2.2 UART Configuration Settings

Access: PROTOCOL > "Bus type" = "UART" "Configuration"

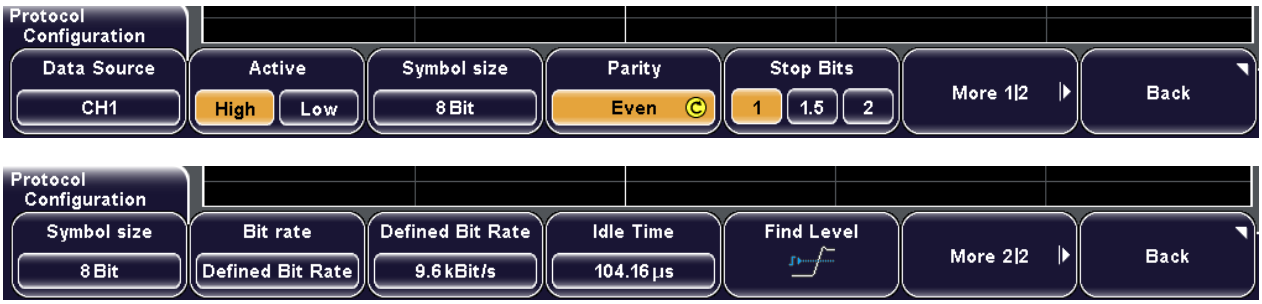

Data Source....177
Active....178
Parity....178
Stop Bits....178
Symbol Size....178
Bit Rate....178
Idle Time....178
Find Level....179

Data Source
Select the input channels of the data line.

If the MSO option R&S RTM-B1 is installed, digital channels can also be used as source.

Remote command:
`BUS<b>:UART:DATA:SOURce` on page 0

Active
Defines the logic levels of the bus. The idle state corresponds to a logic 1, and the start bit to a logic 0. Active-high (high=1) is used, for example, for control signals, while active-low (low=1) is defined for data lines (RS-232).

Remote command:
`BUS<b>:UART:DATA:POLarity` on page 400
`BUS<b>:UART:POLarity` on page 400

Parity
Defines the optional parity bit that is used for error detection.

"None"	No parity bit is used.
"Even"	The parity bit is set to "1" if the number of "1"s in a given set of bits is odd (not including the parity bit).
"Odd"	The parity bit is set to "1" if the number of "1"s in a given set of bits is even (not including the parity bit).

Remote command:
`BUS<b>:UART:PARity` on page 401

Stop Bits
Sets the number of stop bits: 1; 1.5 or 2 stop bits are possible.

Remote command:
`BUS<b>:UART:SBIT` on page 401

Symbol Size
Sets the number of data bits in a word (symbol) in a range from 5 to 9 bits.

Remote command:
`BUS<b>:UART:SSIZe` on page 400

Bit Rate
Sets the number of transmitted bits per second.

"Defined Bit Rate"	Select a standard bit rate value from the list.
"User Bit Rate"	Enter a user defined value.

Remote command:
`BUS<b>:UART:BAUDrate` on page 401

Idle Time
Sets the minimal time between two frames – between the stop bit of the last word in a frame and the start bit of the first word in the next frame.

Remote command:
`BUS<b>:UART:BITime` on page 402

Find Level
The instrument analyzes all lines that are configured for the selected bus and sets the threshold for digitization of analog signals for each channel. If no level can be found, the existing value remains unchanged, and you can set the thresholds manually in the channel menu: CH N > "More" (page 2) > "Threshold".

See: "Threshold" on page 31

"Find Level" is not relevant for digital channels (MSO option R&S RTM-B1). Thresholds for digital channels are set in the "Logic > Threshold" menu.

Remote command:
`CHANnel<m>:THReshold:FINDlevel` on page 379

11.4.3 UART/RS-232 Trigger

- Triggering on UART/RS-232 Interfaces.....179
- UART Trigger Settings.....180

11.4.3.1 Triggering on UART/RS-232 Interfaces

Prerequisites: The UART interface is configured. After configuration, the trigger type "Protocol (UART)" is available. See: chapter 11.4.2.1, "Configuring UART/RS-232 Interfaces", on page 176.

Triggers are only available if "Decode" is enabled.

1. Press the SETUP key in the trigger area of the front panel.
2. Select the "Trigger Type": "Protocol (UART)".
3. Press "Source" and select RX or TX as trigger source.
4. Press "Back".
5. Press "Setup".
6. Press the softkey of the required trigger condition:
   - "Start Bit", or "Frame Start": next start bit, or first start bit after idle time
   - "Symbol<n>": frame number in a data stream
   - "Any Symbol": pattern of the data bits anywhere in the data stream
   - "Pattern": serial pattern of one, two or three symbols at a defined position in the data stream
   - "Parity Error"
   - "Frame Errror"
   - "Break"
7. If "Any Symbol" is selected, press the softkey again and define the symbol pattern, either as binary input, or as hexadecimal input:

- For hex entry, select "Value" and turn the navigation knob to change the bits.
- For binary input, press "Select Bit" and enter the data bit number to be set. Enter the "State" of this bit: 0, 1, or X (don't care).
  Repeat these settings until all bit states are defined.

8. If "Pattern" is selected, press the softkey again and define the pattern:
   a) Set the "Symbol Offset", the number of symbols to be ignored before the pattern starts.
   b) Set the "Number of Symbols" contained in the pattern.
   c) Enter the pattern, either as binary input, or as hexadecimal input:
      - For hexadecimal input, press "Select Symbol" repeatedly to select the symbol to be set. The selected symbol is highlighted in the hex pattern line. Then press "Value" and turn the navigation knob to change the bits.
        Repeat these settings until all symbols are defined.
      - For binary input, press "Select Symbol" until the required symbol is marked in the pattern hex line. Then press "Select Bit" and enter the data bit number to be set. Enter the "State" of this bit: 0, 1, or X (don't care).
        Repeat these settings until all bit states of all symbols are defined.

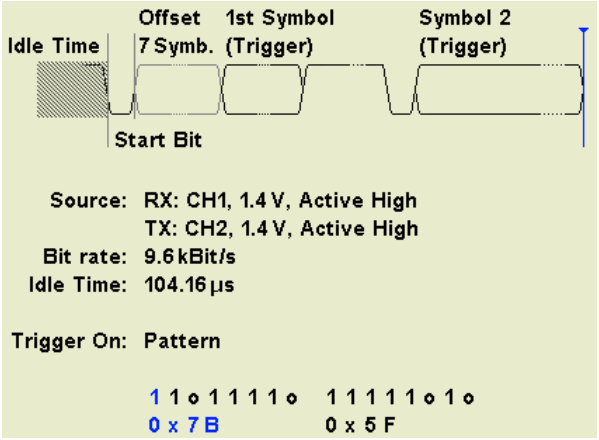

11.4.3.2 UART Trigger Settings

The complete UART trigger is configured in the "Source" and "Setup" menus.

Triggers are only available if "Decode" is enabled.

- UART Trigger Source....181
- UART Trigger Setup....181

UART Trigger Source

Access: TRIGGER SETUP > "Trigger Type" = "Protocol (UART)" > "Source"

RX, TX
Select one of the lines as trigger source.

Remote command:
`TRIGger:A:SOURce:UART` on page 402

UART Trigger Setup

Access: TRIGGER SETUP > "Trigger Type" = "Protocol (UART)" > "Setup"

Start Bit....181
Frame Start....182
Symbol <n>....182
Any Symbol....182
Pattern....182
└ Symbol Offset....182
└ Number of Symb....182
└ Select Bit....182
└ State....182
└ Select Symbol....183
└ Value....183
Parity Error....183
Frame Error....183
Break....183

Start Bit
Triggers on a start bit. The start bit is the first logical 0 after a stop bit.

Remote command:
`TRIGger:A:UART:MODE` on page 402 `(SBIT)`

Frame Start
Triggers on the begin of a frame. The frame start is the first start bit after the idle time.

Remote command:
`TRIGger:A:UART:MODE` on page 402 `(BSTart)`

Symbol <n>
Sets the trigger to the specified symbol - the n-th word - in a frame (package).

Remote command:
`TRIGger:A:UART:MODE` on page 402 `(NTHSymbol)`

Any Symbol
Opens a submenu to trigger if a pattern occurs in a symbol at any position in a frame.

You can enter the pattern in binary or hex, the functions are the same as for "Pattern" setting:

- "Select Bit" on page 182
- "State" on page 182
- "Value" on page 183

Remote command:
`TRIGger:A:UART:MODE` on page 402 `(SYMBol)`

Pattern
Opens a submenu to set the trigger on a serial pattern at a defined position in the frame. The pattern can include several subsequent symbols.

Remote command:
`TRIGger:A:UART:MODE` on page 402 `(PATTern)`
`TRIGger:A:UART:PATTern` on page 403

Symbol Offset ← Pattern
Sets the number of symbols to be ignored before the serial pattern.

Remote command:
`TRIGger:A:UART:POFFset` on page 404

Number of Symb. ← Pattern
Defines the length of the pattern - how many symbols build it up.

Remote command:
`TRIGger:A:UART:PLENgth` on page 403

Select Bit ← Pattern
Selects the bit number inside the selected symbol for binary pattern input.

State ← Pattern
Toggles the logic state of the selected bit: 0 (low), 1 (high), or X (don't care).

Select Symbol ← Pattern
Selects the symbol for binary or hex input.

Value ← Pattern
Sets the hexadecimal value for the selected symbol by turning the navigation knob.

Parity Error
Triggers on a parity error indicating a transmission error.

Remote command:
`TRIGger:A:UART:MODE` on page 402 `(PERRor)`

Frame Error
Triggers on a frame error.

Remote command:
`TRIGger:A:UART:MODE` on page 402 `(FERRor)`

Break
Triggers if a start bit is not followed by a stop bit, the data line remains at logic 0 for longer than a UART word.

Remote command:
`TRIGger:A:UART:MODE` on page 402 `(BREak)`

11.4.4 UART/RS-232 Decode Results

You can enable the decoding results in the "Protocol" main menu. "Decode" shows the decoded values below the waveforms in the format selected with "Display". Additionally, you can display the binary signal with "Bits".

See also: chapter 11.1.2, "Protocol - Common Settings", on page 149

Additionally, you can display and save a "Frame Table" containing decoded data: frame number, start time of the frame, data and state of the frame.

See also: chapter 11.1.5, "Frame Table: Decode Results", on page 154

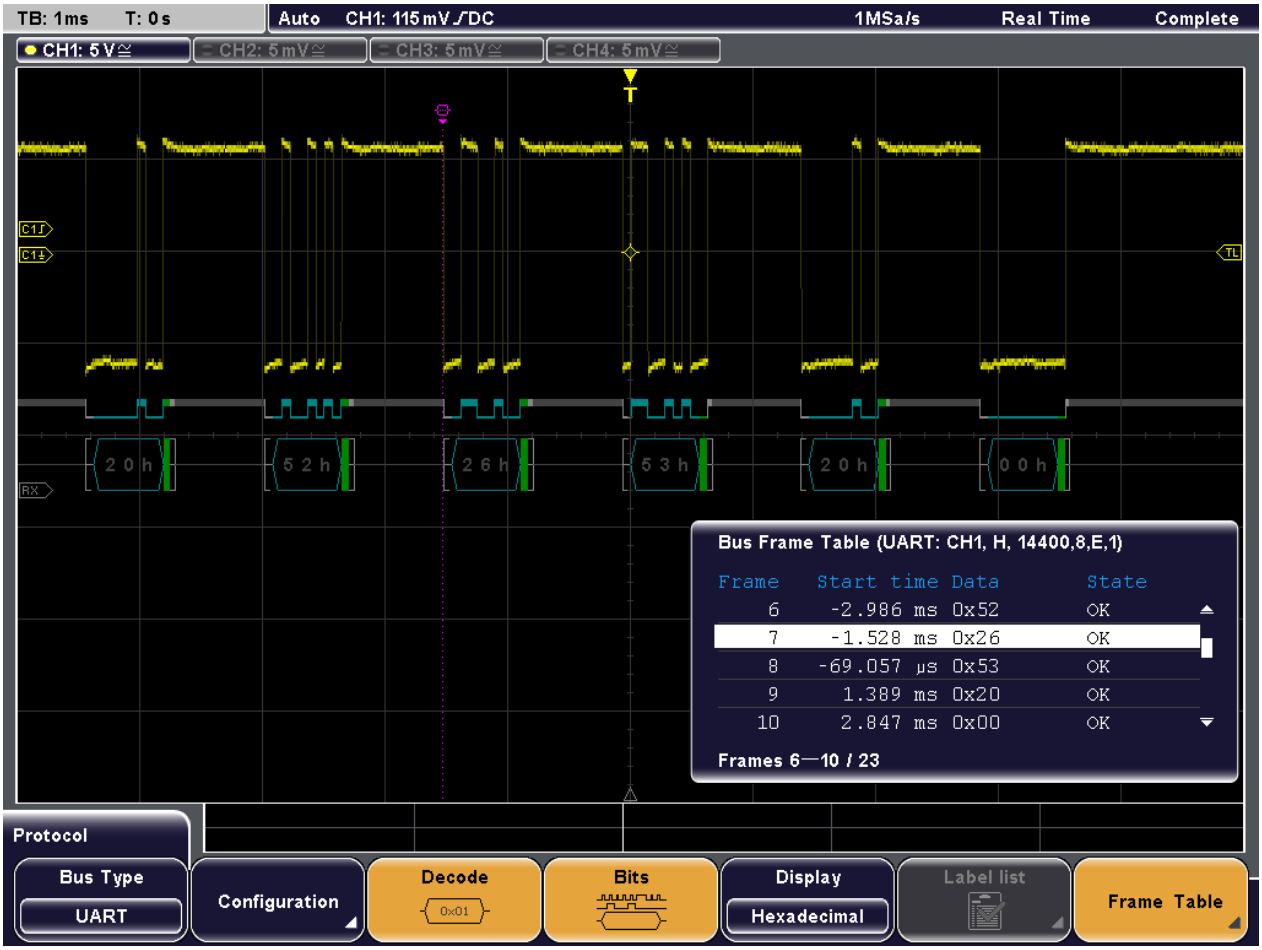

Fig. 11-10: Decoded UART signal

C1 = Data source
blue results = completely decoded words
grey brackets = start and end of complete frames
green results = correct parity bits
red results = Errors or incomplete word that is not completely contained in the acquisition. Change the horizontal scale, or move the"Time Reference" to get a longer acquisition.

Example:

The figure above shows five frames of a UART signal with one source line.

Table 11-3: Content of the UART frame table

Column	Description
Start time	Time of the frame start in relation to the trigger point
Data	Hexadecimal values of the data words
State	Overall state of the frame

Remote commands:

- `BUS<b>:UART:RX:FCOunt?` on page 0

- BUS<b>:UART:RX:FRAMe<n>:WCOunt? on page 404
- BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STATe? on page 0
- BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STARt? on page 0
- BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STOP? on page 0
- BUS<b>:UART:RX:FRAMe<n>:WORD<o>:VALue? on page 0

11.5 CAN (Option R&S RTM-K3)

CAN is the Controller Area Network, a bus system used within automotive network architecture.

11.5.1 CAN Configuration

Access: PROTOCOL > "Bus type" = "CAN" > "Configuration"

Data....185
Type....185
Sample point....186
Bit rate....186
Find Level....186

Data
Sets the source of the data line. All channel waveforms can be used.

If the MSO option R&S RTM-B1 is installed, digital channels can also be used as source.

Remote command:
BUS<b>:CAN:DATA:SOURce on page 406

Type
Selects the CAN-High or CAN-Low line. CAN uses both lines for differential signal transmission.

If you measure with a differential probe, connect the probe to both CAN-H and CAN-L lines, and select the data "Type" "CAN-H".

If you use a single-ended probe, connect the probe to either CAN_L or CAN_H, and select the data type accordingly.

Remote command:
BUS<b>:CAN:TYPE on page 406

Sample point
Sets the position of the sample point within the bit in percent of the nominal bit time. The sample point divides the nominal bit period into two distinct time segments, which are used for resynchronization of the clock.

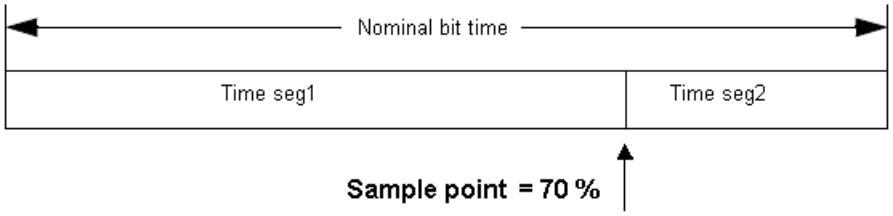

The CAN bus interface uses an asynchronous transmission scheme. The standard specifies a set of rules to resynchronize the local clock of a CAN node to the message.

Remote command:
`BUS<b>:CAN:SAMPlepoint` on page 406

Bit rate
Sets the number of transmitted bits per second. The maximum bit rate for High Speed CAN is 1 Mbit/s. The bit rate is uniform and fixed for a given CAN bus.

To select a bit rate from the list of predefined values, set "Bit rate" to "Defined Bit Rate", and then select the value with "Predefined".

To set another value, set "Bit rate" to "User Bit Rate", and then enter the value with "User".

Remote command:
`BUS<b>:CAN:BITRate` on page 407

Find Level
The instrument analyzes all lines that are configured for the selected bus and sets the threshold for digitization of analog signals for each channel. If no level can be found, the existing value remains unchanged, and you can set the thresholds manually in the channel menu: CH N > "More" (page 2) > "Threshold".

See: "Threshold" on page 31

"Find Level" is not relevant for digital channels (MSO option R&S RTM-B1). Thresholds for digital channels are set in the "Logic > Threshold" menu.

Remote command:
`CHANnel<m>:THReshold:FINDlevel` on page 379

11.5.2 CAN Trigger Settings

Access: SETUP (Trigger) > "Trigger type" = "Protocol (CAN)" > "Setup"

Start of frame....187
End of frame....187
Frame <type>....187
└ Error....187
└ Overload....188
└ Data....188
└ Remote....188
└ Data or remote....188
Error <type>....188
└ Stuff bit....188
└ Form....188
└ Acknowledge....188
└ CRC....189
Identifier....189
└ Frame type....189
└ Symbolic ID....189
└ Identifier Setup....189
└ ID type....190
└ Compare....190
└ Bit....190
└ State....190
└ Byte....190
└ Value....190
Identifier and data....190
└ Data Setup....190
└ Data Length....191

Start of frame
Triggers on the first edge of the dominant SOF bit (synchronization bit).

Remote command:
`TRIGger:A:CAN:TYPE` on page 407 (`STOFrame`)

End of frame
Triggers on the end of the frame (7 recessive bits).

Remote command:
`TRIGger:A:CAN:TYPE` on page 407 (`EOFrame`)

Frame <type>
Selects the frame type to be triggered on. The selected frame type is indicated in the softkey name.

Remote command:
`TRIGger:A:CAN:TYPE` on page 407 (`FTYPe`)
`TRIGger:A:CAN:FTYPe` on page 408

Error ← Frame <type>
An error frame is sent by a node that has detected an error.

Overload ← Frame <type>
An overload frame is sent by a node that needs a delay between data and/or remote frames.

Data ← Frame <type>
Frame for data transmission.

The identifier format is also considered, see "ID type" on page 190.

Remote ← Frame <type>
Data: Frame for data transmission.

A remote frame initiates the transmission of data by another node. The frame format is the same as of data frames but without the data field.

The identifier format is also considered, see "ID type" on page 190.

Data or remote ← Frame <type>
Triggers on remote frames and on data frames.

The identifier format is also considered, see "ID type" on page 190.

Error <type>
Identifies various errors in the frame. You can select one or more error types as trigger condition.

The first key press enables the "Error" trigger type, the second opens the "Error" menu.

Remote command:
`TRIGger:A:CAN:TYPE` on page 407 (`ERRCondition`)

Stuff bit ← Error <type>
The frame segments Start Of Frame, Arbitration Field, Control Field, Data Field and CRC Sequence are coded by the bit stuffing method. The transmitter automatically inserts a complementary bit into the bit stream when it detects five consecutive bits of identical value in the bit stream to be transmitted. A stuff error occurs when the 6th consecutive equal bit level in the mentioned fields is detected.

Remote command:
`TRIGger:A:CAN:BITSterror` on page 410

Form ← Error <type>
A form error occurs when a fixed-form bit field contains one or more illegal bits.

Remote command:
`TRIGger:A:CAN:FORMerror` on page 410

Acknowledge ← Error <type>
An acknowledgement error occurs when the transmitter does not receive an acknowledgment - a dominant bit during the Ack Slot.

Remote command:
`TRIGger:A:CAN:ACKerror` on page 410

CRC ← Error <type>
CAN uses the Cyclic Redundancy Check, which is a complex checksum calculation method. The transmitter calculates the CRC and sends the result in the CRC sequence. The receiver calculates the CRC in the same way. A CRC error occurs when the calculated result differs from the received value in the CRC sequence.

Remote command:
`TRIGger:A:CAN:CRCerror` on page 410

Identifier
Sets the trigger to a specific message identifier or an identifier range.

The first key press enables the "Identifier" trigger type, the second one opens the "Identifier" menu.

If a label list with node names was loaded and applied in the bus configuration, you can select simply the "Symbolic ID" from the list instead of entering the numeric identifier.

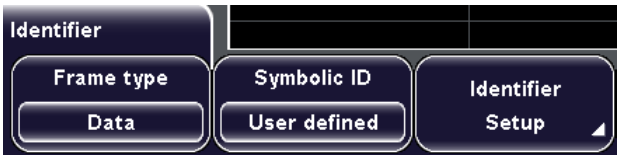

Remote command:
`TRIGger:A:CAN:TYPE` on page 407 (`ID` | `IDDT`)

Frame type ← Identifier
Data frames and remote frames contain an identifier. Select the frame type to be triggered on, or select "Data and remote" if the frame type is not relevant.

Remote command:
`TRIGger:A:CAN:FTYPe` on page 408

Symbolic ID ← Identifier
If a label list with node names was loaded and applied in the bus configuration, you can select simply the node name from the list instead of entering the numeric identifier.

The instrument trriggers on the identifier of the selected node.

Identifier Setup ← Identifier
Opens the menu to set the identifier pattern. After setting the "ID type" and the "Compare" condition, you can enter the value bit-by-bit by setting the state high, low, or don't care for each single bit. Alternatively, you can enter a hexadecimal value for each byte.

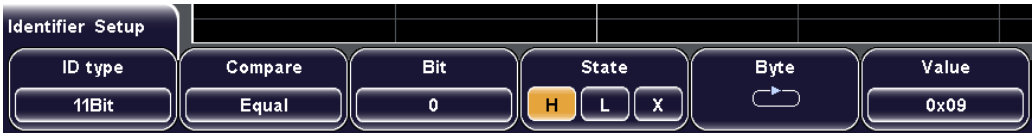

Remote command:
`TRIGger:A:CAN:IDENtifier` on page 409

ID type ← Identifier Setup ← Identifier
Selects the length of the identifier: 11 bit for CAN base frames, or 29 bits for CAN extended frames.

Remote command:
`TRIGger:A:CAN:ITYPe` on page 408

Compare ← Identifier Setup ← Identifier
Sets the comparison condition: If the pattern contains at least one X (don't care), you can trigger on values equal or not equal to the specified value. If the pattern contains only 0 and 1, you can also trigger on a range greater than or lower than the specified value.

Remote command:
`TRIGger:A:CAN:ICONdition` on page 409

Bit ← Identifier Setup ← Identifier
Selects the number of the bit in the pattern for bit-by-bit input. For each selected bit, enter the "State".

State ← Identifier Setup ← Identifier
Toggles the logic state of the selected bit: 0 (low), 1 (high), or X (don't care).

Byte ← Identifier Setup ← Identifier
Selects the byte for input of the pattern. For each selected byte, enter the hexadecimal value, or set the "State" for each selected "Bit".

Value ← Identifier Setup ← Identifier
Sets the hexadecimal value for the selected byte by turning the navigation knob.

Identifier and data
Sets the trigger to a combination of identifier and data condition. The instrument triggers at the end of the last byte of the specified data pattern.

The identifier conditions are the same as for the "Identifier" trigger type, see "Identifier" on page 189.

The first key press enables the trigger type, the second one opens the "Identifier and data" menu.

Remote command:
`TRIGger:A:CAN:TYPE` on page 407 (`IDDT`)

Data Setup ← Identifier and data
Opens a menu to set the data pattern to be triggered on. After setting the "Data length" and the "Compare" condition, you can enter the value bit-by-bit by setting the state high, low, or don't care for each single bit. Alternatively, you can enter a hexadecimal value for each byte.

Most settings are the same as for identifier input. See:

- "Compare" on page 190
- "Bit" on page 190
- "State" on page 190
- "Byte" on page 190
- "Value" on page 190

Remote command:

TRIGger:A:CAN:DCONdition on page 409

TRIGger:A:CAN:DATA on page 410

Data Length ← Data Setup ← Identifier and data

Defines the length of the data pattern - the number of bytes in the pattern.

Remote command:

TRIGger:A:CAN:DLC on page 409

11.5.3 CAN Label List

Label lists are protocol-specific. A PTT file for CAN contains three values for each identifier:

- "Type": identifier type, 11-bit or 29-bit long
- "ID / Addr": hexadecimal identifier value
- "Symbolic label": symbolic name of the identifier, specifiing its function in the bus network.

Example: CAN PTT file

```
# ------------------------------------------------------------------------
@FILE_VERSION  = 1.00
@PROTOCOL_NAME = can
# ------------------------------------------------------------------------
# Labels for CAN protocol
#   Column order: Identifier type, Identifier value, Label
# ------------------------------------------------------------------------
11,0x064,Diag_Response
11,0x1E5,EngineData
11,0x0A2,Ignition_Info
11,0x1BC,TP_Console
11,0x333,ABSdata
11,0x313,Door_Left
11,0x314,Door_Right
29,0x01A54321,Throttle
29,0x13A00FA2,LightState
29,0x0630ABCD,Engine_Status
```

```
29,0x03B1C002,Airbag_Status
29,0x01234ABC,NM_Gateway
# ------------------------------------------------------------------------
```

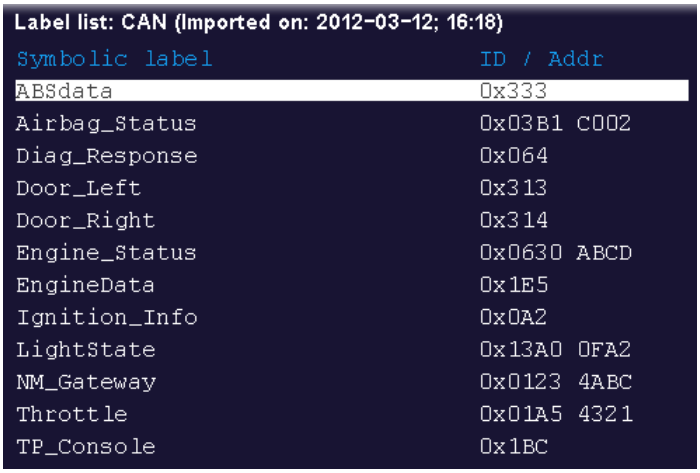

Fig. 11-11: Label list for CAN

For general information, see chapter 11.1.4, "Label List", on page 151.

11.5.4 CAN Decode Results

You can enable the decoding in the "Protocol" main menu. "Decode" shows the decoded values below the waveforms in the format selected with "Display". Additionally, you can display the binary signal with "Bits".

See also: chapter 11.1.2, "Protocol - Common Settings", on page 149

Additionally, you can display and save a "Frame Table" containing decoded data: frame number, start time of the frame, frame type, identifier, data length code, data, checksum, and state of the frame.

See also: chapter 11.1.5, "Frame Table: Decode Results", on page 154

Fig. 11-12: Decoded CAN signal with frame table and applied label list

violet = identifier
gray = DLC, data length code
blue = data words
red = error occured, error frame

Table 11-4: Content of the CAN frame table

Column	Description
Start time	Time of frame start in relation to the trigger point
Type	Frame type: Data, Remote, Error, or Overload
ID	Identifier value, hexadecimal value
Label	Symbolic label, available if a label list was loaded and applied
DLC	Data length code, number of data bytes
Data	Hexadecimal values of the data bytes
CRC	Hexadecimal value of the Cyclic Redundance Check (checksum)
State	Overall state of the frame.

Remote commands:

- BUS<b>:CAN:FCOunt? on page 411
  BUS<b>:CAN:FRAMe<n>:DATA? on page 413
  BUS<b>:CAN:FRAMe<n>:STATus? on page 412
  BUS<b>:CAN:FRAMe<n>:STARt? on page 412
  BUS<b>:CAN:FRAMe<n>:STOP? on page 413
  BUS<b>:CAN:FRAMe<n>:TYPE? on page 411
  BUS<b>:CAN:FRAMe<n>:ACKState? on page 413
  BUS<b>:CAN:FRAMe<n>:ACKValue? on page 414
  BUS<b>:CAN:FRAMe<n>:CSSTate? on page 414
  BUS<b>:CAN:FRAMe<n>:CSValue? on page 414
  BUS<b>:CAN:FRAMe<n>:DLCState? on page 414
  BUS<b>:CAN:FRAMe<n>:DLCValue? on page 415
  BUS<b>:CAN:FRAMe<n>:IDSTate? on page 415
  BUS<b>:CAN:FRAMe<n>:IDTYpe? on page 415
  BUS<b>:CAN:FRAMe<n>:IDValue? on page 416
  BUS<b>:CAN:FRAMe<n>:BSEPosition? on page 416
  BUS<b>:CAN:FRAMe<n>:BCOunt? on page 416
  BUS<b>:CAN:FRAMe<n>:BYTE<o>:STATe? on page 417
  BUS<b>:CAN:FRAMe<n>:BYTE<o>:VALue? on page 417

11.5.5 Search on Decoded CAN Data

Using the search functionality, you can find various events in the decoded data, the same events which you also can trigger on. Before you can start the search, you have to configure the bus correctly and acquire decoded data.

To search on decoded data, use the search type "Protocol". The source is automatically set to the configured protocol.

See also: chapter 10, "Search", on page 132.

11.5.5.1 CAN Search Setup

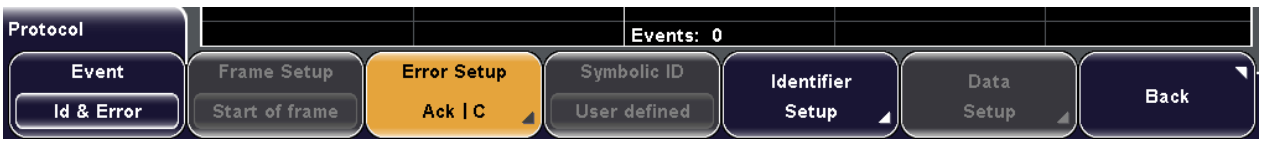

Event
Sets the event or combination of events to be searched for. Depending on the selected event, the appropriate settings in the softkey menu are activated.

Remote command:
SEARch:PROTocol:CAN:CONDition on page 418

Frame Setup
Selects the frame type to be searched for.

If you search for remote or data frames, the search consideres also the ID type, the length of the identifier.

The setting is only available if "Event" = "Frame" is selected.

Remote command:
SEARch:PROTocol:CAN:FRAMe on page 418

Error Setup
Selects the error type to be searched for. You can select one or more error types as search condition.

The error types are the same as in the CAN trigger setup, see "Error <type>" on page 188.

The setting is only available if "Event" = "Error" or "ID & Error" is selected.

Remote command:
SEARch:PROTocol:CAN:ACKerror on page 419
SEARch:PROTocol:CAN:BITSterror on page 419
SEARch:PROTocol:CAN:CRCerror on page 419
SEARch:PROTocol:CAN:FORMerror on page 420

Symbolic ID
If a label list with node names was loaded and applied in the bus configuration, you can select simply the node name from the list instead of entering the numeric identifier.

The instrument trriggers on the identifier of the selected node.

Frame type
Selects the frame type to be searched for, if "Event" = "Identifier" is selected. You can search for data and or remote frames.

Remote command:
SEARch:PROTocol:CAN:FTYPe on page 420

Identifier Setup
Opens the menu to set the identifier pattern, if "Event" = "Identifier" or "ID & Data" or "ID & Error" is selected.

After setting the "ID type" and the "Comparison" condition, you can enter the value bit-by-bit by setting the state high, low, or don't care for each single bit. Alternatively, you can enter a hexadecimal value for each byte.

The settings are the same as for the setup of the identifier trigger, see "Identifier Setup" on page 189.

Remote command:
SEARch:PROTocol:CAN:ITYPe on page 420
SEARch:PROTocol:CAN:ICONdition on page 420
SEARch:PROTocol:CAN:IDENtifier on page 420

Data Setup
Opens the menu to set the data pattern to be searched, if "Event" = "ID & Data" is selected.

After setting the "Data length" and the "Comparison" condition, you can enter the value bit-by-bit by setting the state high, low, or don't care for each single bit. Alternatively, you can enter a hexadecimal value for each byte.

The settings are the same as for the setup of the data trigger, see "Data Setup" on page 190.

Remote command:

SEARch:PROTocol:CAN:DLENgth on page 421
SEARch:PROTocol:CAN:DCONdition on page 421
SEARch:PROTocol:CAN:DATA on page 421

11.5.5.2 CAN Search Results

Search results (events) are marked on the waveform and listed in the event table as usual. Instead of the event table, you can display the frame table, where the search results are also marked. The event flags are not saved in the csv file of the frame table.

Fig. 11-13: Search for data frames with 11 bit identifier, search results are marked in frame table and on the decoded data

11.6 LIN (Option R&S RTM-K3)

The Local Interconnect Network (LIN) is a simple, low-cost bus system used within automotive network architectures. LIN is usually a sub-network of a CAN bus. The primary purpose of LIN is the integration of uncritical sensors and actuators with low bandwidth requirements. Common applications in a motor vehicle are the control of doors, windows, wing mirrors, and wipers.

11.6.1 The LIN Protocol

This chapter provides an overview of protocol characteristics, frame format, identifiers and trigger possibilities. For detailed information, order the LIN specification on http://www.lin-subbus.org/ (free of charge).

LIN characteristics

Main characteristics of LIN are:

- Single-wire serial communications protocol, based on the UART byte-word interface
- Single master, multiple slaves - usually up to 12 nodes
- Master-controlled communication: master coordinates communication with the LIN schedule and sends identifier to the slaves
- Synchronization mechanism for clock recovery by slave nodes without crystal or ceramics resonator

The R&S RTM supports several versions of the LIN standard: v1.3, v2.0, v2.1 and the american SAE J2602.

Data transfer

Basic communication concept of LIN:

- Communication in an active LIN network is always initiated by the master.
- Master sends a message header including the synchronization break, the synchronization byte, and the message identifier.
- The identified node sends the message response: one to eight data bytes and one checksum byte.
- Header and response form the message frame.

The data is transmitted in bytes using the UART byte-word interface without the parity bit. Each byte consists of a start bit, 8 bits and a stop bit.

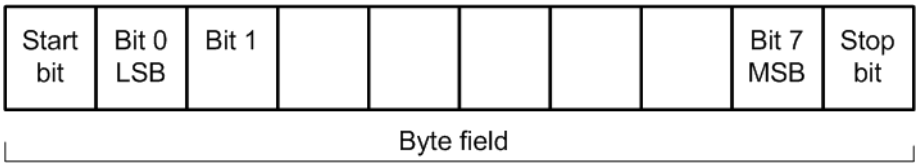

Fig. 11-14: Structure of a byte field

Data bytes are transmitted LSB first.

The identifier byte consists of 6 bits for the frame identifier and two parity bits. This combination is known as protected identifier.

Trigger

The R&S RTM can trigger on various parts of LIN frames. The data line must be connected to an input channel, triggering on math and reference waveforms is not possible.

You can trigger on:

- Frame start (synchronization field)
- Specific slave identifier or identifier range
- Data pattern in the message
- Wake up signal
- Checksum error (error in data), parity error (error in identifier)

11.6.2 LIN Configuration Settings

Access: PROTOCOL > "Bus type" = "LIN" "Configuration"

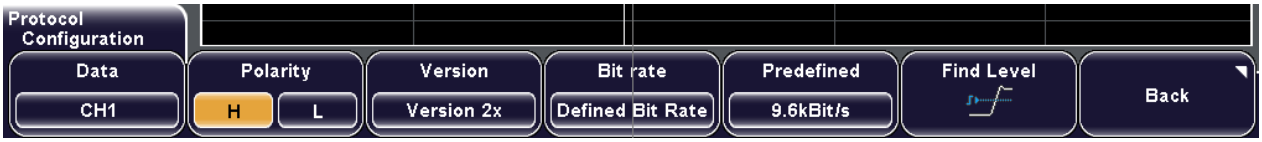

Data....198
Polarity....198
Version....198
Bit rate....199
Find Level....199

Data
Sets the source of the data line. All channel waveforms can be used.

If the MSO option R&S RTM-B1 is installed, digital channels can also be used as source.

Remote command:
`BUS<b>:LIN:DATA:SOURce` on page 422

Polarity
Defines the idle state of the bus. The idle state is the rezessive state and corresponds to a logic 1.

Remote command:
`BUS<b>:LIN:POLarity` on page 422

Version
Selects the version of the LIN standard that is used in the DUT. The setting mainly defines the checksum version used during decoding.

The most common version is LIN 2.x. For mixed networks, or if the standard is unknown, set the LIN standard to "Auto".

Remote command:
`BUS<b>:LIN:STANdard` on page 422

Bit rate
Sets the number of transmitted bits per second. The maximum bit rate is 20 kbit/s.

To select a bit rate from the list of predefined values, set "Bit rate" to "Defined Bit Rate", and then select the value with "Predefined".

To set another value, set "Bit rate" to "User Bit Rate", and then enter the value with "User".

Remote command:
`BUS<b>:LIN:BITRate` on page 423

Find Level
The instrument analyzes all lines that are configured for the selected bus and sets the threshold for digitization of analog signals for each channel. If no level can be found, the existing value remains unchanged, and you can set the thresholds manually in the channel menu: CH N > "More" (page 2) > "Threshold".

See: "Threshold" on page 31

"Find Level" is not relevant for digital channels (MSO option R&S RTM-B1). Thresholds for digital channels are set in the "Logic > Threshold" menu.

Remote command:
`CHANnel<m>:THReshold:FINDlevel` on page 379

11.6.3 LIN Trigger Settings

Access: SETUP (Trigger) > "Trigger type" = "Protocol (LIN)" "Setup"

Start of Frame....200
Wake Up....200
Error <type>....200
└ Checksum....200
└ Parity....200
└ Synchronization....200
Identifier....200
└ Symbolic ID....201
└ Compare....201
└ Bit....201
└ State....201
└ Byte....201
└ Value....201

Identifier and data....201
└ Identifier Setup....202
└ Data Setup....202
└ No. of Bytes....202

Start of Frame
Triggers on the stop bit of the sync field.

Remote command:
`TRIGger:A:LIN:TYPE` on page 423 (`SYNC`)

Wake Up
Triggers after a wakeup frame.

Remote command:
`TRIGger:A:LIN:TYPE` on page 423 (`WKFRame`)

Error <type>
Identifies various errors in the frame. You can select one or more error types as trigger condition.

The first key press enables the "Error" trigger type, the second opens the "Error" menu.

Remote command:
`TRIGger:A:LIN:TYPE` on page 423 (`ERRCondition`)

Checksum ← Error <type>
Triggers on a checksum error. The checksum verifies the correct data transmission. It is the last byte of the frame response. The checksum includes not only the data but also the protected identifier (PID).

Remote command:
`TRIGger:A:LIN:CHKSerror` on page 424

Parity ← Error <type>
Triggers on a parity error. Parity bits are the bits 6 and 7 of the identifier. They verify the correct transmission of the identifier.

Remote command:
`TRIGger:A:LIN:IPERror` on page 424

Synchronization ← Error <type>
Triggers if synchronization caused an error.

Remote command:
`TRIGger:A:LIN:SYERror` on page 424

Identifier
Sets the trigger to a specific identifier or an identifier range. Only the 6 bit identifier without parity bits is considered, not the protected identifier.

The first key press enables the "Identifier" trigger type, the second opens the "Identifier" menu.

After setting the "Compare" condition, you can enter the value bit-by-bit by setting the state high, low, or don't care for each single bit. Alternatively, you can enter a hexadecimal value for each byte.

If a label list with node names was loaded and applied in the bus configuration, you can select simply the "Symbolic ID" from the list instead of entering the numeric identifier.

Remote command:

`TRIGger:A:LIN:TYPE` on page 423 (`ID` | `IDDT`)

`TRIGger:A:LIN:ICONdition` on page 425

`TRIGger:A:LIN:IDENtifier` on page 425

Symbolic ID ← Identifier

If a label list with node names was loaded and applied in the bus configuration, you can select simply the node name from the list instead of entering the numeric identifier.

The instrument trriggers on the identifier of the selected node.

Compare ← Identifier

Sets the comparison condition: If the pattern contains at least one X (don't care), you can trigger on values equal or not equal to the specified value. If the pattern contains only 0 and 1, you can also trigger on a range greater than or lower than the specified value.

Bit ← Identifier

Selects the number of the bit in the pattern for bit-by-bit input. For each selected bit, enter the "State".

State ← Identifier

Toggles the logic state of the selected bit: 0 (low), 1 (high), or X (don't care).

Byte ← Identifier

Selects the byte for input of the data pattern. For each selected byte, enter the hexadecimal value, or set the "State" for each selected "Bit".

For the identifier pattern, byte selection is not relevant, as only the 6 bit identifier without parity bits is considered.

Value ← Identifier

Sets the hexadecimal value for the selected byte by turning the navigation knob.

Identifier and data

Sets the trigger to a combination of identifier and data condition. The instrument triggers at the end of the last byte of the specified data pattern.

The first key press enables the trigger type, the second one opens the "Identifier and data" menu.

Identifier Setup ← Identifier and data
Opens the "Identifier" menu.

The identifier conditions are the same as for the "Identifier" trigger type, see "Identifier" on page 200.

Data Setup ← Identifier and data
Opens a menu to set the data pattern. After setting the "No. of Bytes" and the "Compare" condition, you can enter the value bit-by-bit by setting the state high, low, or don't care for each single bit. Alternatively, you can enter a hexadecimal value for each byte.

The method is the same as for identifier input. See:
- "Compare" on page 201
- "Bit" on page 201
- "State" on page 201
- "Byte" on page 201
- "Value" on page 201

Remote command:
`TRIGger:A:LIN:TYPE` on page 423 (`IDDT`)
`TRIGger:A:LIN:DCONdition` on page 425
`TRIGger:A:LIN:DATA` on page 425

No. of Bytes ← Data Setup ← Identifier and data
Defines the length of the data pattern - the number of bytes in the pattern.

Remote command:
`TRIGger:A:LIN:DLENgth` on page 426

11.6.4 LIN Label List

Label lists are protocol-specific. A LIN PTT file contains two values for each identifier:
- "ID / Addr": hexadecimal identifier value
- "Symbolic label": symbolic name for the identifier

Example: LIN PTT file

```
# ------------------------------------------------------------------------

@FILE_VERSION = 1.0
@PROTOCOL_NAME = lin
# ------------------------------------------------------------------------
# Labels for LIN protocol
#   Column order: Identifier, Label
# ------------------------------------------------------------------------
# Labels for standard addresses
```

```
0x06,Dashboard
0x13,Gateway
0x1C,Temperature
0x21,Mirror
0x37,Indoor lights
# Labels for reserved addresses
0x3C,Master_Request_Frame
0x3D,Slave_Response_Frame
# ------------------------------------------------------------------------------
```

Label list: LIN (Imported on: 2012-04-05; 12:36)

Symbolic label	ID / Addr
Dashboard	0x06
Door controller	0x2E
Gateway	0x13
Indoor lights	0x37
Master_Request_Frame	0x3C
Mirror	0x21
Reserved_Frame	0x3F
Slave_Response_Frame	0x3D
Temperature	0x1C
User_Defined_Frame	0x3E

Fig. 11-15: Label list for CAN

For general information, see chapter 11.1.4, "Label List", on page 151.

11.6.5 LIN Decode Results

You can enable the decoding in the "Protocol" main menu. "Decode" shows the decoded values below the waveforms in the format selected with "Display". Additionally, you can display the binary signal with "Bits".

See also: chapter 11.1.2, "Protocol - Common Settings", on page 149

Additionally, you can display and save a "Frame Table" containing decoded data: frame number, start time of the frame, identifier, data length, data, checksum, and state of the frame.

See also: chapter 11.1.5, "Frame Table: Decode Results", on page 154

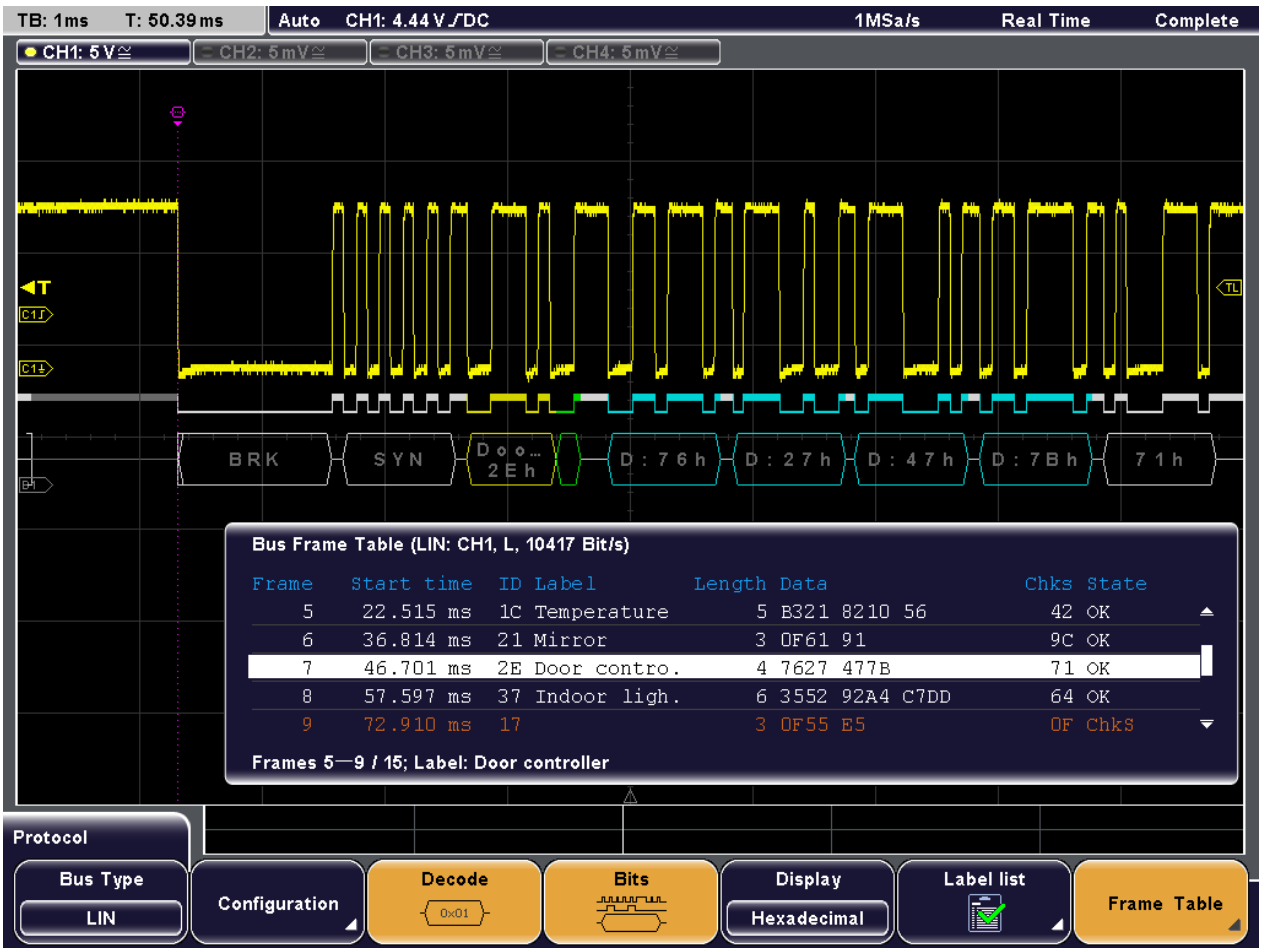

Fig. 11-16: Decoded LIN signal with frame table and applied label list

gray = synchronization break, synchronization byte, correct checksum
yellow = identifier
green = parity bits
blue = data words (UART words)

Table 11-5: Content of the LIN frame table

Column	Description
Start time	Time of frame start in relation to the trigger point
ID	Identifier value, hexadecimal value
Label	Symbolic label, available if a label list was loaded and applied
Length	Number of data bytes
Data	Hexadecimal values of the data bytes
Chks	Checksum value
State	Overall state of the frame.

Remote commands:

- `BUS<b>:LIN:FCOunt?` on page 426

- BUS<b>:LIN:FRAMe<n>:DATA? on page 426
- BUS<b>:LIN:FRAMe<n>:STATus? on page 427
- BUS<b>:LIN:FRAMe<n>:STARt? on page 427
- BUS<b>:LIN:FRAMe<n>:STOP? on page 427
- BUS<b>:LIN:FRAMe<n>:VERSion? on page 430
- BUS<b>:LIN:FRAMe<n>:CSSTate? on page 428
- BUS<b>:LIN:FRAMe<n>:CSValue? on page 428
- BUS<b>:LIN:FRAMe<n>:IDPValue? on page 428
- BUS<b>:LIN:FRAMe<n>:IDSTate? on page 429
- BUS<b>:LIN:FRAMe<n>:IDValue? on page 429
- BUS<b>:LIN:FRAMe<n>:SYSTate? on page 429
- BUS<b>:LIN:FRAMe<n>:SYValue? on page 430
- BUS<b>:LIN:FRAMe<n>:BCOunt? on page 430
- BUS<b>:LIN:FRAMe<n>:BYTE<o>:STATe? on page 431
- BUS<b>:LIN:FRAMe<n>:BYTE<o>:VALue? on page 431

11.6.6 Search on Decoded LIN Data

Using the search functionality, you can find various events in the decoded data, the same events which you also can trigger on. Before you can start the search, you have to configure the bus correctly and acquire decoded data.

To search on decoded data, use the search type "Protocol". The source is automatically set to the configured protocol.

See also: chapter 10, "Search", on page 132.

11.6.6.1 LIN Search Setup

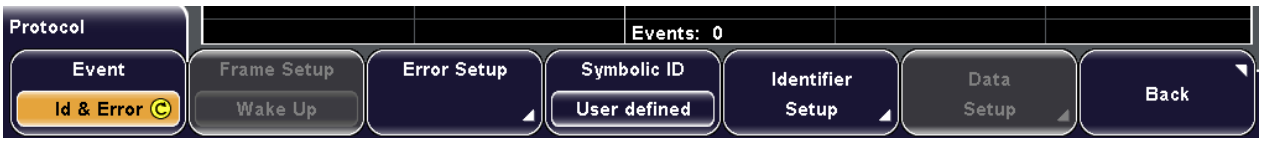

Event
Sets the event or combination of events to be searched for. Depending on the selected event, the appropriate settings in the softkey menu are activated.

Remote command:
SEARch:PROTocol:LIN:CONDition on page 432

Frame Setup
Selects the frame type to be searched for: Start of frame or wakeup frame.

The setting is only available if "Event" = "Frame" is selected.

Remote command:
SEARch:PROTocol:LIN:FRAMe on page 432

Error Setup
Selects the error type to be searched for. You can select one or more error types as search condition.

The error types are the same as in the LIN trigger setup, see "Error <type>" on page 200.

The setting is only available if "Event" = "Error" or "ID & Error" is selected.

Remote command:
SEARch:PROTocol:LIN:CHKSerror on page 433
SEARch:PROTocol:LIN:IPERror on page 433
SEARch:PROTocol:LIN:SYERror on page 433

Symbolic ID
If a label list with node names was loaded and applied in the bus configuration, you can select simply the node name from the list instead of entering the numeric identifier.

The instrument trriggers on the identifier of the selected node.

Identifier Setup
Opens the menu to set the identifier pattern, if "Event" = "Identifier" or "ID & Data" or "ID & Error" is selected.

The settings are the same as for the setup of the identifier trigger, see "Identifier" on page 200.

Remote command:
SEARch:PROTocol:LIN:ICONdition on page 433
SEARch:PROTocol:LIN:IDENtifier on page 433

Data Setup
Opens the menu to set the data pattern to be searched, if "Event" = "ID & Data" is selected.

After setting the "No. of Bytes" and the "Comparison" condition, you can enter the value bit-by-bit by setting the state high, low, or don't care for each single bit. Alternatively, you can enter a hexadecimal value for each byte.

The settings are the same as for the setup of the data trigger, see "Data Setup" on page 202.

Remote command:
SEARch:PROTocol:LIN:DLENgth on page 434
SEARch:PROTocol:LIN:DCONdition on page 434
SEARch:PROTocol:LIN:DATA on page 434

11.6.6.2 LIN Search Results

Search results (events) are marked on the waveform and listed in the event table as usual. Instead of the event table, you can display the frame table, where the search results are also marked. The event flags are not saved in the csv file of the frame table.

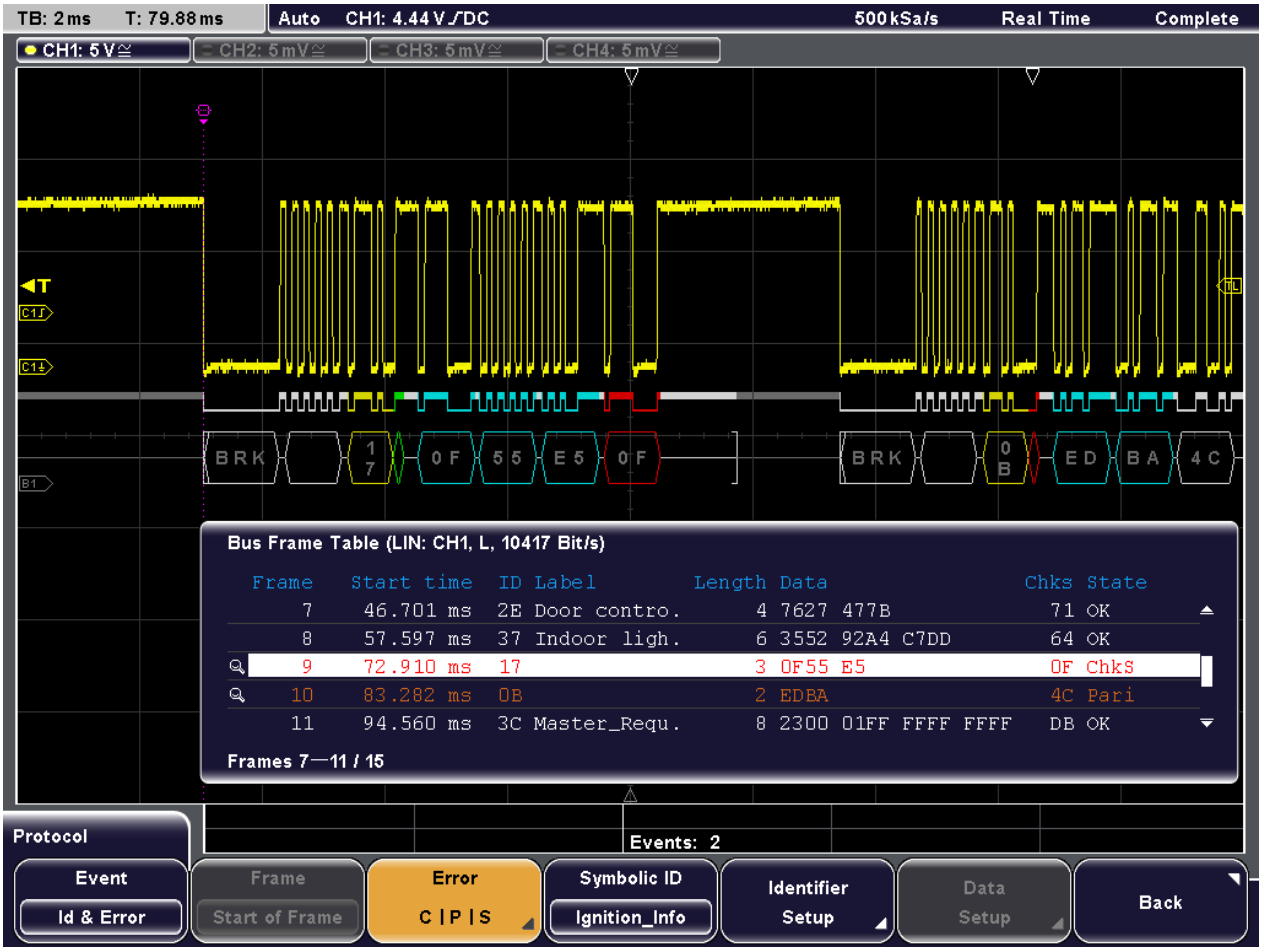

Fig. 11-17: Search for data frames with 11 bit identifier, search results are marked in frame table and on the decoded data

12 Mixed Signal Option (MSO, R&S RTM-B1)

The Mixed Signal Option R&S RTM-B1 adds logic analyzer functions to the classical oscilloscope functions. Using the MSO option, you can analyze and debug embedded systems with mixed-signal designs that use analog signals and correlated digital signals simultaneously.

12.1 About MSO

The Mixed Signal Option provides 16 digital channels grouped in two logic probes (pods) with 8 channels each. The instrument ensures that analog and digital waveforms are timealigned and synchronized so that critical timing interactions between analog and digital signals can be displayed and tested. The automatic alignment compensates the skew between the probe connectors of the analog channels and the probe boxes of the digital channels.

Digital channels and parallel buses

Each digital channel can be displayed on the screen and used as trigger source of some trigger types. A pod of digital signals can be saved as reference waveform.

Digital channels may be grouped and displayed as a parallel bus. Up to 4 parallel buses can be configured; and two bus types are supported: clocked bus and unclocked bus.

Trigger possibilities

One of the digital channels can be used as trigger source for edge and width triggers. However, digital channels are not selectable if the B-trigger is enabled. Using the pattern trigger, you can trigger on parallel buses and logical combinations of analog and digital channels. For all digital trigger sources, the trigger level is the logical threshold. Additionally, you can define a trigger holdoff time for the edge and width trigger.

Cursor measurements

Cursor measurements can be performed on single digital channels and on pods. As for all measurements, the instrument provides only sources that are active and appropriate for the selected measurement type.

The sources D0 to D15 are available for time, ratio X, count, duty ratio and burst width measurements. The pods D0...D7 and D8...D15 are available for V-marker measurements, which delivers the 8-bit value of the pod.

Automatic measurements and statistics

Automatic time and count measurements can be performed on active digital channels. As for all measurements, the instrument provides only sources that are active and appropriate for the selected measurement type.

The following measurement types are available for single digital channels (bits): frequency, period, edge and pulse counts, phase, delay, duty cycle, burst width. Statistical evaluation of these measurements is also possible.

12.2 Digital Channels

12.2.1 Digital Channels - Configuration Settings

Access: PROTOCOL LOGIC > if "Protocol" menu is displayed: "Logic"

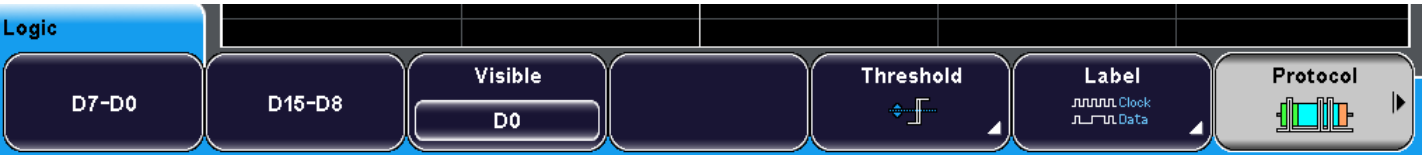

D7-D0 / D15-D8
Enables or disables all digital channels of the pod at once.

Visible
Enables or disables individual digital channels.

Turn the navigation knob to select the digital channel, then press the knob to enable or disable the channel.

Remote command:
`DIGital<m>:DISPlay` on page 435

Threshold
Opens the "Threshold" menu.

You can set the digital threshold in several ways:

- The same threshold and hysteresis is used for all digital channels: Enable "Couple Levels" and set the values.
- Different thresholds and hysteresis are used for individual channel groups (nibbles): Disable "Couple Levels" and set the threshold and hysteresis for each nibble.

Nibble ← Threshold
Selects a group of 4 digital channels for which the threshold and the hysteresis can be set.

Threshold ← Threshold
Sets the threshold value for the selected nibble, or for all digital channels if "Couple Levels" is enabled.

The threshold setting is available if "Technology" is "User Level".

For each acquired sample, the instrument compares the input voltage with the threshold value. If the input voltage is above the threshold, the signal state "1" is stored. Otherwise, the signal state "0" is stored if the input voltage is below the threshold.

Remote command:
`DIGital<m>:THReshold` on page 435

Technology ← Threshold
Selects the threshold voltage for various types of integrated circuits from a list. The value is applied to the selected nibble, or to all digital channels if "Couple Levels" is enabled.

Remote command:
`DIGital<m>:TECHnology` on page 435

Hysteresis ← Threshold
Hysteresis avoids the change of signal states due to noise oscillation around the threshold level. Set a small hysteresis for clean signals, and large hysteresis for noisy signals.

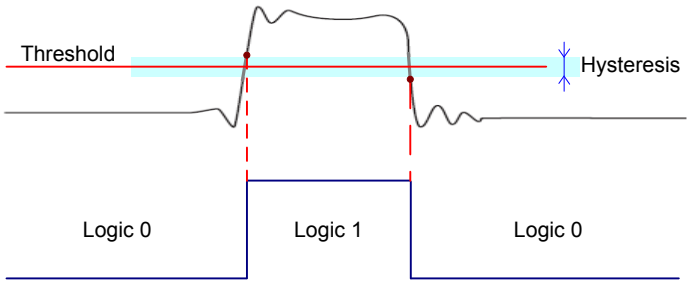

Remote command:
`DIGital<m>:Hysteresis` on page 436

Couple Levels ← Threshold
Applies the threshold and hysteresis values of the first nibble (D0 to D3) to all digital channels.

Remote command:
`DIGital<m>:THCoupling` on page 436

Label
Opens the "Label" menu.

You can define a label for each digital channel, and display each label individually. The labels are shown on the the right side of the display. You can enter a label text in several ways:

- Select a predefined string from the "Library".
- Enter a user-defined text using "Edit Label".

Remote command:
`DIGital<m>:LABel` on page 436

Bit ← Label
Selects the digital channel for which the label is to be defined.

Label ← Label
Displays or hides the label of the selected digital channel.

Remote command:
`DIGital<m>:LABel:STATe` on page 437

Library ← Label
Selects a label text from a list of frequently used terms.

Edit Label ← Label
Opens the on-screen keyboard to enter any label text

The maximum name length is 8 characters, and only ASCII characters provided on the on-screen keyboard can be used.

POSITION
The vertical POSITION rotary knob moves the digital channels vertically on the screen. It affects all visible dgital channels.

Remote command:
`DIGital<m>:POSition` on page 436

SCALE
The vertical SCALE rotary knob sets the size of the digital channels. Three sizes are available: small, medium and large display. The setting affects all visible dgital channels.

Remote command:
`DIGital<m>:SIZE` on page 437

12.3 Parallel Buses

The R&S RTM can display and decode up to 16 lines of a parallel bus. To trigger on parallel buses, use the pattern trigger. See: chapter 3.3.2.6, "Pattern", on page 48.

12.3.1 Analyzing Parallel Buses

Similar to serial protocols, the parallel buses - unclocked and clocked - need configuration to decode and display the signal.

To configure parallel buses

1. Press the PROTOCOL LOGIC key on the front panel.
2. If the "Logic" menu is displayed, press "Protocol".
3. Press "Bus" and select the bus to be configured.
4. Press the "Bus Type" and select "Parallel" or "Parallel Clocked".
5. Press "Configuration".
6. To configure the "Parallel" (unclocked) bus, select the "Bus Width".

7. To configure the "Parallel Clocked" bus:
   a) Select the "Bus Width".
   b) Press "Chip Select" and select the digital channel connected to CS.
   c) Select the "Active" state of chip select.
   d) Press "Clock" and select the digital channel connected to the clock line.
   e) Select the clock "Slope".
8. Make sure that the thresholds are set correctly.
   See:
9. Press "Back" and configure the data display.
   See: "To configure decoding and data display" on page 149

12.3.2 Parallel Clocked Bus

12.3.2.1 Parallel Clocked Bus - Configuration

For the parallel clocked bus, the bus width and, in addition, a clock line and a chip select line are defined.

Access: PROTOCOL LOGIC > if "Logic" menu is displayed: "Protocol" > "Bus Type = Parallel Clocked" > "Configuration "

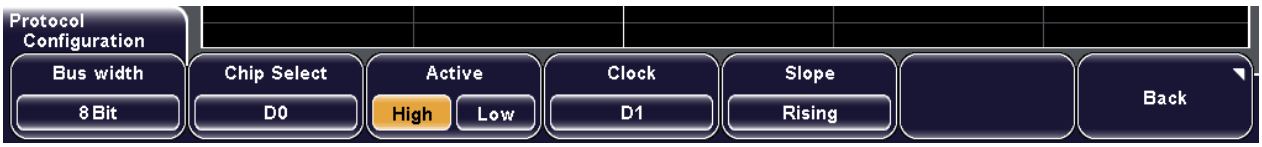

Bus width
Sets the number of lines to be analyzed. The maximum number is 14 bits if all digital channels are used. D0 and D1 are reserved for chip select and clock.

Remote command:
`BUS<b>:CPARallel:WIDTh` on page 438

Chip Select
The chip select must be connected to D0.

Active
Selects wether the chip select signal is high active (high = 1) or low active (low = 1).

Remote command:
`BUS<b>:CPARallel:CS:POLarity` on page 438

Clock
The clock must be connected to D1.

Slope
Selects if the data is sampled on the rising or falling slope of the clock, or on both edges of a double data rate clock. The clock slope marks the begin of a new bit.

Remote command:
`BUS<b>:CPARallel:CLOCK:SLOPe` on page 438

12.3.2.2 Parallel Clocked Bus - Decode Results

You can enable the decoding in the "Protocol" main menu. "Decode" shows the decoded values below the waveforms in the format selected with "Display". Additionally, you can display the binary signal with "Bits".

See also: chapter 11.1.2, "Protocol - Common Settings", on page 149

Additionally, you can display and save a "Frame Table" containing decoded data: frame number, start time of the frame, identifier, data length, data, checksum, and state of the frame.

See also: chapter 11.1.5, "Frame Table: Decode Results", on page 154

Remote commands:

- `BUS<b>:CPARallel:FCOunt?` on page 439
- `BUS<b>:CPARallel:FRAMe<n>:DATA?` on page 439
- `BUS<b>:CPARallel:FRAMe<n>:STATe?` on page 440
- `BUS<b>:CPARallel:FRAMe<n>:STARt?` on page 440
- `BUS<b>:CPARallel:FRAMe<n>:STOP?` on page 440

12.3.3 Parallel Bus (Unclocked)

12.3.3.1 Parallel Bus - Configuration

The unclocked parallel bus can analyze up to 16 digital channels. The configuration is simple, the only setting is the "Bus width".

Bus width
Sets the number of lines to be analyzed. The maximum number is 16 bits if all 16 digital channels are used.

Remote command:
`BUS<b>:PARallel:WIDTh` on page 437

12.3.3.2 Parallel Bus - Decode Results

You can enable the decoding in the "Protocol" main menu. "Decode" shows the decoded values below the waveforms in the format selected with "Display". Additionally, you can display the binary signal with "Bits".

See also: chapter 11.1.2, "Protocol - Common Settings", on page 149

Additionally, you can display and save a "Frame Table" containing decoded data: frame number, start time of the frame, identifier, data length, data, checksum, and state of the frame.

See also: chapter 11.1.5, "Frame Table: Decode Results", on page 154

Remote commands:

- `BUS<b>:PARallel:FCOunt?` on page 439
- `BUS<b>:PARallel:FRAMe<n>:DATA?` on page 439
- `BUS<b>:PARallel:FRAMe<n>:STATe?` on page 440
- `BUS<b>:PARallel:FRAMe<n>:STARt?` on page 440
- `BUS<b>:PARallel:FRAMe<n>:STOP?` on page 440

13 Data and File Management

This chapter describes how to print screenshots and how to manage measurement settings and data.

- Printing....215
- Saving and Loading....217

13.1 Printing

You can create a sceenshot of the current display of your waveforms and measurement results and print it on a printer. To optimize the output, you can configure different color modes. The printer has to be connected to a Type A USB port. Alternatively, you can save screenshots to files, see also: chapter 13.2.5, "Screenshots", on page 230.

If you want to print many screenshots, you can assign the printout function to the PRINT key. This key is a shortcut key that initiates the assigned action at a single keypress. Infrequent printouts can be started from the "File" menu, see also: chapter 13.1.1.3, "Quick Printing with the PRINT Key", on page 216.

13.1.1 Printing a Screenshot

Before you can print, you have to:

- Connect and configure the printer
- Configure the PRINT key if you need quick printout

Then you can start the printout from the "File" menu or with the PRINT key.

13.1.1.1 Configuring the Printer Output

For the printout, you configure the format and colors. The individual settings are described in chapter 13.1.2, "Printer Settings", on page 216.

1. Connect the printer to a Type A USB port on the front or rear panel of the instrument.
2. Press SETUP > "Printer" to open the "Printer" menu.
3. Press "Paper Format" and select the required format using the "Navigation" knob.
4. In the "Printer" menu, press "Color Mode".
5. Select the required color format using the "Navigation" knob.
6. Most printers support PCL (Printer Command Language). If your printer does not, select the appropriate "Command Set".

13.1.1.2 Starting the Printout

Infrequent printouts can be started from the "File" menu.

1. Make sure that the printer is configured correctly.
   See: chapter 13.1.1.1, "Configuring the Printer Output", on page 215
2. Press the FILE key.
3. Press "Screenshots > Print".

13.1.1.3 Quick Printing with the PRINT Key

You assign the print function to the PRINT key. After this configuration a screenshot will be printed on the connected printer whenever you press the PRINT key.

See also: chapter 13.2.2, "Quick Access with PRINT key", on page 223.

1. Configure the PRINT key:
   a) Press FILE > "Print-Key".
   b) Press "(Print) Screenshots".
2. Make sure that the printer is configured correctly.
   See: chapter 13.1.1.1, "Configuring the Printer Output", on page 215
3. Press the PRINT key.

13.1.2 Printer Settings

Access: SETUP key > "More" (switch to page 2/3) > "Printer"

Paper Format
Defines the paper format and the orientation (portrait or landscape) for printing.

Remote command:
`HCOPy:PAGE:SIZE` on page 442
`HCOPy:PAGE:ORIentation` on page 442

Color Mode
Defines the color mode for output on printer.

"Grayscale" Black and white output
"Color" Color output

"Inverted" Inverts the colors of the output, i.e. a dark waveform is printed on a white background.

Remote command:
`HCOPy:COLor:SCHeme` on page 442

Command Set
Sets the printer language that is supported by the printer. When you connect a printer, the supported command set is shown in the "Device Information" window.

13.2 Saving and Loading

With R&S RTM, you can save and recall your measurement data: device settings, mask definitions, equation sets, waveform data, and screenshots. Data can be stored in the instrument or on external device, it can be copied and converted (depending on the available formats).

- Storage Locations....217
- Quick Access with PRINT key....223
- Device Settings....225
- Waveforms....227
- Screenshots....230
- References, Masks, and Equation Sets: Import/Export....232

13.2.1 Storage Locations

The R&S RTM provides three basic storage locations to store any data. In the following, these locations are refered to as storage devices:

- The "Internal" storage device is a flash memory in the instrument with about 8 MB memory size.
- The "Front USB" storage device indicates a USB flash drive that is connected to the USB connector on the front panel of the instrument.
- The "Rear USB" storage device indicates a USB flash drive that is connected to the USB connector on the rear panel of the instrument.

On each storage device, data can be organized in folders as usual. Therefore, the R&S RTM allows you to create folders or remove them wherever you need.

Device settings, reference waveforms, masks, and equations sets can be directly saved to and loaded from any storage device. Waveforms and screenshots can be saved to USB storage devices only.

To copy data from one storage device to another, the "Import/Export" functions are used. The name of the target file can be changed, so you can copy and rename in one operation. For references and masks, you can also change the target file format and convert the data during export/import.

This chapter describes the general procedures and settings to save, load, and export/ import data.

13.2.1.1 Configuring Storage Locations

You must configure the storage settings for the various data types initially: select the storage location and the storage directory, and define the file name. For some data types, further storage settings are available. Then you can save data simply by pressing the "Save" softkey in the FILE menu or, if configured accordingly, by pressing the PRINT key on the front panel.

To select the storage directory

Whenever you want to save, copy or load data, you have to set the directory where the data will be stored or loaded from.

1. Press "Storage" to open the storage directory menu and display the file explorer for the currently selected storage location.
   See also: "Storage Directory Menu" on page 221.
2. Press "Storage (Internal/Front/Rear)" until the required storage device is highlighted. For waveforms and screenshots, only a USB flash drive can be selected as a storage location. If no USB flash drive is connected to the instrument, this function is not available.
3. Use the "Navigation" knob to scroll through the directories. To change the directory, scroll to the name of the directory and press the knob, or press "Change dir.".
4. Press "Create dir." to create a new subdirectory under the selected directory. Enter a name for the subdirectory as described in "To define a new file or directory name" on page 218.
5. Press "Remove dir." to remove a directory that you no longer need.
6. Press "Accept" to confirm the selected storage directory.

To define a new file or directory name

When you create a new directory or press "File name" to define the name of the storage file, a text editor is displayed in which you can enter the new name.

1. Use the "Navigate" knob to select a character.
2. Press "Character Set", if available, to display additional characters.
3. Press "Backspace" to delete the character to the left of the cursor.
4. Press the "Cursor →" and "Cursor←" softkeys to scroll through the characters of the name.
5. Press "Default name" to restore the default name.
6. Press "Accept" to save the defined name.

13.2.1.2 Importing and Exporting Data

To copy data from one storage device to another, the "Import/Export" functions are used. The procedures is the same for all data types.

The name of the target file can be changed, so you can copy and rename in one operation. For references and masks, you can also change the target file format and convert the data during export/import.

1. In the FILE menu, press the "Import/Export" softkey for the required data type.
2. Define the source file for the copy operation.
   a) Press "Source".
      A file explorer is displayed.
   b) If necessary, switch to the storage location that contains the source file by pressing "Storage (Internal/Front/Rear)".
   c) Select the source file. Use the "Navigation" knob to scroll through the directories. To change the directory, scroll to the name of the directory and press the knob, or press "Change dir.".
   d) Press "Load".
      The source file is selected, but not yet loaded to the R&S RTM.
3. Define the destination directory for the copy operation. The source file will be copied here.
   a) Press "Destination".
      A file explorer is displayed.
   b) If necessary, switch to the storage location that contains the storage directory by pressing "Storage (Internal/Front/Rear)".
   c) Select the storage directory. Use the "Navigation" knob to scroll through the directories. To change the directory, scroll to the name of the directory and press the knob, or press "Change dir.".
      Press "Create dir." to create a new subdirectory under the selected directory. Enter a name for the subdirectory as described in "To define a new file or directory name" on page 218.
   d) Press "Accept" to confirm the selection.
4. Change the "File Name" of the destination file if necessary.

   Note: If a file with the same file name already exists in the destination directory, it will be overwritten without notification.
5. If you want to change the file format for references or masks, press "Format" and select the target format.
6. Press "Import/Export".

   The source file is copied to the destination directory.

Imported data is not loaded to the instrument automatically. You must explicitly load it after import with the "Load" function in the relevant menu (Masks, Reference, Math menu, or File menu for instrument settings).

13.2.1.3 General Storage Settings

This chapter describes the general settings to save, load, and export/import data.

- Save Menu....220
- Load Menu....221
- Storage Directory Menu....221
- Import/Export Menu....222

Save Menu

The "Save" menu provides functions to configure how the data is saved and to start the save process. Its main functions are displayed whenever some data has to be stored. Depending on the data type, additional specific functions may be provided. These functions are described in the relevant chapters.

Storage....220
File name....220
Comment....220
Save....221

Storage
Opens the storage directory submenu, see "Storage Directory Menu" on page 221.

File name
Opens on-screen keyboard to define a new file name to which the data is stored.

Note: If a file with the same file name already exists in the destination directory, it will be overwritten without notification.

Turn the NAVIGATION knob to mark a character and press the knob to select it. Press "Backspace" to delete the character to the left of the cursor. Press the "Cursor →" and "Cursor ←" softkeys to scroll through the characters of the name. Press "Default name" to restore the standard file name.

Press "Accept" to save the defined name.

Remote command:
`MMEMory:NAME` on page 441

Comment
Opens an on-screen keyboard to insert a comment to the stored data. Comments are available for all file formats that can be read by the R&S RTM: device settings, reference waveforms (trf format), masks, equation sets.

Save
Saves the data to the selected storage directory. The used file name is displayed when storage is completed.

Remote command:
Device settings: `MMEMory:STORe:STATe` on page 449
Other data: `MMEMory:DATA` on page 449

Load Menu

The "Load" menu provides functions and a file explorer to select data files and to load it for usage. It is displayed whenever some data has to be loaded.

Storage....221
Remove File....221
Load....221

Storage
Opens the storage directory submenu, see "Storage Directory Menu" on page 221.

Remove File
Deletes the selected file.

Remote command:
`MMEMory:DELete` on page 448

Load
Loads the selected file to the instrument.

During an import/export operation, this command confirms the selection of a file and loads it temporarily. In order to actually copy the file to the selected destination, press "Import/Export".

Remote command:
Device settings: `MMEMory:LOAD:STATe` on page 449

Storage Directory Menu

The storage directory menu is opened with the "Storage" softkey that is available in all "Save" and "Load" menus. Here you define the storage device and the directory where the file will be saved or loaded from. If appropriate, you can also create new directories or delete existing ones.

Waveforms and screenshots can only be stored on a USB stick connected to the front or rear panel, not to an internal directory. If you want to store a waveform or scrrenshot, and no USB stick is currently connected, the "Storage" softkey is not available.

See also: chapter 13.2.1, "Storage Locations", on page 217.

Storage (Internal/Front/Rear).....222
Change Directory.....222
Create Directory.....222
Remove Directory.....222

Storage (Internal/Front/Rear)
Defines the storage device.

Waveforms and screenshots can only be stored on a USB stick connected to the front or rear panel, not to an internal directory. In this case, the softkey is only available if a USB stick is connected to the rear or front panel.

"Internal"	Directly in the internal memory of the instrument
"Front"	On a USB stick connected to the front panel
"Rear"	On a USB stick connected to the rear panel

Remote command:
`MMEMory:MSIS` on page 444

Change Directory
Switches to the selected directory.

See also: "To select the storage directory" on page 218.

Remote command:
`MMEMory:CDIRectory` on page 445

Create Directory
Creates a new subdirectory of the currently selected storage directory.

See also: "To define a new file or directory name" on page 218.

Remote command:
`MMEMory:MDIRectory` on page 445

Remove Directory
Removes the currently selected directory.

Remote command:
`MMEMory:RDIRectory` on page 445

Import/Export Menu

The "Import/Export" menu provides functions to copy data between the instrument and a USB flash device.

See also: chapter 13.2.1.2, "Importing and Exporting Data", on page 218

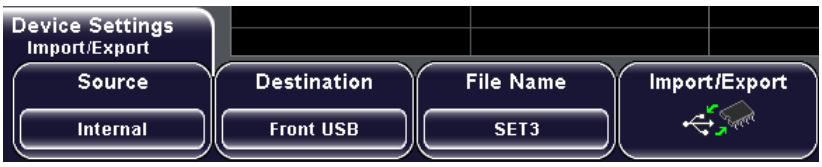

Source....223
Destination....223
Import/Export....223

Source
Opens the "Load" menu and a file explorer to select the source file of the import/export operation.

See "Load Menu" on page 221.

Destination
Opens the "Storage" menu and a file explorer to select the destination of the import/export operation.

See "Storage Directory Menu" on page 221.

Import/Export
Copies the selected source file to the specified file in the selected destination directory.

Note: If a file with the same file name already exists in the destination directory, it will be overwritten without notification.

Remote command:
`MMEMory:COPY` on page 448

13.2.2 Quick Access with PRINT key

The PRINT key is a shortcut key that initiates the associated action. With this key it is easy to save, for example, a series of waveform data or screenshots.

You can assign one of the following actions to the PRINT key:

- Save device settings
- Save a waveform
- Save a screenshot
- Save a screenshot and the device settings
- Print a screenshot

Saving data
You also can save data without changing the behavior of the PRINT key by pressing "Save" for the selected data type in the FILE menu.

13.2.2.1 Configuring the PRINT-Key Behavior

The PRINT key can either be used to print screenshots to a connected printer, or to save data to a specified storage location just by pressing a single key.

1. Press FILE > "Print Key".
2. Press the softkey of the action that you want to assign to the PRINT key.
3. Configure the settings for the selected action:
   - Save device settings: FILE > "Device Settings > Save"
   - Save a waveform: FILE > "Waveforms"
   - Save a screenshot: FILE > "Screenshots"
   - Save a screenshot and the device settings: FILE > "Screenshots" and FILE > "Device Settings > Save"
   - Print screenshots: SETUP > "More > Printer"

   After this configuration the selected action is started whenever you press the PRINT key.

13.2.2.2 PRINT-Key Settings

With FILE > "Print Key" you define an action that will be executed by pressing the PRINT key.

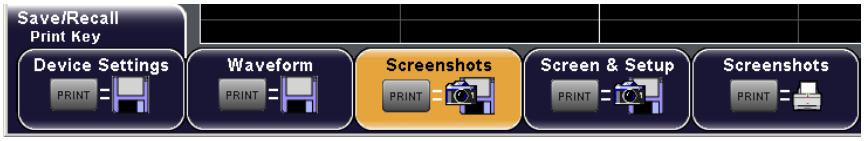

Device Settings.....224
Waveforms.....224
(Save) Screenshots.....224
Screen & Setup.....225
(Print) Screenshots.....225

Device Settings
If selected, the device settings are stored when you press the PRINT key. Storage settings are configured with FILE > "Device Settings".

See also: chapter 13.2.3.2, "Device Settings Menu", on page 226.

Waveforms
If selected, the current waveform is stored when you press the PRINT key. Storage settings are configured with FILE > "Waveforms".

See also: chapter 13.2.4.3, "Waveform Storage Settings", on page 229.

(Save) Screenshots
If selected, a screenshot of the current display is stored when you press the PRINT key. Storage settings are configured with FILE > "Screenshots".

See also: chapter 13.2.5.2, "Screenshot Storage Settings", on page 231.

Screen & Setup
If selected, the device settings and a screenshot of the current display are stored when you press the PRINT key. Storage settings are configured with FILE > "Screenshots" and FILE > "Device Settings".

See also: chapter 13.2.5.2, "Screenshot Storage Settings", on page 231

(Print) Screenshots
If selected, a screenshot of the current display is sent to the USB printer when you press the PRINT key. Printer settings are configured with SETUP > "Printer".

See also: chapter 13.1, "Printing", on page 215

13.2.3 Device Settings

In order to repeat measurements at different times or perform similar measurements with different test data, it is useful to save the used instrument settings and load them again later. Furthermore, it can be helpful to refer to the instrument settings of a particular measurement when analyzing the results. Therefore, functions are provided so you can easily save the instrument settings of a measurement, with or without the corresponding screenshot.

The instrument settings can be saved to and loaded from any storage device - internal memory or external USB flash device. It is also possible to copy the stored settings to another storage device with "Export/Import". The file format is always `.SET`, and the file size is about 2.76 kB.

You can exchange stored device settings between R&S RTM instruments, also between 2-channel and 4-channel instruments.

The default instrument settings can be restored with PRESET or FILE > "Device Settings > Default sett.".

13.2.3.1 Saving and Loading Device Settings

- "To save device settings" on page 225
- "To load device settings" on page 226

To save device settings

1. Press FILE > "Device Settings > Save".
2. Configure the storage location as described in "To select the storage directory" on page 218.
3. Enter the file name as described in "To define a new file or directory name" on page 218.
4. Optionally, press "Comment" and enter a description of the settings.
5. Press "Save".

Note: To save the device settings several times by pressing simply the PRINT key, assign the "Device Settings" to the PRINT key as described in chapter 13.2.2.1, "Configuring the PRINT-Key Behavior", on page 224.

To load device settings

1. Press FILE > "Device Settings > Load".

   A file explorer is displayed.

2. If necessary, select the storage device and directory described in "To select the storage directory" on page 218.

3. Select the file that contains the device settings. Use the "Navigation" knob to scroll through the files.

4. Press "Load".

   The saved settings are loaded to the R&S RTM.

13.2.3.2 Device Settings Menu

With FILE > "Device Settings" you open a menu to manage instrument configuration files.

Save....226
└ Setup & Label....226
Load....226
Import/Export Device Settings....227
Memory Usage....227
Default sett....227

Save
Opens the "Save" menu, see "Save Menu" on page 220.

In addition to the common save functions, specific functions are available.

Setup & Label ← Save
Saves the the device settings together with the label list to the selected storage directory in one file. The used file name is displayed when storage is completed.

This function is available if option R&S RTM-K1 or K3 is installed (protocols I^2C, LIN, CAN), and a label list was loaded and applied to the protocol data.

When you load a setting file with label list to an instrument, the label list is loaded together with the instrument settings. A previously loaded label list will be overwritten.

Load
Opens the "Load" menu, see "Load Menu" on page 221.

Import/Export Device Settings
Opens the "Import/Export" menu, see "Import/Export Menu" on page 222.

Memory Usage
Displays information on the instrument and information on used and available memory space on all available storage devices.

Default sett.
Restores the default device settings. These settings, among others, are also restored with the PRESET key.

13.2.4 Waveforms

A waveform can be saved in two ways:

- As a reference waveform for later use with R&S RTM: REF key
  See: chapter 5, "Reference Waveforms", on page 74
- As data in various formats directly to a USB flash drive for analysis by other means: FILE > "Waveforms".
  This way is described in the current chapter.
  If you want to save many waveforms, you can assign the function to the PRINT key. Infrequent save operations can be started from the "File" menu. See also: chapter 13.2.2, "Quick Access with PRINT key", on page 223.

13.2.4.1 Waveform File Formats

Data of all waveforms - channel, reference, and math waveforms - is saved as a succession of values or pairs of values. Pairs of values are written as two consecutive single values. Depending on the file format, only amplitude values are stored, or the amplitude values are stored together with their time value, or frequency value in FFT mode.

With export/import, you can change the target file format and convert the data.

In order to reload waveform data as a reference waveform, it must be stored in TRF or CSV format.

TRF Format

TRF is the specific binary format for reference waveforms of the R&S RTM. It contains amplitude values or pairs of values, time information (time of the first sample and the sample interval) and current instrument settings. The data can be loaded as reference waveform for further use on the instrument. It is not intended for analysis outside the R&S RTM.

CSV Format

In a Comma Separated Values text file, the waveform is stored in a two-columned table. Columns are separated by a comma, and the lines are separated by line breaks `\r\n` (`0x0D 0x0A`). Values are listed in scientific notation.

The first column contains the time values of the samples in relation to the trigger point, and the second column contains the associated amplitude values. The first line indicates the units of the values in each column, and the name of the waveform. Pairs of values are listed as two single values with the same time value (minimum and maximum).

The data can be loaded back to the instrument for further use.

Example CSV1: Waveform of channel 1, single values

```
[s],CH1[V]
-1.1996E-02,1.000E-02
-1.1992E-02,1.000E-02
-1.1988E-02,1.000E-02
-1.1984E-02,1.000E-02
```

Example CSV2: Waveform of channel 1, pairs of values

```
[s],CH1[V]
-2.9980E+00,2.000E-05
-2.9980E+00,1.400E-04
-2.9960E+00,-1.800E-04
-2.9960E+00,1.400E-04
-2.9940E+00,-1.800E-04
-2.9940E+00,1.400E-04
```

Example CSV3: FFT

```
[Hz],FFT[dBm]
0.000000E+00,1.03746E+01
1.525879E+02,7.49460E+00
3.051758E+02,-1.19854E+01
4.577637E+02,-1.56854E+01
```

Import of CSV files: If you import a CSV file as reference waveform from a USB flash drive to the instrument, the import converts the data to TRF format. The instrument reads the first and the last time value and calculates the total time of the waveform, and it counts the number of values. Then all amplitude values are read one by one and written with an equidistant time distribution to the TRF file. If the first two time values are identical, the waveform is considered to consist of pairs of values.

TXT Format

TXT files are ASCII files that contain only amplitude values in scientific notation but no time values. Amplitude values are separated by commas. Pairs of values are listed as two subsequent single values, without any identification. There is no comma at the end of the file.

Example: TXT file

```
1.000E-02,1.000E-02,1.000E-02,1.000E-02,3.000E-02
```

BIN Format

BIN files contain binary amplitude values only but no time values. Each value has a word size of 8, or 16, or 32 bit, the word size is the same throughout the file.

Words are given in Big Endian order - beginning with the MSB (Most Significant Byte) and ending with the LSB (Least Significant Byte). Pairs of values are listed as two subsequent single values, without any identification.

13.2.4.2 Saving a Waveform to USB flash drive

If you want to save many waveforms, you can assign the function to the PRINT key. Infrequent savings can be started from the "File" menu. Before you can save the waveform, you have to configure the storage location and file format.

1. Press FILE > "Waveforms".
2. Configure the storage location as described in "To select the storage directory" on page 218.
3. Press "Waveform" and select the waveform to be stored. All active waveforms are listed.
4. Enter the file name as described in "To define a new file or directory name" on page 218.
5. Select the "Format".
   For details, see chapter 13.2.4.1, "Waveform File Formats", on page 227.
6. Press "Data" and select whether to save the displayed data or the data stored in the memory.
   For details, see "Data" on page 230.
7. Press "Save".

To save waveforms several times by pressing simply the PRINT key, assign the "Waveforms" to the PRINT key as described in chapter 13.2.2.1, "Configuring the PRINT-Key Behavior", on page 224.

13.2.4.3 Waveform Storage Settings

With FILE > "Waveforms" you open a menu to store one of the active waveforms to a USB flash drive.

For a description of the common save functions "Storage", "File Name", and "Save", see chapter 13.2.1.3, "General Storage Settings", on page 220. Specific settings for saving waveforms are described below.

Waveform....230
Format....230
Data....230

Waveform
Selects the waveform to be stored. Turn the "Navigation" knob to select one of the available waveforms (channel, reference, and math waveforms).

Format
Defines the format of the waveform storage file: BIN, CSV, TXT, or TRF. For details, see chapter 13.2.4.1, "Waveform File Formats", on page 227.

Data
Selects the amount of data points to be saved in the waveform file.

"Display Data" All waveform samples that are displayed on the screen will be saved. Exception: The "Waveform Rate" ist set to maximum sample rate, and the acquisition is stopped. In this case, the memory can contain more data samples than the display shows (decimation). To save the waveform with maximum resolution, the instrument stores the samples that are saved in the memory.

"Acq. Memory" All data samples that are stored in the memory will be saved. This setting takes effect only for stopped acquisitions and it is not available for math waveforms. For running acquisitions, always display data is stored.

Remote command:
`CHANnel<m>:DATA:POINts` on page 295

13.2.5 Screenshots

You can create a screenshot of the current display of your waveforms and measurement results and save it to a file. To optimize the output, you can configure different color modes and file formats. Alternatively, you can print screenshots to a printer.

See also: chapter 13.1, "Printing", on page 215.

If you want to save many screenshots - together with the instrument or the image only - you can assign the function to the PRINT key. Infrequent save operations can be started from the "File" menu.

See also: chapter 13.2.2, "Quick Access with PRINT key", on page 223.

13.2.5.1 Saving a Screenshot

Before you can save the screenshot, you have to configure the storage location and file format.

1. Press FILE > "Screenshots".

2. Configure the storage location as described in "To select the storage directory" on page 218.
3. Enter the file name as described in "To define a new file or directory name" on page 218.
4. Select the "Format" and the "Color mode".
   For details, see chapter 13.2.5.2, "Screenshot Storage Settings", on page 231.
5. Press "Save".

See also: chapter 13.2.2, "Quick Access with PRINT key", on page 223.

13.2.5.2 Screenshot Storage Settings

With FILE > "Screenshots" you open a menu to save or print screenshots of the current display.

For a description of the common save functions "Storage", "File Name", and "Save", see chapter 13.2.1.3, "General Storage Settings", on page 220. Specific settings for saving screenshots are described below.

Format....231
Color mode....231
Print....232

Format
Defines the format of the screenshot file. The following formats are available:

- BMP
  BitMaP is an uncompressed format, files are large and saving might take some time.
- PNG
  Portable Network Graphics is a graphic format with lossless data compression.

Remote command:
`HCOPy:LANGuage` on page 442

Color mode
Defines the color mode for saved screenshots.

"Grayscale"	Black and white output
"Color"	Color output
"Inverted"	Inverts the colors of the output, i.e. a dark waveform is printed on a white background

Remote command:
`HCOPy:COLor:SCHeme` on page 442

Print
Prints the screenshot on a printer connected to the USB connector on the front or rear panel. The printer output is configured with SETUP > "Printer".

The function is only available if a printer is connected.

Remote command:
`HCOPy[:IMMediate]` on page 442

13.2.6 References, Masks, and Equation Sets: Import/Export

The "File" menu provides the functions to copy mask files, equation sets, and reference waveform files from one storage device to another.

For details, refer to the relevant chapters:

- Reference waveforms: chapter 5, "Reference Waveforms", on page 74
- Masks: chapter 9, "Masks", on page 122
- Equation sets: chapter 7, "Mathematics", on page 98
- Export/Import procedure: chapter 13.2.1.2, "Importing and Exporting Data", on page 218

14 General Instrument Setup

This chapter describes the firmware update, the activation of new options, and all softkeys of the "Setup" menu.

The usage of the functions except of update is described in other chapters depending on the usage context:

- chapter "Defining General Instrument Settings" in the "Getting Started" manual: configuring date, time, interface and help language, and sounds;
- chapter 15.1.2, "Setting Up a LAN Connection", on page 243.

14.1 Firmware and Options

- Updating Firmware....233
- Activating Options....234

14.1.1 Updating Firmware

This chapter describes how to update the instrument's firmware and the interface firmware.

You should update the instrument and interface firmware in regular intervals to take advantage of new functions and solve possible problems.

1. Download the current firmware package from the instrument's Web page: http://www.scope-of-the-art.com/product/rtm.html under "Downloads > Firmware".

   The zip package contains the instrument firmware and interface firmware for all R&S RTM20xx types.
2. Extract the zip package and copy the required files to a USB flash drive.
3. Insert the USB flash drive in the instrument.
4. Press SETUP.
5. Press "More".
6. Press "Update > Firmware".

   The currently installed firmware version as well as all available update versions are displayed.
7. Press "Execute" to start the firmware update.

To update the interface firmware

1. Insert a USB flash drive containing an interface update file in the instrument.

2. Press SETUP > "Update > Interface".

   The currently installed firmware version as well as all available update versions are displayed.

3. Press "Execute" to install the available updates.

14.1.2 Activating Options

You need the material number and serial number of your instrument to get a license key. New R&S RTM options must be activated using the license key supplied by Rohde & Schwarz. The license key can be read from a license file or entered manually.

A detailed description of the key activation procedure is delivered together with the license key information.

14.2 Reference for Setup

The SETUP key provides functions for basic instrument settings and allows you to update the instrument's firmware and help files:

Time Reference....235
Menu Off....235
Language....236
Date & Time....236
└ Year/Month/Day/Hour/Minute....236
Interface....236
└ USB....236
└ LAN....236
└ IEEE488....236
└ Parameter....237
└ DHCP....237
└ Next....237
└ Up....237

└ Down....237
└ Default....237
└ Save....237
Device Information....237
Update....237
└ Firmware....237
└ Execute....237
└ Interface....238
└ Execute....238
└ Upgrade....238
└ Read keys from license file....238
└ Input key manually....238
Printer....238
Sound....238
└ Control Beep....238
└ Error Beep....238
└ Trigger Beep....238
Self Alignment....239
└ Self Test & Self Alignment....239
└ Self Alignment....239
└ Start....239
└ Abort....239
└ Log File....239
Probe Adjust....239
└ 1kHz....239
└ 1MHz....239
└ Automatic....240
Secure Erase....240
Device Name....240
LED Intensity....240
Trigger Output....240
└ Output....240
└ Polarity....240
└ Pulse width....240

Time Reference
Defines the time reference point in the diagram, i.e. the point at which the trigger is 0s. The reference point is defined as an offset of divisions from the center in the diagram. By default, the reference point 0s is displayed in the center of the window, which corresponds to 0 divisions.

The scaling of the waveform depends on this reference point.

Remote command:
`TIMebase:REFerence` on page 284

Menu Off
Defines how long a selection menu for a softkey is displayed before it automatically closes again.

Language
Selects the language in which the key labels, help and other screen information is displayed. Currently, the help is available only in English.

Remote command:
DISPlay:LANGuage on page 450

Date & Time
Provides softkeys to set the current date and time in the instrument.

Year/Month/Day/Hour/Minute ← Date & Time
Change the date and time settings individually. Changes are only adopted by the instrument after you press "Save and Back".

Remote command:
SYSTem:DATE on page 451
SYSTem:TIME on page 451

Interface
Activates or deactivates additional instrument interfaces. Using these interfaces you can communicate with the instrument, for example to read out data or automate the measuring station. Various interfaces are available as options for the instrument and are installed in a specific slot at the rear. Depending on the installed interface, additional parameters may be definable via the "Parameter" softkey after the interface has been activated.

USB ← Interface
Activates the (Type B) USB interface for remote control. The USB interface provides a simple way to connect the instrument to a PC. The USB 2.0 standard is supported. Use a connection cable that is suitable for a "Type B" USB interface.

No settings are available for the USB interface.

Note: You cannot connect a printer via the Type B USB interface. Use one of the Type A USB interfaces on the rear or front panel to connect a printer.

LAN ← Interface
Activates the LAN interface which allows you to connect the instrument to various other devices. Access to the instrument is controlled via its IP address.

By default, the instrument is set to use DHCP. If the instrument cannot find a DHCP server, it takes about two minutes until the LAN menu is available.

The interface is configured using the Parameter softkey. See also: chapter 15.1.2, "Setting Up a LAN Connection", on page 243.

IEEE488 ← Interface
Activates the IEEE488 interface, also known as a "General Purpose Interface Bus" (GPIB). Using this interface, up to 15 devices can be connected to the instrument. Each device is identified by a unique number, which is defined within the device.

The interface is configured using the Parameter softkey. For details see chapter 15.1.2, "Setting Up a LAN Connection", on page 243.

Parameter ← Interface
Provides a settings dialog to configure the active additional interface. Changes are only adopted by the instrument after you press "Save".

DHCP ← Parameter ← Interface
Activates or deactivates usage of the Dynamic Host Configuration Protocol (DHCP). If the network supports dynamic TCP/IP configuration using DHCP, all address information can be assigned automatically.

Next ← Parameter ← Interface
For settings that require several entries in one row, "Next" selects the next entry.

To select the next setting in the dialog, press "Down", to select the previous setting, press "Up".

Up ← Parameter ← Interface
Selects the previous setting in the dialog.

Down ← Parameter ← Interface
Selects the next setting in the dialog.

Default ← Parameter ← Interface
Restores the default interface settings.

Save ← Parameter ← Interface
Saves the changes to the instrument and closes the dialog.

Device Information
Displays insformation on the instrument, such as its serial number, the installed software version and hardware information. This information is required in case of a support request.

Update
Provides functions to update the help files or firmware of the instrument or interfaces.

Firmware ← Update
Allows you to update the instrument firmware. The currently installed firmware version is displayed, as well as all available update versions if a USB flash drive containing an update is identified. The instrument is only updated when you press "Execute".

Note: You should update the instrument firmware in regular intervals to take advantage of new functions and solve possible problems.
The online help is not included in the firmware update package. Update the online help separately to get the latest information.

Execute ← Firmware ← Update
The instrument firmware is updated.

Interface ← Update
Some interfaces are provided with their own instrument-independant firmware. This interface firmware can also be updated. The currently installed firmware version is displayed, as well as all available update versions, if a USB flash drive containing an update is identified. The instrument is only updated when you press "Execute".

Note: You should update the interface firmware in regular intervals to take advantage of new functions and solve possible problems.

Execute ← Interface ← Update
The interface firmware is updated.

Upgrade ← Update
Provides functions to activate options.

Read keys from license file ← Upgrade ← Update
Select the storage and directory where your license file is stored, and press "Load" to activate the options.

Input key manually ← Upgrade ← Update
Opens the on-screen keyboard to enter the license key of the option.

Printer
Opens a menu to configure the output on the printer: paper format, orientation, color, and printer language. The printer has to be connected to a (Type A) USB port.

For details, see chapter 13.1.2, "Printer Settings", on page 216.

Sound
Defines the event types for which a sound is to be generated by the instrument. Switch the sound for a particular event type on or off by selecting the corresponding softkey. Active sounds are highlighted.

Control Beep ← Sound
Generates a sound for general control events, e.g. reaching the rotary encoder end or changing the measuring mode in the "Automeasure" menu.

Remote command:
`SYSTem:BEEPer:CONTrol:STATe` on page 452

Error Beep ← Sound
Generates a a sound if an error occurs in the instrument, e.g. when the input exceeds 50 Ω or a false value is entered in a dialog.

Remote command:
`SYSTem:BEEPer:ERRor:STATe` on page 452

Trigger Beep ← Sound
Generates a sound when the trigger condition is fulfilled.

Remote command:
`SYSTem:BEEPer:TRIG:STATe` on page 452

Self Alignment
Opens a submenu to perform selftest and self-alignment of the instrument and to check the results.

Self Test & Self Alignment ← Self Alignment
Checks if a self-alignment has been executed successfully. If not, the self-alignment is executed. To start the process, press the "Start" softkey.

Self Alignment ← Self Alignment
Allows you to execute an internal self-alignment of the instrument. Alignment is only executed when you press the "Start" softkey.

When data from several input channels is displayed at the same time, it may be necessary to align the data in order to synchronize the time bases, amplitudes, and positions. This is the case, for example, when strong temperature changes occur.

Start ← Self Alignment
Starts the internal self-calibration of the instrument. Status information is displayed on the screen.

Abort ← Self Alignment
Aborts the internal self-calibration of the instrument.

Log File ← Self Alignment
The log file records the results of the self-alignment. You can set et the extend of the log file and export it.

"No Log File"	No log file is written
"Standard Log File"	Default logging
"Extended Log File"	Complete log results are written
"Export"	Opens the submenu to store the log file on USB stick. See also: "Storage Directory Menu" on page 221.

Probe Adjust
A R&S RTM allows you to adjust a probe without further devices. Two connector pins are located on the front panel. The left pin is on ground level. The right pin supplies a square wave signal for the adjustment. In this menu you can choose between two frequencies (1 kHz, 1 MHz) or allow the detection of an automatic setting by the instrument. The rise time does not differ between the settings.

1kHz ← Probe Adjust
A square wave with a frequency of f = 1 kHz is generated at the "Probe Adjust" pin. Use this setting to adjust the LF band of the probe.

1MHz ← Probe Adjust
A square wave with a frequency of f = 1 MHz is generated at the "Probe Adjust" pin. Use this setting to adjust the HF band of the probe.

Automatic ← Probe Adjust
A square wave is generated at the "Probe Adjust" pin. The frequency of the square wave depends on the defined time base. If the time base becomes too small to display the 1 kHz wave, it is automatically switched to a 1 MHz wave.

Secure Erase
Deletes current instrument configuration data and user data (for example, reference files, equation sets, masks) from the internal storage. Calibration data remains in the storage.

Use this function before you send the instrument to the service. If the instrument is used in a secured environment, the function ensures that all sensitive data is removed before the instrument leaves the secured area.

To start secure erase, select "OK". Do not turn off the instrument before the process has been completed!

See also: document "Resolving Security Issues When Working in Secure Areas" that is delivered on the documentation CD-ROM and on the R&S RTM internet web page.

Device Name
Enter the name of the instrument.

LED Intensity
Defines the luminosity of illuminated front panel keys and rotary knobs.

Trigger Output
Opens the "Trigger Output" menu.

Output ← Trigger Output
Enables the trigger out signal and defines when a trigger out pulse is generated: on trigger event, or on mask violation.

Remote command:
`TRIGger:OUT:MODE` on page 450

Polarity ← Trigger Output
Sets the polarity of the trigger out pulse.

Remote command:
`TRIGger:OUT:POLarity` on page 451

Pulse width ← Trigger Output
Defines the pulse width of the trigger out pulse.

Remote command:
`TRIGger:OUT:PLENgth` on page 451

15 Remote Control

15.1 Basics

This chapter provides basic information on operating an instrument via remote control.

15.1.1 Remote Control Interfaces

For remote control, the LAN, USB or the GPIB interface can be used. The GPIB interface (Option RTM-B10) replaces the LAN / USB type B interface module on the rear panel.

Table 15-1: Remote control interfaces and protocols

Interface	Protocols, address string	Remarks
Local Area Network (LAN)	VXI-11 protocol: TCPIP::<IP_address>[::inst0]::INSTR Raw socket mode: TCPIP::<IP_address>::<IP_port>::SOCKET	The LAN connector is located on the rear panel of the instrument. See also: • chapter 15.1.1.1, "LAN Interface", on page 242 • chapter 15.1.2, "Setting Up a LAN Connection", on page 243
USB	The instrument is addressed by the COM port number.	A USB type B connector is located on the rear panel of the instrument. Connection requires installation of an USB driver. Contact your Rohde & Schwarz service center to get the driver. See also: • chapter 15.1.1.2, "USB Interface", on page 242
GPIB (IEC/IEEE Bus Interface)	GPIB::primary address[::INSTR] (no secondary address)	An optional GPIB bus interface according to standard IEC 625.1/IEEE 488.1 can be mounted on the rear panel of the instrument. See also: chapter 15.1.1.3, "GPIB Interface (IEC/IEEE Bus Interface)", on page 242.

Within this interface description, the term GPIB is used as a synonym for the IEC/IEEE bus interface.

SCPI compatibility

SCPI commands (Standard Commands for Programmable Instruments) are used for remote control. The SCPI standard is based on standard IEEE 488.2 and aims at the standardization of device-specific commands, error handling and the status registers. The tutorial "Automatic Measurement Control - A tutorial on SCPI and IEEE 488.2" from John M. Pieper (R&S order number 0002.3536.00) offers detailed information on concepts and definitions of SCPI. The instrument supports the SCPI version 1999.

SCPI-confirmed commands are explicitly marked in the command reference chapters. Commands without SCPI label are device-specific, however, their syntax follows SCPI rules.

15.1.1.1 LAN Interface

The R&S RTM is equipped with a network interface and can be connected to an Ethernet LAN (local area network) for remote control of the instrument. The instrument accepts remote commands via the LAN interface using the VISA library. VISA must be installed on the control computer.

The R&S RTM supports two ways of LAN communication:

- VXI-11 protocol: a protocol that has been specifically developed for test and measurement instruments. It is the recommended protocol for remote control via LAN.
- Raw socket mode: a synchronous, streaming oriented protocol. Consequently, raw socket communication does not support asynchronous events like Service Request (SRQ) or Device Clear (DCL).

See also: chapter 15.1.2, "Setting Up a LAN Connection", on page 243.

VXI-11 Protocol

The VXI-11 standard is based on the ONC RPC (Open Network Computing Remote Procedure Call) protocol which in turn relies on TCP/IP as the network/transport layer. The TCP/IP network protocol and the associated network services are preconfigured. TCP/IP ensures connection-oriented communication, where the order of the exchanged messages is adhered to and interrupted links are identified. With this protocol, messages cannot be lost.

15.1.1.2 USB Interface

For remote control via the USB connection, the PC and the instrument must be connected via the USB type B interface. The USB connection requires the VISA library and the USB driver to be installed. VISA detects the R&S instrument at the assigned serial port when the USB connection is established. You do not have to enter an address string.

Contact your Rohde & Schwarz service center to get the USB driver.

15.1.1.3 GPIB Interface (IEC/IEEE Bus Interface)

The GBIP interface is optional (option RTM-B10). It replaces the LAN / USB type B interface module on the rear panel. Thus, remote control is possible either with LAN or USB connection, or with GBIP.

To be able to control the instrument via the GPIB bus, the instrument and the controller must be linked by a GPIB bus cable. A GPIB bus card, the card drivers and the program libraries for the programming language must be provided in the controller. The controller must address the instrument with the GPIB instrument address.

Characteristics

The GPIB interface is described by the following characteristics:

- Up to 15 instruments can be connected
- The total cable length is restricted to a maximum of 15 m; the cable lenth between two instruments should not exceed 2m.
- A wired "OR"-connection is used if several instruments are connected in parallel.

GPIB Instrument Address

In order to operate the instrument via remote control, it must be addressed using the GPIB address. The remote control address is factory-set to 20, but it can be changed in the network environment settings or in the "Setup" menu under "Interface > Parameter". For remote control, addresses 0 through 30 are allowed. The GPIB address is maintained after a reset of the instrument settings.

15.1.2 Setting Up a LAN Connection

15.1.2.1 Connecting the Instrument to the Network

The network card can be operated with a 10 Mbps Ethernet IEEE 802.3 or a 100 Mbps Ethernet IEEE 802.3u interface.

NOTICE

Risk of network failure

Before connecting the instrument to the network or configuring the network, consult your network administrator. Errors may affect the entire network.

► To establish a network connection, connect a commercial RJ-45 cable to one of the LAN ports of the instrument and to a PC.

15.1.2.2 Configuring LAN Parameters

Depending on the network capacities, the TCP/IP address information for the instrument can be obtained in different ways.

- If the network supports dynamic TCP/IP configuration using the Dynamic Host Configuration Protocol (DHCP), and a DHCP server is available, all address information can be assigned automatically.
- Otherwise, the address must be set manually. Automatic Private IP Addressing (APIPA) is not supported.
  See: "Configuring LAN parameters manually (no DHCP)" on page 244

By default, the instrument is configured to use dynamic TCP/IP configuration and obtain all address information automatically. This means that it is safe to establish a physical connection to the LAN without any previous instrument configuration.

NOTICE

Risk of network errors

Connection errors can affect the entire network. If your network does not support DHCP, or if you choose to disable dynamic TCP/IP configuration, you must assign valid address information before connecting the instrument to the LAN. Contact your network administrator to obtain a valid IP address.

Configuring LAN parameters manually (no DHCP)

1. Disconnect the R&S RTM from the LAN.
2. Restart the instrument.
3. Press the SETUP key and then the "Interface" softkey.
4. Wait about two minutes until the LAN menu is available. Press the "LAN" softkey.

   Note: By default, the instrument is set to use DHCP. If the instrument cannot find a DHCP server, it takes some time until the LAN settings can be accessed.
5. Press the "Parameter" softkey.

   The "LAN settings" dialog box is displayed.

Some data is displayed for information only and cannot be edited. This includes the "MAC" (physical) address of the connector and the "Link" status information.

6. If the LAN does not support DHCP, or the instrument is directly connected with a computer, disable DHCP: Press the "DHCP" softkey so that it is not highlighted (off).
7. Define the IP address of the instrument by entering each of the four blocks individually.
   a) Define the first block number using the Navigation knob.
   b) Press "Next" to move to the next block and define the number.
   c) When the IP address is complete, press "Down" to continue with the next setting.
8. Define the "Subnetmask" and "Gateway" in the same way as the IP address.
9. Select the "IP Port" - the port number for raw socket communication.
10. Select the "HTTP Port" used by the instrument.
11. Select the "Transfer" mode. This mode can either be determined automatically ("Auto" setting), or you can select a combination of a transfer rate and half or full duplex manually.

12. Press "Save" to save the LAN parameters on the instrument.

    The "Link" status information at the bottom of the dialog box indicates whether a LAN connection was established successfully.

Checking LAN and SCPI connection

1. Check the LAN connection using ping: `ping xxx.yyy.zzz.xxx`.
2. If the computer can access the instrument, enter the IP address of the R&S RTM in the address line of the internet browser on your computer: *http//:xxx.yyy.zzz.xxx*

   The "Instrument Home" page appears. It provides information on the instrument and the LAN connection.

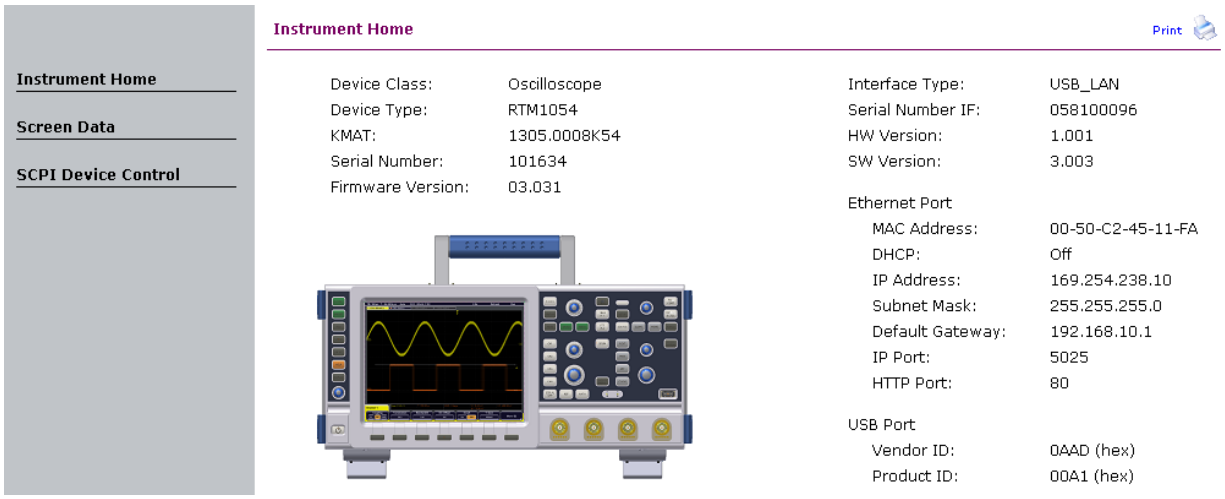

3. On the "Screen Data" page, a copy of the instrument screen is shown. To get the current screen content from the instrument, click "Update".
   To save the screen copy, right-click the picture and select "Save picture as".
4. On the "SCPI Device Control" page, you can check if the transfer of remote commands is working. You can enter a single command, for example; `*IDN?`, and transmit it with "Send". Do not press the Enter key.

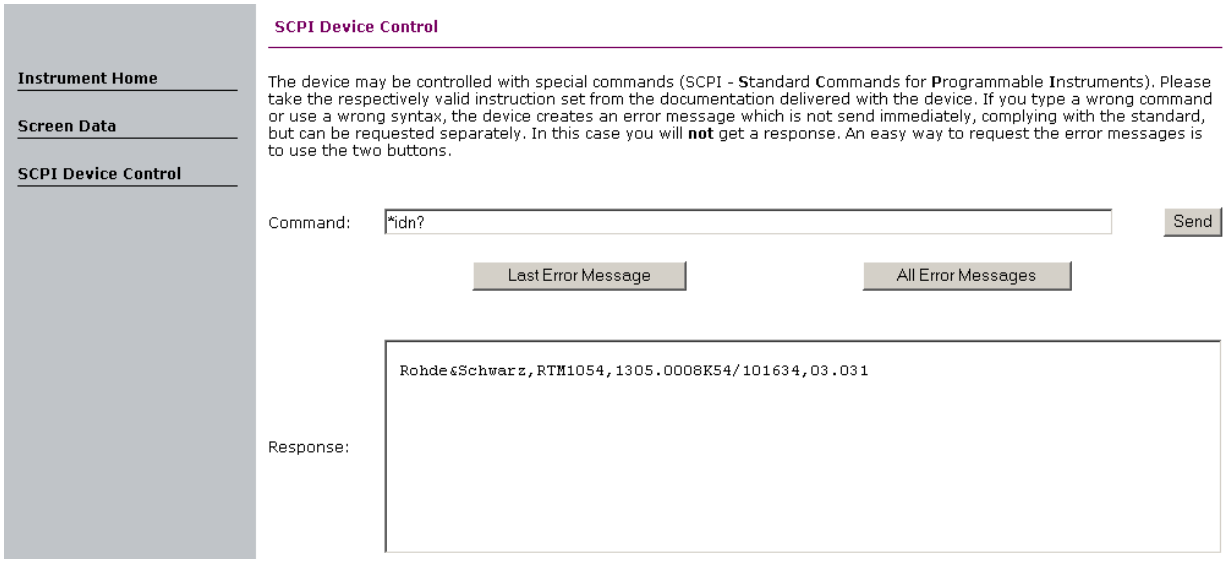
SCPI Device Control
Instrument Home
Screen Data
SCPI Device Control
The device may be controlled with special commands (SCPI - Standard Commands for Programmable Instruments). Please take the respectively valid instruction set from the documentation delivered with the device. If you type a wrong command or use a wrong syntax, the device creates an error message which is not send immediately, complying with the standard, but can be requested separately. In this case you will not get a response. An easy way to request the error messages is to use the two buttons.
Command:
*idn?
Send
Last Error Message
All Error Messages
Response:
Rohde&Schwarz,RTM1054,1305.0008K54/101634,03.031

15.1.2.3 Connecting with the Instrument: VISA Address String

Only the IP address of the instrument is required to set up the connection. It identifies the instrument in the network and is part of the resource string used by the programs to identify and control the instrument. Depending on the communication mode - VXI-11 protocol or raw socket mode - the resource string has different forms.

IP address and port number are listed in the "Ethernet Settings" of R&S RTM, see also: chapter 15.1.2.2, "Configuring LAN Parameters", on page 243.

If the LAN is supported by a DNS server, the host name can be used instead of the IP address. The DNS server (Domain Name System server) translates the host name to the IP address. To assign a host name to the R&S RTM, select SETUP > "More" > "Device Name".

VXI-11 protocol

`TCPIP::<IP address>[::inst0]::INSTR`

where:

- `inst0` is the LAN device name. VISA supports several devices running on the instrument. On R&S RTM, only one device is configured, so the LAN device name can be omitted.
- `INSTR` indicates that the VXI-11 protocol is used

Example: If the instrument has the IP address *192.1.2.3*, the valid resource string is:
`TCPIP::192.1.2.3::INSTR`

With host name instead of IP address:

`TCPIP::<host name>[::inst0]::INSTR`

Example: If the computer name is *RSRT1*, the valid resource string is:
`TCPIP::RSRT1::INSTR`.

Raw socket mode

`TCPIP::<IP_address>::<IP_port>::SOCKET`

The default port number for SCPI socket communication is 5025.

Example: If the instrument has the IP address *192.1.2.3*; the valid resource string is: `TCPIP::192.1.2.3::5025::SOCKET`

With host name instead of IP address:

`TCPIP::<host_name>::<IP_port>::SOCKET`

Example: If the host name is *RSRT1*; the valid resource string is: `TCPIP::RSRT1::5025::SOCKET`

The end character must be set to linefeed.

15.1.3 Switching to Remote Control

When you switch on the instrument, it is always in manual operation state ("local" state) and can be operated via the front panel.

When you send a command from the control computer, it is received and executed by the R&S RTM. The display remains on, manual operation via the front panel is always possible.

15.1.4 Messages and Command Structure

15.1.4.1 Messages

Instrument messages are employed in the same way for all interfaces, if not indicated otherwise in the description.

See also:

- Structure and syntax of the instrument messages: chapter 15.1.4.2, "SCPI Command Structure", on page 251
- Detailed description of all messages: chapter 15.2, "Command Reference", on page 273

There are different types of instrument messages, depending on the direction they are sent:

- Commands
- Instrument responses

Commands

Commands (program messages) are messages the controller sends to the instrument. They operate the instrument functions and request information. The commands are subdivided according to two criteria:

- According to the effect they have on the instrument:
  - **Setting commands** cause instrument settings such as a reset of the instrument or setting the frequency.
  - **Queries** cause data to be provided for remote control, e.g. for identification of the instrument or polling a parameter value. Queries are formed by directly appending a question mark to the command header.
- According to their definition in standards:
  - **Common commands**: their function and syntax are precisely defined in standard IEEE 488.2. They are employed identically on all instruments (if implemented). They refer to functions such as management of the standardized status registers, reset and self test.
  - **Instrument control commands** refer to functions depending on the features of the instrument such as frequency settings. Many of these commands have also been standardized by the SCPI committee. These commands are marked as "SCPI compliant" in the command reference chapters. Commands without this SCPI label are device-specific, however, their syntax follows SCPI rules as permitted by the standard.

Instrument responses

Instrument responses (response messages and service requests) are messages the instrument sends to the controller after a query. They can contain measurement results, instrument settings and information on the instrument status.

LAN Interface Messages

In the LAN connection, the interface messages are called low–level control messages. These messages can be used to emulate interface messages of the GPIB bus.

Command	Long term	Effect on the instrument
&ABO	Abort	Aborts processing of the commands just received.
&DCL	Device Clear	Aborts processing of the commands just received and sets the command processing software to a defined initial state. Does not change the instrument setting.
&GTL	Go to Local	Transition to the "local" state (manual control).
&GTR	Go to Remote	Transition to the "remote" state (remote control).
&GET	Group Execute Trigger	Triggers a previously active instrument function (e.g. a sweep). The effect of the command is the same as with that of a pulse at the external trigger signal input.
&LLO	Local Lockout	Disables switchover from remote control to manual control by means of the front panel keys.

Command	Long term	Effect on the instrument
&NREN	Not Remote Enable	Enables switchover from remote control to manual operation by means of the front panel keys
&POL	Serial Poll	Starts a serial poll.

GPIB Interface Messages

Interface messages are transmitted to the instrument on the data lines, with the attention line (ATN) being active (LOW). They are used for communication between the controller and the instrument and can only be sent by a computer which has the function of a GPIB bus controller. GPIB interface messages can be further subdivided into:

- **Universal commands**: act on all instruments connected to the GPIB bus without previous addressing
- **Addressed commands**: only act on instruments previously addressed as listeners

Universal Commands

Universal commands are encoded in the range 10 through 1F hex. They affect all instruments connected to the bus and do not require addressing.

Command	Effect on the instrument
DCL (Device Clear)	Aborts the processing of the commands just received and sets the command processing software to a defined initial state. Does not change the instrument settings.
IFC (Interface Clear) *)	Resets the interfaces to the default setting.
LLO (Local Lockout)	The LOC/IEC ADDR key is disabled.
SPE (Serial Poll Enable)	Ready for serial poll.
SPD (Serial Poll Disable)	End of serial poll.
PPU (Parallel Poll Unconfigure)	End of the parallel-poll state.
*) IFC is not a real universal command, it is sent via a separate line; however, it also affects all instruments connected to the bus and does not require addressing	

Addressed Commands

Addressed commands are encoded in the range 00 through 0F hex. They only affect instruments addressed as listeners.

Command	Effect on the instrument
GET (Group Execute Trigger)	Triggers a previously active instrument function (e.g. a sweep). The effect of the command is the same as with that of a pulse at the external trigger signal input.
GTL (Go to Local)	Transition to the "local" state (manual control).
GTR (Go to Remote)	Transition to the "remote" state (remote control).

Command	Effect on the instrument
PPC (Parallel Poll Configure)	Configures the instrument for parallel poll.
SDC (Selected Device Clear)	Aborts the processing of the commands just received and sets the command processing software to a defined initial state. Does not change the instrument setting.

15.1.4.2 SCPI Command Structure

SCPI commands consist of a so-called header and, in most cases, one or more parameters. The header and the parameters are separated by a "white space" (ASCII code 0 to 9, 11 to 32 decimal, e.g. blank). The headers may consist of several mnemonics (keywords). Queries are formed by appending a question mark directly to the header.

The commands can be either device-specific or device-independent (common commands). Common and device-specific commands differ in their syntax.

Syntax for Common Commands

Common (=device-independent) commands consist of a header preceded by an asterisk (*) and possibly one or more parameters.

Examples:

*RST	RESET	Resets the instrument.
*ESE	EVENT STATUS ENABLE	Sets the bits of the event status enable registers.
*ESR?	EVENT STATUS QUERY	Queries the contents of the event status register.
*IDN?	IDENTIFICATION QUERY	Queries the instrument identification string.

Syntax for Device-Specific Commands

Not all commands used in the following examples are necessarily implemented in the instrument.

For demonstration purposes only, assume the existence of the following commands for this section:

- `DISPlay[:WINDow<1...4>]:MAXimize <Boolean>`
- `FORMat:READings:DATA <type>[,<length>]`
- `HardCOPy:DEVice:COLor <Boolean>`
- `HardCOPy:DEVice:CMAP:COLor:RGB <red>,<green>,<blue>`
- `HardCOPy[:IMMediate]`
- `HardCOPy:ITEM:ALL`
- `HardCOPy:ITEM:LABel <string>`
- `HardCOPy:PAGE:DIMensions:QUADrant[<N>]`
- `HardCOPy:PAGE:ORIentation LANDscape | PORTrait`
- `HardCOPy:PAGE:SCALe <numeric value>`
- `MMEMory:COPY <file_source>,<file_destination>`
- `SENSE:BANDwidth|BWIDth[:RESolution] <numeric_value>`
- `SENSe:FREQuency:STOP <numeric value>`
- `SENSe:LIST:FREQuency <numeric_value>{,<numeric_value>}`

Long and short form

The mnemonics feature a long form and a short form. The short form is marked by upper case letters, the long form corresponds to the complete word. Either the short form or the long form can be entered; other abbreviations are not permitted.

Example:

`HardCOPy:DEVice:COLor ON` is equivalent to `HCOP:DEV:COL ON`.

Case-insensitivity

Upper case and lower case notation only serves to distinguish the two forms in the manual, the instrument itself is case-insensitive.

Numeric suffixes

If a command can be applied to multiple instances of an object, e.g. specific channels or sources, the required instances can be specified by a suffix added to the command. Numeric suffixes are indicated by angular brackets (<1...4>, <n>, <i>) and are replaced by a single value in the command. Entries without a suffix are interpreted as having the suffix 1.

Example:

Definition: `HardCOPy:PAGE:DIMensions:QUADrant[<N>]`

Command: `HCOP:PAGE:DIM:QUAD2`

This command refers to the quadrant 2.

Different numbering in remote control

For remote control, the suffix may differ from the number of the corresponding selection used in manual operation. SCPI prescribes that suffix counting starts with 1. Suffix 1 is the default state and used when no specific suffix is specified.

Optional mnemonics

Some command systems permit certain mnemonics to be inserted into the header or omitted. These mnemonics are marked by square brackets in the description. The instrument must recognize the long command to comply with the SCPI standard. Some commands are considerably shortened by these optional mnemonics.

Example:

Definition: `HardCOPy[:IMMediate]`

Command: `HCOP:IMM` is equivalent to `HCOP`

Optional mnemonics with numeric suffixes

Do not omit an optional mnemonic if it includes a numeric suffix that is relevant for the effect of the command.

Example:

Definition:`DISPlay[:WINDow<1...4>]:MAXimize <Boolean>`

Command: `DISP:MAX ON` refers to window 1.

In order to refer to a window other than 1, you must include the optional `WINDow` parameter with the suffix for the required window.

`DISP:WIND2:MAX ON` refers to window 2.

Parameters

Parameters must be separated from the header by a "white space". If several parameters are specified in a command, they are separated by a comma (,). For a description of the parameter types, refer to "SCPI Parameters" on page 254.

Example:

Definition:`HardCOPy:DEVice:CMAP:COLor:RGB <red>,<green>,<blue>`

Command:`HCOP:DEV:CMAP:COL:RGB 3,32,44`

Special characters

|	**Parameters**
	A vertical stroke in parameter definitions indicates alternative possibilities in the sense of "or". The effect of the command differs, depending on which parameter is used.
	Example:
	Definition:`HardCOPy:PAGE:ORIentation LANDscape | PORTrait`
	Command `HCOP:PAGE:ORI LAND` specifies landscape orientation
	Command `HCOP:PAGE:ORI PORT` specifies portrait orientation
	Mnemonics
	A selection of mnemonics with an identical effect exists for several commands. These mnemonics are indicated in the same line; they are separated by a vertical stroke. Only one of these mnemonics needs to be included in the header of the command. The effect of the command is independent of which of the mnemonics is used.
	Example:
	Definition`SENSE:BANDwidth|BWIDth[:RESolution] <numeric_value>`
	The two following commands with identical meaning can be created:
	`SENS:BAND:RES 1`
	`SENS:BWID:RES 1`

[ ]	mnemonics in square brackets are optional and may be inserted into the header or omitted. **Example**: `HardCOPy[:IMMediate]` `HCOP:IMM` is equivalent to `HCOP`

{ }	Parameters in curly brackets are optional and can be inserted once or several times, or omitted.
	Example: `SENSe:LIST:FREQuency <numeric_value>{,<numeric_value>}`
	The following are valid commands:
	`SENS:LIST:FREQ 10`
	`SENS:LIST:FREQ 10,20`
	`SENS:LIST:FREQ 10,20,30,40`

SCPI Parameters

Many commands are supplemented by a parameter or a list of parameters. The parameters must be separated from the header by a "white space" (ASCII code 0 to 9, 11 to 32 decimal, e.g. blank). Allowed parameters are:

- Numeric values
- Special numeric values
- Boolean parameters
- Text
- Character strings
- Block data

The parameters required for each command and the allowed range of values are specified in the command description.

Numeric values

Numeric values can be entered in any form, i.e. with sign, decimal point and exponent. Values exceeding the resolution of the instrument are rounded up or down. The mantissa may comprise up to 255 characters, the exponent must lie inside the value range -32000 to 32000. The exponent is introduced by an "E" or "e". Entry of the exponent alone is not allowed. In the case of physical quantities, the unit can be entered. Allowed unit prefixes are G (giga), MA (mega), MOHM and MHZ are also allowed), K (kilo), M (milli), U (micro) and N (nano). If the unit is missing, the basic unit is used.

Example: `SENSe:FREQ:STOP 1.5GHz` = `SENSe:FREQ:STOP 1.5E9`

Units

For physical quantities, the unit can be entered. Allowed unit prefixes are:

- G (giga)
- MA (mega), MOHM, MHZ
- K (kilo)
- M (milli)
- U (micro)
- N (nano)

If the unit is missing, the basic unit is used.

Example:

`SENSe:FREQ:STOP 1.5GHz` = `SENSe:FREQ:STOP 1.5E9`

Some settings allow relative values to be stated in percent. According to SCPI, this unit is represented by the `PCT` string.

Example:

`HCOP:PAGE:SCAL 90PCT`

Special numeric values

The texts listed below are interpreted as special numeric values. In the case of a query, the numeric value is provided.

- **MIN/MAX**
  MINimum and MAXimum denote the minimum and maximum value.

Example:

Setting command: `SENSe:LIST:FREQ MAXimum`

Query: `SENS:LIST:FREQ?, Response: 3.5E9`

Queries for special numeric values

The numeric values associated to `MAXimum/MINimum` can be queried by adding the corresponding mnemonics to the command. They must be entered following the quotation mark.

Example: `SENSe:LIST:FREQ? MAXimum`

Returns the maximum numeric value as a result.

Boolean Parameters

Boolean parameters represent two states. The "ON" state (logically true) is represented by "ON" or a numeric value 1. The "OFF" state (logically untrue) is represented by "OFF" or the numeric value 0. The numeric values are provided as the response for a query.

Example:

Setting command: `HCOPy:DEV:COL ON`

Query: `HCOPy:DEV:COL?`

Response: `1`

Text parameters

Text parameters observe the syntactic rules for mnemonics, i.e. they can be entered using a short or long form. Like any parameter, they have to be separated from the header by a white space. In the case of a query, the short form of the text is provided.

Example:

Setting command: `HardCOPy:PAGE:ORIentation LANDscape`

Query: `HCOP:PAGE:ORI?`

Response: `LAND`

Character strings

Strings must always be entered in quotation marks (' or ").

Example:

`HCOP:ITEM:LABel "Test1"` or `HCOP:ITEM:LABel 'Test1'`

Block data

Block data is a format which is suitable for the transmission of large amounts of data. A command using a block data parameter has the following structure:

Example:

```
FORMat:READings:DATA  #45168xxxxxxxx
```

The ASCII character # introduces the data block. The next number indicates how many of the following digits describe the length of the data block. In the example the 4 following digits indicate the length to be 5168 bytes. The data bytes follow. During the transmission of these data bytes all end or other control signs are ignored until all bytes are transmitted.

#0 specifies a data block of indefinite length. The use of the indefinite format requires a `NL^END` message to terminate the data block. This format is useful when the length of the transmission is not known or if speed or other considerations prevent segmentation of the data into blocks of definite length.

Overview of Syntax Elements

The following table provides an overview of the syntax elements:

:	The colon separates the mnemonics of a command. In a command line the separating semicolon marks the uppermost command level.
;	The semicolon separates two commands of a command line. It does not alter the path.
,	The comma separates several parameters of a command.
?	The question mark forms a query.
*****	The asterisk marks a common command.
"	Quotation marks introduce a string and terminate it.
#	The hash symbol introduces binary, octal, hexadecimal and block data. • Binary: #B10110 • Octal: #O7612 • Hexa: #HF3A7 • Block: #21312
	A "white space" (ASCII-Code 0 to 9, 11 to 32 decimal, e.g. blank) separates the header from the parameters.

Structure of a command line

A command line may consist of one or several commands. It is terminated by one of the following:

- a <New Line>
- a <New Line> with EOI
- an EOI together with the last data byte

Several commands in a command line must be separated by a semicolon ";". If the next command belongs to a different command system, the semicolon is followed by a colon.

Example:

```
MMEM:COPY "Test1","MeasurementXY";:HCOP:ITEM ALL
```

This command line contains two commands. The first command belongs to the MMEM system, the second command belongs to the HCOP system.

If the successive commands belong to the same system, having one or several levels in common, the command line can be abbreviated. To this end, the second command after the semicolon starts with the level that lies below the common levels. The colon following the semicolon must be omitted in this case.

Example:

```
HCOP:ITEM ALL; HCOP:IMM
```

This command line is represented in its full length and contains two commands separated from each other by the semicolon. Both commands are part of the `HCOP` command system, i.e. they have one level in common.

When abbreviating the command line, the second command begins with the level below HCOP. The colon after the semicolon is omitted. The abbreviated form of the command line reads as follows:

```
HCOP:ITEM ALL;IMM
```

However, a new command line always begins with the complete path.

Example:

```
HCOP:ITEM ALL
HCOP:IMM
```

Responses to Queries

A query is defined for each setting command unless explicitly specified otherwise. It is formed by adding a question mark to the associated setting command. According to SCPI, the responses to queries are partly subject to stricter rules than in standard IEEE 488.2.

- The requested parameter is transmitted without a header.
  Example: `HCOP:PAGE:ORI?`, Response: `LAND`
- Maximum values, minimum values and all other quantities that are requested via a special text parameter are returned as numeric values.
  Example: `SENSe:FREQuency:STOP? MAX`, Response: `3.5E9`
- Numeric values are output without a unit. Physical quantities are referred to the basic units or to the units set using the `Unit` command. The response `3.5E9` in the previous example stands for 3.5 GHz.
- Truth values (Boolean values) are returned as `0` (for OFF) and `1` (for ON).
  Example:
  Setting command: `HCOPy:DEV:COL ON`
  Query: `HCOPy:DEV:COL?`
  Response: `1`
- Text (character data) is returned in a short form.
  Example:
  Setting command: `HardCOPy:PAGE:ORIentation LANDscape`
  Query: `HCOP:PAGE:ORI?`
  Response: `LAND`

15.1.5 Command Sequence and Synchronization

IEEE 488.2 defines a distinction between overlapped and sequential commands:

- A sequential command is one which finishes executing before the next command starts executing. Commands that are processed quickly are usually implemented as sequential commands.
- An overlapping command is one which does not automatically finish executing before the next command starts executing. Usually, overlapping commands take longer to process and allow the program to do other tasks while being executed. If overlapping commands do have to be executed in a defined order, e.g. in order to avoid wrong measurement results, they must be serviced sequentially. This is called synchronization between the controller and the instrument.

Setting commands within one command line, even though they may be implemented as sequential commands, are not necessarily serviced in the order in which they have been received. In order to make sure that commands are actually carried out in a certain order, each command must be sent in a separate command line.

Example: Commands and queries in one message

The response to a query combined in a program message with commands that affect the queried value is not predictable.

The following commands always return the specified result:

```
:FREQ:STAR 1GHZ;SPAN 100 :FREQ:STAR?
```

Result:

`1000000000` (1 GHz)

Whereas the result for the following commands is not specified by SCPI:

```
:FREQ:STAR 1GHz;STAR?;SPAN 1000000
```

The result could be the value of `STARt` before the command was sent since the instrument might defer executing the individual commands until a program message terminator is received. The result could also be 1 GHz if the instrument executes commands as they are received.

As a general rule, send commands and queries in different program messages.

Example: Overlapping command with *OPC

The instrument implements `SINGle` as an overlapped (asynchronous) command. Assuming that `SINGle` takes longer to execute than `*OPC`, sending the following command sequence results in initiating a sweep and, after some time, setting the `OPC` bit in the `ESR`:

```
SINGle; *OPC.
```

Sending the following commands still initiates a sweep:

```
SINGle; *OPC; *CLS
```

However, since the operation is still pending when the instrument executes `*CLS`, forcing it into the "Operation Complete Command Idle" State (OCIS), `*OPC` is effectively skipped. The `OPC` bit is not set until the instrument executes another `*OPC` command.

15.1.5.1 Preventing Overlapping Execution

To prevent an overlapping execution of commands, one of the commands *OPC, *OPC? or *WAI can be used. All three commands cause a certain action only to be carried out after the hardware has been set. By suitable programming, the controller can be forced to wait for the corresponding action to occur.

Table 15-2: Synchronization using *OPC, *OPC? and *WAI

Command	Action	Programming the controller
*OPC	Sets the Operation Complete bit in the ESR after all previous commands have been executed.	• Setting bit 0 in the ESE • Setting bit 5 in the SRE • Waiting for service request (SRQ)
*OPC?	Stops command processing until 1 is returned. This is only the case after the Operation Complete bit has been set in the ESR. This bit indicates that the previous setting has been completed.	Sending *OPC? directly after the command whose processing should be terminated before other commands can be executed.
*WAI	Stops further command processing until all commands sent before *WAI have been executed.	Sending *WAI directly after the command whose processing should be terminated before other commands are executed.

Command synchronization using *WAI or *OPC? appended to an overlapped command is a good choice if the overlapped command takes only little time to process. The two synchronization techniques simply block overlapped execution of the command.

For time consuming overlapped commands it is usually desirable to allow the controller or the instrument to do other useful work while waiting for command execution. Use one of the following methods:

***OPC with a service request**

1. Set the OPC mask bit (bit no. 0) in the ESE: *ESE 1
2. Set bit no. 5 in the SRE: *SRE 32 to enable ESB service request.
3. Send the overlapped command with *OPC

4. Wait for a service request

   The service request indicates that the overlapped command has finished.

***OPC? with a service request**

1. Set bit no. 4 in the SRE: *SRE 16 to enable MAV service request.
2. Send the overlapped command with *OPC?
3. Wait for a service request

   The service request indicates that the overlapped command has finished.

Event Status Register (ESE)

1. Set the OPC mask bit (bit no. 0) in the ESE: *ESE 1
2. Send the overlapped command without *OPC, *OPC? or *WAI
3. Poll the operation complete state periodically (by means of a timer) using the sequence: *OPC; *ESR?

   A return value (LSB) of 1 indicates that the overlapped command has finished.

***OPC? with short timeout**

1. Send the overlapped command without *OPC, *OPC? or *WAI
2. Poll the operation complete state periodically (by means of a timer) using the sequence: <short timeout>; *OPC?
3. A return value (LSB) of 1 indicates that the overlapped command has finished. In case of a timeout, the operation is ongoing.
4. Reset timeout to former value
5. Clear the error queue with `SYStem:ERRor?` to remove the "-410, Query interrupted" entries.

Using several threads in the controller application

As an alternative, provided the programming environment of the controller application supports threads, separate threads can be used for the application GUI and for controlling the instrument(s) via SCPI.

A thread waiting for a *OPC? thus will not block the GUI or the communication with other instruments.

15.1.6 Status Reporting System

The status reporting system stores all information on the current operating state of the instrument, and on errors which have occurred. This information is stored in the status registers and in the error queue. Both can be queried via GPIB bus or LAN interface (`STATus`... commands).

15.1.6.1 Structure of a SCPI Status Register

Each standard SCPI register consists of 5 parts. Each part has a width of 16 bits and has different functions. The individual bits are independent of each other, i.e. each hardware status is assigned a bit number which is valid for all five parts. Bit 15 (the most significant bit) is set to zero for all parts. Thus the contents of the register parts can be processed by the controller as positive integers.

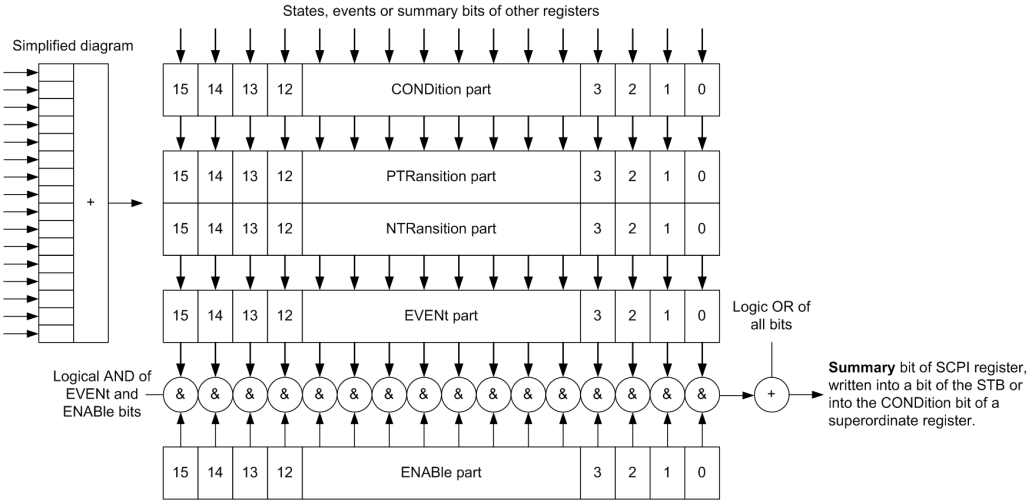
States, events or summary bits of other registers
Simplified diagram
15 14 13 12 CONDition part 3 2 1 0
15 14 13 12 PTRansition part 3 2 1 0
15 14 13 12 NTRansition part 3 2 1 0
15 14 13 12 EVENt part 3 2 1 0
Logic OR of all bits
Logical AND of EVENt and ENABle bits
Summary bit of SCPI register, written into a bit of the STB or into the CONDition bit of a superordinate register.
15 14 13 12 ENABle part 3 2 1 0

Fig. 15-1: The status-register model

Description of the five status register parts

The five parts of a SCPI register have different properties and functions:

- **CONDition**
  The `CONDition` part is written into directly by the hardware or the sum bit of the next lower register. Its contents reflect the current instrument status. This register part can only be read, but not written into or cleared. Its contents are not affected by reading.
- **PTRansition / NTRansition**
  The two transition register parts define which state transition of the `CONDition` part (none, 0 to 1, 1 to 0 or both) is stored in the `EVENt` part.
  The **Positive-TRansition** part acts as a transition filter. When a bit of the `CONDition` part is changed from 0 to 1, the associated `PTR` bit decides whether the `EVENt` bit is set to 1.
  – PTR bit =1: the `EVENt` bit is set.
  – PTR bit =0: the `EVENt` bit is not set.

  This part can be written into and read as required. Its contents are not affected by reading.
  The **Negative-TRansition** part also acts as a transition filter. When a bit of the `CONDition` part is changed from 1 to 0, the associated `NTR` bit decides whether the `EVENt` bit is set to 1.
  – NTR bit =1: the `EVENt` bit is set.
  – NTR bit =0: the `EVENt` bit is not set.

This part can be written into and read as required. Its contents are not affected by reading.

- **EVENt**
  The EVENt part indicates whether an event has occurred since the last reading, it is the "memory" of the condition part. It only indicates events passed on by the transition filters. It is permanently updated by the instrument. This part can only be read by the user. Reading the register clears it. This part is often equated with the entire register.
- **ENABle**
  The ENABle part determines whether the associated EVENt bit contributes to the sum bit (see below). Each bit of the EVENt part is "ANDed" with the associated ENABle bit (symbol '&'). The results of all logical operations of this part are passed on to the sum bit via an "OR" function (symbol '+').
  ENABle bit = 0: the associated EVENt bit does not contribute to the sum bit
  ENABle bit = 1: if the associated EVENt bit is "1", the sum bit is set to "1" as well.
  This part can be written into and read by the user as required. Its contents are not affected by reading.

Sum bit

The sum bit is obtained from the EVENt and ENABle part for each register. The result is then entered into a bit of the CONDition part of the higher-order register.

The instrument automatically generates the sum bit for each register. Thus an event can lead to a service request throughout all levels of the hierarchy.

15.1.6.2 Hierarchy of status registers

As shown in the following figure, the status information is of hierarchical structure.

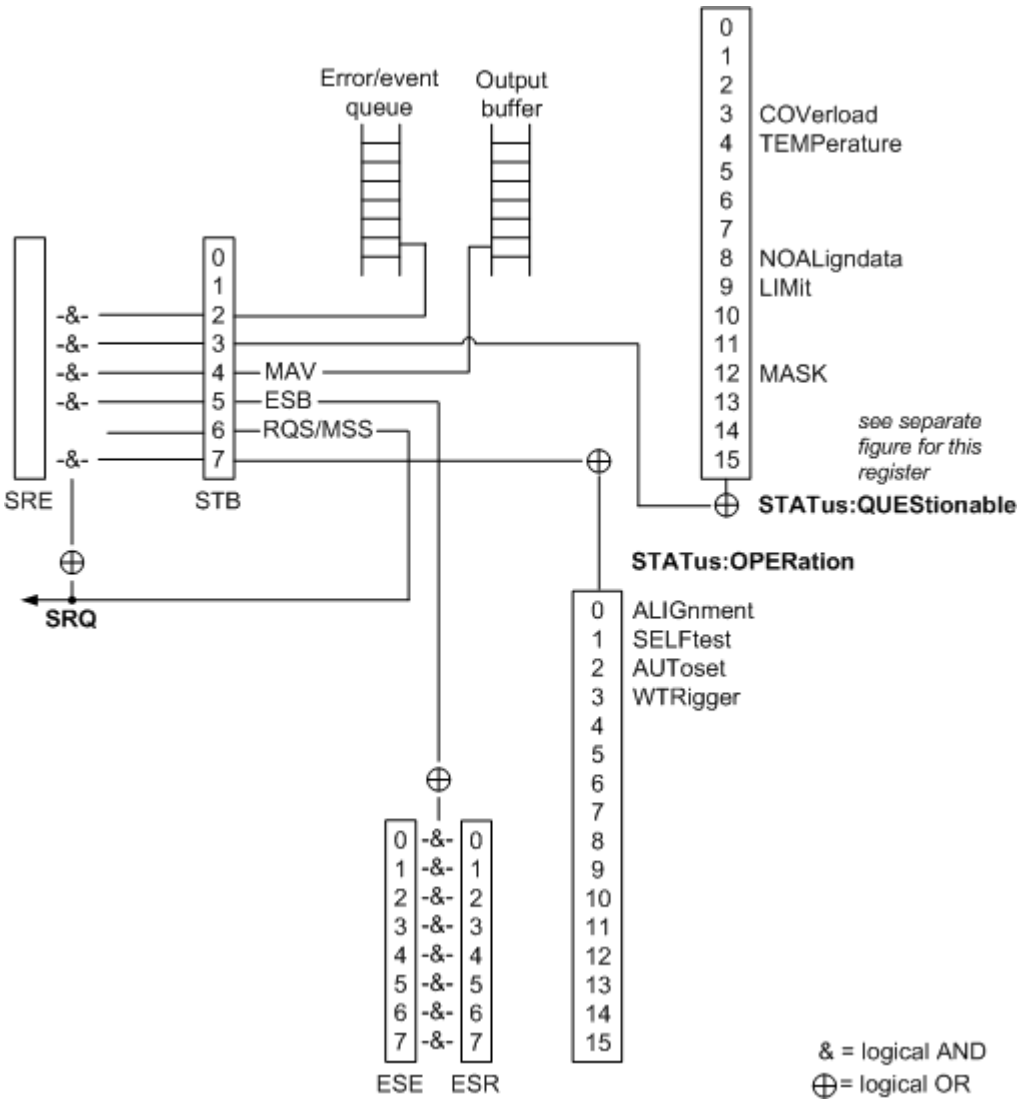

Fig. 15-2: Overview of the status registers hierarchy

- **STB, SRE**
  The STatus Byte (`STB`) register and its associated mask register Service Request Enable (`SRE`) form the highest level of the status reporting system. The `STB` provides a rough overview of the instrument status, collecting the information of the lower-level registers.
- **ESR, SCPI registers**
  The STB receives its information from the following registers:
  – The Event Status Register (`ESR`) with the associated mask register standard Event Status Enable (`ESE`).
  – The `STATus:OPERation` and `STATus:QUEStionable` registers which are defined by SCPI and contain detailed information on the instrument.
- **Output buffer**

The output buffer contains the messages the instrument returns to the controller. It is not part of the status reporting system but determines the value of the MAV bit in the STB and thus is represented in the overview.

All status registers have the same internal structure.

SRE, ESE

The service request enable register SRE can be used as ENABle part of the STB if the STB is structured according to SCPI. By analogy, the ESE can be used as the ENABle part of the ESR.

15.1.6.3 Contents of the Status Registers

In the following sections, the contents of the status registers are described in more detail.

Status Byte (STB) and Service Request Enable Register (SRE)

The STatus Byte (STB) is already defined in IEEE 488.2. It provides a rough overview of the instrument status by collecting the pieces of information of the lower registers. A special feature is that bit 6 acts as the sum bit of the remaining bits of the status byte.

The STB can thus be compared with the CONDition part of an SCPI register and assumes the highest level within the SCPI hierarchy.

The STB is read using the command *STB? or a serial poll.

The STatus Byte (STB) is linked to the Service Request Enable (SRE) register. Each bit of the STB is assigned a bit in the SRE. Bit 6 of the SRE is ignored. If a bit is set in the SRE and the associated bit in the STB changes from 0 to 1, a service request (SRQ) is generated. The SRE can be set using the command *SRE and read using the command *SRE?.

Table 15-3: Meaning of the bits used in the status byte

Bit No.	Meaning
0...1	Not used
2	Error Queue not empty The bit is set when an entry is made in the error queue. If this bit is enabled by the SRE, each entry of the error queue generates a service request. Thus an error can be recognized and specified in greater detail by polling the error queue. The poll provides an informative error message. This procedure is to be recommended since it considerably reduces the problems involved with remote control.
3	QUEStionable status register summary bit The bit is set if an EVENt bit is set in the QUEStionable status register and the associated ENABle bit is set to 1. A set bit indicates a questionable instrument status, which can be specified in greater detail by querying the STATus:QUEStionable status register.
4	MAV bit (message available) The bit is set if a message is available in the output queue which can be read. This bit can be used to enable data to be automatically read from the instrument to the controller.

Bit No.	Meaning
5	ESB bit Sum bit of the event status register. It is set if one of the bits in the event status register is set and enabled in the event status enable register. Setting of this bit indicates a serious error which can be specified in greater detail by polling the event status register.
6	MSS bit (master status summary bit) The bit is set if the instrument triggers a service request. This is the case if one of the other bits of this registers is set together with its mask bit in the service request enable register SRE.
7	`STATus:OPERation` status register summary bit The bit is set if an `EVENt` bit is set in the `OPERation` status register and the associated `ENABle` bit is set to 1. A set bit indicates that the instrument is just performing an action. The type of action can be determined by querying the `STATus:OPERation` status register.

Event Status Register (ESR) and Event Status Enable Register (ESE)

The ESR is defined in IEEE 488.2. It can be compared with the `EVENt` part of a SCPI register. The event status register can be read out using command *ESR?.

The ESE corresponds to the `ENABle` part of a SCPI register. If a bit is set in the ESE and the associated bit in the ESR changes from 0 to 1, the ESB bit in the STB is set. The ESE register can be set using the command `*ESE` and read using the command `*ESE?`.

Table 15-4: Meaning of the bits used in the event status register

Bit No.	Meaning
0	Operation Complete This bit is set on receipt of the command *OPC exactly when all previous commands have been executed.
1	Not used
2	Query Error This bit is set if either the controller wants to read data from the instrument without having sent a query, or if it does not fetch requested data and sends new instructions to the instrument instead. The cause is often a query which is faulty and hence cannot be executed.
3	Device-dependent Error This bit is set if a device-dependent error occurs. An error message with a number between -300 and -399 or a positive error number, which denotes the error in greater detail, is entered into the error queue.
4	Execution Error This bit is set if a received command is syntactically correct but cannot be performed for other reasons. An error message with a number between -200 and -300, which denotes the error in greater detail, is entered into the error queue.
5	Command Error This bit is set if a command is received, which is undefined or syntactically incorrect. An error message with a number between -100 and -200, which denotes the error in greater detail, is entered into the error queue.

Bit No.	Meaning
6	User Request This bit is set when the instrument is switched over to manual control.
7	Power On (supply voltage on) This bit is set on switching on the instrument.

STATus:OPERation Register

In the `CONDition` part, this register contains information on which actions the instrument is being executing. In the `EVENt` part, it contains information on which actions the instrument has executed since the last reading. It can be read using the commands `STATus:OPERation:CONDition?` or `STATus:OPERation[:EVENt]?`.

See also: figure 15-2

The remote commands for the STATus:OPERation register are described in chapter 15.2.17.1, "STATus:OPERation Register", on page 453.

Table 15-5: Bits in the STATus:OPERation register

Bit No.	Meaning
0	`ALIGnment` This bit is set as long as the instrument is performing a self alignment.
1	`SELFtest` This bit is set while the selftest is running.
2	`AUToset` This bit is set while the instrument is performing an auto setup.
3	`WTRIgger` This bit is set while the instrument is waiting for the trigger.
4 to 14	Not used
15	This bit is always 0.

STATus:QUEStionable Register

This register contains information about indefinite states which may occur if the unit is operated without meeting the specifications. It can be read using the commands `STATus:QUEStionable:CONDition?` on page 456 and `STATus:QUEStionable[:EVENt]?` on page 457

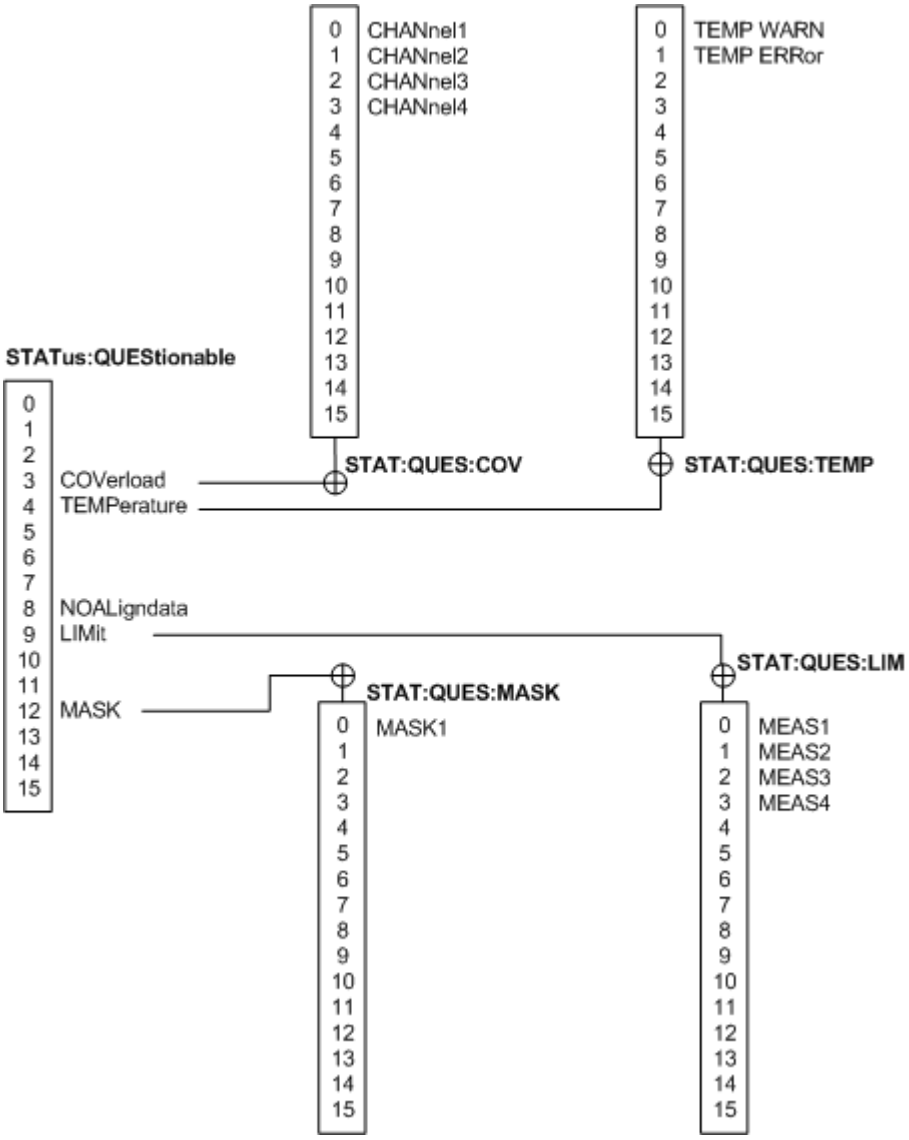
0 CHANnel1
1 CHANnel2
2 CHANnel3
3 CHANnel4
4 5 6 7 8 9 10 11 12 13 14 15
0 TEMP WARN
1 TEMP ERRor
2 3 4 5 6 7 8 9 10 11 12 13 14 15
STATus:QUEStionable
0 1 2 3 COVerload
4 TEMPerature
5 6 7 8 NOALigndata
9 LIMit
10 11 12 MASK
13 14 15
STAT:QUES:COV
STAT:QUES:TEMP
STAT:QUES:MASK
0 MASK1
1 2 3 4 5 6 7 8 9 10 11 12 13 14 15
STAT:QUES:LIM
0 MEAS1
1 MEAS2
2 MEAS3
3 MEAS4
4 5 6 7 8 9 10 11 12 13 14 15

Fig. 15-3: Overview of the STATus:QUEStionable register

Table 15-6: Bits in the STATus:QUEStionable register

Bit No.	Meaning
0 to 2	not used
3	`COVerload` This bit is set if a questionable channel overload occurs (see "STATus:QUEStionable:COVerload register" on page 269).
4	`TEMPerature` This bit is set if a questionable temperature occurs (see "STATus:QUEStionable:TEMPerature register" on page 269).
5 to 7	Not used

Bit No.	Meaning
8	NOALigndata This bit is set if no alignment data is available - the instrument is uncalibrated.
9	LIMit This bit is set if a limit value is violated (see "STATus:QUEStionable:LIMit register" on page 269).
10 to 11	Not used
12	MASK This bit is set if a mask value is violated (see "STATus:QUEStionable:MASK register" on page 270
13 to 14	Not used
15	This bit is always 0.

STATus:QUEStionable:COVerload register

This register contains all information about overload of the channels. The bit is set if the assigned channel is overloaded.

Table 15-7: Bits in the STATus:QUEStionable:COVerload register

Bit No.	Meaning
0	CHANnel1
1	CHANnel2
2	CHANnel3
3	CHANnel4

STATus:QUEStionable:TEMPerature register

This register contains information about the instrument's temperature.

Table 15-8: Bits in the STATus:QUEStionable:TEMPerature register

Bit No.	Meaning
0	TEMP WARN This bit is set if a temperature warning on channel 1, 2, 3 or 4 occured.
1	TEMP ERRor This bit is set if a temperature error on channel 1, 2, 3 or 4 occured.

STATus:QUEStionable:LIMit register

This register contains information about the observance of the limits of measurements. This bit is set if the limits of the main or additional measurement of the assigned measurement are violated.

Table 15-9: Bits in the STATus:QUEStionable:LIMit register

Bit No.	Meaning
0	MEAS1
1	MEAS2
2	MEAS3
3	MEAS4

STATus:QUEStionable:MASK register

This register contains information about the violation of masks. This bit is set if the assigned mask is violated.

Table 15-10: Bits in the STATus:QUEStionable:MASK register

Bit No.	Meaning
0	MASK1

15.1.6.4 Application of the Status Reporting System

The purpose of the status reporting system is to monitor the status of one or several devices in a measuring system. To do this and react appropriately, the controller must receive and evaluate the information of all devices. The following standard methods are used:

- **Service request** (SRQ) initiated by the instrument
- **Serial poll** of all devices in the bus system, initiated by the controller in order to find out who sent a SRQ and why
- **Parallel poll** of all devices
- Query of a **specific instrument status** by means of commands
- Query of the **error queue**

Service Request

Under certain circumstances, the instrument can send a service request (SRQ) to the controller. Usually this service request initiates an interrupt at the controller, to which the control program can react appropriately. As evident from figure 15-2, an SRQ is always initiated if one or several of bits 2, 3, 4, 5 or 7 of the status byte are set and enabled in the SRE. Each of these bits combines the information of a further register, the error queue or the output buffer. The ENABle parts of the status registers can be set such that arbitrary bits in an arbitrary status register initiate an SRQ. In order to make use of the possibilities of the service request effectively, all bits should be set to "1" in enable registers SRE and ESE.

The SRQ is the only possibility for the instrument to become active on its own. Each controller program should cause the instrument to initiate a service request if errors occur. The program should react appropriately to the service request.

Serial Poll

In a serial poll, just as with command `*STB`, the status byte of an instrument is queried. However, the query is realized via interface messages and is thus clearly faster.

The serial poll method is defined in IEEE 488.1 and used to be the only standard possibility for different instruments to poll the status byte. The method also works for instruments which do not adhere to SCPI or IEEE 488.2.

The serial poll is mainly used to obtain a fast overview of the state of several instruments connected to the controller.

Query of an instrument status

Each part of any status register can be read using queries. There are two types of commands:

- The common commands `*ESR?`, `*IDN?`, `*IST?`, `*STB?` query the higher-level registers.
- The commands of the `STATus` system query the SCPI registers (`STATus:QUEStionable...`)

The returned value is always a decimal number that represents the bit pattern of the queried register. This number is evaluated by the controller program.

Queries are usually used after an SRQ in order to obtain more detailed information on the cause of the SRQ.

Decimal representation of a bit pattern

The STB and ESR registers contain 8 bits, the SCPI registers 16 bits. The contents of a status register are specified and transferred as a single decimal number. To make this possible, each bit is assigned a weighted value. The decimal number is calculated as the sum of the weighted values of all bits in the register that are set to 1.

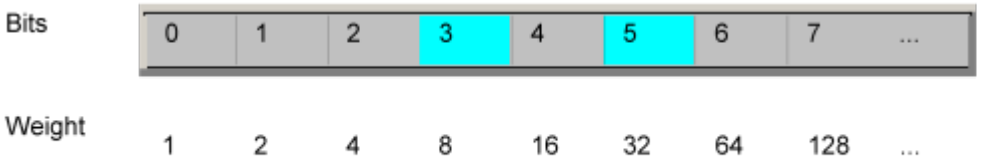

Example:

The decimal value 40 = 32 + 8 indicates that bits no. 3 and 5 in the status register (e.g. the `QUEStionable` status summary bit and the `ESB` bit in the `STatus` Byte) are set.

Error Queue

Each error state in the instrument leads to an entry in the error queue. The entries of the error queue are detailed plain text error messages that can be looked up in the Error Log or queried via remote control using `SYSTem:ERRor[:NEXT]?` or `SYSTem:ERRor:ALL?`. Each call of `SYSTem:ERRor[:NEXT]?` provides one entry from the error queue. If no error messages are stored there any more, the instrument responds with 0, "No error".

The error queue should be queried after every SRQ in the controller program as the entries describe the cause of an error more precisely than the status registers. Especially in the test phase of a controller program the error queue should be queried regularly since faulty commands from the controller to the instrument are recorded there as well.

15.1.6.5 Reset Values of the Status Reporting System

The following table contains the different commands and events causing the status reporting system to be reset. None of the commands, except `*RST` and `SYSTem:PRESet`, influence the functional instrument settings. In particular, `DCL` does not change the instrument settings.

Table 15-11: Resest of the status reporting system

Event	**Switching on supply voltage** **Power-On-Status-Clear**		**DCL, SDC** **(Device Clear, Selected Device Clear)**	***RST or SYS-Tem:PRE–Set**	**STA-Tus:PRE–Set**	***CLS**
Effect	**0**	**1**				
Clear STB, ESR	-	yes	-	-	-	yes
Clear SRE, ESE	-	yes	-	-	-	-
Clear EVENt parts of the registers	-	yes	-	-	-	yes
Clear ENABle parts of all OPERation and QUEStionable registers; Fill ENABle parts of all other registers with "1".	-	yes	-	-	yes	-
Fill PTRansition parts with "1"; Clear NTRansition parts	-	yes	-	-	yes	-
Clear error queue	yes	yes	-	-	-	yes
Clear output buffer	yes	yes	yes	1)	1)	1)
Clear command processing and input buffer	yes	yes	yes	-	-	-
1) The first command in a command line that immediately follows a <PROGRAM MESSAGE TERMINATOR> clears the output buffer.						

15.1.7 General Programming Recommendations

Initial instrument status before changing settings

Manual operation is designed for maximum possible operating convenience. In contrast, the priority of remote control is the "predictability" of the instrument status. Thus, when a command attempts to define incompatible settings, the command is ignored and the instrument status remains unchanged, i.e. other settings are not automatically adapted.

Therefore, control programs should always define an initial instrument status (e.g. using the *RST command) and then implement the required settings.

Command sequence

As a general rule, send commands and queries in different program messages. Otherwise, the result of the query may vary depending on which operation is performed first (see also Preventing Overlapping Execution).

Reacting to malfunctions

The service request is the only possibility for the instrument to become active on its own. Each controller program should instruct the instrument to initiate a service request in case of malfunction. The program should react appropriately to the service request.

Error queues

The error queue should be queried after every service request in the controller program as the entries describe the cause of an error more precisely than the status registers. Especially in the test phase of a controller program the error queue should be queried regularly since faulty commands from the controller to the instrument are recorded there as well.

15.2 Command Reference

This chapter provides the description of all remote commands available for R&S RTM. The commands are sorted according to the menu structure of the instrument. A list of commands in alphabetical order ist given in the "List of Commands" at the end of this documentation.

15.2.1 Conventions used in Remote Command Description

Note the following conventions used in the remote command descriptions:

- **Command usage**
  If not specified otherwise, commands can be used both for setting and for querying parameters.
  If a command can be used for setting or querying only, or if it initiates an event, the usage is stated explicitely.
- **Parameter usage**
  If not specified otherwise, a parameter can be used to set a value and it is the result of a query.
  Parameters required only for setting are indicated as **Setting parameters**.
  Parameters required only to refine a query are indicated as **Query parameters**.
  Parameters that are only returned as the result of a query are indicated as **Return values**.
- **Conformity**

Commands that are taken from the SCPI standard are indicated as **SCPI confirmed**. All commands used by the R&S RTM follow the SCPI syntax rules.

- **Asynchronous commands**
  A command which does not automatically finish executing before the next command starts executing (overlapping command) is indicated as an **Asynchronous command**.
- **Reset values (*RST)**
  Default parameter values that are used directly after resetting the instrument (`*RST` command) are indicated as ***RST** values, if available.

15.2.2 Common Commands

Common commands are described in the IEEE 488.2 (IEC 625-2) standard. These commands have the same effect and are employed in the same way on different devices. The headers of these commands consist of "*" followed by three letters. Many common commands are related to the Status Reporting System.

Available common commands:

*CAL?....274
*CLS....274
*ESE....275
*ESR?....275
*IDN?....275
*OPC....275
*OPT?....275
*PSC....276
*RST....276
*SRE....276
*STB?....276
*TRG....276
*TST?....277
*WAI....277

***CAL?**

Performs a self-alignment of the instrument and then generates a status response. Return values ≠ 0 indicate an error.

Usage: Query only

***CLS**

CLear Status

Sets the status byte (STB), the standard event register (ESR) and the `EVENt` part of the `QUEStionable` and the `OPERation` registers to zero. The command does not alter the mask and transition parts of the registers. It clears the output buffer.

Usage: Setting only

***ESE** <Value>

Event Status Enable

Sets the event status enable register to the specified value. The query returns the contents of the event status enable register in decimal form.

Parameters:
<Value> Range: 0 to 255

***ESR?**

Event Status Read

Returns the contents of the event status register in decimal form and subsequently sets the register to zero.

Return values:
<Contents> Range: 0 to 255

Usage: Query only

***IDN?**

IDeNtification: returns the instrument identification.

Return values:
<ID> "Rohde&Schwarz,<device type>,<serial number>,<firmware version>"

Example: `Rohde&Schwarz,RTO,1316.1000k14/200153,1.30.0.25`

Usage: Query only

***OPC**

OPeration Complete

Sets bit 0 in the event status register when all preceding commands have been executed. This bit can be used to initiate a service request. The query form writes a "1" into the output buffer as soon as all preceding commands have been executed. This is used for command synchronization.

***OPT?**

OPTion identification query

Queries the options included in the instrument. For a list of all available options and their description refer to the CD-ROM.

Return values:
<Options> The query returns a list of options. The options are returned at fixed positions in a comma-separated string. A zero is returned for options that are not installed.

Usage: Query only

***PSC** <Action>

Power on Status Clear

Determines whether the contents of the `ENABle` registers are preserved or reset when the instrument is switched on. Thus a service request can be triggered when the instrument is switched on, if the status registers ESE and SRE are suitably configured. The query reads out the contents of the "power-on-status-clear" flag.

Parameters:

<Action> 0 | 1

0
The contents of the status registers are preserved.

1
Resets the status registers.

***RST**

ReSeT

Sets the instrument to a defined default status. The default settings are indicated in the description of commands.

Usage: Setting only

***SRE** <Contents>

Service Request Enable

Sets the service request enable register to the indicated value. This command determines under which conditions a service request is triggered.

Parameters:

<Contents> Contents of the service request enable register in decimal form. Bit 6 (MSS mask bit) is always 0.

Range: 0 to 255

***STB?**

STatus Byte query

Reads the contents of the status byte in decimal form.

Usage: Query only

***TRG**

TRiGger

Triggers all actions waiting for a trigger event. In particular, *TRG generates a manual trigger signal (Manual Trigger). This common command complements the commands of the TRIGger subsystem.

Usage: Event

***TST?**

self TeST query

Triggers selftests of the instrument and returns an error code in decimal form (see Service Manual supplied with the instrument). "0" indicates no errors occured.

Usage: Query only

***WAI**

WAIt to continue

Prevents servicing of the subsequent commands until all preceding commands have been executed and all signals have settled (see also command synchronization and *OPC).

Usage: Event

15.2.3 General Remote Settings and Queries

This chapter describes commands that have effect on many other commands in different applications of the instrument.

FORMat[:DATA] ... 278
FORMat:BORDer ... 279
CHANnel<m>:DATA:XORigin? ... 279
CHANnel<m>:DATA:ENVelope:XORigin? ... 279
CALCulate:MATH<m>:DATA:XORigin? ... 279
REFCurve<m>:DATA:XORigin? ... 279
CHANnel<m>:DATA:XINCrement? ... 280
CHANnel<m>:DATA:ENVelope:XINCrement? ... 280
CALCulate:MATH<m>:DATA:XINCrement? ... 280
REFCurve<m>:DATA:XINCrement? ... 280
CHANnel<m>:DATA:YORigin? ... 280
CHANnel<m>:DATA:ENVelope:YORigin? ... 280
CALCulate:MATH<m>:DATA:YORigin? ... 280
REFCurve<m>:DATA:YORigin? ... 280
CHANnel<m>:DATA:YINCrement? ... 280
CHANnel<m>:DATA:ENVelope:YINCrement? ... 280
CALCulate:MATH<m>:DATA:YINCrement? ... 280
REFCurve<m>:DATA:YINCrement? ... 280
CHANnel<m>:DATA:YRESolution? ... 281

CHANnel<m>:DATA:ENVelope:YRESolution?....281
CALCulate:MATH<m>:DATA:YRESolution?....281
REFCurve<m>:DATA:YRESolution?....281

FORMat[:DATA] <DataFormat>,<Accuracy>

Defines the format for data export with

- `CHANnel<m>:DATA?` on page 293
- `CHANnel<m>:DATA:ENVelope?` on page 294
- `CALCulate:MATH<m>:DATA?` on page 347
- `REFCurve<m>:DATA?` on page 325

Parameters:

<DataFormat> ASCii | REAL | UINTeger

ASCii
List of values, for example, 1.23,1.22,1.24,..
<Accuracy> is 0 which means that the instrument selects the number of digits to be returned. The query returns ASC,0.

REAL
Binary format. <Accuracy> is 32. The query returns REAL,32.
The data is stored as binary data (Definite Length Block Data according to IEEE 488.2). Each waveform value is formatted in 32 Bit IEEE 754 Floating-Point-Format.
The schema of the result string is as follows:
`#41024<value1><value2>…<value n>` with:
`#4` = number of digits (= 4 in the example) of the following number
`1024` = number of following data bytes (= 1024 in the example)
`<value>` = 4-byte floating point values

UINTeger
Unsigned integer format, binary values with length 8 bit (1 byte per sample), 16 bit (2 bytes per sample) or 32 bit (4 bytes per sample): `UINT,8` or `UINT,16` or `UINT,32`.
The data range for `UINT,8` is 0 to 255, the data range for `UINT,16` is 0 to 65.535 and for `UINT,16` is $2^{32} - 1$.
For data conversion, you need the results of following commands: `...:DATA:XORigin?`; `...:DATA:XINCrement?`; `..:DATA:Yorigin?`; `...:DATA:YINCrement?`; `...:DATA:YRESolution?`. They are described below in this chapter. The way of data conversion is described in chapter 15.3.1.2, "Reading Waveform Data in Unsigned Integer Format", on page 458.
32 bit data is relevant for average waveforms if averaging 512 or 1024 waveforms. The resulting data is 17 bits long (512 waveforms) or 18 bit (1024 waveforms).

*RST: ASC

<Accuracy> 0 | 8 | 16 | 32

Length of a data value in bit
0 - for ASC only
32 - for REAL
8 | 16 | 32 - for UINT

*RST: 0

Example: Set the ASCII data format:
```
FORM ASC
```

Example: Query for data format:
```
FORM?
-> ASC,0
```

Example: Set the unsigned integer format, 16 bit data length:
```
FORM UINT,16
```

FORMat:BORDer <ByteOrder>

Defines the byte order for binary data export if `FORMat[:DATA]` is set to `REAL` or `UINT,16|32`.

Parameters:

<ByteOrder> MSBFirst | LSBFirst

MSBFirst
Big endian, most significant byte first

LSBFirst
Little endian, least significant byte first

*RST: MSBF

Example: See chapter 15.3.1.1, "Reading Waveform Data from Memory", on page 458

ByteOrder	8 bit	16 bit	32 bit
MSBF	0xab	0xAB CD	0xAB CD 00 00
LSBF	not relevant	0xCD AB	0x00 00 CD AB

CHANnel<m>:DATA:XORigin?
CHANnel<m>:DATA:ENVelope:XORigin?
CALCulate:MATH<m>:DATA:XORigin?
REFCurve<m>:DATA:XORigin?

Return the time of the first sample of the indicated waveform.

The commands are relevant for data conversion if binary data format is defined (FORM UINT, 8|16|32).

Return values:

<Xorigin> Time in s

Example: See chapter 15.3.1.2, "Reading Waveform Data in Unsigned Integer Format", on page 458

Usage: Query only

CHANnel<m>:DATA:XINCrement?
CHANnel<m>:DATA:ENVelope:XINCrement?
CALCulate:MATH<m>:DATA:XINCrement?
REFCurve<m>:DATA:XINCrement?

Return the time difference between two adjacent samples of the indicated waveform.

The commands are relevant for data conversion if binary data format is defined (FORM UINT, 8|16|32).

Return values:
<Xincrement> Time in s

Example: See chapter 15.3.1.2, "Reading Waveform Data in Unsigned Integer Format", on page 458

Usage: Query only

CHANnel<m>:DATA:YORigin?
CHANnel<m>:DATA:ENVelope:YORigin?
CALCulate:MATH<m>:DATA:YORigin?
REFCurve<m>:DATA:YORigin?

Return the voltage value for binary value 0 of the indicated waveform.

The commands are relevant for data conversion if binary data format is defined (FORM UINT, 8|16|32).

Return values:
<Yorigin> Voltage in V

Example: See chapter 15.3.1.2, "Reading Waveform Data in Unsigned Integer Format", on page 458

Usage: Query only

CHANnel<m>:DATA:YINCrement?
CHANnel<m>:DATA:ENVelope:YINCrement?
CALCulate:MATH<m>:DATA:YINCrement?
REFCurve<m>:DATA:YINCrement?

Return the voltage value per bit of the indicated waveform.

The commands are relevant for data conversion if binary data format is defined (FORM UINT, 8|16|32).

Return values:
<Yincrement> Voltage in V

Example: See chapter 15.3.1.2, "Reading Waveform Data in Unsigned Integer Format", on page 458

Usage: Query only

CHANnel<m>:DATA:YRESolution?
CHANnel<m>:DATA:ENVelope:YRESolution?
CALCulate:MATH<m>:DATA:YRESolution?
REFCurve<m>:DATA:YRESolution?

Return the vertical bit resolution of the indicated waveform.

The commands are relevant for data conversion if binary data format is defined (FORM UINT, 8|16|32).

Return values:

<Yresolution> For default waveforms, the resolution is 8 bit.
If high resolution, average or filter are set for the waveform, the resolution is 16 bit.

Example: See chapter 15.3.1.2, "Reading Waveform Data in Unsigned Integer Format", on page 458

Usage: Query only

15.2.4 Acquisition and Setup

- Starting and Stopping Acquisition....281
- Time Base....282
- Acquisition....284
- Vertical....288
- Waveform Data....293
- Probes....296

15.2.4.1 Starting and Stopping Acquisition

RUN....281
RUNContinous....282
SINGle....282
RUNSingle....282
ACQuire:NSINgle:COUNt....282
STOP....282

RUN

Starts the continuous acquisition.

Usage: Event
Asynchronous command

RUNContinous

Same as `RUN`.

Usage: Event
Asynchronous command

SINGle

Starts a defined number of acquisitions. The number of acquisitions is set with `ACQuire:NSINgle:COUNt`.

Usage: Event
Asynchronous command

RUNSingle

Same as `SINGle`.

Usage: Event
Asynchronous command

ACQuire:NSINgle:COUNt <NSingleCount>

Sets the number of waveforms acquired with `RUNSingle`.

Parameters:
<NSingleCount> Number of waveforms
Range: 1 to 10
Increment: 1
*RST: 1

STOP

Stops the running acquistion.

Usage: Event
Asynchronous command

15.2.4.2 Time Base

TIMebase:SCALe....283
TIMebase:RATime?....283
TIMebase:ACQTime....283
TIMebase:RANGe....283
TIMebase:DIVisions?....283
TIMebase:POSition....284
TIMebase:REFerence....284

TIMebase:SCALe <TimeScale>

Sets the horizontal scale for all channel and math waveforms.

Parameters:

<TimeScale>
Range: 1,00E-009 to 50; lower limits are possible if zoom or FFT is enabled.
Increment: 1, 2, 5 progression, for example, 1 ms/div, 2 ms/div, 5 ms/div, 10, 20, 50...
*RST: 1,00E-004
Default unit: s/div

TIMebase:RATime?

Queries the real acquisition time used in the hardware. If FFT analysis is performed, the value can differ from the adjusted acquisition time (`TIMebase:ACQTime`).

Return values:

<HWAcqTime>
Range: Depends on various settings
Default unit: s

Usage: Query only

TIMebase:ACQTime <AcquisitionTime>

Defines the time of one acquisition, that is the time across the 10 divisions of the diagram: *Timebase Scale*10*.

Parameters:

<AcquisitionTime>
*RST: 1 ms
Default unit: s

TIMebase:RANGe <AcquisitionTime>

Defines the time of one acquisition, that is the time across the 10 divisions of the diagram: *Timebase Scale*10*.

Parameters:

<AcquisitionTime>
Range and increment depend on time base and other settings
*RST: 1 ms
Default unit: s

TIMebase:DIVisions?

Queries the number of horizontal divisions on the screen.

Return values:

<HorizDivCount>
Range: 10 to 10
Increment: 0
*RST: 10
Default unit: div

Usage: Query only

TIMebase:POSition <Offset>

Defines the trigger position (trigger offset) - the time interval between trigger point and reference point to analize the signal some time before or after the trigger event.

See also: `TIMebase:REFerence` on page 284

Parameters:

<Offset>
Range: Depends on time base setting
*RST: 0
Default unit: s

TIMebase:REFerence <ReferencePoint>

Sets the reference point of the time scale (Time Reference) in % of the display. The reference point defines which part of the waveform is shown. If the trigger position is zero, the trigger point matches the reference point.

See also: `TIMebase:POSition` on page 284

Parameters:

<ReferencePoint>
Range: 10 to 90
Increment: 10
*RST: 50
Default unit: %

15.2.4.3 Acquisition

AUToscale....284
ACQuire:MODE....285
ACQuire:INTerpolate....285
ACQuire:AVERage:COUNt....285
ACQuire:WRATe....286
CHANnel<m>:TYPE....286
CHANnel<m>:ARIThmetics....287
TIMebase:ROLL:ENABle....287
ACQuire:FILTer:FREQuency....287
ACQuire:POINts:ARATe?....288
ACQuire:SRATe?....288

AUToscale

Performs an autoset process: analyzes the enabled channel signals, and obtains appropriate horizontal, vertical, and trigger settings to display stable waveforms.

Usage: Event
Asynchronous command

ACQuire:MODE <AcquisitionMode>

Selects the method of adding waveform points to the samples of the ADC in order to fill the record length.

Parameters:

<AcquisitionMode> RTIMe | ETIMe

RTIMe
Real Time Mode: At slow time base settings the sampled points of the input signal are used to build the waveform, no waveform points are added. With fast time base settings, the sample rate is higher than the ADC sample rate. Waveform samples are added to the ADC samples with sin(x)/x interpolation.

ETIMe
Equivalent time: The waveform points are taken from several acquisitions of a repetive signal at a different time in relation to the trigger point.

*RST: RTIME

ACQuire:INTerpolate <Interpolation>

Defines the interpolation mode.

See also: "Interpolation" on page 27

Parameters:

<Interpolation> SINX

LINear
Linear interpolation between two adjacent sample points.

SINX
Interpolation by means of a sin(x)/x curve.

SMHD
Sample & Hold causes a histogram-like interpolation.

*RST: SINX

ACQuire:AVERage:COUNt <AverageCount>

Defines the number of waveforms used to calculate the average waveform. The higher the number, the better the noise is reduced.

Parameters:

<AverageCount> Only numbers from the 2^n progression are permitted (2, 4, 8, ...)

Range: 2 to 1024
*RST: 2

ACQuire:WRATe <WaveformRate>

Defines the mode to set the sample rate (samples per second saved in the memory) and the waveform acquisition rate (waveforms per second).

Parameters:

<WaveformRate> AUTO | MWAVeform | MSAMples | MANual

AUTO
To display the best waveform, the instrument selects the optimum combination of waveform acquisition rate and sample rate using the full memory depth (maximum record length).

MWAVeform
Maximum waveform rate: The instrument combines sample rate and memory depth to acquire at maximum waveform acquisition rate. In connection with persistence, the mode can display rare signal anomalies.

MSAMples
Maximum sample rate: The instrument acquires the signal at maximum sample rate and uses the full memory depth. The result is a waveform with maximum number of waveform samples, high degree of accuracy, and low risk of aliasing.

MANual
The instrument acquires the signals at a sample rate that fills up an user-defined record length. Set the record length using ACQuire:POINts[:VALue].

*RST: AUTO

CHANnel<m>:TYPE <DecimationMode>

Selects the method to reduce the data stream of the ADC to a stream of waveform points with lower sample rate.

Suffix:

<m> The command affects all channels regardless of the indicated channel number. The suffix can be omitted.

Parameters:

<DecimationMode> SAMPle | PDETect | HRESolution

SAMPle
Input data is acquired with a sample rate which is aligned to the time base (horizontal scale) and the record length.

PDETect
Peak Detect: the minimum and the maximum of n samples in a sample interval are recorded as waveform points.

HRESolution
High resolution: The average of n sample points is recorded as waveform point.

*RST: SAMPle

CHANnel<m>:ARIThmetics <TrArithmetic>

Selects the method to build the resulting waveform from several consecutive acquisitions of the signal.

Suffix:
<m> The command affects all channels regardless of the indicated channel number. The suffix can be omitted.

Parameters:
<TrArithmetic> OFF | ENVelope | AVERage | SMOoth | FILTer

OFF
The data of the current acquisition is recorded according to the decimation settings.

ENVelope
Detects the minimum and maximum values in an sample interval over a number of acquisitions.

AVERage
Calculates the average from the data of the current acquisition and a number of acquisitions before. The number of used acquisitions is set with `ACQuire:AVERage:COUNt`.

SMOoth
Calculates a mean value of several adjacent sample points. Thus, smoothing is a moving average that uses the full data and can be used for non-periodic signals. It works like a low-pass, and increases the vertical resolution at the expense of bandwidth reduction.

FILTer
Sets a low-pass filter with 3 db attenuation at a configurable limit frequency set with `ACQuire:FILTer:FREQuency`. The filter removes higher frequencies from the channel signals.

*RST: OFF

TIMebase:ROLL:ENABle <Roll>

Enables the roll mode.

Parameters:
<Roll> ON | OFF

*RST: OFF

ACQuire:FILTer:FREQuency <FilterFrequency>

Sets the limit frequency for `CHANnel<m>:ARIThmetics` is set to `FILTer`.

Parameters:
<FilterFrequency> Limit frequency with 3 dB attenuation

Default unit: Hz

ACQuire:POINts:ARATe?

Retrieves the sample rate of the ADC, that is the number of points that are sampled by the ADC in one second.

Return values:

<AcquisitionRate> ADC sample rate

Range: 2.5E3 to 5,00E+009
Increment: 1,00E+003
*RST: 5,00E+009
Default unit: Hz

Usage: Query only

ACQuire:SRATe?

Returns the sample rate, that is the number of recorded waveform samples per second.

Return values:

<SampleRate>

Range: 2 to 1,00E+011
Increment: depends on time base, waveform rate, number of active channels
*RST: 1,00E+007
Default unit: Sa/s

Usage: Query only

15.2.4.4 Vertical

CHANnel<m>:STATe....288
CHANnel<m>:COUPling....289
CHANnel<m>:SCALe....289
CHANnel<m>:RANGe....289
CHANnel<m>:POSition....290
CHANnel<m>:OFFSet....290
CHANnel<m>:BANDwidth....290
CHANnel<m>:POLarity....291
CHANnel<m>:OVERload....291
CHANnel<m>:SKEW....291
CHANnel<m>:THReshold....292
CHANnel<m>:LABel....292
CHANnel<m>:LABel:STATe....292

CHANnel<m>:STATe <State>

Switches the channel signal on or off.

Suffix:

<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:
<State> ON | OFF

CHANnel<m>:COUPling <Coupling>

Selects the connection of the indicated channel signal.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:
<Coupling> DC | DCLimit | AC | ACLimit

DC
Direct connection with 50 Ω termination.

DCLimit
Direct connection with 1 MΩ termination.

AC
Connection through DC capacitor that removes the DC offset voltage from the input signal.

ACLimit
Connection through DC capacitor with 1 MΩ termination. The capacitor removes the DC offset voltage from the input signal.

*RST: DCLimit

CHANnel<m>:SCALe <Scale>

Sets the vertical scale for the indicated channel.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:
<Scale> Scale value, given in Volts per division.

Range: 1,00E-003 to 10; without probe attenuation
*RST: 5,00E-003
Default unit: V/div

CHANnel<m>:RANGe <Range>

Sets the voltage range across the 10 vertical divisions of the diagram. Use the command alternativly instead of `CHANnel<m>:SCALe`.

Suffix:
<m> Selects the input channel. The maximum channel number is instrument-dependent.

Parameters:

<Range> Voltage range value

Range: 8,00E-003 to 80; without probe attenuation
*RST: 4,00E-002
Default unit: V

CHANnel<m>:POSition <Position>

Sets the vertical position of the indicated channel and its horizontal axis in the window.

Suffix:

<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:

<Position> Position value, given in divisions.

Range: -5 to 5
*RST: 0
Default unit: div

CHANnel<m>:OFFSet <Offset>

The offset voltage is subtracted to correct an offset-affected signal.

Suffix:

<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:

<Offset> Offset value

Range: Values depend on vertical scale and probe attenuation.
Increment: Value depends on vertical scale and probe attenuation.
Default unit: V

CHANnel<m>:BANDwidth <BandwidthLimit>

Selects the bandwidth limit for the indicated channel.

Suffix:

<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:

<BandwidthLimit> FULL | B400 | B200 | B20

FULL
Use full bandwidth.

B400 | B200 | B20
Limit to 400MHz, 200 MHz, or 20 MHz respectively.
B400 is not available for 350 MHz instruments (R&S RTM203x).

*RST: FULL

CHANnel<m>:POLarity <Polarity>

Turns the inversion of the signal amplitude on or off. To invert means to reflect the voltage values of all signal components against the ground level. Inversion affects only the display of the signal but not the trigger.

Suffix:

<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:

<Polarity> NORMal | INVerted

*RST: NORM

CHANnel<m>:OVERload <Overload>

Retrieves the overload status of the specified channel from the status bit. When the overload problem is solved, the command resets the status bit.

Suffix:

<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:

<Overload> ON | OFF

Use OFF to reset the overload status bit.

*RST: OFF

Example: `CHANnel2:OVERload?`
Queries the overload status of channel 2.
`CHANnel2:OVERload OFF`
Resets the overload status bit.

CHANnel<m>:SKEW <Skew>

Skew or deskew compensates delay differences between channels caused by the different length of cables, probes, and other sources. Correct deskew values are important for accurate triggering.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:
<Skew> Deskew value
Default unit: s

CHANnel<m>:THReshold <Threshold>

Threshold value for digitization of analog signals. If the signal value is higher than the threshold, the signal state is high (1 or true for the boolean logic). Otherwise, the signal state is considered low (0 or false) if the signal value is below the threshold.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:
<Threshold> Default values are:
TTL: 1.4 V
ECL: -1.3 V
CMOS: 2.5 V
*RST: 1.4
Default unit: V

CHANnel<m>:LABel <Label>

Specifies a name for the selected channel.

Suffix:
<m> 1..4
Selects the input channel. The number of channels depends on the instrument.

Parameters:
<Label> String value
String with max. 8 characters, only ASCII characters can be used

---

CHANnel<m>:LABel:STATe

Shows or hides the channel name.

Suffix:
<m> 1..4
Selects the input channel. The number of channels depends on the instrument.

Parameters:
<State> ON | OFF
*RST: OFF

15.2.4.5 Waveform Data

Consider also the following commands:

- FORMat[:DATA] on page 278
- CHANnel<m>:DATA:XINCrement? on page 280
- CHANnel<m>:DATA:XORigin? on page 279
- CHANnel<m>:DATA:YINCrement? on page 280
- CHANnel<m>:DATA:YORigin? on page 280
- CHANnel<m>:DATA:YRESolution? on page 281
- CHANnel<m>:DATA:ENVelope:XINCrement? on page 280
- CHANnel<m>:DATA:ENVelope:XORigin? on page 279
- CHANnel<m>:DATA:ENVelope:YINCrement? on page 280
- CHANnel<m>:DATA:ENVelope:YORigin? on page 280
- CHANnel<m>:DATA:ENVelope:YRESolution? on page 281

CHANnel<m>:DATA?....293
CHANnel<m>:DATA:HEADer?....294
CHANnel<m>:DATA:ENVelope?....294
CHANnel<m>:DATA:ENVelope:HEADer?....294
CHANnel<m>:DATA:POINts....295

CHANnel<m>:DATA?

Returns the data of the channel waveform points for transmission from the instrument to the controlling computer. The waveforms data can be used in MATLAB, for example.

To set the export format, use FORMat[:DATA] on page 278.

To set the range of samples to be returned, use CHANnel<m>:DATA?.

For envelope waveforms, use the CHANnel<m>:DATA:ENVelope? command.

Suffix:

<m> Selects the input channel. The number of channels depends on the instrument.

Return values:

<Data> List of values according to the format settings - the voltages of recorded waveform samples.

Example:

```
FORM ASC
CHAN1:DATA?
-0.125000,-0.123016,-0.123016,-0.123016,
-0.123016,-0.123016,...
```

Example: See chapter 15.3.1, "Data Export", on page 458

Usage: Query only

CHANnel<m>:DATA:HEADer?

Returns information on the channel waveform. For envelope waveforms, use the `CHANnel<m>:DATA:ENVelope:HEADer?` command.

Table 15-12: Header data

Position	Meaning	Example
1	XStart in s	-9.477E-008 = - 94,77 ns
2	XStop in s	9.477E-008 = 94,77 ns
3	Record length of the waveform in Samples	200000
4	Number of values per sample interval, usually 1.	1

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Return values:
<DataHeader> Comma-separated value list

Example: `-9.477E-008,9.477E-008,200000,1`

Usage: Query only

CHANnel<m>:DATA:ENVelope?

Returns the data of the envelope. The envelope consists of two waveforms. The waveforms data can be used in MATLAB, for example.

Use this command only for envelope waveforms. For other channel waveforms use `CHANnel<m>:DATA?`.

To set the export format, use `FORMat[:DATA]` on page 278.

To set the range of samples to be returned, use `CHANnel<m>:DATA?`.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Return values:
<Data> List of values according to the format settings - the voltages of the envelope points. The list contains two values for each sample interval.

Usage: Query only

CHANnel<m>:DATA:ENVelope:HEADer?

Returns information on the envelope waveform.

Use this command only for envelope waveforms. for all other channel waveforms use `CHANnel<m>:DATA:HEADer?`.

Table 15-13: Header data

Position	Meaning	Example
1	XStart in s	-9.477E-008 = - 94,77 ns
2	XStop in s	9.477E-008 = 94,77 ns
3	Number of samples	200000
4	Number of values per sample interval. For envelope waveforms the value is 2.	2

Suffix:
<m>

Return values:
<DataHeader> Comma-separated value list
Example: `-9.477E-008,9.477E-008,200000,2`

Usage: Query only

CHANnel<m>:DATA:POINts <Points>

As a setting, the command selects a range of samples that will be returned with `CHANnel<m>:DATA?` and `CHANnel<m>:DATA:ENVelope?`. As a query, it returns the number of returned samples for the selected range.

If `ACQuire:WRATe` is set to `MSAMples` (maximum sample rate), the memory usually contains more data samples than the screen can display. In this case, you can decide which data will be saved: samples stored in the memory or only the displayed samples.

Note: The sample range can be change only in STOP mode. If the acquisition is running, DEF is always used automatically. If the acquisition has been stopped, data can be read from the memory, and all settings are available.

Suffix:
<m> The command affects all channels, and the suffix is irrelevant.

Setting parameters:

<Points> DEFault | MAXimum | DMAXimum

Sets the range for data queries.

DEFault
Waveform samples that are visible as waveform points on the screen.

MAXimum
All waveform samples that are stored in the memory. Only available if acquisition is stopped.

DMAXimum
Display maximum: Waveform samples stored in the current waveform record but only for the displayed time range. At maximum waveform rate, the instrument stores more samples than visible on the screen, and DMAX returns more values than DEF. Only available if acquisition is stopped.

*RST: DEFault

Return values:

<Points> Number of data points in the selected range.

Default unit: Samples

Example:

```
CHAN:DATA:POIN DEF
CHAN:DATA:POIN?;:CHAN2:DATA:POIN?
```
Returned values: `10416;10416`
```
CHAN:DATA:POIN DMAX
CHAN:DATA:POIN?;:CHAN2:DATA:POIN?
```
Returned values: `124992;124992`
```
CHAN:DATA:POIN MAX
CHAN:DATA:POIN?;:CHAN2:DATA:POIN?
```
Returned values: `4194302;4194302`

Example: See chapter 15.3.1.1, "Reading Waveform Data from Memory", on page 458

15.2.4.6 Probes

PROBe<m>:SETup:ATTenuation[:AUTO]?....297
PROBe<m>:SETup:ATTenuation:UNIT....297
PROBe<m>:SETup:ATTenuation:MANual....297
PROBe<m>:SETup:BANDwidth?....297
PROBe<m>:SETup:CAPacitance?....298
PROBe<m>:SETup:DCOFfset?....298
PROBe<m>:SETup:IMPedance?....298
PROBe<m>:SETup:MODE....299
PROBe<m>:SETup:NAME?....299
PROBe<m>:SETup:OFFSwitch....299
PROBe<m>:SETup:TYPE?....299
PROBe<m>:SETup:UOFFset....300
PROBe<m>:ID:BUILd?....300

PROBe<m>:ID:PARTnumber?.....300
PROBe<m>:ID:PRDate?.....301
PROBe<m>:ID:SRNumber?.....301
PROBe<m>:ID:SWVersion?.....301

PROBe<m>:SETup:ATTenuation[:AUTO]?

Returns the attenuation of an automatically detected probe.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Return values:
<ProbeAttenuation> Range: 1 to 1000

Usage: Query only

PROBe<m>:SETup:ATTenuation:UNIT <Unit>

Selects the unit that the probe can measure.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:
<Unit> V | A

Firmware/Software: FW 03.700

PROBe<m>:SETup:ATTenuation:MANual <ManualAttenuation>

Sets the attenuation or gain of the probe if the probe was not detected by the instrument.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:
<ManualAttenuation> Range: 1 to 10000
*RST: 1

Firmware/Software: FW 03.700

PROBe<m>:SETup:BANDwidth?

Queries the bandwidth of the probe.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Return values:

<Bandwidth> Range: 1,00E+006 to 2,00E+009
Increment: 10
Default unit: Hz

Usage: Query only

PROBe<m>:SETup:CAPacitance?

Queries the input capacity of the probe.

Suffix:

<m> Selects the input channel. The number of channels depends on the instrument.

Return values:

<InputCapacitance> Range: 0.1e-12 to 1.0e-9
Increment: 1.0e-12
Default unit: F

Usage: Query only

PROBe<m>:SETup:DCOFfset?

Retrieves the DC voltage that is measured by the integrated voltmeter of R&S active probes. Switch the voltmeter on before, see `PROBe<m>:SETup:OFFSwitch` on page 299.

Suffix:

<m> Selects the input channel. The number of channels depends on the instrument.

Return values:

<Offset> Range: -1.0e26 to 1.0e-26
Increment: 1,00E-003
Default unit: V

Usage: Query only

PROBe<m>:SETup:IMPedance?

Queries the termination of the probe.

Suffix:

<m> Selects the input channel. The number of channels depends on the instrument.

Return values:

<Termination> 50OHm | 1MOHm | UNKNown

Usage: Query only

PROBe<m>:SETup:MODE <Mode>

Select the action that is started with the probe button.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:
<Mode> RCONtinuous | RSINgle | AUToset | NOACtion

RCONtinuous
Run continuous: The acquisition is running as long as the probe button is pressed.

RSINgle
Run single: starts one acquisition.

AUTOSET
Starts the autoset procedure.

NOACtion
Nothing is started on pressing the micro button.

*RST: RCONtinuous

PROBe<m>:SETup:NAME?

Queries the name of the probe.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Return values:
<Name> string

Usage: Query only

PROBe<m>:SETup:OFFSwitch <DCOffsetOnOff>

Switches the integrated voltmeter of an R&S active probe on or off.

The command is only available if an R&S active probe with R&S ProbeMeter is used.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:
<DCOffsetOnOff> ON | OFF

*RST: OFF

PROBe<m>:SETup:TYPE?

Queries the type of the probe.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Return values:
<Type> NONE | ACTive | PASSive

NONE
not detected

ACTive
active probe

PASSive
passive probe

Usage: Query only

PROBe<m>:SETup:UOFFset <UserOffset>

Sets an additional probe offset.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Parameters:
<UserOffset>
Range: Depends on the probe characteristics.
*RST: 0
Default unit: V

PROBe<m>:ID:BUILd?

Queries the build number of the probe software.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Return values:
<BuildNumber> 32 bit number

Range: 0 to 4294967295
Increment: 1

Usage: Query only

PROBe<m>:ID:PARTnumber?

Queries the R&S part number of the probe.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Return values:
<PartNumber> string
Returns the part number in a string.

Usage: Query only

PROBe<m>:ID:PRDate?

Queries the production date of the probe.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Return values:
<ProductionDate> string
Returns the date in a string.

Usage: Query only

PROBe<m>:ID:SRNumber?

Queries the serial number of the probe.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Return values:
<SerialNumber> string

Usage: Query only

PROBe<m>:ID:SWVersion?

Queries the version of the probe firmware.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Return values:
<SoftwareVersion> string
Returns the version number in a string.

Usage: Query only

15.2.5 Trigger

- General A Trigger Settings....302
- Edge Trigger....304
- Width Trigger....305

- Video/TV Trigger....307
- Pattern Trigger....308
- Rise Time / Fall Time Trigger....310
- B-Trigger....312

15.2.5.1 General A Trigger Settings

TRIGger:A:MODE....302
TRIGger:A:LEVel<n>[:VALue]....302
TRIGger:A:FINDlevel....302
TRIGger:A:SOURce....303
TRIGger:EXTern:COUPling....303
TRIGger:A:TYPE....303
TRIGger:A:HYSTeresis....304
TRIGger:A:HOLDoff:MODE....304
TRIGger:A:HOLDoff:TIME....304

TRIGger:A:MODE <TriggerMode>

Sets the trigger mode. The trigger mode determines the behaviour of the instrument if no trigger occurs.

Parameters:

<TriggerMode> AUTO | NORMal

AUTO
The instrument triggers repeatedly after a time interval if the trigger conditions are not fulfilled. If a real trigger occurs, it takes precedence.

NORMal
The instrument acquires a waveform only if a trigger occurs.

*RST: AUTO

TRIGger:A:LEVel<n>[:VALue] <Level>

Sets the trigger treshold voltage for all A trigger types that require a trigger level.

Suffix:

<n> 1..5
Selects the trigger input. 1...4 select the corresponding channel, 5 is the external trigger input. The number of channels depends on the instrument.

Parameters:

<Level> Range: Depends on vertical scale.
Default unit: V

TRIGger:A:FINDlevel

Sets the trigger level of the A-trigger event to 50% of the signal amplitude.

Usage: Event

TRIGger:A:SOURce <Source>

Sets the trigger source for the selected A trigger type.

Parameters:

<Source> CH1 | CH2 | CH3 | CH4 | EXTernanalog | LINE | SBUS1 .. SBUS4 | D0..D15

CH1 | CH2 | CH3 | CH4
One of the input channels is the trigger source. Available channels depend on the instrument type.

EXTernanalog
External Trigger Input on the rear panel

LINE
AC line for the edge trigger

SBUS
Serial buses 1 to 4

D0..D15
If MSO option R&S RTM-B1 is installed, the digital channels D0 to D15 can be used as trigger sources for edge, width and pattern trigger.

TRIGger:EXTern:COUPling <ExternCoupling>

Sets the coupling for the external trigger input. The command is relevant if `TRIGger:B:SOURce` is set to `EXTernanalog`.

Parameters:

<ExternCoupling> AC | DC

*RST: AC

TRIGger:A:TYPE <Type>

Sets the trigger type for the A trigger.

Parameters:

<Type> EDGE | WIDTh | TV | BUS | LOGic

EDGE: edge trigger
WIDTh: width trigger
TV: video trigger
BUS: only available if at least one option R&S RTM-K1 or R&S RTM-K2 is installed.
LOGic: pattern trigger, logic trigger
See: chapter 11, "Protocol Analysis", on page 148

TRIGger:A:HYSTeresis <Hysteresis>

Sets a hysteresis range around the trigger level of the A trigger event. If the signal jitters inside this range and crosses the trigger level thereby, no trigger event occurs.

Hysteresis is available for edge and width trigger.

Parameters:

<Hysteresis> AUTO | SMALl | MEDium | LARGE

*RST: AUTO

TRIGger:A:HOLDoff:MODE <HoldOffMode>

Enables or disables the holdoff time.

Parameters:

<HoldOffMode> TIME | OFF

*RST: Off

TRIGger:A:HOLDoff:TIME <HoldOffTime>

Defines the holdoff time. The next trigger occurs only after the holdoff time has passed.

Parameters:

<HoldOffTime> Default unit: s

15.2.5.2 Edge Trigger

TRIGger:A:EDGE:SLOPe....304
TRIGger:A:EDGE:COUPling....305
TRIGger:A:EDGE:FILTer:LPASs....305
TRIGger:A:EDGE:FILTer:NREJect....305

TRIGger:A:EDGE:SLOPe <Slope>

Sets the slope for the edge trigger (A trigger).

Parameters:

<Slope> POSitive | NEGative | EITHer

POSitive
Rising edge, a positive voltage change

NEGative
Falling edge, a negative voltage change

EITHer
Rising as well as the falling edge

*RST: POSitive

TRIGger:A:EDGE:COUPling <Coupling>

Sets the coupling for the trigger source.

Parameters:

<Coupling> DC | AC | HF

DC
Direct Current coupling. The trigger signal remains unchanged.

AC
Alternating Current coupling. A 5 Hz high pass filter removes the DC offset voltage from the trigger signal.

HF
High frequency coupling. A 15 kHz high-pass filter removes lower frequencies from the trigger signal. Use this mode only with very high frequency signals.

*RST: DC

TRIGger:A:EDGE:FILTer:LPASs <State>

Turns an additional 5 kHz low-pass filter in the trigger path on or off. This filter removes higher frequencies and is available with AC and DC coupling.

Parameters:

<State> ON | OFF

*RST: OFF

TRIGger:A:EDGE:FILTer:NREJect <State>

Turns an additional 100 MHz low-pass filter in the trigger path on or off. This filter removes higher frequencies and is available with AC and DC coupling.

Parameters:

<State> ON | OFF

*RST: OFF

15.2.5.3 Width Trigger

TRIGger:A:WIDTh:POLarity....305
TRIGger:A:WIDTh:RANGe....306
TRIGger:A:WIDTh:DELTa....306
TRIGger:A:WIDTh:WIDTh....306

TRIGger:A:WIDTh:POLarity <Polarity>

Sets the polarity of the pulse.

Parameters:

<Polarity> POSitive | NEGative

POSitive
Positive going pulse, the width is defined from the rising to the falling slopes.

NEGative
Negative going pulse, the width is defined from the falling to the rising slopes.

*RST: POSitive

TRIGger:A:WIDTh:RANGe <RangeMode>

Defines how the measured pulse width is compared with the given limit(s).

Parameters:

<RangeMode> WITHin | OUTSide | SHORter | LONGer

WITHin | OUTSide
Triggers on pulses inside or outside a range defined by *time* ± *delta*. The time is specified with `TRIGger:A:WIDTh:WIDTh`, the range around is defined with `TRIGger:A:WIDTh:DELTa`.

SHORter | LONGer
Triggers on pulses shorter or longer than a time set with `TRIGger:A:WIDTh:WIDTh`.

*RST: LONGer

TRIGger:A:WIDTh:DELTa <Delta>

Defines a range around the width value specified using `TRIGger:A:WIDTh:WIDTh`.

Parameters:

<Delta> Range ±Δt ("Variation" softkey)

Range: Depends on the defined pulse width (TRIG:A:WIDTH:WITDH)

TRIGger:A:WIDTh:WIDTh <Time1>

For the ranges WITHin and OUTSide (defined using `TRIGger:A:WIDTh:RANGe`), the <Time1> defines the center of a range which is defined by the limits ±<Delta> (set with `TRIGger:A:WIDTh:DELTa`).

For the ranges SHORter and LONGer, the width defines the maximum and minimum pulse width, respectively.

Parameters:

<Time1> Center value, maximum value or minimum value depending on the defined range type.

Range: 2,00E-008 to 6.87194685440
Increment: Depends on the <Time1> value
*RST: 2,00E-008

15.2.5.4 Video/TV Trigger

TRIGger:A:TV:STANdard....307
TRIGger:A:TV:POLarity....307
TRIGger:A:TV:FIELd....307
TRIGger:A:TV:LINE....308

TRIGger:A:TV:STANdard <Standard>

Selects the color television standard.

Parameters:

<Standard> PAL | NTSC | SECam | PALM | I576 | P720 | P1080 | I1080

PALM = PAL-M
I576 = SDTV 576i (PAL and SECAM)
P720 | P1080 = HDTV 720/1080p (progressive scanning)
I1080 = HDTV 1080i (interlaced scanning)

*RST: PAL

TRIGger:A:TV:POLarity <Polarity>

Selects the polarity of the signal. Note that the sync pulse has the opposite polarity. The edges of the sync pulses are used for triggering,

See also: "Signal" on page 47

Parameters:

<Polarity> POSitive | NEGative

POSitive
If the video modulation is positive, the sync pulses are negative.

NEGative
If the modulation is negative, sync pulses are positive.

*RST: NEGative

TRIGger:A:TV:FIELd <Field>

Sets the trigger on the beginning of the video signal fields, or on the beginning of video signal lines.

Parameters:

<Field> EVEN | ODD | ALL | LINE | ALINe

EVEN | ODD
Triggers only on the field start of even or odd fields. Only available for interlaced scanning.

ALL
All fields, triggers on the frame start (progressive scanning) or any field start (interlaced scanning).

LINE
Triggers on the beginning of a specified line in any field. The line number is set with `TRIGger:A:TV:LINE`.

ALINe
Triggers on the beginning of all video signal lines.

*RST: ALL

TRIGger:A:TV:LINE <Line>

Sets an exact line number if `TRIGger:A:TV:FIELd` is set to LINE.

Parameters:

<Line>
Range: 1 to 525 (NTSC, PAL-M); 625 (PAL, SECAM, SDTV I-576); 750 (HDTV P720); 1125 (HDTV I1080, HDTV P1080)
Increment: 1
*RST: 1

15.2.5.5 Pattern Trigger

Pattern

TRIGger:A:PATTern:SOURce <SourceString>

Parameters:

<SourceString> string containing 0, 1, or X for each channel

1: high, the signal voltage is higher than the trigger level.
0: low, the signal voltage is lower than the trigger level.
X: Don't care. the channel does not affect the trigger.
Without MSO option, the pattern has 4 or 2 bits, depending on the number of channels: <ch1><ch2>[<ch3><ch4>].
With MSO option, the pattern has 18 or 20 bits: <ch1><ch2>[<ch3><ch4>]<d0><d1><d2>...<d15>.

Example: Without MSO option R&S RTM-B1:
`TRIG:A:PATT:SOUR "1X10"`
CH1, CH3, and NOT CH4 are logically combined with `TRIGger:A:PATTern:FUNCtion`, CH2 does not matter (don't care).

Example: With MSO option R&S RTM-B1:
`TRIG:A:PATT:SOUR "XXXX111101010011XXXX"`
Analog channels CH1 to CH4 do not matter (don't care). Digital channels D0 to D15 are logically combined with `TRIGger:A:PATTern:FUNCtion`.

TRIGger:A:PATTern:FUNCtion <Function>

Sets the logical combination of the trigger states of the channels.

Parameters:

<Function> AND | OR

AND
The required states of all channels must appear in the input signal at the same time.

OR
At least one of the channels must have the required state.

*RST: AND

TRIGger:A:PATTern:CONDition <ConditionString>

Sets the trigger point depending on the result of the logical combination of the channel states.

Parameters:

<ConditionString> "TRUE" | "FALSE"

*RST: "TRUE"

Time Limitation

TRIGger:A:PATTern:MODE <PatternMode>

Disables the time limitation or sets the time comparison mode.

Parameters:

<PatternMode> OFF | TIMeout | WIDTh

OFF
Disables the time limitation.

TIMeout
Defines how long at least the result of the state pattern condition must be true or false.

WIDTh
Defines a time range for keeping up the true result of the pattern condition. The range is defined using `TRIGger:A:PATTern:WIDTh:RANGe`.

TRIGger:A:PATTern:WIDTh:RANGe <PatternRange>

Selects how the time limit of the pattern state is defined.

The time is specified using `TRIGger:A:PATTern:WIDTh[:WIDTh]` on page 310, the range around is specified using `TRIGger:A:PATTern:WIDTh:DELTa` on page 310.

Parameters:

<PatternRange> WITHin | OUTSide | SHORter | LONGer

WITHin
Triggers if the pattern state remains unchanged longer than *Time - Delta* and shorter than *Time + Delta*.

OUTSide
Triggers if the pattern state remains unchanged either shorter than *Time - Delta* or longer than *Time + Delta*.

SHORter | LONGer
Triggers if the pattern state changes before or after the specified time.

TRIGger:A:PATTern:WIDTh[:WIDTh] <PatternWidth>

For the ranges WITHin and OUTSide, the <PatternWidth> defines the center of a range which is defined by the limits ±<Delta>.

For the ranges SHORter and LONGer, the pattern width defines the maximum and minimum values, respectively.

Parameters:

<PatternWidth> Default unit: s

TRIGger:A:PATTern:WIDTh:DELTa <PatternDelta>

Defines a range around the pattern width value specified using `TRIGger:A:PATTern:WIDTh[:WIDTh]`.

Parameters:

<PatternDelta> Default unit: s

15.2.5.6 Rise Time / Fall Time Trigger

TRIGger:A:LEVel<n>:RISetime:LOWer....311
TRIGger:A:LEVel<n>:RISetime:UPPer....311
TRIGger:A:RISetime:SLOPe....311
TRIGger:A:RISetime:RANGe....311
TRIGger:A:RISetime:TIME....311
TRIGger:A:RISetime:DELTa....312

TRIGger:A:LEVel<n>:RISetime:LOWer <Level>
TRIGger:A:LEVel<n>:RISetime:UPPer <Level>

Set the loer and upper voltage threshold, respectively. When the signal crosses these levels, the slew rate measurement starts or stops depending on the selected polarity.

Suffix:
<n> 1..5
The suffix is not relevant, the level applies to all sources.

Parameters:
<Level> Default unit: V

TRIGger:A:RISetime:SLOPe <Polarity>

Sets the edge of whic the transition time is to be analyzed:

Parameters:
<Polarity> POSitive | NEGative
POSitive: rise time trigger
NEGative: Fall time trigger
*RST: POS

TRIGger:A:RISetime:RANGe <Range>

Selects how the time limit of the rise or fall time is defined.

Parameters:
<Range> LONGer | SHORter | WITHin | OUTSide

LONGer | SHORter
Triggers on transition times longer or shorter than the time `TRIGger:A:RISetime:TIME`.

WITHin | OUTSide
Triggers on transition times inside or outside the time range TIMe ± DELTa. Use `TRIGger:A:RISetime:TIME` and `TRIGger:A:RISetime:DELTa` to set the time range.

*RST: LONG

TRIGger:A:RISetime:TIME <RiseTime>

For the ranges LONGer and SHORter, the command defines the minimum and maximum transition times, respectively.

For the ranges WITHin and OUTSide, the command defines the center of a time range which is defined using `TRIGger:A:RISetime:DELTa`.

See also: `TRIGger:A:RISetime:RANGe`

Parameters:
<RiseTime> Default unit: s

TRIGger:A:RISetime:DELTa <Variation>

Sets a time range around the time value defined using `TRIGger:A:RISetime:TIME` if `TRIGger:A:RISetime:RANGe` is set to WITHin | OUTSide.

Parameters:
<Variation> Default unit: s

15.2.5.7 B-Trigger

TRIGger:B:ENABle....312
TRIGger:B:SOURce....312
TRIGger:B:EDGE:SLOPe....312
TRIGger:B:LEVel....312
TRIGger:B:FINDlevel....313
TRIGger:B:MODE....313
TRIGger:B:DELay....313
TRIGger:B:EVENt:COUNt....313
TRIGger:B:HYSTeresis....314

TRIGger:B:ENABle <State>

Activates or deactivates the second trigger. The instrument triggers if both trigger event conditions (A and B) are fulfilled.

Parameters:
<State> ON | OFF
*RST: OFF

TRIGger:B:SOURce <Source>

Selects one of the input channels as B-trigger source. Available channels depend on the instrument type.

Parameters:
<Source> CH1 | CH2 | CH3 | CH4
*RST: CH1

TRIGger:B:EDGE:SLOPe <Slope>

Sets the edge for the B-trigger.

Parameters:
<Slope> POSitive | NEGative | EITHer
*RST: POSitive

TRIGger:B:LEVel <Level>

Sets the trigger level for the B-trigger event.

Parameters:

<Level> *RST: 0
Default unit: V

TRIGger:B:FINDlevel

Sets the trigger level of the B-trigger event to 50% of the signal amplitude.

Usage: Event

TRIGger:B:MODE <Mode>

Defines the delay type of the B-trigger.

Parameters:

<Mode> DELay | EVENts

DELay
Time delay, set with `TRIGger:B:DELay`

EVENts
Event count delay, set with `TRIGger:B:EVENt:COUNt`

*RST: DELay

TRIGger:B:DELay <DelayTime>

Sets the time the instrument waits after an A-event until it recognizes B-events.

Before setting the dalay time, `TRIGger:B:MODE` must be set to `DELAy`.

Parameters:

<DelayTime> Range: 2,00E-008 to 6,87
Increment: Depends on the <DelayTime> value. The longer the <DelayTime>, the longer is the increment value.
*RST: 2,00E-008
Default unit: s

TRIGger:B:EVENt:COUNt <EventCnt>

Sets a number of B-trigger events that fulfill all B-trigger conditions but do not cause the trigger. The oscilloscope triggers on the n-th event (the last of the specified number of events).

Before setting the event number, `TRIGger:B:MODE` must be set to `EVENts`.

Parameters:

<EventCnt> Number of B-events

Range: 1 to 65535
Increment: 1
*RST: 1

TRIGger:B:HYSTeresis <Hysteresis>

Sets a hysteresis range around the trigger level of the B trigger event. If the signal jitters inside this range and crosses the trigger level thereby, no trigger event occurs.

Parameters:

<Hysteresis> AUTO | SMALl | MEDium | LARGE

*RST: AUTO

15.2.6 Display

15.2.6.1 Basic Display Settings

This chapter describes commands that configure the screen display.

General Display Settings

DISPlay:MODE....314
DISPlay:PALette....314

DISPlay:MODE <Mode>

Sets the diagram mode.

Parameters:

<Mode> YT | XY

YT
Default time diagram with a time axis in x-direction and the signal amplitudes displayed in y-direction.

XY
XY-diagram, combines the voltage levels of two waveforms in one diagram.

*RST: YT

DISPlay:PALette <Palette>

Sets the color and brightness of the displayed waveform samples depending on their cumulative occurance.

Parameters:

<Palette> NORMal | INVerse | FCOLor | IFColor

NORMal
Values that occur frequently are brighter than rare values.

INVerse
Rare values are brighter than frequent values, inverse to the NORMal brightness.

FColor
Rare values are displayed in blue, while more frequent values are red and very frequent values are displayed in yellow or white, with various colors inbetween.

IFColor
Inverses the FColor setting: rare values are yellow or white while frequent values are blue.

*RST: NORMal

XYZ-Setup

DISPlay:XY:XSOurce....315
DISPlay:XY:Y1Source....315
DISPlay:XY:Y2Source....316
DISPlay:XY:ZMODe....316
DISPlay:XY:ZTHReshold....316
DISPlay:XY:ZSOurce....316

DISPlay:XY:XSOurce <Source>

Defines the source to be displayed in x direction in an XY-diagram, replacing the usual time base.

Parameters:

<Source> CH1 | CH2 | CH3 | CH4

CH3 and CH4 are only available with 4-channel R&S RTM oscilloscopes.

*RST: CH1

DISPlay:XY:Y1Source <Source>

Defines the (first) source to be displayed in y direction in an XY-diagram.

Parameters:

<Source> CH1 | CH2 | CH3 | CH4

CH3 and CH4 are only available with 4-channel R&S RTM oscilloscopes.

*RST: CH2

DISPlay:XY:Y2Source <Source>

Defines an optional second source to be displayed in y direction in an XY-diagram. The command is only relevant for 4-channel R&S RTM instruments.

Parameters:

<Source> NONE | CH1 | CH2 | CH3 | CH4

*RST: NONE

DISPlay:XY:ZMODe <Mode>

Activates or deactivates the intensity control of the waveform via an additional signal source and sets the intensity mode.

Parameters:

<Mode> ANALog | DIGital | OFF

ANALog
Modulated intensity; Intensity is modulated continuously according to the selected Source Z.

DIGital
Intensity is determined by a threshold value defined with `DISPlay:XY:ZTHReshold`. If the Z signal value is below the selected threshold, the corresponding x/y point is not displayed. If the Z signal value is above the threshold, the x/y point is displayed with the defined intensity level.

OFF
Intensity control is deactivated.

*RST: OFF

DISPlay:XY:ZTHReshold <Zthreshold>

Defines the threshold for intensity with a two-state modulation, if `DISPlay:XY:ZMODe` is set to `DIGital`.

Parameters:

<Zthreshold> Threshold for visibility on the screen

Range: -10 to 10
Increment: depends on the scaling of the channel that is assigned to Z
*RST: 0
Default unit: V

DISPlay:XY:ZSOurce <Source>

Defines the source to be used to determine the intensity of the xy-waveform.

Parameters:

<Source> CH1 | CH2 | CH3 | CH4

CH3 and CH4 are only available with 4-channel R&S RTM oscilloscopes.

*RST: CH1

Intensities

DISPlay:INTensity:WAVeform....317
DISPlay:INTensity:BACKlight....317
DISPlay:INTensity:GRID....317
DISPlay:PERSistence:STATe....318
DISPlay:PERSistence:TIME....318
DISPlay:PERSistence:INFinite....318
DISPlay:PERSistence:TIME:AUTO....318
DISPlay:PERSistence:CLEar....319

DISPlay:INTensity:WAVeform <Intensity>

Defines the strength of the waveform line in the diagram.

Parameters:

<Intensity> Value in percent

Range: 0 to 100
Increment: 1
*RST: not available, *RST does not change the intensity
Default unit: %

DISPlay:INTensity:BACKlight <Intensity>

Defines the intensity of the background lighting of the display.

Parameters:

<Intensity> Value in percent

Range: 10 to 100
Increment: 1
*RST: not available, *RST does not change the intensity
Default unit: %

DISPlay:INTensity:GRID <Intensity>

Defines the intensity of the grid on the screen.

Parameters:

<Intensity> Value in percent

Range: 0 to 100
Increment: 1
*RST: not available, *RST does not change the intensity
Default unit: %

DISPlay:PERSistence:STATe <State>

Defines whether the waveform persists on the screen or whether the screen is refreshed continuously.

Parameters:

<State> ON | OFF

ON
The waveform persists for the time defined using `DISPlay:PERSistence:TIME`.

OFF
The waveform does not persist on the screen. Only the currently measured values are displayed at any time.

*RST: OFF

DISPlay:PERSistence:TIME <Time>

Persistence time if persistence is active (see `DISPlay:PERSistence:STATe` on page 318).

Each new data point in the diagram area remains on the screen for the duration defined here. To set infinite persistence, use `DISPlay:PERSistence:INFinite`.

Parameters:

<Time>
Range: 5,00E-002 to Infinite
Increment: minimum 50E-3 s, increasing increment with increasing persistence time
*RST: 5,00E-002
Default unit: s

DISPlay:PERSistence:INFinite <InfPersistence>

Sets the persistence time to infinite if `DISPlay:PERSistence:STATe` is ON. each new data point remains on the screen infinitely until this setting is changed or the persistence is cleared.

Parameters:

<InfPersistence> ON | OFF

*RST: OFF

DISPlay:PERSistence:TIME:AUTO <Auto>

The optimal persistence time is determined automatically by the instrument.

Parameters:

<Auto> ON | OFF

*RST: OFF

DISPlay:PERSistence:CLEar

Removes the displayed persistent waveform from the screen.

Usage: Event

Waveform, Auxilary Cursors and Grid Settings

DISPlay:STYLe....319
DISPlay:GRID:STYLe....319

DISPlay:STYLe <Style>

Defines how the waveform data is displayed

Parameters:

<Style> VECTors | DOTS

VECTors
Individual data points are connected by a line.

DOTS
Only the data points are displayed.

*RST: VECT

DISPlay:GRID:STYLe <Style>

Defines how the grid is displayed.

Parameters:

<Style> LINes | RETicle | NONE

LINes
Displays the grid as horizontal and vertical lines.

RETicle
Displays crosshairs instead of a grid.

NONE
No grid is displayed.

*RST: LIN

Virtual Screen

DISPlay:VSCReen:ENABle....319
DISPlay:VSCReen:POSition....320

DISPlay:VSCReen:ENABle <Enable>

Enables or disables the virtual screen. If enabled, the virtual screen has 20 divisions, 8 of them are displayed.

Parameters:
<Enable> ON | OFF
*RST: OFF

DISPlay:VSCReen:POSition <Position>

Selects the divisions to be displayed on the virtual screen. The virtual screen has 20 divisions, 8 of them are displayed.

Parameters:
<Position> Indicated the position of the middle visible division.
Range: -6 to 6. At -6, the lower 8 divisons are visible. 0 indicates the center of the virtual screen, and the divions -4 to 4 are visible.

15.2.6.2 Zoom

TIMebase:ZOOM:STATe....320
TIMebase:ZOOM:SCALe....320
TIMebase:ZOOM:TIME....320
TIMebase:ZOOM:POSition....321

TIMebase:ZOOM:STATe <ZoomState>

Switches the zoom window on or off.

Parameters:
<ZoomState> ON | OFF
*RST: OFF

TIMebase:ZOOM:SCALe <ZoomScale>

Defines the time base in the zoom diagram in seconds per division.

Parameters:
<ZoomScale> Range: Depends on various other settings
Default unit: s/div

TIMebase:ZOOM:TIME <Time>

Defines the offset of the trigger point to the reference point of the zoom diagram.

Parameters:
<Time> *RST: 0
Default unit: s

TIMebase:ZOOM:POSition <Position>

Defines the position of the zoom reference point (the reference point of the zoom window) in relation to the reference point of original time base.

Parameters:

<Position>	Range:	Depends on the zoom time base, nearly 0 to 100 % for large zoom
	*RST:	50
	Default unit:	%

15.2.6.3 Markers (Timestamps)

TSTamp:SET....321
TSTamp:NEXT....321
TSTamp:PREVious....321
TSTamp:CLEar....321
TSTamp:ACLear....321

TSTamp:SET

Sets a new marker (timestamp) at the reference point of the display, unless an existing marker is already set there. The reference point is set with `TIMebase:REFerence`.

Usage: Event

TSTamp:NEXT

Usage: Event

Moves the next marker (timestamp, to the right) to the reference point of the display or zoom area.

TSTamp:PREVious

Moves the previous marker (timestamp, to the left) to the reference point of the display or zoom area.

Usage: Event

TSTamp:CLEar

Deletes the marker (timestamp) at the reference point. The reference point is set with `TIMebase:REFerence`.

Usage: Event

TSTamp:ACLear

Deletes all markers (timestamps).

Usage: Event

15.2.7 Reference Waveforms

For data queries and conversion, consider also the following commands:

- `FORMat[:DATA]` on page 278
- `REFCurve<m>:DATA:XINCrement?` on page 280
- `REFCurve<m>:DATA:XORigin?` on page 279
- `REFCurve<m>:DATA:YINCrement?` on page 280
- `REFCurve<m>:DATA:YORigin?` on page 280
- `REFCurve<m>:DATA:YRESolution?` on page 281

REFCurve<m>:STATe....322
REFCurve<m>:SOURce....322
REFCurve<m>:SOURce:CATalog?....323
REFCurve<m>:UPDate....323
REFCurve<m>:SAVE....323
REFCurve<m>:LOAD....324
REFCurve<m>:LOAD:STATe....324
REFCurve<m>:HORizontal:SCALe....324
REFCurve<m>:HORizontal:POSition....324
REFCurve<m>:VERTical:SCALe....325
REFCurve<m>:VERTical:POSition....325
REFCurve<m>:DATA?....325
REFCurve<m>:DATA:HEADer?....325

REFCurve<m>:STATe

Displays or hides the selected reference waveform.

Suffix:
<m> 1..4
Selects the reference waveform, the internal reference storage.

Parameters:
<State> ON | OFF
*RST: OFF

REFCurve<m>:SOURce <Source>

Defines the source of the reference waveform.

Suffix:
<m> 1..4
Selects the reference waveform, the internal reference storage.

Parameters:

<Source> CH1 | CH2 | CH3 | CH4 | MA1 | MA2 | MA3 | MA4 | RE1 | RE2 | RE3 | RE4 | D70 | D158

Any active channel, math, or reference waveform. Available channels depend on the instrument type.
If MSO option R&S RTM-B1 is installed, you can use also the pods as reference source: D70 is the pod with digital channels D0 to D7, and D158 is the pod with D8 to D15.

*RST: CH1

REFCurve<m>:SOURce:CATalog?

Returns the source waveform - channel, math or reference waveform.

If MSO option R&S RTM-B1 is installed, the source can also be a pod: D70 is the pod with digital channels D0 to D7, and D158 is the pod with D8 to D15.

Suffix:

<m> 1..4
Selects the reference waveform, the internal reference storage.

Return values:

<Catalog> CH1 | CH2 | CH3 | CH4 | MA1 | MA2 | MA3 | MA4 | RE1 | RE2 | RE3 | RE4 | D70 | D158

Usage: Query only

REFCurve<m>:UPDate

Updates the selected reference by the waveform defined with `REFCurve<m>:SOURce`.

Suffix:

<m> 1..4
Selects the reference waveform, the internal reference storage.

Usage: Event

REFCurve<m>:SAVE <FileName>

Stores the reference waveform the specified file.

Suffix:

<m> 1..4
Selects the reference waveform, the internal reference storage.

Setting parameters:

<FileName> String with path and file name

Usage: Setting only

REFCurve<m>:LOAD <FileName>

Loads the waveform data from the indicated reference file to the reference storage.

To load the instrument settings, use `REFCurve<m>:LOAD:STATe`.

Suffix:
<m> 1..4
Selects the reference waveform, the internal reference storage.

Setting parameters:
<FileName> String with path and file name

Usage: Setting only

REFCurve<m>:LOAD:STATe

Loads the instrument settings in addition to the reference waveform data. The waveform data must be loaded before the settings, see `REFCurve<m>:LOAD` on page 324.

The settings are only available if the file was stored to the internal storage `/INT/REFERENCE` and never written to an external storage (USB stick).

Suffix:
<m> 1..4
Selects the reference waveform.

Usage: Event

REFCurve<m>:HORizontal:SCALe <Scale>

Changes the horizontal scale (timebase) of the reference waveform independent of the channel waveform settings.

Suffix:
<m> 1..4
Selects the reference waveform, the internal reference storage.

Parameters:
<Scale> *RST: 1,00E-004
Default unit: s/div

REFCurve<m>:HORizontal:POSition <Position>

Changes the horizontal position of the reference waveform independent of the channel waveform settings.

Suffix:
<m> 1..4
Selects the reference waveform, the internal reference storage.

Parameters:
<Position> *RST: 0
Default unit: s

REFCurve<m>:VERTical:SCALe <Scale>

Changes the vertical scale of the reference waveform.

Suffix:
<m> 1..4
Selects the reference waveform, the internal reference storage.

Parameters:
<Scale> *RST: 1
Default unit: V/div

REFCurve<m>:VERTical:POSition <Position>

Changes the vertical position of the reference waveform.

Suffix:
<m> 1..4
Selects the reference waveform, the internal reference storage.

Parameters:
<Position> *RST: 0
Default unit: div

REFCurve<m>:DATA?

Returns the data of the reference waveform for transmission from the instrument to the controlling computer. The waveforms data can be used in MATLAB, for example.

To set the export format, use `FORMat[:DATA]` on page 278.

Suffix:
<m> 1..4
Selects the reference waveform, the internal reference storage.

Return values:
<Data> List of values according to the format settings.

Usage: Query only

REFCurve<m>:DATA:HEADer?

Returns information on the reference waveform.

Table 15-14: Header data

Position	Meaning	Example
1	XStart in s	-9.477E-008 = - 94,77 ns
2	XStop in s	9.477E-008 = 94,77 ns
3	Record length of the waveform in Samples	200000
4	Number of values per sample interval, usually 1.	1

Suffix:
<m> 1..4
Selects the reference waveform, the internal reference storage.

Parameters:
<Header> Comma-separated value list
Example: `-9.477E-008,9.477E-008,200000,1`

Usage: Query only

15.2.8 Measurements

This chapter describes functions that configure or perform cursor and automatic measurements.

- Cursor Measurements....326
- Quick Measurements....334
- Automatic Measurements....335
- Reference Level....341
- Automatic Measurements - Statistic....342

15.2.8.1 Cursor Measurements

CURSor<m>:AOFF....327
CURSor<m>:STATe....327
CURSor<m>:SOURce....327
CURSor<m>:FUNCtion....328
CURSor<m>:TRACking[:STATe]....330
CURSor<m>:X1Position....330
CURSor<m>:X2Position....330
CURSor<m>:X3Position....330
CURSor<m>:Y1Position....330
CURSor<m>:Y2Position....330
CURSor<m>:Y3Position....330
CURSor<m>:YCOupling....330
CURSor<m>:XCOupling....330
CURSor<m>:SWAVe....331
CURSor<m>:SSCReen....331
CURSor<m>:SPPeak....331
CURSor<m>:SNPeak....331
CURSor<m>:TRACking:SCALe[:STATe]....331
CURSor<m>:RESult?....332
CURSor<m>:XDELta:INVerse?....332
CURSor<m>:XDELta[:VALue]?....332
CURSor<m>:YDELta:SLOPe?....333
CURSor<m>:YDELta[:VALue]?....333
CURsor<m>:XRATio:UNIT....333
CURSor<m>:XRATio[:VALue]?....333
CURSor<m>:YRATio:UNIT....334
CURSor<m>:YRATio[:VALue]?....334

CURSor<m>:AOFF

Switches the cursor off.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Usage: Event

CURSor<m>:STATe <State>

Activates or deactivates the cursor measurement.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Parameters:
<State> ON | OFF
*RST: OFF

CURSor<m>:SOURce <Source>

Defines the source of the cursor measurement.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Parameters:

<Source> NONE | CH1 | CH2 | CH3 | CH4 | MA1 | MA2 | MA3 | MA4 | MA5 | RE1 | RE2 | RE3 | RE4 | XY1 | D0..D15 | D70 | D158

CH1 | CH2 | CH3 | CH4
Active channel waveform 1 to 4

MA1 | MA2 | MA3 | MA4 | MA5
Active math channels 1 to 5

RE1 | RE2 | RE3 | RE4
Active reference channels 1 to 4

XY1
Active XY-waveform

D0..D15
Active igital channels D0 to D15, available if MSO option R&S RTM-B1 is installed. The following cursor measurements are possible: time, ratio X, count, duty ratio, burst width. Available sources depend on the selected measurement type.

D70 | D158
Active digital pods D0...D7 and D8...D15, available if MSO option R&S RTM-B1 is installed. The following cursor measurements are possible: V-marker.

*RST: CH1

CURSor<m>:FUNCtion <Type>

Defines the cursor measurement type.

Suffix:

<m> 1
The numeric suffix is irrelevant.

Parameters:

<Type> HORizontal | VERTical | PAIRed | HRATio | VRATio | PPCount | NPCount | RECount | FECount | MEAN | RMS | RTIMe | FTIMe | PEAK | UPEakvalue | LPEakvalue | BWIDth

*RST: VERT

Value	Description	Queries for results

HORizontal	Sets two horizontal cursor lines and measures the voltages at the two cursor positions and the delta of the two values.	`CURSor<m>:Y1Position`
		`CURSor<m>:Y2Position`
		`CURSor<m>:YDELta[:VALue]?`
		`CURSor<m>:YDELta:SLOPe?`

VERTical	Sets two vertical cursor lines and measures the time from the trigger point to each cursor, the time between the two cursors and the frequency calculated from that time.	`CURSor<m>:X1Position`
		`CURSor<m>:X2Position`
		`CURSor<m>:XDELta[:VALue]?`
		`CURSor<m>:XDELta:INVerse?`

Value	Description	Queries for results
PAIRed	V-Marker same as CURSor<m>:TRACking[:STATe]	CURSor<m>:Y1Position CURSor<m>:Y2Position CURSor<m>:XDELta[:VALue]? CURSor<m>:YDELta[:VALue]?
HRATio	Sets three horizontal cursor lines. Queries return the ratio of the y-values (e.g. overshooting) between the first and second cursors and the first and third cursors.	CURSor<m>:YRATio:UNIT CURSor<m>:YRATio[:VALue]? CURSor<m>:Y1Position CURSor<m>:Y2Position CURSor<m>:Y3Position
VRATio	Sets three vertical cursor lines. Queries return the ratio of the x-values (e.g. a duty cycle) between the first and second cursors and the first and third cursors.	CURsor<m>:XRATio:UNIT CURSor<m>:XDELta[:VALue]? CURSor<m>:X1Position CURSor<m>:X2Position CURSor<m>:X3Position
PPCount NPCount RECount FECount	Count positive pulses Count negative pulses Count rising edges Count falling edges Sets two vertical and one horizontal cursor line. The time base is defined by the vertical cursors, the horizontal cursor defines the threshold value.	CURSor<m>:RESult?
MEAN RMS	Mean value Root mean square Values are measured between two vertical cursor lines.	CURSor<m>:RESult?
RTIMe FTIMe	Rise time, tr Fall time, tf Measures the rise or fall time of the first edge after the first vertical cursor between the upper and lower reference levels. The reference level for rise and fall time measurement is set with REFLevel:RELative:MODE.	CURSor<m>:RESult?
PEAK UPEakvalue LPEakvalue	Vpp, absolute difference between the two peak values Vp+, upper peak value Vp-, lower peak value Values are measured between two vertical cursor lines.	CURSor<m>:RESult?
BWIDth	Burst width, the duration of a burst. Two vertical cursors mark the beginning and the end of the burst. The horizontal cursor sets the threshold value, and the time between the first and the last edge of the burst is returned.	CURSor<m>:RESult?

CURSor<m>:TRACking[:STATe] <State>

If set to ON, the V-Marker cursor measurement is enabled.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Parameters:
<State> ON | OFF
*RST: OFF

CURSor<m>:X1Position <Xposition1>
CURSor<m>:X2Position <Xposition2>
CURSor<m>:X3Position <Xposition3>

The commands specify the x-positions of vertical cursor lines on the time axis. The third cursor is only used for Ratio X measurement.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Parameters:
<Position> Range: Depends on horizontal settings.

CURSor<m>:Y1Position <Yposition1>
CURSor<m>:Y2Position <Yposition2>
CURSor<m>:Y3Position <Yposition3>

The commands specify the positions of horizontal cursor lines on the y-axis. The third cursor is only used for Ratio Y measurements.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Parameters:
<Position> Range: Depends on various other settings.

CURSor<m>:YCOupling <Coupling>
CURSor<m>:XCOupling <Coupling>

If enabled, the cursors of a set are coupled so that the distance between the two remains the same if one cursor is moved.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Parameters:
<Coupling> ON | OFF
*RST: OFF

CURSor<m>:SWAVe

Autoset for cursor lines, sets the cursor lines to typical points of the waveform depending on the selected measurement type. For example, for voltage measurement, the cursor lines are set to the upper and lower peaks of the waveform. For time measurement, the cursor lines are set to the edges of two consecutive positive or two consecutive negative pulses.

Usage: Event

Firmware/Software: FW 03.700

CURSor<m>:SSCReen

Resets the cursors to their initial positions. This is helpful if the cursors have disappeared from the display or need to be moved for a larger distance.

Usage: Event

Firmware/Software: FW 03.700

CURSor<m>:SPPeak

For FFT analysis only: sets the selected cursor to the previous (left) level peak.

Usage: Event

Firmware/Software: FW 03.700

CURSor<m>:SNPeak

For FFT analysis only: sets the selected cursor to the next (right) level peak.

Usage: Event

Firmware/Software: FW 03.700

CURSor<m>:TRACking:SCALe[:STATe] <State>

Enables the adjustment of cursor lines if the vertical or horizontal scales are changed.

Suffix:

<m> 1
The numeric suffix is irrelevant.

Parameters:

<State> ON | OFF

ON
Cursor lines keep their relative position to the waveform.

OFF
Cursor lines remain on their position on the display if the scaling is changed.

*RST: OFF

CURSor<m>:RESult?

Returns the measurement result for count, mean, RMS, rise and fall time, peak measurements, and burst width. Make sure to set `CURSor<m>:FUNCtion` correctly.

Suffix:

<m> 1
The numeric suffix is irrelevant.

Return values:

<Value> Measurement result

Usage: Query only

CURSor<m>:XDELta:INVerse?

Returns the inverse time difference between the two cursors (1/Δt).

Suffix:

<m> 1
The numeric suffix is irrelevant.

Return values:

<DeltaInverse> Range: -1,00E+026 to 1,00E+026
Increment: 0.1
*RST: 0
Default unit: 1/s

Usage: Query only

CURSor<m>:XDELta[:VALue]?

Returns the time difference between the two cursors (Δt).

Suffix:

<m> 1
The numeric suffix is irrelevant.

Return values:

<Delta> Range: -1,00E+026 to 1,00E+026
Increment: 0.1
*RST: 0
Default unit: s

Usage: Query only

CURSor<m>:YDELta:SLOPe?

Returns the inverse value of the voltage difference - the reciprocal of the vertical distance of two horizontal cursor lines: *1/ΔV*.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Return values:
<DeltyYslope> Inverse value

Usage: Query only

CURSor<m>:YDELta[:VALue]?

Queries the delta of the values in y-direction at the two cursors.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Return values:
<DeltaY> Delta value in V

Usage: Query only

CURsor<m>:XRATio:UNIT <Unit>

Sets the unit for X Ratio measurements with `CURSor<m>:XRATio[:VALue]?`.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Parameters:
<Unit> RATio | PCT | GRD | PI
RATio - floating value
PCT - percent
GRD - degree
PI - radian
*RST: RAT

CURSor<m>:XRATio[:VALue]?

Returns the ratio of the x-values (e.g. a duty cycle) between the first and second cursors and the first and third cursors: *(x2-x1)/(x3-x1)*.

Set the unit of the result with `CURsor<m>:XRATio:UNIT`.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Return values:
<Ratio> Numeric value corresponding to the specified unit.

Usage: Query only

CURSor<m>:YRATio:UNIT <Unit>

Sets the unit for Y Ratio measurements with `CURSor<m>:YRATio[:VALue]?` on page 334.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Parameters:
<Unit> RATio | PCT
RATio - floating value
PCT - percent
*RST: RAT

CURSor<m>:YRATio[:VALue]?

Returns the ratio of the y-values (e.g. overshooting) between the first and second cursors and the first and third cursors: *(y2-y1)/(y3-y1)*.

For this measurement, set the cursor measurement type `CURSor<m>:FUNCtion` to `HRATio`.

Set the unit of the result with `CURSor<m>:YRATio:UNIT`.

Suffix:
<m> 1
The numeric suffix is irrelevant.

Return values:
<Ratio> Numeric value corresponding to the specified unit.

Usage: Query only

15.2.8.2 Quick Measurements

MEASurement<m>:ALL[:STATe]....335
MEASurement<m>:AON....335
MEASurement<m>:AOFF....335
MEASurement<m>:ARESult?....335

MEASurement<m>:ALL[:STATe]

Starts or stops the quick measurement and sets the status bit.

Parameters:

<State> ON | OFF
*RST: OFF

Firmware/Software: FW 03.800

MEASurement<m>:AON

Starts the quick measurement.

Suffix:

<m> 1..4
The numeric suffix is irrelevant.

Usage: Event

MEASurement<m>:AOFF

Stops the quick measurement.

Suffix:

<m> 1..4
The numeric suffix is irrelevant.

Usage: Event

MEASurement<m>:ARESult?

Returns the results of the quick measurement.

Suffix:

<m> 1..4
Selects the measurement.

Return values:

<QuickMeasData> List of values
Quick measurement results are listed in the following order: PEAK, UPE, LPE, CYCR, CYCM, PER, FREQ, RTIM , FTIM

Usage: Query only

15.2.8.3 Automatic Measurements

MEASurement<m>[:ENABle]....336
MEASurement<m>:MAIN....336
MEASurement<m>:SOURce....338

MEASurement<m>:DELay:SLOPe....339
MEASurement<m>:RESult[:ACTual]?....340
MEASurement<m>:CATegory?....340

MEASurement<m>[:ENABle] <State>

Activates or deactivates the selected measurement (1-4). Only the results of active measurements are displayed in the result table.

Suffix:
<m> 1..4
Selects the measurement.

Parameters:
<State> ON | OFF
*RST: OFF

MEASurement<m>:MAIN <MeasType>

Defines the measurement type to be performed on the selected source. To query the results, use `MEASurement<m>:RESult[:ACTual]?`.

Suffix:
<m> 1..4
Selects the measurement.

Parameters:

<MeasType> FREQuency | PERiod | PEAK | UPEakvalue | LPEakvalue | PPCount | NPCount | RECount | FECount | HIGH | LOW | AMPLitude | MEAN | RMS | RTIMe | FTIMe | PDCYcle | NDCYcle | PPWidth | NPWidth | CYCMean | CYCRms | STDDev | CYCStddev | TFRequency | TPERiode | DELay | PHASe | BWIDth | POVershoot | NOVershoot | TBFRequency | TBPeriod

For a detailed description, see "Meas. Type" on page 95.

FREQuency
Frequency of the signal. The result is based on the length of the left-most signal period within the displayed section of the waveform of the selected channel.

PERiod
Length of the left-most signal period within the displayed section of the waveform of the selected channel.

PEAK
Peak-to-peak value within the displayed section of the waveform of the selected channel.

UPEakvalue
Maximum value within the displayed section of the waveform of the selected channel.

LPEakvalue
Minimum value within the displayed section of the waveform of the selected channel.

PPCount
Counts positive pulses.

NPCount
Counts negative pulses.

RECount
Counts the number of rising edges.

FECount
Counts the number of falling edges.

HIGH
Mean value of the high level of a square wave.

LOW
Mean value of the low level of a square wave.

AMPLitude
Amplitude of a square wave.

MEAN
Mean value of the complete displayed waveform of the selected channel.

RMS
RMS (Root Mean Square) value of the voltage of the complete displayed waveform of the selected channel.

RTIMe | FTIMe

Rise or falling time of the left-most rising edge within the displayed section of the waveform of the selected channel. The reference level for this mesurement is set with `REFLevel:RELative:MODE`.

PDCycle | NDCycle
Measure the positive or negative duty cycle.

PPWidth | NPWidth
Measure the width of positive or negative pulses.

CYCMean
Mean value of the left-most signal period of the waveform of the selected channel.

CYCRms
RMS (Root Mean Square) value of the voltage of the left-most signal period of the waveform of the selected channel.

STDDev
Measures the standard deviation of the waveform.

CYCStddev
Measures the standard deviation of one cycle, usually of the first, left-most signal period.

TFRequency | TPERiode
Measure the frequency of the trigger signal and the length of the its periods (hardware counter).

DELay
Time difference between two edges of the same or different waveforms. The waveforms are selected with `MEASurement<m>:SOURce`, and the edges with `MEASurement<m>:DELay:SLOPe`.

PHASe
Phase difference between two waveforms (time difference/period * 360). The waveforms are selected with `MEASurement<m>:SOURce`.

BWIDth
Burst width, the duration of one burst, measured from the first edge to the last edge that cross the middle reference level.

POVershoot | NOVershoot
Positive and negative overshoot of a square wave.

TBFRequency | TBPeriod
Measures the frequency of the B-trigger signal and the length of the B-trigger signal periods.

*RST: NONE (measurement is off)

MEASurement<m>:SOURce <SignalSource>[,<ReferenceSource>]

Selects one of the active signal, reference or math channels as the source(s) of the selected measurement. Available sources depend on the selected measurement type.

Suffix:

<m> 1..4
Selects the measurement place.

Parameters:

<SignalSource> NONE | CH1 | CH2 | CH3 | CH4 | MA1 | MA2 | MA3 | MA4 | MA5 | RE1 | RE2 | RE3 | RE4 TRIGger | CH1 | CH2 | CH3 | CH4 | MA1 | MA2 | MA3 | MA4 | MA5 | RE1 | RE2 | RE3 | RE4 | TRIGger | D0..D15 | D70 | D158

Waveform to be measured, required for all measurement types

CH1 | CH2 | CH3 | CH4
Active signal channels 1 to 4

MA1 | MA2 | MA3 | MA4 | MA5
Active math channels 1 to 5

RE1 | RE2 | RE3 | RE4
Active reference channels 1 to 4

TRIGger
Only return value. TRIG is returned if the measurement type is a trigger measurement: TFRequency | TPERiode measure the A-trigger source, TBFRequency | TBPeriod measure the B-trigger source.

D0..D15
Active digital channels, if MSO option R&S RTM-B1 is installed. The following automatic measurements are possible: frequency, period, edge and pulse counts, phase, delay, duty cycle, burst width.

D70 | D158
Active digital pods D0...D7 and D8...D15, available if MSO option R&S RTM-B1 is installed.

*RST: CH1

<ReferenceSource> NONE | CH1 | CH2 | CH3 | CH4 | MA1 | MA2 | MA3 | MA4 | MA5 | RE1 | RE2 | RE3 | RE4 | NONE | CH1 | CH2 | CH3 | CH4 | MA1 | MA2 | MA3 | MA4 | MA5 | RE1 | RE2 | RE3 | RE4 | D0..D15 | D70 | D158

Second waveform, reference source that is required for delay and phase mesurements.

MEASurement<m>:DELay:SLOPe <SignalSlope>,<ReferenceSlope>

Sets the edges to be used for delay measurement. The associated waveforms are defined with `MEASurement<m>:SOURce`

Parameters:

<SignalSlope> POSitive | NEGative

Slope of source 1 (first waveform)

*RST: POS

<ReferenceSlope> POSitive | NEGative
Slope of source 2 (second waveform)
*RST: POS

Firmware/Software: 03.400

MEASurement<m>:RESult[:ACTual]? [<MeasType>]

Returns the result of the specified measurement type.

Suffix:
<m> 1..4
Selects the measurement place.

Query parameters:
<MeasType> FREQuency | PERiod | PEAK | UPEakvalue | LPEakvalue | PPCount | NPCount | RECount | FECount | HIGH | LOW | AMPLitude | MEAN | RMS | RTIMe | FTIMe | PDCYcle | NDCYcle | PPWidth | NPWidth | CYCMean | CYCRms | STDDev | CYCStddev | TFRequency | TPERiode | DELay | PHASe | BWIDth | POVershoot | NOVershoot | TBFRequency | TBPeriod
Specifies the measurement type. See MEASurement<m>:MAIN on page 336.

Return values:
<Value> Measurement result. If no measurement was executed, no value (NAN) is returned.

Usage: Query only

MEASurement<m>:CATegory?

Returns the measurement category. Currently, the instrument supports only yt-measurements.

Suffix:
<m> 1..4
Selects the measurement.

Return values:
<Category> AMPTime
AMPtime: yt-measurements
*RST: AMPT

Usage: Query only

15.2.8.4 Reference Level

REFLevel:RELative:MODE....341
REFLevel:RELative:LOWer....341
REFLevel:RELative:UPPer....341
REFLevel:RELative:MIDDle....342

REFLevel:RELative:MODE <RelativeMode>

Sets the lower and upper reference levels for rise and fall time mesurements (cursor and automatic mesurements) as well as the middle reference level for phase and delay measurements. The levels are defined as percentages of the high signal level. The setting is valid for all measurement places.

Parameters:

<RelativeMode> TEN | TWENty | FIVE | USER

TEN: 10, 50 and 90%
TWENty: 20, 50 and 80%
FIVE: 5, 50 and 95 %
USER: levels are defined with `REFLevel:RELative:LOWer`, `REFLevel:RELative:MIDDle`, and `REFLevel:RELative:UPPer`.

*RST: TEN

Example:

```
REFL:REL:MODE TWENty
MEAS2:MAIN RTIM
```

Sets the reference levels for all measurement places and measures the rise time between these levels for measurement place 2:
lower reference level = 20% of high signal level
upper reference level = 80% of high signal level

REFLevel:RELative:LOWer <LowerLevel>
REFLevel:RELative:UPPer <UpperLevel>

Set the lower and upper reference levels for rise and fall time mesurements (cursor and automatic mesurements) if `REFLevel:RELative:MODE` is set to `USER`. The levels are defined as percentages of the high signal level. They are valid for all measurement places.

Parameters:

<LowerLevel> *RST: 10
Default unit: %

<UpperLevel> *RST: 90
Default unit: %

Firmware/Software: 03.400

REFLevel:RELative:MIDDle <MiddleLevel>

Set the middle reference level used for phase and delay measurements, if `REFLevel:RELative:MODE` is set to `USER`. The level is defined as percentages of the high signal level. The setting is valid for all measurement places.

Parameters:
<MiddleLevel> *RST: 50
Default unit: %

Firmware/Software: 03.400

15.2.8.5 Automatic Measurements - Statistic

MEASurement<m>:STATistics[:ENABle] 342
MEASurement<m>:STATistics:WEIGht 342
MEASurement<m>:STATistics:RESet 343
MEASurement<m>:RESult:AVG? 343
MEASurement<m>:RESult:STDDev? 343
MEASurement<m>:RESult:NPEak? 344
MEASurement<m>:RESult:PPEak? 344
MEASurement<m>:RESult:WFMCount? 344
MEASurement<m>:STATistics:VALue:ALL? 344
MEASurement<m>:STATistics:VALue<n>? 345

MEASurement<m>:STATistics[:ENABle] <StatisticEnable>

Activates or deactivates the statistical evaluation for the selected measurement.

Suffix:
<m> 1..4
Selects the measurement place.

Parameters:
<StatisticEnable> ON | OFF
*RST: OFF

Firmware/Software: FW 03.700

MEASurement<m>:STATistics:WEIGht <AverageCount>

Sets the number of measured waveforms used for calculation of average and standard deviation.

Suffix:
<m> 1..4
Selects the measurement place.

Parameters:
<AverageCount> Range: 2 to 1000
Increment: 1
*RST: 1000

Firmware/Software: FW 03.700

MEASurement<m>:STATistics:RESet

Deletes the statistical results for the selected measurement, and starts a new statistical evaluation if the acquisition is running. The waveform count is set to 0 and all measurement values are set to NAN.

Suffix:
<m> 1..4
Selects the measurement place.

Usage: Event

Firmware/Software: FW 03.700

MEASurement<m>:RESult:AVG? <AverageValue>

Returns the average value of the current mesurement series.

The number of waveforms used for calculation is defined with `MEASurement<m>:STATistics:WEIGht`.

Suffix:
<m> 1..4
Selects the measurement place.

Query parameters:
<AverageValue> Statistic value

Usage: Query only

Firmware/Software: FW 03.700

MEASurement<m>:RESult:STDDev? <StandardDeviation>

Returns the statistical standard deviation of the current mesurement series.

The number of waveforms used for calculation is defined with `MEASurement<m>:STATistics:WEIGht`.

Suffix:
<m> 1..4
Selects the measurement place.

Query parameters:
<StandardDeviation> Statistic value

Usage: Query only

Firmware/Software: FW 03.700

MEASurement<m>:RESult:NPEak? <NegativePeak>

Returns the minimum measurement value of the current measurement series.

Suffix:
<m> 1..4
Selects the measurement place.

Query parameters:
<NegativePeak> Minimum measurement value

Usage: Query only

Firmware/Software: FW 03.700

MEASurement<m>:RESult:PPEak? <PositivePeak>

Returns the maximum measurement value of the current measurement series.

Suffix:
<m> 1..4
Selects the measurement place.

Query parameters:
<PositivePeak> Maximum measurement value

Usage: Query only

Firmware/Software: FW 03.700

MEASurement<m>:RESult:WFMCount? <WaveformCount>

Returns the current number of measured waveforms.

Suffix:
<m> 1..4
Selects the measurement place.

Query parameters:
<WaveformCount> Number of measured waveforms

Usage: Query only

Firmware/Software: FW 03.700

MEASurement<m>:STATistics:VALue:ALL?

Returns all values from the statistics buffer.

Note that valid buffered values can only be read if the acquisition is stopped. As long as the acquisition is running, the buffer contents is changing and the buffered values are not valid for reading.

Suffix:
<m> 1..4
Selects the measurement place.

Return values:
<ValueList> Comma-separated list of statistical values

Usage: Query only

MEASurement<m>:STATistics:VALue<n>?

Returns one statistical value from the indicated buffer place.

Note that valid buffered values can only be read if the acquisition is stopped. As long as the acquisition is running, the buffer contents is changing and the buffered values are not valid for reading.

Suffix:
<m> 1..4
Selects the measurement place.

<n> *
Buffer place. The buffer size is limited by `MEASurement<m>:STATistics:WEIGht`.

Return values:
<StatisticValue> Statistical value

Usage: Query only

15.2.9 Mathematics

This chapter describes commands that configure or perform mathematical functions.

For data queries and conversion, consider also the following commands:

- `FORMat[:DATA]` on page 278
- `CALCulate:MATH<m>:DATA:XINCrement?` on page 280
- `CALCulate:MATH<m>:DATA:XORigin?` on page 279
- `CALCulate:MATH<m>:DATA:YINCrement?` on page 280
- `CALCulate:MATH<m>:DATA:YORigin?` on page 280
- `CALCulate:MATH<m>:DATA:YRESolution?` on page 281

CALCulate:MATH<m>:STATe....345
CALCulate:MATH<m>:SCALe....346
CALCulate:MATH<m>:POSition....346
CALCulate:MATH<m>[:EXPRession][:DEFine]....346
CALCulate:MATH<m>:DATA?....347
CALCulate:MATH<m>:DATA:HEADer?....348

CALCulate:MATH<m>:STATe <State>

Defines whether the selected mathematical channel is active or not. Only if a channel is active it is visible on the screen and can be selected as a source for analysis and display functions.

Suffix:
<m> 1..4
Selects the math waveform.

Parameters:
<State> ON | OFF
*RST: OFF

CALCulate:MATH<m>:SCALe <Scale>

Sets the vertical scale for the specified math waveform.

In FFT mode, the command sets the vertical scale of the FFT window. The scale unit for FFT is set with `CALCulate:MATH<m>:FFT:MAGNitude:SCALe`.

Suffix:
<m> 1..4
Selects the math waveform.
IN FFT mode, the numeric suffix is irrelevant.

Parameters:
<Scale> Scale value
Range: -1.0E-24 to 5.0E+25
Increment: 1, 2, 5 progression, for example, 1mV/div, 2mV/div, 5mV/div, 10, 20, 50...
*RST: 1

CALCulate:MATH<m>:POSition <Position>

Sets the vertical position of the specified math waveform in the window.

Suffix:
<m> 1..4
Selects the math waveform.

Parameters:
<Position> Position value, given in divisions.
Range: -1,88E+005 to 2,12E+005
Increment: 0.01 in reset state
*RST: 2

CALCulate:MATH<m>[:EXPRession][:DEFine] <RemComplExpr>

Defines the equation to be calculated for the selected math waveform as a regular expression.

For details on available operators, see "Operator" on page 103.

Suffix:
<m> 1..4
Selects the math waveform.

Parameters:

<RemComplExpr> String parameter, consisting of the mathematical operation and the source(s) written in parenthesis.

Example: `CALC:MATH<2>:EXPR:DEF "CH1+CH2"`

Operation	Expression string	Comment
Addition	"ADD(CH1,CH2)"	"CH1+CH2" is also possible
Subtraction	"SUB(CH1,CH2)"	"CH1-CH2" is also possible
Multiplication	"MUL(CH1,CH2)"	"CH1*CH2" is also possible
Division	"DIV(CH1,CH2)"	"CH1/CH2" is also possible
Maximum amplitude	"MAX(CH1,CH2)"	
Minimum amplitude	"MIN(CH1,CH2)"	
Square	"SQR(CH1)"	
Square Root	"SQRT(CH1)"	
Absolute value	"ABS(CH1)"	
Positive wave	"POS(CH1)"	
Negative wave	"NEG(CH1)"	
Reciprocal	"REC(CH1)"	
Inverse	"INV(CH1)"	
Common logarithm (basis 10)	"LOG(CH1)"	
Natural logarithm (basis e)	"LN(CH1)"	
Derivative	"DERI(CH1)"	
Integral	"INT(CH1)"	
IIR low pass	"IIRL(CH1,1E6)"	CH1 – Source waveform 1e6 – constant value, cut-off frequency of the low or high pass
IIR high pass	"IIRH(CH1,1E6)"	
FFT	"FFTMAG(CH1)"	FFT function of the source waveform See also: chapter 15.2.10, "FFT", on page 348

CALCulate:MATH<m>:DATA?

Returns the data of the math waveform points for transmission from the instrument to the controlling computer. The waveforms data can be used in MATHLAB, for example.

To set the export format, use `FORMat[:DATA]` on page 278.

Suffix:

<m> 1..4
Selects the math waveform.

Return values:

<Data> List of values according to the format settings - voltages, or magnitudes of a spectrum.

Usage: Query only

CALCulate:MATH<m>:DATA:HEADer?

Returns information on the math waveform.

Table 15-15: Header data

Position	Meaning	Example
1	XStart in s	-9.477E-008 = - 94,77 ns
2	XStop in s	9.477E-008 = 94,77 ns
3	Record length of the waveform in Samples	200000
4	Number of values per sample interval, usually 1.	1

Suffix:

<m> 1..4
Selects the math waveform.

Return values:

<Header> Comma-separated value list
Example: `-9.477E-008,9.477E-008,200000,1`

Usage: Query only

15.2.10 FFT

To define an FFT for a channel waveform, use `CALC:MATH:EXPR "FFTMAG(CHx)"`.

CALCulate:MATH<m>:FFT:WINDow:TYPE....349
CALCulate:MATH<m>:ARIThmetics....349
CALCulate:MATH<m>:FFT:AVERage:COUNt....350
CALCulate:MATH<m>:FFT:MAGNitude:SCALe....350
CALCulate:MATH<m>:FFT:BANDwidth[:RESolution]:ADJusted?....351
CALCulate:MATH<m>:FFT:BANDwidth[:RESolution]:AUTO....351
CALCulate:MATH<m>:FFT:BANDwidth[:RESolution]:RATio....351
CALCulate:MATH<m>:FFT:BANDwidth[:RESolution][:VALue]....352
CALCulate:MATH<m>:FFT:CFRequency....352
CALCulate:MATH<m>:FFT:FULLspan....352
CALCulate:MATH<m>:FFT:SPAN....352
CALCulate:MATH<m>:FFT:STARt....353
CALCulate:MATH<m>:FFT:STOP....353
CALCulate:MATH<m>:FFT:TIME:RANGe....353
CALCulate:MATH<m>:FFT:TIME:POSition....354
CALCulate:MATH<m>:FFT:SRATe?....354

CALCulate:MATH<m>:FFT:WINDow:TYPE <WindowType>

Window functions are multiplied with the input values and thus can improve the FFT display.

Suffix:
<m> 1..4
The numeric suffix is irrelevant.

Parameters:
<WindowType> RECTangular | HAMMing | HANNing | BLACkmanharris

RECTangular
The rectangular window multiplies all points by one. The result is a high frequency accuracy with thin spectral lines, but also with increased noise. Use this function preferably with pulse response tests where start and end values are zero.

HAMMing
The Hamming window is bell shaped. Its value is not zero at the borders of the measuring interval. Thus, the noise level inside the spectrum is higher than Hanning or Blackman, but smaller than the rectangular window. The width of the spectral lines is thinner than the other bell-shaped functions. Use this window to measure amplitudes of a periodical signal precisely.

HANNing
The Hanning window is bell shaped. Unlike the Hamming window, its value is zero at the borders of the measuring interval. Thus, the noise level within the spectrum is reduced and the width of the spectral lines enlarges. Use this window to measure amplitudes of a periodical signal precisely.

BLACkmanharris
The Blackman window is bell shaped and has the steepest fall in its wave shape of all other available functions. Its value is zero at both borders of the measuring interval. In the Blackman window the amplitudes can be measured very precisely. However, determining the frequency is more difficult. Use this window to measure amplitudes of a periodical signal precisely.

*RST: HANNing

CALCulate:MATH<m>:ARIThmetics <Arithmetics>

Defines the mode for FFT calculation and display.

Suffix:
<m> 1..4
The numeric suffix is irrelevant.

Parameters:

<Arithmetics> OFF | ENVelope | AVERage

OFF
The FFT is performed without any additional weighting or post-processing of the acquired data. The new input data is acquired and displayed, and thus overwrites the previously saved and displayed data.

ENVelope
In addition to the normal spectrum, the maximal oscillations are saved separately and updated for each new spectrum. The maximum values are displayed together with the newly acquired values and form an envelope. This envelope indicates the range of all FFT trace values that occurred.

AVERage
The average of several spectrums is calculated. The number of spectrums used for the averaging is defined using the command. This mode is useful for noise rejection.

*RST: OFF

CALCulate:MATH<m>:FFT:AVERage:COUNt

Defines the number of spectrums used for averaging if `CALCulate:MATH<m>:ARIThmetics` is set to `AVERage`.

Suffix:

<m> 1..4
The numeric suffix is irrelevant.

Parameters:

<AverageCount> Integer value

Range: 2 to 512
Increment: 2^n
*RST: 2

CALCulate:MATH<m>:FFT:MAGNitude:SCALe

Defines the scaling unit of the y-axis.

To set the scale value, use `CALCulate:MATH<m>:SCALe`.

Suffix:

<m> 1..4
The numeric suffix is irrelevant.

Parameters:

<Magnitude Scale> LINear | DBM | DBV

LINear
linear scaling; displays the RMS value of the voltage.

DBM
logarithmic scaling; related to 1 mW

DBV
logarithmic scaling; related to 1 Veff

*RST: DBM

Example:
```
CALC:MATH:FFT:MAGN:SCAL DBM
CALC:MATH:SCAL 20
```
Set the Y-scale of the FFT window to 20 dBm.

CALCulate:MATH<m>:FFT:BANDwidth[:RESolution]:ADJusted?

Queries the effective resolution bandwidth.

Suffix:

<m> 1..4
The numeric suffix is irrelevant.

Return values:

<AdjResBW> Range: Depends on various other settings.
Default unit: Hz

Usage: Query only

CALCulate:MATH<m>:FFT:BANDwidth[:RESolution]:AUTO <SpanRBWCoupling>

Couples the frequency span to the RBW.

Suffix:

<m> 1..4
The numeric suffix is irrelevant.

Parameters:

<SpanRBWCoupling> ON | OFF

CALCulate:MATH<m>:FFT:BANDwidth[:RESolution]:RATio <SpanRBWRatio>

Defines the ratio of span (Hz) / resolution bandwidth (Hz). The span/RBW ratio is half the number of points used for FFT which is defined with manual operation in the menu.

Suffix:

<m> 1..4
The numeric suffix is irrelevant.

Parameters:

<SpanRBWRatio> Range: The value is changed in 2^n steps from 2^10 to 2^15 (1024, 2048,4096,8192,16384, 32768).

Example: CALC:MATH:FFT:BAND:RAT 32768
Sets the number of points to 65536.

CALCulate:MATH<m>:FFT:BANDwidth[:RESolution][:VALue] <ResolutionBW>

Defines the resolution bandwidth - the minimum frequency step at which the individual components of a spectrum can be distinguished

Suffix:
<m> 1..4
The numeric suffix is irrelevant.

Parameters:
<ResolutionBW> Range: Depends on various other settings.
Default unit: Hz

CALCulate:MATH<m>:FFT:CFRequency <CenterFreq>

Defines the position of the displayed frequency domain, which is (Center - Span/2) to (Center + Span/2). The width of the domain is defined using the CALCulate:MATH<m>:FFT:SPAN command.

Suffix:
<m> 1..4
The numeric suffix is irrelevant.

Parameters:
<CenterFreq> Range: Limited by the first data point (minimum) and last data point (maximum) of the FFT curve.
Increment: Depends on the span and the number of data points (span/RBW ratio).
Default unit: Hz

CALCulate:MATH<m>:FFT:FULLspan

Performs FFT calculation for the full frequency span.

Suffix:
<m> 1..4
The numeric suffix is irrelevant.

Usage: Event

CALCulate:MATH<m>:FFT:SPAN <FreqSpan>

The span is specified in Hertz and defines the width of the displayed frequency range, which is (Center - Span/2) to (Center + Span/2). The position of the span is defined using the CALCulate:MATH<m>:FFT:CFRequency command.

Suffix:
<m> 1..4
The numeric suffix is irrelevant.

Parameters:
<FreqSpan> Range: Depends on various other settings, mainly on time base and span/RBW ratio.
Increment: Only 1 | 2 | 5 in first digit
Default unit: Hz

CALCulate:MATH<m>:FFT:STARt <StartFreq>

Defines the start frequency of the displayed frequency domain at the left display edge: *Center - Span/2*

You can set start and stop frequency instead of defining a center frequency and span.

Suffix:
<m> 1..4
The numeric suffix is irrelevant.

Parameters:
<StartFreq> Range: Depends on various other settings, mainly on time base, span/RBW ratio, and center frequency.
Default unit: Hz

CALCulate:MATH<m>:FFT:STOP <StopFreq>

Defines the stop frequency of the displayed frequency domain at the right display edge: *Center + Span/2*

You can set start and stop frequency instead of defining a center frequency and span.

Suffix:
<m> 1..4
The numeric suffix is irrelevant.

Parameters:
<StopFreq> Range: Depends on various other settings, mainly on time base, span/RBW ratio, and center frequency.
Default unit: Hz

CALCulate:MATH<m>:FFT:TIME:RANGe

Defines the width of the time base extract from the Y(t)-window for which the FFT is calculated.

Parameters:
<WindowWidth> Range: depends on the time base
Default unit: s

Firmware/Software: FW 03.800

CALCulate:MATH<m>:FFT:TIME:POSition

Defines the position of the time base extract in the Y(t)-window for which the FFT is calculated.

Parameters:

<WindowPosition>	Range:	depends on the time base and the width of the FFT time base extract
	Default unit:	s

Firmware/Software: FW 03.800

CALCulate:MATH<m>:FFT:SRATe?

Returns the sample rate of data used in an FFT analysis.

Return values:

<SampleRate>	Default unit:	Sa/s

Usage: Query only

15.2.11 Masks

MASK:STATe....355
MASK:TEST....355
MASK:LOAD....355
MASK:SAVE....355
MASK:SOURce....355
MASK:CHCopy....355
MASK:YPOSition....356
MASK:YSCale....356
MASK:YWIDth....356
MASK:XWIDth....356
MASK:COUNt?....357
MASK:VCOunt?....357
MASK:RESet:COUNter....357
MASK:ACTion:SOUNd:EVENt:MODE....357
MASK:ACTion:STOP:EVENt:MODE....357
MASK:ACTion:SCRSave:EVENt:MODE....357
MASK:ACTion:PRINt:EVENt:MODE....357
MASK:ACTion:WFMSave:EVENt:MODE....357
MASK:ACTion:SOUNd:EVENt:COUNt....358
MASK:ACTion:STOP:EVENt:COUNt....358
MASK:ACTion:SCRSave:EVENt:COUNt....358
MASK:ACTion:PRINt:EVENt:COUNt....358
MASK:ACTion:WFMSave:EVENt:COUNt....358

MASK:STATe <State>

Turns the mask test mode on or off. When turning off, any temporarily stored new masks are deleted.

Parameters:

<State> ON | OFF

*RST: OFF

MASK:TEST <Test>

Starts, finishes or interrupts a mask test.

Parameters:

<Test> RUN | STOP | PAUSe

*RST: STOP

MASK:LOAD <FileName>

Loads a stored mask from the specified file.

Setting parameters:

<FileName> String parameter

Path and file name

Usage: Setting only

MASK:SAVE <FileName>

Saves the current mask in the specified file.

Setting parameters:

<FileName> String parameter

Path and file name

Usage: Setting only

MASK:SOURce <Source>

Defines the channel to be compared with the mask.

Parameters:

<Source> CH1 | CH2 | CH3 | CH4

CH3 and CH4 are only available on 4-channel R&S RTM models.

*RST: CH1

MASK:CHCopy

Creates a mask from the envelope waveform of the test source set with `MASK:SOURce`.

Usage: Event

MASK:YPOSition <Yposition>

Moves the mask vertically within the display.

Parameters:

<Yposition> Mask offset from the vertical center

Range: -200 to 200
Increment: 0,02
*RST: 0
Default unit: div

MASK:YSCale <Yscale>

Changes the vertical scaling to stretch or compress the mask in y-direction.

Parameters:

<Yscale> A value over 100% stretches the amplitudes; a value less than 100% compresses the amplitudes.

Range: 10 to 1000
Increment: 1
*RST: 100
Default unit: %

MASK:YWIDth <Yaddition>

Changes the width of the mask in vertical direction.

Parameters:

<Yaddition> The value is added to the y-values of the upper mask limit and subtracted from the y-values of the lower mask limit.

Range: 0 to 5,12
Increment: 0,04
*RST: 0
Default unit: div

MASK:XWIDth <Xaddition>

Changes the width of the mask in horizontal direction.

Parameters:

<Xaddition> The value is added to the positive x-values and subtracted from the negative x-values of the mask limits in relation to the mask center.

Range: 0 to 10
Increment: 0,01
*RST: 0
Default unit: div

MASK:COUNt?

Returns the number of tested acquisitions.

Return values:
<TotalCount> Total number of tested acquisitions

Usage: Query only

MASK:VCOunt?

Returns the number of acquistions that hit the mask.

Return values:
<ViolationCount> Acquisition count

Usage: Query only

MASK:RESet:COUNter

Sets the counters of passed and failed acquisitions to Zero.

Usage: Event

Firmware/Software: FW 03.800

MASK:ACTion:SOUNd:EVENt:MODE <EventMode>
MASK:ACTion:STOP:EVENt:MODE <EventMode>
MASK:ACTion:SCRSave:EVENt:MODE <EventMode>
MASK:ACTion:PRINt:EVENt:MODE <EventMode>
MASK:ACTion:WFMSave:EVENt:MODE <EventMode>

Defines when and how often the action will be executed.

- SOUNd: Generates a beep sound.
- STOP: Stops the waveform acquisition.
- PRINt: Prints a screenshot to a printer connected to the USB connector on the front or rear panel.
- SCRSave: Saves a screenshot according to printer output settings.
- WFMSave: Saves the waveform data according to the screenshot output settings. For output settings, see chapter 15.2.15.1, "Screenshots", on page 441.

Parameters:

<EventMode> OFF | EACH | SINGle | CYCLic

OFF
No action is executed.

EACH
The selected action is executed on each violation of the mask.

SINGle
The selected action is executed once after the n-th violation.

CYCLic
The selected action is executed repeatedly after each n-th violation.
The number of violations <n> is set with the relevant MASK:ACTion:...:EVENt:COUNt command.

*RST: OFF

Firmware/Software: FW 03.800

MASK:ACTion:SOUNd:EVENt:COUNt <EventCount>
MASK:ACTion:STOP:EVENt:COUNt <EventCount>
MASK:ACTion:SCRSave:EVENt:COUNt <EventCount>
MASK:ACTion:PRINt:EVENt:COUNt <EventCount>
MASK:ACTion:WFMSave:EVENt:COUNt <EventCount>

Sets the number of mask violations after which the action is executed. The command is only relevant if the associated MASK:ACTion:...:EVENt:MODE is set to `SINGle` or `CYCLic`.

Parameters:

<EventCount> Integer value, number of mask violations

Firmware/Software: FW 03.800

15.2.12 Search

- General Search Configuration....359
- Edge Search Configuration....362
- Width Search Configuration....362
- Peak Search Configuration....364
- Rise/Fall Time Search Configuration....365
- Runt Search Configuration....366
- Data2Clock Search Configuration....368
- Pattern Search Configuration....370
- Search Results....372

15.2.12.1 General Search Configuration

SEARch:STATe....359
SEARch:CONDition....359
SEARch:SOURce....361
SEARch:GATE:MODE....361
SEARch:GATE:ABSolute:START....361
SEARch:GATE:ABSolute:STOP....361

SEARch:STATe <SearchState>

Enables and disables the search mode.

Parameters:

<SearchState> ON | OFF

*RST: OFF

Example: chapter 15.3.2.1, "Searching for a Pulse of Specified Width", on page 460

Firmware/Software: FW 03.400

SEARch:CONDition <SearchCondition>

Selects the event you want to search for.

Parameters:

<SearchCondition> EDGE | WIDTh | PEAK | RUNT | RTIMe | DATatoclock | PATTern | PROTocol

EDGE
An edge search result is found when the waveform passes the given level in the specified direction.

WIDTH
A width search finds pulses with an exact pulse width, or pulses shorter or longer than a given time, or pulses inside or outside the allowable time range.

PEAK
The peak search finds pulses exceeding a given amplitude.

RUNT
The runt search finds pulses lower than normal in amplitude. The amplitude crosses the first threshold twice without crossing the second one. In addition to the threshold amplitudes, you can define a time limit for the runt in the same way as for width search: runts with exact width, shorter or longer than a given time, or runts inside or outside the allowable time range.

RTIMe
The rise or fall time search finds slopes with an exact rise or fall time, or rise/fall times shorter or longer than a given limit, or rise/fall times inside or outside the allowable time range.

DATatoclock
The Data2Clock search - also known as setup/hold - finds violation of setup and hold times. It analyzes the relative timing between two signals: a data signal and the synchronous clock signal. Setup time is the time that the data signal is steady before clock edge. Hold time is the time that the data signal is steady after clock edge.

PATTern
The pattern search finds logical combinations of channel states inside or outside a specified time range. For each channel, its state and threshold level is defined. The states are combined logically, and the time of true pattern results is compared with a specified time range.

PROTocol
The protocol search finds various events in decoded data of CAN or LIN signals, for example, a specified frame type, identifier, data, and errors. Available search settings depend on the configured bus type. For bus types PARallel, I2C, SPI, SSPI, and UART no search is available.
See also: `BUS<b>:TYPE` on page 375

*RST: EDGE

Example: chapter 15.3.2.1, "Searching for a Pulse of Specified Width", on page 460

Firmware/Software: FW 03.400

SEARch:SOURce <SearchSource>

Selects the waveform to be analyzed. One of the active channel, math, and reference waveforms can be searched.

Parameters:

<SearchSource> CH1 | CH2 | CH3 | CH4 | MA1 | MA2 | MA3 | MA4 | RE1 | RE2 | RE3 | RE4

*RST: CH1

Example: chapter 15.3.2.1, "Searching for a Pulse of Specified Width", on page 460

Firmware/Software: FW 03.400

SEARch:GATE:MODE

Defines the search area. If the search is performed on a running acquisition series, the instrument analyzes the displayed data. The search on a stopped acquisition analyzes the contents of the memory.

Parameters:

<GateMode> OFF | DISPlay | ABSolute

OFF
Running acquisition: all waveform samples that are displayed on the screen.
Stopped acquisition: all data samples that are stored in the memory.

DISPlay
Search is restricted to the time range of the display.

ABSolute
Search is restricted to the time range defined by `SEARch:GATE:ABSolute:START` and `SEARch:GATE:ABSolute:STOP`.

SEARch:GATE:ABSolute:START <StartTime>

Sets the start time of the search area in relation to the trigger point if `SEARch:GATE:MODE` on page 361 is set to `ABSolute`.

Parameters:

<StartTime> Default unit: s

SEARch:GATE:ABSolute:STOP <StopTime>

Sets the end time of the search area in relation to the trigger point if `SEARch:GATE:MODE` on page 361 is set to `ABSolute`.

Parameters:

<StopTime> Default unit: s

15.2.12.2 Edge Search Configuration

SEARch:TRIGger:EDGE:SLOPe....362
SEARch:TRIGger:EDGE:LEVel....362
SEARch:TRIGger:EDGE:LEVel:DELTa....362

SEARch:TRIGger:EDGE:SLOPe <Slope>

Sets the slope to be found.

Parameters:

<Slope> POSitive | NEGative | EITHer
*RST: POS

Firmware/Software: FW 03.400

SEARch:TRIGger:EDGE:LEVel <Level>

Sets the voltage level for the edge search.

Parameters:

<Level> *RST: 0.6 V

Firmware/Software: FW 03.400

SEARch:TRIGger:EDGE:LEVel:DELTa <DeltaLevel>

Sets a hysteresis range above and below the search level to avoid unwanted search results caused by noise oscillation around the level.

Parameters:

<DeltaLevel> Range: Lower limit depends on vertical scale and other settings, no upper limit
*RST: 0.2 V

Firmware/Software: FW 03.400

15.2.12.3 Width Search Configuration

SEARch:TRIGger:WIDTh:POLarity....362
SEARch:TRIGger:WIDTh:LEVel....363
SEARch:TRIGger:WIDTh:LEVel:DELTa....363
SEARch:TRIGger:WIDTh:RANGe....363
SEARch:TRIGger:WIDTh:WIDTh....364
SEARch:TRIGger:WIDTh:DELTa....364

SEARch:TRIGger:WIDTh:POLarity <Polarity>

Indicates the polarity of the pulse to be searched for.

Parameters:

<Polarity> POSitive | NEGative

*RST: POS

Example: chapter 15.3.2.1, "Searching for a Pulse of Specified Width", on page 460

Firmware/Software: FW 03.400

SEARch:TRIGger:WIDTh:LEVel <Level>

Sets the voltage level on which the pulse width is measured.

Parameters:

<Level> *RST: 500 mV

Firmware/Software: FW 03.400

SEARch:TRIGger:WIDTh:LEVel:DELTa <DeltaLevel>

Sets a hysteresis range above and below the search level to avoid unwanted search results caused by noise oscillation around the level.

Parameters:

<DeltaLevel> Range: Lower limit depends on vertical scale and other settings, no upper limit

*RST: 200 mV

Firmware/Software: FW 03.400

SEARch:TRIGger:WIDTh:RANGe <Range>

Sets how the measured pulse width is compared with the given limit(s).

To set the width, use `SEARch:TRIGger:WIDTh:WIDTh`.

To set the range ± Δt, use `SEARch:TRIGger:WIDTh:DELTa`.

Parameters:

<Range> WITHin | OUTSide | SHORter | LONGer

WITHin
Finds pulses inside the range *width* ± *Δt*.

OUTSide
Finds pulses outside the range *width* ± *Δt*.

SHORter
Finds pulses shorter than the given width.

LONGer
Finds pulses longer than the given width.

*RST: WITH

Example: chapter 15.3.2.1, "Searching for a Pulse of Specified Width", on page 460

Firmware/Software: FW 03.400

SEARch:TRIGger:WIDTh:WIDTh <Width>

Sets the reference pulse width, the nominal value for comparisons.

Parameters:
<Width> Default unit: s

Example: chapter 15.3.2.1, "Searching for a Pulse of Specified Width", on page 460

Firmware/Software: FW 03.400

SEARch:TRIGger:WIDTh:DELTa <DeltaWidth>

Sets a range Δt to the reference pulse width set with `SEARch:TRIGger:WIDTh:WIDTh` if `SEARch:TRIGger:WIDTh:RANGe` is set to `WITHin` or `OUTSide`

Parameters:
<DeltaWidth> Range: Lower limit depends on the resolution, practically no upper limit

Example: chapter 15.3.2.1, "Searching for a Pulse of Specified Width", on page 460

Firmware/Software: FW 03.400

15.2.12.4 Peak Search Configuration

SEARch:MEASure:PEAK:POLarity....364
SEARch:MEASure:LEVel:PEAK:MAGNitude....364

SEARch:MEASure:PEAK:POLarity <Polarity>

Indicates the polarity of a the pulse to be searched for a peak.

Parameters:
<Polarity> POSitive | NEGative | EITHer
*RST: POS

Firmware/Software: FW 03.400

SEARch:MEASure:LEVel:PEAK:MAGNitude <Magnitude>

Sets the amplitude limit.

Parameters:
<Magnitude> Default unit: V

Firmware/Software: FW 03.400

15.2.12.5 Rise/Fall Time Search Configuration

SEARch:TRIGger:RISetime:SLOPe....365
SEARch:TRIGger:LEVel:RISetime:LOWer....365
SEARch:TRIGger:LEVel:RISetime:UPPer....365
SEARch:TRIGger:RISetime:RANGe....365
SEARch:TRIGger:RISetime:TIME....366
SEARch:TRIGger:RISetime:DELTa....366

SEARch:TRIGger:RISetime:SLOPe <Polarity>

Sets the slope to be found.

Parameters:

<Polarity> POSitive | NEGative | EITHer

POSitive: to search for rise time.
NEGative to search for fall time.
EITHer: to search for rise and fall time

*RST: POS

Firmware/Software: FW 03.700

SEARch:TRIGger:LEVel:RISetime:LOWer <LowerLevel>

Sets the lower voltage threshold. When the signal crosses this level, the rise time measurement starts or stops depending on the selected slope.

Parameters:

<LowerLevel> *RST: 400 mV
Default unit: V

Firmware/Software: FW 03.700

SEARch:TRIGger:LEVel:RISetime:UPPer <UpperLevel>

Sets the upper voltage threshold. When the signal crosses this level, the rise/fall time measurement starts or stops depending on the selected slope.

Parameters:

<UpperLevel> *RST: 600 mV
Default unit: V

Firmware/Software: FW 03.700

SEARch:TRIGger:RISetime:RANGe <Range>

Sets how the measured rise or fall time is compared with the given limit(s).

To set the rise/fall time, use `SEARch:TRIGger:RISetime:TIME`.

To set the range ± Δt, use `SEARch:TRIGger:RISetime:DELTa`.

Parameters:

<Range> LONGer | SHORter | WITHin | OUTSide

LONGer
Finds rise/fall times longer than the given time.

SHORter
Finds rise/fall times shorter than the given time.

WITHin
Finds rise/fall times inside the range *time* ± *Δt*.

OUTSide
Finds rise/fall times outside the range *time* ± *Δt*.

*RST: LONG

Firmware/Software: FW 03.700

SEARch:TRIGger:RISetime:TIME <Time>

Sets the reference rise or fall time, the nominal value for comparisons.

Parameters:

<Time> Range: Depends on various settings, mainly time base and sample rate
*RST: 200e-6
Default unit: s

Firmware/Software: FW 03.700

SEARch:TRIGger:RISetime:DELTa <DeltaTime>

Sets a range Δt to the reference rise/fall time set with `SEARch:TRIGger:RISetime:TIME` if `SEARch:TRIGger:RISetime:RANGe` on page 365 is set to `Within` or `Outside`. The instrument finds rise/fall times inside or outside the range *time* ± *Δt*.

Parameters:

<DeltaTime> Range: Depends on various settings, mainly time base and sample rate
*RST: 50e-6
Default unit: s

Firmware/Software: FW 03.700

15.2.12.6 Runt Search Configuration

SEARch:TRIGger:RUNT:POLarity....367
SEARch:TRIGger:LEVel:RUNT:LOWer....367
SEARch:TRIGger:LEVel:RUNT:UPPer....367
SEARch:TRIGger:RUNT:RANGe....367
SEARch:TRIGger:RUNT:WIDTh....368
SEARch:TRIGger:RUNT:DELTa....368

SEARch:TRIGger:RUNT:POLarity <Polarity>

Indicates the polarity of a the runt to be searched for.

Parameters:

<Polarity> POSitive | NEGative | EITHer
*RST: POS

Firmware/Software: FW 03.700

SEARch:TRIGger:LEVel:RUNT:LOWer <LowerLevel>

Sets the lower voltage threshold for runt detection. A positive runt crosses the lower level twice without crossing the upper level.

Parameters:

<LowerLevel> *RST: 400 mV
Default unit: V

Firmware/Software: FW 03.700

SEARch:TRIGger:LEVel:RUNT:UPPer <UpperLevel>

Sets the upper voltage threshold for runt detection. A negative runt crosses the upper level twice without crossing the lower level.

Parameters:

<UpperLevel> *RST: 600 mV
Default unit: V

Firmware/Software: FW 03.700

SEARch:TRIGger:RUNT:RANGe <Range>

Sets how the measured pulse width is compared with the given limit(s).

To set the width, use `SEARch:TRIGger:RUNT:WIDTh`.

To set the range ± Δt, use `SEARch:TRIGger:RUNT:DELTa`.

Parameters:

<Range> LONGer | SHORter | WITHin | OUTSide

LONGer
Finds pulses longer than the given width.

SHORter
Finds pulses shorter than the given width.

WITHin
Finds pulses inside the range *width ± Δt*.

OUTSide
Finds pulses outside the range *width ± Δt*.

*RST: LONG

Firmware/Software: FW 03.700

SEARch:TRIGger:RUNT:WIDTh <Width>

Sets the reference runt pulse width, the nominal value for comparisons.

Parameters:

<Width>
Range: Depends on various settings, mainly time base and sample rate
*RST: 200e-6
Default unit: s

Firmware/Software: FW 03.700

SEARch:TRIGger:RUNT:DELTa <DeltaWidth>

Sets a range Δt to the reference pulse width set with `SEARch:TRIGger:RUNT:WIDTh` if `SEARch:TRIGger:RUNT:RANGe` on page 367 is set to `WITHin` or `OUTSide`.

Parameters:

<DeltaWidth>
Range: Depends on various settings, mainly time base and sample rate
*RST: 50e-6
Default unit: s

Firmware/Software: FW 03.700

15.2.12.7 Data2Clock Search Configuration

SEARch:TRIGger:DATatoclock:CSOurce....368
SEARch:TRIGger:DATatoclock:CLEVel....369
SEARch:TRIGger:DATatoclock:DLEVel....369
SEARch:TRIGger:DATatoclock:CLEVel:DELTa....369
SEARch:TRIGger:DATatoclock:DLEVel:DELTa....369
SEARch:TRIGger:DATatoclock:CEDGe....369
SEARch:TRIGger:DATatoclock:HTIMe....369
SEARch:TRIGger:DATatoclock:STIMe....370

SEARch:TRIGger:DATatoclock:CSOurce <ClockSource>

Selects the input channel of the clock signal.

Parameters:

<ClockSource>
CH1 | CH2 | CH3 | CH4 | MA1 | MA2 | MA3 | MA4 | MA5 | RE1 | RE2 | RE3 | RE4
*RST: CH1

Firmware/Software: FW 03.800

SEARch:TRIGger:DATatoclock:CLEVel <ClockLevel>

Sets the voltage level for the clock signal. Clock level and clock edge define the reference point for setup and hold time.

Parameters:
<ClockLevel> Range: depends on vertical scale

Firmware/Software: FW 03.800

SEARch:TRIGger:DATatoclock:DLEVel <DataLevel>

Sets the voltage level for the data signal. The data lavel defines the point of data transition.

Parameters:
<DataLevel> Range: depends on vertical scale

Firmware/Software: FW 03.800

SEARch:TRIGger:DATatoclock:CLEVel:DELTa <LevelDelta>
SEARch:TRIGger:DATatoclock:DLEVel:DELTa <LevelDelta>

Set a hysteresis range to the clock and data levels in order to avoid unwanted search results caused by noise oscillation around the level. For a rising edge, the hysteresis is below the search level. Otherwise, for a falling edge the hysteresis is above the level.

Parameters:
<LevelDelta> Range: Lower limit depends on vertical scale and other settings, no upper limit

Firmware/Software: FW 03.800

SEARch:TRIGger:DATatoclock:CEDGe <ClockEdge>

Sets the edge of the clock signal to define the time reference point for the setup and hold time.

Parameters:
<ClockEdge> POSitive | NEGative | EITHer
*RST: POS

Firmware/Software: FW 03.800

SEARch:TRIGger:DATatoclock:HTIMe <HoldTime>

Sets the minimum time **after** the clock edge while the data signal must stay steady above or below the data level. The hold time can be negative. In this case, the hold time ends before the clock edge, and the setup time must be positive and longer than the absolute value of the hold time.

Parameters:
<HoldTime> Range: depends on time base and sample interval

Firmware/Software: FW 03.800

SEARch:TRIGger:DATatoclock:STIMe <SetupTime>

Sets the minimum time **before** the clock edge while the data signal must stay steady above or below the data level. The setup time can be negative. In this case, the setup interval starts after the clock edge, and the hold time must be positive and longer than the absolute value of the setup time.

Parameters:

<SetupTime> Range: depends on time base and sample interval

Firmware/Software: FW 03.800

15.2.12.8 Pattern Search Configuration

SEARch:TRIGger:PATTern:SOURce....370
SEARch:TRIGger:PATTern:FUNCtion....370
SEARch:TRIGger:PATTern:LEVel<n>....371
SEARch:TRIGger:PATTern:LEVel<n>:DELTa....371
SEARch:TRIGger:PATTern:WIDTh:RANGe....371
SEARch:TRIGger:PATTern:WIDTh[:WIDTh]....372
SEARch:TRIGger:PATTern:WIDTh:DELTa....372

SEARch:TRIGger:PATTern:SOURce <Pattern>

Specifies the search pattern - the state for each channel.

Parameters:

<Pattern> String parameter

String containing 0, 1, X|x for each channel. The order of channels is fixed: CH1 CH2 [CH3 CH4].

Example: `SEAR:TRIG:PATT:SOUR '1X10'`
CH1, CH3 are high, CH4 is low. These states are logically combined with `SEARch:TRIGger:PATTern:FUNCtion`. CH2 does not matter (don't care).

SEARch:TRIGger:PATTern:FUNCtion <Function>

Sets the logical combination of the channel states.

Parameters:

<Function> AND | OR | NAND | NOR

AND
The required states of all channels must appear in the input signal at the same time.

OR
At least one of the channels must have the required state.

NAND
"Not and" operator, at least one of the channels does not have the required state.

NOR
"Not or" operator, none of the channels has the required state.

*RST: AND

SEARch:TRIGger:PATTern:LEVel<n> <ThresholdLevel>

Sets the threshold value for each specified source channel. You can set different levels for the channels

Suffix:

<n> 1..4
Selects the input channel. The number of channels depends on the instrument.

Parameters:

<ThresholdLevel> Range: Depends on vertical scale

SEARch:TRIGger:PATTern:LEVel<n>:DELTa <LevelDelta>

Sets a hysteresis range to the level of the specified source channel in order to avoid unwanted search results caused by noise oscillation around the level. For a rising edge, the hysteresis is below the search level. Otherwise, for a falling edge the hysteresis is above the level.

Suffix:

<n> 1..4
Selects the input channel. The number of channels depends on the instrument.

Parameters:

<LevelDelta> Range: Lower limit depends on vertical scale and other settings, no upper limit

---

SEARch:TRIGger:PATTern:WIDTh:RANGe <Range>

Sets the condition how the duration of a steady pattern is compared with the given reference time.

To set the reference value *width*, use `SEARch:TRIGger:PATTern:WIDTh[:WIDTh]` on page 372.

To set a range *Δt*, use SEARch:TRIGger:PATTern:WIDTh:DELTa on page 372

Parameters:

<Range> WITHin | OUTSide | LONGer | SHORter

WITHin
Finds patterns steady for a time range *width* ± *Δt*.

OUTSide
Finds patterns outside a time range *width* ± *Δt*.

LONGer
Finds patterns steady for at least the given *width*.

SHORter
Finds patterns shorter than the given *width*.

*RST: LONG

SEARch:TRIGger:PATTern:WIDTh[:WIDTh] <Width>

Sets the reference time of a steady pattern, the nominal value for comparisons.

Parameters:

<Width> Default unit: s

SEARch:TRIGger:PATTern:WIDTh:DELTa <DeltaTime>

Sets a range Δt to the reference pattern duration set with SEARch:TRIGger:PATTern:WIDTh[:WIDTh] if SEARch:TRIGger:PATTern:WIDTh:RANGe is set to WITHin or OUTSide.

Parameters:

<DeltaTime> Default unit: s

15.2.12.9 Search Results

SEARch:RESDiagram:SHOW....372
SEARch:RESult:ALL?....373
SEARch:RESult<n>?....373
SEARch:RCOunt?....374

SEARch:RESDiagram:SHOW <ResultShow>

Shows or hides the table of search results.

Parameters:

<ResultShow> ON | OFF

*RST: OFF

Example: chapter 15.3.2.1, "Searching for a Pulse of Specified Width", on page 460

Firmware/Software: FW 03.400

SEARch:RESult:ALL?

Returns all result values of the search.

Return values:

<AllResults> List of results items seperated by comma

For each result, six values are returned:
1. Result number as indicated in the search results table
2. X-position (time) of the search result
3. Y-position of the search result, currently not relevant
4. Type of the search result (Edge, Peak, ...)
5. Slope or polarity of the search result
6. For peak searches, the value contains the peak voltage. For width searches, it contains the pulse width. For edge searches, the value is not relevant.

Example: `SEARch:RESult:ALL?`
Returns all four results of a peak search:
```
1,-4.7750e-04,0,PEAK,NEGATIVE,-1.530e-02,2,
-4.4630e-04,0,PEAK,NEGATIVE,-1.530e-02,3,
-4.1660e-04,0,PEAK,NEGATIVE,-1.530e-02,4,
-3.8690e-04,0,PEAK,NEGATIVE,-1.530e-02
```

Example: chapter 15.3.2.1, "Searching for a Pulse of Specified Width", on page 460

Usage: Query only

Firmware/Software: FW 03.400

SEARch:RESult<n>?

Returns the result values of the specified search result.

See also: `SEARch:RESult:ALL?`

Suffix:

<n> *
Number of the search result

Return values:

<Result> Comma-separated value list

Meaning of the values:
Result number, time value, y-position (not relevant), search type, slope or polarity, optional value: voltage for peak search, pulse width for width search.

Example: `SEARch:RESult3?`
Returns the result values of the third search result.
```
3,-4.1660e-04,0,PEAK,NEGATIVE,-1.530e-02
```

Usage: Query only

Firmware/Software: FW 03.400

SEARch:RCOunt?

Returns the number of search results.

Return values:
<ResultCount> *RST: 0

Example: chapter 15.3.2.1, "Searching for a Pulse of Specified Width", on page 460

Usage: Query only

Firmware/Software: FW 03.400

15.2.13 Protocol Analysis

- General....374
- SPI....377
- SSPI....386
- I²C....388
- UART....399
- CAN....405
- LIN....421

15.2.13.1 General

Note: SPI/SSPI and UART protocols occupy two bus lines (bus 1 and 2 or bus 3 and 4). If one of these buses is configured, the number of buses (suffix <b>) is reduced. Bus 2 and/or bus 4 is not available.

BUS<b>:STATe....374
BUS<b>:TYPE....375
BUS<b>:FORMat....375
BUS<b>:DSIGnals....375
BUS<b>:DSIZe....375
BUS<b>:POSition....376
BUS<b>:RESult....376
BUS<b>:LIST?....376
BUS<b>:LIST:SAVE....376

BUS<b>:STATe <State>

Switches the protocol display on or off.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:
<State> ON | OFF
*RST: OFF

BUS<b>:TYPE <Type>

Defines the bus or interface type for analysis. For most types, a special option to the instrument is required.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:
<Type> PARallel | CPARallel | I2C | SPI | SSPI | UART | CAN | LIN
*RST: PARallel

BUS<b>:FORMat <Format>

Sets the decoding format for the display on the screen.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:
<Format> ASCii | HEXadecimal | BINary | DECimal
*RST: HEX

BUS<b>:DSIGnals <BitsSignals>

Displays the individual bit lines above the decoded bus line.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:
<BitsSignals> ON | OFF
*RST: ON

BUS<b>:DSIZe <DisplaySize>

Sets the height of the decoded bus signal on the sreen.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:
<DisplaySize> SMALl | MEDium | LARGe
*RST: MEDium

BUS<b>:POSition <Position>

Sets the vertical position of the decoded bus signal in divisions on the sreen.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:
<Position> Range: 4 to -4
Increment: 0.02
*RST: -3.5
Default unit: div

BUS<b>:RESult

Displays or hides the table of decode results.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:
<ShowResultTable> ON | OFF

BUS<b>:LIST?

Returns the contents of the frame table in block data format.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Return values:
<DataTable> Block data

Usage: Query only

BUS<b>:LIST:SAVE <FilePath>

Saves the decoded data (frame table) to the specified CSV file (comma-separated list).

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Setting parameters:
<FilePath> String containing the storage device, path, and file name

Example: `BUS:LIST:SAVE "/USB_FRONT/MYTABLE.CSV"`
Saves the frame table data to the MYTABLE.CSV file on a USB flash device connected to the front panel.

Usage: Setting only

15.2.13.2 SPI

The Serial Peripheral Interface SPI is used for communication with slow peripheral devices, in particular, for transmission of data streams. A 4-channel instrument is required for full support of the SPI protocol.

The SPI/SSPI protocol require two bus lines (bus 1 and 2 or bus 3 and 4), so the number of buses (suffix <b>) is reduced. Bus 2 and/or bus 4 is not available.

- SPI - Configuration....377
- SPI - Trigger....380
- SPI - Decode Results....381

SPI - Configuration

BUS<b>:SPI:CS:SOURce....377
BUS<b>:SPI:CS:POLarity....377
BUS<b>:SPI:CLOCk:SOURce....378
BUS<b>:SPI:CLOCk:POLarity....378
BUS<b>:SPI:DATA:SOURce....378
BUS<b>:SPI:DATA:POLarity....379
BUS<b>:SPI:BORDer....379
BUS<b>:SPI:SSIZe....379
CHANnel<m>:THReshold:FINDlevel....379

BUS<b>:SPI:CS:SOURce <Source>

Selects the input channel of the chip select line.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:
<Source> CH1 | CH2 | CH3 | CH4 | D0..D15
*RST: CH1

BUS<b>:SPI:CS:POLarity <Polarity>

Selects whether the chip select signal is high active (high = 1) or low active (low = 1).

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Polarity> POSitive | NEGative

POSitive = high active
NEGative = low active

*RST: POSitive

BUS<b>:SPI:CLOCk:SOURce <Source>

Selects the input channel of the clock line.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Source> CH1 | CH2 | CH3 | CH4 | D0..D15

*RST: CH1

BUS<b>:SPI:CLOCk:POLarity <Polarity>

Selects if data is stored with the rising or falling slope of the clock. The slope marks the begin of a new bit.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Polarity> POSitive | NEGative

POSitive: rising slope
NEGative: falling slope

*RST: NEGative

BUS<b>:SPI:DATA:SOURce <Source>

Selects the input channel of the data line.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Source> CH1 | CH2 | CH3 | CH4 | D0..D15

*RST: CH1

BUS<b>:SPI:DATA:POLarity <Polarity>

Selects whether transmitted data is high active (high = 1) or low active (low = 1) on the data line.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Polarity> POSitive | NEGative

POSitive = high active
NEGative = low active

*RST: POSitive

BUS<b>:SPI:BORDer <BitOrder>

Defines if the data of the messages starts with MSB (most significant bit) or LSB (least significant bit).

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<BitOrder> MSBFirst | LSBFirst

*RST: MSBFirst

BUS<b>:SPI:SSIZe <SymbolSize>

Sets the word length, the number of bits in a message.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<SymbolSize> Range: 4 to 32
Increment: 1
*RST: 8
Default unit: Bit

CHANnel<m>:THReshold:FINDlevel

Executes the analysis of all analog channels that are configured for the selected bus and sets the threshold for digitization of analog signals for each channel.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Usage: Event

SPI - Trigger

TRIGger:A:SPI:MODE....380
TRIGger:A:SPI:PATTern....380
TRIGger:A:SPI:PLENgth....381
TRIGger:A:SPI:POFFset....381

TRIGger:A:SPI:MODE <Mode>

Specifies the trigger mode for SPI/SSPI protocols.

Parameters:
<Mode> BSTart | BEND | NTHBit | PATTern

BSTart
Burst start, sets the trigger event to the start of the frame. The frame starts when the chip select signal CS changes to the active state.

BEND
Burst end, sets the trigger event to the end of the message.

NTHBit
Sets the trigger event to the specified bit number. To define the bit number, use `TRIGger:A:SPI:POFFset`.

PATTern
Sets the trigger event to a serial pattern. To define the pattern, use `TRIGger:A:SPI:PATTern`.
For a complete configuration of the pattern mode, you also have to set `TRIGger:A:SPI:PLENgth` and `TRIGger:A:SPI:POFFset`.

*RST: BSTart

TRIGger:A:SPI:PATTern <DataPattern>

Defines the bit pattern as trigger condition. The pattern length is adjusted to the number of bits defined in the pattern.

Parameters:
<DataPattern> String with max. 32 characters (4 byte + 8 bit) . Characters 0, 1, and X are allowed.

Example: `TRIG:A:SPI:PATT "0011XXXX0110"`
Sets a 12bit pattern.

TRIGger:A:SPI:PLENgth <PatternLength>

Returns the number of bits in the previously defined bit pattern (`TRIGger:A:SPI:PATTern`). The command can also be used to shorten a previously defined bit pattern.

Parameters:

<PatternLength> Range: 1 to 32
Increment: 1
*RST: 4

Example:

```
TRIG:A:SPI:PATT "0011XXXX0110"
TRIG:A:SPI:PLEN?
12
TRIG:A:SPI:PLEN 4
TRIG:A:SPI:PATT?
"0011"
```

TRIGger:A:SPI:POFFset <PatternBitOffset>

Sets the number of bits before the first bit of the pattern.

Parameters:

<PatternBitOffset> Number of ignored bits
Range: 0 to 4095
Increment: 1
*RST: 0

SPI - Decode Results

BUS<b>:SPI:FCOunt?....381
BUS<b>:SPI:FRAME<n>:STATus?....382
BUS<b>:SPI:FRAME<n>:STARt?....382
BUS<b>:SPI:FRAME<n>:STOP?....382
BUS<b>:SPI:FRAME<n>:DATA:MOSI?....383
BUS<b>:SPI:FRAME<n>:DATA:MISO?....383
BUS<b>:SPI:FRAME<n>:WCOunt?....383
BUS<b>:SPI:FRAME<n>:WORD<o>:STARt?....384
BUS<b>:SPI:FRAME<n>:WORD<o>:STOP?....384
BUS<b>:SPI:FRAME<n>:WORD<o>:MOSI?....385
BUS<b>:SPI:FRAME<n>:WORD<o>:MISO?....385

BUS<b>:SPI:FCOunt?

Returns the number of decoded frames.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Return values:

<FrameCount> Total number of decoded frames.

Usage: Query only

BUS<b>:SPI:FRAME<n>:STATus?

Returns the overall state of the specified frame.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

Return values:
<Status> OK | INCFirst | INCLast | INSufficient

INCFirst
First frame is incomplete

INCLast
Last frame is incomplete

Usage: Query only

BUS<b>:SPI:FRAME<n>:STARt?

Returns the start time of the specified frame.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

Return values:
<StartTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:SPI:FRAME<n>:STOP?

Returns the end time of the specified frame.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

Return values:
<StopTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:SPI:FRAME<n>:DATA:MOSI?

Returns the data words of the specified frame of the MOSI line.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

Return values:
<DataMosi> List of decimal values of data bytes

Example:
```
BUS:SPI:FRAM3:DATA:MOSI?
-> 94,177,171,60,242,219,100,0
```

Usage: Query only

BUS<b>:SPI:FRAME<n>:DATA:MISO?

Returns the data words of the specified frame of the MISO line.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

Return values:
<DataMiso> List of decimal values of data bytes

Example:
```
BUS:SPI:FRAM3:DATA:MISO?
-> 94,177,171,60,242,219,100,0
```

Usage: Query only

BUS<b>:SPI:FRAME<n>:WCOunt?

Returns the number of words in the specified frame.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

Return values:

<WordCount> Number of words

Usage: Query only

BUS<b>:SPI:FRAME<n>:WORD<o>:STARt?

Returns the start time of the specified data word.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

<o> *
Selects the word number.

Return values:

<StartTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:SPI:FRAME<n>:WORD<o>:STOP?

Returns the end time of the specified data word.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

<o> *
Selects the word number.

Return values:

<StopTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:SPI:FRAME<n>:WORD<o>:MOSI?

Returns the data value of the specified word on the MOSI line.

Use this command if only one line is defined.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame (1...n)

<o> *
Selects the word number (1...m)

Return values:

<Data> Decimal value of the data word

Usage: Query only

BUS<b>:SPI:FRAME<n>:WORD<o>:MISO?

Returns the data value of the specified word on the optional MISO line.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame (1...n)

<o> *
Selects the word number (1...m)

Return values:

<Data> Decimal value of the data word

Usage: Query only

15.2.13.3 SSPI

BUS<b>:SSPI:CLOCk:SOURce....386
BUS<b>:SSPI:CLOCk:POLarity....386
BUS<b>:SSPI:DATA:SOURce....386
BUS<b>:SSPI:DATA:POLarity....387
BUS<b>:SSPI:BITime....387
BUS<b>:SSPI:BORDer....387
BUS<b>:SSPI:SSIZe....388
CHANnel<m>:THReshold:FINDlevel....388

BUS<b>:SSPI:CLOCk:SOURce <Source>

Selects the input channel of the clock line.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Source> CH1 | CH2 | CH3 | CH4 | D0..D15

CH3 and CH4 are only available with 4-channel R&S RTM oscilloscopes.

*RST: CH1

BUS<b>:SSPI:CLOCk:POLarity <Polarity>

Selects if data is stored with the rising or falling slope of the clock. The slope marks the begin of a new bit.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Polarity> POSitive | NEGative

POSitive: rising slope
NEGative: falling slope

*RST: POSitive

BUS<b>:SSPI:DATA:SOURce <Source>

Selects the input channel of the data line.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Source> CH1 | CH2 | CH3 | CH4 | D0..D15

CH3 and CH4 are only available with 4-channel R&S RTM oscilloscopes.

*RST: CH1

BUS<b>:SSPI:DATA:POLarity <Polarity>

Selects whether transmitted data is high active (high = 1) or low active (low = 1) on the data line.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Polarity> POSitive | NEGative

POSitive = high active
NEGative = low active

*RST: POSitive

BUS<b>:SSPI:BITime <BurstIdleTime>

Within the idle time the data and clock lines are low. A new frame begins when the idle time has expired and the clock line has been inactive during that time. If the time interval between the data words is shorter than the idle time, the words are part of the same frame.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<BurstIdleTime> Range: 1,60E-008 to 8,39E-001
Increment: 1,60E-008
*RST: 1,00E-004
Default unit: s

BUS<b>:SSPI:BORDer <BitOrder>

Defines if the data of the messages starts with MSB (most significant bit) or LSB (least significant bit).

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:
<BitOrder> MSBFirst | LSBFirst
*RST: MSBFirst

BUS<b>:SSPI:SSIZe <SymbolSize>

Sets the word length, the number of bits in a message.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:
<SymbolSize> Range: 4 to 32
Increment: 1
*RST: 8
Default unit: Bit

CHANnel<m>:THReshold:FINDlevel

Executes the analysis of all analog channels that are configured for the selected bus and sets the threshold for digitization of analog signals for each channel.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Usage: Event

15.2.13.4 I²C

The Inter-Integrated Circuit is a simple, lowbandwidth, low-speed protocol used for communication between on-board devices, for example, in LCD and LED drivers, RAM, EEPROM, and others.

Note: SPI/SSPI and UART protocols occupy two bus lines (bus 1 and 2 or bus 3 and 4). If one of these buses is configured, the number of buses (suffix <b>) is reduced. Bus 2 and/or bus 4 is not available.

- I²C - Configuration....388
- I²C - Trigger....389
- I²C - Decode Results....392

I²C - Configuration

BUS<b>:I2C:CLOCk:SOURce....389
BUS<b>:I2C:DATA:SOURce....389
CHANnel<m>:THReshold:FINDlevel....389

BUS<b>:I2C:CLOCk:SOURce <Source>

Sets the input channel to which the clock line is connected.

Suffix:
<b> 1..4
Selects the bus.

Parameters:
<Source> CH1 | CH2 | CH3 | CH4 | D0..D15
CH3 and CH4 are only available with 4-channel R&S RTM oscilloscopes.
*RST: CH1

BUS<b>:I2C:DATA:SOURce <Source>

Sets the input channel to which the data line is connected.

Suffix:
<b> 1..4
Selects the bus.

Parameters:
<Source> CH1 | CH2 | CH3 | CH4 | D0..D15
CH3 and CH4 are only available with 4-channel R&S RTM oscilloscopes.
*RST: CH1

CHANnel<m>:THReshold:FINDlevel

Executes the analysis of all analog channels that are configured for the selected bus and sets the threshold for digitization of analog signals for each channel.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Usage: Event

I²C - Trigger

TRIGger:A:I2C:MODE....390
TRIGger:A:I2C:ACCess....390
TRIGger:A:I2C:AMODe....390
TRIGger:A:I2C:ADDRess....391
TRIGger:A:I2C:PATTern....391
TRIGger:A:I2C:PLENgth....391
TRIGger:A:I2C:POFFset....392

TRIGger:A:I2C:MODE <Mode>

Specifies the trigger mode for I²C.

Parameters:

<Mode> STARt | RESTart | STOP | MACKnowledge | PATTern

STARt
Start of the message. The start condition is a falling slope on SDA while SCL is high.

RESTart
Restarted message. The restart is a repeated start condition.

STOP
End of the message. The stop condition is a rising slope on SDA while SCL is high.

MACKnowledge
Missing acknowledge. If the transfer failed, at the moment of the acknowledge bit the SCL and the SDA lines are both on high level.

PATTern
Triggers on a set of trigger conditions: read or write access of the master, to an address, or/and to a bit pattern in the message.
For a complete configuration of the pattern mode, you have to set:
`TRIGger:A:I2C:ACCess` (read/write access), and
`TRIGger:A:I2C:AMODe` and `TRIGger:A:I2C:ADDRess` (address), and/or
`TRIGger:A:I2C:POFFset` and `TRIGger:A:I2C:PLENgth` and `TRIGger:A:I2C:PATTern` (pattern)

*RST: STARt

TRIGger:A:I2C:ACCess <Access>

Toggles the trigger condition between Read and Write access of the master.

Parameters:

<Access> READ | WRITe

*RST: READ

TRIGger:A:I2C:AMODe <AdrMode>

Sets the lenght of the slave address.

Parameters:

<AdrMode> NORMal | EXTended

NORMal: 7 bit address
EXTended: 10 bit address

*RST: NORMal

TRIGger:A:I2C:ADDRess <AddressString>

Sets the address of the slave device. The address can have 7 bits or 10 bits.

Parameters:

<AddressString> String with max. 7 or 10 characters, depending on the address length. Characters 0, 1, and X are allowed, but X cannot be assigned to a specified bit. If at least one X occurs in the address, the complete address is set to X.

Example:
```
TRIG:A:I2C:AMOD NORM
TRIG:A:I2C:ADDR "1011"
TRIG:A:I2C:ADDR?
```
Return value (7bit address): `"0001011"`

Example:
```
TRIG:A:I2C:AMOD EXT
TRIG:A:I2C:ADDR "10X1"
TRIG:A:I2C:ADDR?
```
Return value (10bit address): `"XXXXXXXXXX"`

TRIGger:A:I2C:PATTern <DataPattern>

Defines the bit pattern as trigger condition. Make sure that the correct pattern length has been defined before with `TRIGger:A:I2C:PLENgth`.

Parameters:

<DataPattern> String with max. 24 characters (3 byte + 8 bit) . Characters 0, 1, and X are allowed. X can be assigned to a specified bit. If you define a pattern shorter than the pattern length, the missing LSB are filled with X. If you define a pattern longer than the pattern length, the pattern string is not valid

Example:
```
TRIG:A:I2C:PLEN 2
TRIG:A:I2C:PATT "10X10000XXXX1111"
TRIG:A:I2C:PATT?
```
Return value (2 bytes): `"10X10000XXXX1111"`

Example:
```
TRIG:A:I2C:PLEN 1
TRIG:A:I2C:PATT "110"
TRIG:A:I2C:PATT?
```
Return value (1 byte): `"110XXXXX"`

TRIGger:A:I2C:PLENgth <PatternLength>

Defines how many bytes are considered in the trigger condition. To set the pattern for these bytes, use `TRIGger:A:I2C:PATTern`.

Parameters:

<PatternLength> Number of bytes

Range: 1 to 3
Increment: 1
*RST: 1

TRIGger:A:I2C:POFFset <PatternByteOffset>

Sets the number of bytes before the first byte of interest, relating to the end of the address bytes.

Parameters:

<PatternByteOffset> Number of ignored bytes

Range: 0 to 4095
Increment: 1
*RST: 0

I²C - Decode Results

BUS<b>:I2C:FCOunt?....392
BUS<b>:I2C:FRAMe<n>:DATA?....392
BUS<b>:I2C:FRAMe<n>:STATus?....393
BUS<b>:I2C:FRAMe<n>:STARt?....393
BUS<b>:I2C:FRAMe<n>:STOP?....394
BUS<b>:I2C:FRAMe<n>:AACCess?....394
BUS<b>:I2C:FRAMe<n>:ACCess?....394
BUS<b>:I2C:FRAMe<n>:ACOMplete?....395
BUS<b>:I2C:FRAMe<n>:ADBStart?....395
BUS<b>:I2C:FRAMe<n>:ADDRess?....395
BUS<b>:I2C:FRAMe<n>:ADEVice?....396
BUS<b>:I2C:FRAMe<n>:AMODe?....396
BUS<b>:I2C:FRAMe<n>:ASTart?....396
BUS<b>:I2C:FRAMe<n>:BCOunt?....397
BUS<b>:I2C:FRAMe<n>:BYTE<o>:ACCess?....397
BUS<b>:I2C:FRAMe<n>:BYTE<o>:ACKStart?....397
BUS<b>:I2C:FRAMe<n>:BYTE<o>:COMPlete?....398
BUS<b>:I2C:FRAMe<n>:BYTE<o>:STARt?....398
BUS<b>:I2C:FRAMe<n>:BYTE<o>:VALue?....398

BUS<b>:I2C:FCOunt?

Returns the number of received frames.

Suffix:

<b> 1..4
Selects the bus.

Return values:

<FrameCount> Total number of decoded frames.

Usage: Query only

BUS<b>:I2C:FRAMe<n>:DATA?

Returns the data words of the specified frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:
<DataWordsInFrame> Comma-separated list of decimal values of the data bytes.

Example: `BUS:I2C:FRAM2:DATA?`
returns four data bytes:
`-> 69,158,174,161`

Usage: Query only

BUS<b>:I2C:FRAMe<n>:STATus?

Returns the overall state of the frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:
<State> INComplete | OK | UNEXpstop | INSufficient | ADDifferent

INComplete
The frame is not completely contained in the acquisition.

Usage: Query only

BUS<b>:I2C:FRAMe<n>:STARt?

Returns the start time of the specified frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:
<StartTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:I2C:FRAMe<n>:STOP?

Returns the end time of the specified frame.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:

<EndTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:I2C:FRAMe<n>:AACCess?

Returns the address acknowledge bit value for the indicated frame.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:

<Acknowledge> INComplete | ACK | NACK | EITHer

Usage: Query only

BUS<b>:I2C:FRAMe<n>:ACCess?

Returns the transfer direction - read or write access from master to slave.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:

<Access> INComplete | READ | WRITE | EITHer | UNDF

INComplete
The frame is not completely contained in the acquisition.

UNDF
Access is not defined.

Usage: Query only

BUS<b>:I2C:FRAMe<n>:ACOMplete?

Returns the state of the address.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:
<AddressComplete> ON | OFF

ON
Address was received completely.

Usage: Query only

BUS<b>:I2C:FRAMe<n>:ADBStart?

Returns the start time of the address acknowledge bit.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:
<AckStartTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:I2C:FRAMe<n>:ADDRess?

Returns the decimal address value of the indicated frame **including** the R/W bit.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:
<AddressValue> Decimal value

Range: 0 to 2047
Increment: 1

Usage: Query only

BUS<b>:I2C:FRAMe<n>:ADEVice?

Returns the decimal address value of the indicated frame **without** R/W bit.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:
<SlaveAddress> Decimal value
Range: 0 to 1023
Increment: 1

Usage: Query only

BUS<b>:I2C:FRAMe<n>:AMODe?

Returns the address length.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:
<AddressMode> BIT7 | BIT10

Usage: Query only

BUS<b>:I2C:FRAMe<n>:ASTart?

Returns the start time of the address for the indicated frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:
<StartTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:I2C:FRAMe<n>:BCOunt?

Returns the number of data bytes in the specified frame.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame.

Return values:

<ByteCount im Frame> Number of words (bytes)

Example:
```
BUS:I2C:FRAM2:BCO?
-> 4
```

Usage: Query only

BUS<b>:I2C:FRAMe<n>:BYTE<o>:ACCess?

Returns the acknowledge bit value of the specified data byte.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame.

<o> *
Selects the byte number.

Return values:

<Acknowledge> INComplete | ACK | NACK | EITHer

Usage: Query only

BUS<b>:I2C:FRAMe<n>:BYTE<o>:ACKStart?

Returns the start time of the acknowledge bit of the specified byte.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame.

<o> *
Selects the byte number.

Return values:

<AckStartTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:I2C:FRAMe<n>:BYTE<o>:COMPlete?

Returns the state of the byte.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame.

<o> *
Selects the byte number.

Return values:

<ByteComplete> ON | OFF

ON
Data byte was received completely.

Usage: Query only

BUS<b>:I2C:FRAMe<n>:BYTE<o>:STARt?

Returns the start time of the specified data byte.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame.

<o> *
Selects the byte number.

Return values:

<StartTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:I2C:FRAMe<n>:BYTE<o>:VALue?

Returns the decimal value of the specified byte.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame.

<o> *
Selects the byte number.

Return values:

<ByteValue> Decimal value

Range: 0 to 255
Increment: 1

Example:
```
BUS:I2C:FRAM2:BYTE2:VAL?
-> 158
```

Usage: Query only

15.2.13.5 UART

The Universal Asynchronous Receiver/Transmitter (UART) converts a word of data into serial data, and vice versa.

The UART protocol requires two bus lines (bus 1 and 2 or bus 3 and 4), so the number of buses (suffix <b>) is reduced. Bus 2 and/or bus 4 is not available.

- UART - Configuration....399
- UART - Trigger....402
- UART - Decode Results....404

UART - Configuration

BUS<b>:UART:DATA:SOURce....399
BUS<b>:UART:POLarity....400
BUS<b>:UART:DATA:POLarity....400
BUS<b>:UART:SSIZe....400
BUS<b>:UART:PARity....401
BUS<b>:UART:SBIT....401
BUS<b>:UART:BAUDrate....401
BUS<b>:UART:BITime....402
CHANnel<m>:THReshold:FINDlevel....402

BUS<b>:UART:DATA:SOURce <Source>

Selects the input channel of the data line.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Source> CH1 | CH2 | CH3 | CH4 | D0..D15

CH3 and CH4 are only available with 4-channel R&S RTM oscilloscopes.

*RST: CH1

BUS<b>:UART:POLarity <IdleState>

Defines the logic levels of the bus. The idle state corresponds to a logic 1, and the start bit to a logic 0.

Alternative command for `BUS<b>:UART:DATA:POLarity`

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<IdleState> IDLLow | IDLHigh

IDLLow: idle low, low = 1
IDLHigh: idle high, high = 1

*RST: IDLH

BUS<b>:UART:DATA:POLarity <Polarity>

Defines if the transmitted data on the bus is high (high = 1) or low (low = 1) active.

Alternative command for `BUS<b>:UART:POLarity` .

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Polarity> POSitive | NEGative

POSitive = high active
NEGative = low active

*RST: POS

BUS<b>:UART:SSIZe <SymbolSize>

Sets the number of data bits in a message.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<SymbolSize>
Range: 5 to 9
Increment: 1
*RST: 8
Default unit: Bit

BUS<b>:UART:PARity <Parity>

Defines the optional parity bit that is used for error detection.

Suffix:

<b>
1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Parity>
ODD | EVEN | NONE
See: "Parity" on page 178
*RST: NONE

BUS<b>:UART:SBIT <StopBitNumber>

Sets the stop bits.

Suffix:

<b>
1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<StopBitNumber>
B1 | B1_5 | B2
1; 1.5 or 2 stop bits are possible.
*RST: B1

BUS<b>:UART:BAUDrate <Baudrate>

Sets the number of transmitted bits per second.

Suffix:

<b>
1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Baudrate>
Range: 100 to 78.1E6
Increment: 100
*RST: 115200
Default unit: Bit

BUS<b>:UART:BITime <BurstIdleTime>

Sets the minimal time between two data frames (packets), that is, between the last stop bit and the start bit of the next frame.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<BurstIdleTime> Range: Range depends on the bus configuration, mainly on bit rate and symbol size.
Default unit: s

CHANnel<m>:THReshold:FINDlevel

Executes the analysis of all analog channels that are configured for the selected bus and sets the threshold for digitization of analog signals for each channel.

Suffix:

<m> Selects the input channel. The number of channels depends on the instrument.

Usage: Event

UART - Trigger

TRIGger:A:SOURce:UART....402
TRIGger:A:UART:MODE....402
TRIGger:A:UART:PATTern....403
TRIGger:A:UART:PLENgth....403
TRIGger:A:UART:POFFset....404

TRIGger:A:SOURce:UART <UartSource>

Selects one of the Rx and Tx lines as trigger source.

Parameters:

<UartSource> RX | TX
*RST: RX

TRIGger:A:UART:MODE <Mode>

Specifies the trigger mode for UART/RS-232 interfaces.

Parameters:

<Mode> BSTart | SBIT | NTHSymbol | SYMBol | PATTern | PRERror | FERRor | BREak

BSTart
Burst start. Sets the trigger to the begin of a data frame. The frame start is the first start bit after the idle time.

SBIT
Start bit. The start bit is the first low bit after a stop bit.

NTHSymbol
Sets the trigger to the n-th symbol of a burst.

SYMBol
Triggers if a pattern occurs in a symbol at any position in a burst.

PATTern
Triggers on a serial pattern at a defined position in the burst.
To define the pattern, use `TRIGger:A:UART:PLENgth` and `TRIGger:A:UART:PATTern`.
To define the position, use `TRIGger:A:UART:POFFset` on page 404.

PRERror
Parity Error: Triggers if a bit error occured in transmission.

FERRor
Triggers on frame error.

BREak
Triggers if a start bit is not followed by a stop bit within a defined time. During the break the stop bits are at low state.

*RST: SBIT

TRIGger:A:UART:PATTern <DataPattern>

Defines the bit pattern as trigger condition.

Parameters:

<DataPattern> Binary pattern with max. 32 bit. Characters 0, 1, and X are allowed.

*RST: 1 = "00000001"

TRIGger:A:UART:PLENgth <PatternLength>

Defines how many symbols build up the serial pattern.

Parameters:

<PatternLength> Number of symbols

Range: 1 to 3
Increment: 1
*RST: 1

TRIGger:A:UART:POFFset <PatternByteOffset>

Sets the number of symbols before the first symbol of the pattern.

Parameters:

<PatternByteOffset> Number of ignored symbols

Range: 0 to 4095
Increment: 1
*RST: 0

UART - Decode Results

BUS<b>:UART:RX:FCOunt?....404
BUS<b>:UART:RX:FRAMe<n>:WCOunt?....404
BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STATe?....404
BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STARt?....405
BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STOP?....405
BUS<b>:UART:RX:FRAMe<n>:WORD<o>:VALue?....405

BUS<b>:UART:RX:FCOunt?

Suffix:

<b> 1..4

Return values:

<FrameCount>

Usage: Query only

BUS<b>:UART:RX:FRAMe<n>:WCOunt?

Suffix:

<b> 1..4

<n> *

<o> *

Return values:

<WordCount>

Usage: Query only

BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STATe?

Suffix:

<b> 1..4

<n> *

<o> *

Return values:

<Status> OK | FRSTart | FRENd | FRMError | STERror | SPERror | PRERror | INSufficient | BREak

Usage: Query only

BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STARt?
Suffix:
<b> 1..4
<n> *
<o> *

Return values:
<StartTime>

Usage: Query only

BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STOP?
Suffix:
<b> 1..4
<n> *
<o> *

Return values:
<StopTime>

Usage: Query only

BUS<b>:UART:RX:FRAMe<n>:WORD<o>:VALue?
Suffix:
<b> 1..4
<n> *
<o> *

Return values:
<Value> Range: 0 to 511
Increment: 1

Usage: Query only

15.2.13.6 CAN

CAN is the Controller Area Network, a bus system used within automotive network architecture.

Note: SPI/SSPI and UART protocols occupy two bus lines (bus 1 and 2 or bus 3 and 4). If one of these buses is configured, the number of buses (suffix <b>) is reduced. Bus 2 and/or bus 4 is not available.

- CAN - Configuration....406
- CAN - Trigger....407
- CAN - Decode Results....411
- CAN - Search....417

CAN - Configuration

BUS<b>:CAN:DATA:SOURce....406
BUS<b>:CAN:TYPE....406
BUS<b>:CAN:SAMPlepoint....406
BUS<b>:CAN:BITRate....407
CHANnel<m>:THReshold:FINDlevel....407

BUS<b>:CAN:DATA:SOURce <Source>

Sets the source of the data line. All channel waveforms can be used.

Suffix:
<b> 1..4
Selects the bus.

Parameters:
<Source> CH1 | CH2 | CH3 | CH4 | D0..D15
*RST: CH1

BUS<b>:CAN:TYPE <SignalType>

Selects the CAN-High or CAN-Low line. CAN uses both lines for differential signal transmission.

If you measure with a differential probe, connect the probe to both CAN-H and CAN-L lines, and set the type CANH.

If you use a single-ended probe, connect the probe to either CAN_L or CAN_H, and select the data type accordingly.

Suffix:
<b> 1..4
Selects the bus.

Parameters:
<SignalType> CANH | CANL
*RST: CANH

BUS<b>:CAN:SAMPlepoint <SamplePoint>

Sets the position of the sample point within the bit in percent of the nominal bit time.

See also: "Sample point" on page 186

Suffix:
<b> 1..4
Selects the bus.

Parameters:

<SamplePoint>	Range:	10 to 90
	Increment:	1
	*RST:	50
	Default unit:	%

BUS<b>:CAN:BITRate <BitRate>

Sets the number of transmitted bits per second.

Suffix:

<b>	1..4 Selects the bus.

Parameters:

<BitRate>	Range:	100 to 5,04E06, depends on instrument type, ADC clock rate
	Increment:	depends on the bit rate value
	*RST:	5,00E+004
	Default unit:	Bit/s

CHANnel<m>:THReshold:FINDlevel

Executes the analysis of all analog channels that are configured for the selected bus and sets the threshold for digitization of analog signals for each channel.

Suffix:

<m>	Selects the input channel. The number of channels depends on the instrument.

Usage: Event

CAN - Trigger

TRIGger:A:CAN:TYPE <TriggerType>

Specifies the trigger mode for CAN.

Parameters:

<TriggerType> STOFrame | EOFrame | ID | IDDT | FTYPe | ERRCondition

STOFrame
Start of frame

EOFrame
End of frame

ID
Sets the trigger to a specific message identifier or an identifier range.
Specify the identifier with `TRIGger:A:CAN:ITYPe`, `TRIGger:A:CAN:ICONdition`, and `TRIGger:A:CAN:IDENtifier`.

IDDT
Sets the trigger to a combination of identifier and data condition. The instrument triggers at the end of the last byte of the specified data pattern.
Specify the identifier (see ID), and the data with `TRIGger:A:CAN:DLC`, `TRIGger:A:CAN:DCONdition`, and `TRIGger:A:CAN:DATA`.

FTYPe
Triggers on a specified frame type. Specify the frame type with `TRIGger:A:CAN:FTYPe`.

ERRCondition
Identifies various errors in the frame. Specify the errors with `TRIGger:A:CAN:ACKerror`, `TRIGger:A:CAN:BITSterror`, `TRIGger:A:CAN:CRCerror`, and `TRIGger:A:CAN:FORMerror`.

*RST: STOF

TRIGger:A:CAN:FTYPe <FrameType>

Specifies the frame type to be triggered on if `TRIGger:A:CAN:TYPE` is set to `FTYPe`.

Parameters:

<FrameType> DATA | REMote | ERRor | OVERload | ANY

*RST: ERR

TRIGger:A:CAN:ITYPe <IdentifierType>

Selects the length of the identifier: 11 bit for CAN base frames, or 29 bits for CAN extended frames.

The command is relevant if `TRIGger:A:CAN:TYPE` is set to `ID` or `IDDT`.

Parameters:

<IdentifierType> B11 | B29 | ANY

ANY: only available for CAN trigger type `IDDT`

*RST: B11

TRIGger:A:CAN:ICONdition <IdentifierCondition>

Sets the comparison condition: If the pattern contains at least one X (don't care), you can trigger on values equal or not equal to the specified value. If the pattern contains only 0 and 1, you can also trigger on a range greater than or lower than the specified value.

The command is relevant if `TRIGger:A:CAN:TYPE` is set to `ID` or `IDDT`.

Parameters:

<IdentifierCondition> EQUual | NEQual | GTHan | LTHan
*RST: EQ

TRIGger:A:CAN:IDENtifier <Identifier>

Defines the identifier pattern. The pattern length is defined with `TRIGger:A:CAN:ITYPe` on page 408.

The command is relevant if `TRIGger:A:CAN:TYPE` is set to `ID` or `IDDT`.

Parameters:

<Identifier> String containing binary pattern with max. 29 bit. Characters 0, 1, and X are allowed.

TRIGger:A:CAN:DLC <DataLength>

Defines the length of the data pattern - the number of bytes in the pattern.

The command is relevant if `TRIGger:A:CAN:TYPE` is set to `IDDT`.

Parameters:

<DataLength> Range: 0 to 8
Increment: 1
*RST: 1
Default unit: Byte

TRIGger:A:CAN:DCONdition <DataCondition>

Sets the comparison condition for data: If the pattern contains at least one X (don't care), you can trigger on values equal or not equal to the specified value. If the pattern contains only 0 and 1, you can also trigger on a range greater than or lower than the specified value.

The command is relevant if `TRIGger:A:CAN:TYPE` is set to `IDDT`.

Parameters:

<DataCondition> EQUal | NEQual | GTHan | LTHan
*RST: EQ

TRIGger:A:CAN:DATA <Data>

Defines the data pattern. The number of bytes in the data pattern is defined with `TRIGger:A:CAN:DLC`.

The command is relevant if `TRIGger:A:CAN:TYPE` is set to `IDDT`.

Parameters:

<Data> String containing binary pattern with max. 64 bit. Characters 0, 1, and X are allowed. Make sure to enter complete bytes.

TRIGger:A:CAN:ACKerror <AcknowledgeError>

Triggers on acknowledgement errors. An acknowledgement error occurs when the transmitter does not receive an acknowledgment - a dominant bit during the Ack Slot.

The command is relevant if `TRIGger:A:CAN:TYPE` is set to `ERRCondition`.

Parameters:

<AcknowledgeError> ON | OFF

*RST: OFF

TRIGger:A:CAN:BITSterror <BitStuffingError>

Triggers on bit stuffing errors.

See also: "Stuff bit" on page 188.

The command is relevant if `TRIGger:A:CAN:TYPE` is set to `ERRCondition`.

Parameters:

<BitStuffingError> ON | OFF

*RST: ON

TRIGger:A:CAN:CRCerror <CRCerror>

Triggers on errors in the Cyclic Redundancy Check.

The command is relevant if `TRIGger:A:CAN:TYPE` is set to `ERRCondition`.

Parameters:

<CRCerror> ON | OFF

*RST: OFF

TRIGger:A:CAN:FORMerror <FormError>

Triggers on form errors. A form error occurs when a fixed-form bit field contains one or more illegal bits.

The command is relevant if `TRIGger:A:CAN:TYPE` is set to `ERRCondition`.

Parameters:
<FormError> ON | OFF
*RST: OFF

CAN - Decode Results

BUS<b>:CAN:FCOunt?....411
BUS<b>:CAN:FRAMe<n>:TYPE?....411
BUS<b>:CAN:FRAMe<n>:STATus?....412
BUS<b>:CAN:FRAMe<n>:STARt?....412
BUS<b>:CAN:FRAMe<n>:STOP?....413
BUS<b>:CAN:FRAMe<n>:DATA?....413
BUS<b>:CAN:FRAMe<n>:ACKState?....413
BUS<b>:CAN:FRAMe<n>:ACKValue?....414
BUS<b>:CAN:FRAMe<n>:CSSTate?....414
BUS<b>:CAN:FRAMe<n>:CSValue?....414
BUS<b>:CAN:FRAMe<n>:DLCState?....414
BUS<b>:CAN:FRAMe<n>:DLCValue?....415
BUS<b>:CAN:FRAMe<n>:IDSTate?....415
BUS<b>:CAN:FRAMe<n>:IDTYpe?....415
BUS<b>:CAN:FRAMe<n>:IDValue?....416
BUS<b>:CAN:FRAMe<n>:BSEPosition?....416
BUS<b>:CAN:FRAMe<n>:BCOunt?....416
BUS<b>:CAN:FRAMe<n>:BYTE<o>:STATe?....417
BUS<b>:CAN:FRAMe<n>:BYTE<o>:VALue?....417

BUS<b>:CAN:FCOunt?

Returns the number of received frames.

Suffix:
<b> 1..4
Selects the bus.

Return values:
<FrameCount> Total number of decoded frames.

Usage: Query only

BUS<b>:CAN:FRAMe<n>:TYPE?

Returns the type of the specified frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:

<FrameType> DATA | REMote | ERR | OVLD
Data, remote, error or overload frame

Usage: Query only

BUS<b>:CAN:FRAMe<n>:STATus?

Returns the overall state of the specified frame.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:

<FrameStatus> OK | BTST | CRCD | ACKD | CRC | EOFD | NOACk | INSufficient
OK: frame is valid.
BTST: bit stuffing error occured
CRCD: wrong CRC delimiter occured
ACKD: Wrong ACK delimiter occured
CRC: cyclic redundancy check failed
EOFD: wrong end of frame
NOACk: acknowlegde is missing
INSufficient: frame is not completely contained in the acquisition. The acquired part of the frame is valid.

Usage: Query only

BUS<b>:CAN:FRAMe<n>:STARt?

Returns the start time of the specified frame.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:

<StartTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:CAN:FRAMe<n>:STOP?

Returns the end time of the specified frame.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:

<StopTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:CAN:FRAMe<n>:DATA?

Returns the data words of the specified frame.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:

<FrameData> Comma-separated list of decimal values of the data bytes.

Usage: Query only

BUS<b>:CAN:FRAMe<n>:ACKState?

Returns the state of the acknowledge field.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:

<AcknowledgeState> OK | UNDF
UNDF: Undefined

Usage: Query only

BUS<b>:CAN:FRAMe<n>:ACKValue?

Returns the value of the acknowledge field.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<AcknowledgeValue> Decimal value

Usage: Query only

BUS<b>:CAN:FRAMe<n>:CSSTate?

Returns the state of the checksum.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<ChecksumState> OK | UNDF
UNDF: Undefined

Usage: Query only

BUS<b>:CAN:FRAMe<n>:CSValue?

Returns the checksum value.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<ChecksumValue> Decimal value

Usage: Query only

BUS<b>:CAN:FRAMe<n>:DLCState?

Returns the state of the data length code.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<DLCState> OK | UNDF
UNDF: Undefined

Usage: Query only

BUS<b>:CAN:FRAMe<n>:DLCValue?

Returns the number of data bytes in the specified frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<DLCValue> non-negative integer

Usage: Query only

BUS<b>:CAN:FRAMe<n>:IDSTate?

Returns the state of the identifier.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<IdentifierState> OK | UNDF
UNDF: Undefined

Usage: Query only

BUS<b>:CAN:FRAMe<n>:IDTYpe?

Returns the length of the identifier: 11 bit for CAN base frames, or 29 bits for CAN extended frames.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<IdentifierType> ANY | B11 | B29
ANY
No length specified, for example, for triggering on data only.

Usage: Query only

BUS<b>:CAN:FRAMe<n>:IDValue?

Returns the decimal address value of the specified frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<IdentifierValue> Decimal value

Usage: Query only

BUS<b>:CAN:FRAMe<n>:BSEPosition?

Returns the position of the bit stuffing error in the specified frame (if available).

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<ErrorPosition> *RST: 0
Default unit: s

Usage: Query only

BUS<b>:CAN:FRAMe<n>:BCOunt?

Returns the number of data bytes in the specified frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<ByteCount> Number of words (bytes)

Usage: Query only

BUS<b>:CAN:FRAMe<n>:BYTE<o>:STATe?

Returns the state of the specified data byte.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

<o> *
Selects the byte number (1...n).

Return values:
<ByteStatus> OK | UNDF
UNDF: Undefined

Usage: Query only

BUS<b>:CAN:FRAMe<n>:BYTE<o>:VALue?

Returns the decimal value of the specified byte.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

<o> *
Selects the byte number (1...n).

Return values:
<ByteValue> Decimal value

Usage: Query only

CAN - Search

SEARch:PROTocol:CAN:CONDition....418
SEARch:PROTocol:CAN:FRAMe....418
SEARch:PROTocol:CAN:ACKerror....419
SEARch:PROTocol:CAN:BITSterror....419
SEARch:PROTocol:CAN:CRCerror....419
SEARch:PROTocol:CAN:FORMerror....420
SEARch:PROTocol:CAN:FTYPe....420
SEARch:PROTocol:CAN:ITYPe....420

SEARch:PROTocol:CAN:ICONdition....420
SEARch:PROTocol:CAN:IDENtifier....420
SEARch:PROTocol:CAN:DLENgth....421
SEARch:PROTocol:CAN:DCONdition....421
SEARch:PROTocol:CAN:DATA....421

SEARch:PROTocol:CAN:CONDition <SearchCondition>

Sets the event or combination of events to be searched for. Depending on the selected event, further settings are required.

Parameters:

<SearchCondition> FRAMe | ERRor | IDENtifier | IDData | IDERror

FRAMe
Search for a frame type. Set the frame type with `SEARch:PROTocol:CAN:FRAMe`.

ERRor
Search for errors of one or more error types. Set the error types with `SEARch:PROTocol:CAN:ACKerror`, `SEARch:PROTocol:CAN:BITSterror`, `SEARch:PROTocol:CAN:CRCerror`, and `SEARch:PROTocol:CAN:FORMerror`.

IDENtifier
Search for identifier.
Specifiy the identifier with `SEARch:PROTocol:CAN:FTYPe`, `SEARch:PROTocol:CAN:ITYPe`, `SEARch:PROTocol:CAN:ICONdition`, and `SEARch:PROTocol:CAN:IDENtifier`.

IDData
Search for identifier and data.
Set the identifier (see IDENtifier) and the data with `SEARch:PROTocol:CAN:DLENgth`, `SEARch:PROTocol:CAN:DCONdition`, and `SEARch:PROTocol:CAN:DATA`.

IDERror
Search for errors that occur with a specified identifier.
Set the identifier (see IDENtifier) and the errors to be found (see ERRor)

*RST: FRAM

SEARch:PROTocol:CAN:FRAMe <Frame>

Selects the frame type to be searched for.

The command is relevant if `SEARch:PROTocol:CAN:CONDition` is set to `FRAMe`.

Parameters:

<Frame> SOF | EOF | OVERload | ERRor | DTA11 | DTA29 | REM11 | REM29

SOF: start of frame
EOF: end of frame
OVERload: overload frame
ERRor: error frame
DTA11: data frame with 11bit identifier
DTA29: data frame with 29bit identifier
REM11: remote frame with 11bit identifier
REM29: remote frame with 29bit identifier

*RST: SOF

SEARch:PROTocol:CAN:ACKerror <AcknowledgeError>

Searches for acknowledgement errors. An acknowledgement error occurs when the transmitter does not receive an acknowledgment - a dominant bit during the Ack Slot.

The command is relevant if `SEARch:PROTocol:CAN:CONDition` is set to `ERRor` or `IDERror`.

Parameters:

<AcknowledgeError> ON | OFF

*RST: OFF

SEARch:PROTocol:CAN:BITSterror <BitStuffingError>

Searches for bit stuffing errors.

See also: "Stuff bit" on page 188.

The command is relevant if `SEARch:PROTocol:CAN:CONDition` is set to `ERRor` or `IDERror`.

Parameters:

<BitStuffingError> ON | OFF

*RST: OFF

SEARch:PROTocol:CAN:CRCerror <CRCerror>

Searches for errors in the Cyclic Redundancy Check.

The command is relevant if `SEARch:PROTocol:CAN:CONDition` is set to `ERRor` or `IDERror`.

Parameters:

<CRCerror> ON | OFF

*RST: OFF

SEARch:PROTocol:CAN:FORMerror <FormError>

Searches for form errors. A form error occurs when a fixed-form bit field contains one or more illegal bits.

The command is relevant if `SEARch:PROTocol:CAN:CONDition` is set to `ERRor` or `IDERror`.

Parameters:

<FormError> ON | OFF

*RST: OFF

SEARch:PROTocol:CAN:FTYPe

Specifies the frame type to be searched for if `SEARch:PROTocol:CAN:CONDition` is set to `IDENtifier`.

Parameters:

<FrameType> DATA | REMote | ANY

SEARch:PROTocol:CAN:ITYPe

Selects the length of the identifier: 11 bit for CAN base frames, or 29 bits for CAN extended frames.

The command is relevant if `SEARch:PROTocol:CAN:CONDition` is set to `IDENtifier`, `IDData`, or `IDERror`.

Parameters:

<IdType> B11 | B29

*RST: B11

SEARch:PROTocol:CAN:ICONdition <IdCondition>

Sets the comparison condition for the identifier: If the pattern contains at least one X (don't care), you can trigger on values equal or not equal to the specified value. If the pattern contains only 0 and 1, you can also trigger on a range greater than or lower than the specified value.

The command is relevant if `SEARch:PROTocol:CAN:CONDition` is set to `IDENtifier`, `IDData`, or `IDERror`.

Parameters:

<IdCondition> EQUal | NEQual | GTHan | LTHan

*RST: EQU

SEARch:PROTocol:CAN:IDENtifier <Identifier>

Defines the identifier pattern. The pattern length is defined with `SEARch:PROTocol:CAN:ITYPe`.

The command is relevant if SEARch:PROTocol:CAN:CONDition is set to IDENtifier, IDData, or IDERror.

Parameters:

<Identifier> String containing binary pattern with max. 29 bit. Characters 0, 1, and X are allowed.

SEARch:PROTocol:CAN:DLENgth <DataLength>

Defines the length of the data pattern - the number of bytes in the pattern.

The command is relevant if SEARch:PROTocol:CAN:CONDition is set to IDData.

Parameters:

<DataLength> Range: 0 to 8
Increment: 1
*RST: 1
Default unit: Byte

SEARch:PROTocol:CAN:DCONdition <DataCondition>

Sets the comparison condition for data: If the pattern contains at least one X (don't care), you can trigger on values equal or not equal to the specified value. If the pattern contains only 0 and 1, you can also trigger on a range greater than or lower than the specified value.

The command is relevant if SEARch:PROTocol:CAN:CONDition is set to IDData.

Parameters:

<DataCondition> EQUal | NEQual | GTHan | LTHan
*RST: EQU

SEARch:PROTocol:CAN:DATA <Data>

Defines the data pattern. The pattern length is defined with SEARch:PROTocol:CAN:DLENgth.

The command is relevant if SEARch:PROTocol:CAN:CONDition is set to IDData.

Parameters:

<Data> String containing binary pattern with max. 64 bit. Characters 0, 1, and X are allowed. Make sure to enter complete bytes.

15.2.13.7 LIN

The Local Interconnect Network (LIN) is a simple, low-cost bus system used within automotive network architectures.

Note: SPI/SSPI and UART protocols occupy two bus lines (bus 1 and 2 or bus 3 and 4). If one of these buses is configured, the number of buses (suffix <b>) is reduced. Bus 2 and/or bus 4 is not available.

- LIN - Configuration....422
- LIN - Trigger....423
- LIN - Decode Results....426
- LIN - Search....431

LIN - Configuration

BUS<b>:LIN:DATA:SOURce....422
BUS<b>:LIN:POLarity....422
BUS<b>:LIN:STANdard....422
BUS<b>:LIN:BITRate....423
CHANnel<m>:THReshold:FINDlevel....423

BUS<b>:LIN:DATA:SOURce <Source>

Sets the source of the data line. All channel waveforms can be used.

Suffix:
<b> 1..4
Selects the bus.

Parameters:
<Source> CH1 | CH2 | CH3 | CH4 | D0..D15
*RST: CH1

BUS<b>:LIN:POLarity <Polarity>

Defines the idle state of the bus. The idle state is the rezessive state and corresponds to a logic 1.

Suffix:
<b> 1..4
Selects the bus.

Parameters:
<Polarity> IDLHigh | IDLLow
IDLHigh: Low active, negative polarity
IDLLow: High active, positive polarity
*RST: IDLL

BUS<b>:LIN:STANdard <Standard>

Selects the version of the LIN standard that is used in the DUT. The setting mainly defines the checksum version used during decoding.

The most common version is LIN 2.x. For mixed networks, or if the standard is unknown, set the LIN standard to AUTO.

Suffix:
<b> 1..4
Selects the bus.

Parameters:
<Standard> V1X | V2X | J2602 | AUTO
*RST: V1X

BUS<b>:LIN:BITRate <BitRate>

Sets the number of transmitted bits per second.

Suffix:
<b> 1..4
Selects the bus.

Parameters:
<BitRate> *RST: 9,60E+003
Default unit: Bit/s

CHANnel<m>:THReshold:FINDlevel

Executes the analysis of all analog channels that are configured for the selected bus and sets the threshold for digitization of analog signals for each channel.

Suffix:
<m> Selects the input channel. The number of channels depends on the instrument.

Usage: Event

LIN - Trigger

TRIGger:A:LIN:TYPE....423
TRIGger:A:LIN:CHKSerror....424
TRIGger:A:LIN:IPERror....424
TRIGger:A:LIN:SYERror....424
TRIGger:A:LIN:ICONdition....425
TRIGger:A:LIN:IDENtifier....425
TRIGger:A:LIN:DATA....425
TRIGger:A:LIN:DCONdition....425
TRIGger:A:LIN:DLENgth....426

TRIGger:A:LIN:TYPE <TriggerType>

Specifies the trigger mode for LIN.

Parameters:

<TriggerType> SYNC | WKFRame | ID | IDDT | ERRCondition

SYNC
Start of frame, triggers on the stop bit of the sync field.

WKFRame
Triggers after a wakeup frame.

ID
Sets the trigger to a specific identifier or an identifier range.
Set the identifier with `TRIGger:A:LIN:ICONdition` and `TRIGger:A:LIN:IDENtifier`.

IDDT
Set the identifier (see ID) and the data with `TRIGger:A:LIN:DLENgth`, `TRIGger:A:LIN:DCONdition`, and `TRIGger:A:LIN:DATA`.

ERRCondition
Identifies various errors in the frame. You can select one or more error types as trigger condition.
Select the error types with `TRIGger:A:LIN:CHKSerror`, `TRIGger:A:LIN:IPERror`, and `TRIGger:A:LIN:SYERror`.

*RST: SYNC

TRIGger:A:LIN:CHKSerror <ChecksumError>

Triggers on a checksum error. The checksum verifies the correct data transmission. It is the last byte of the frame response. The checksum includes not only the data but also the protected identifier (PID).

The command is relevant if `TRIGger:A:LIN:TYPE` is set to `ERRCondition`.

Parameters:

<ChecksumError> ON | OFF

*RST: ON

TRIGger:A:LIN:IPERror <IdParityError>

Triggers on a parity error. Parity bits are the bits 6 and 7 of the identifier. They verify the correct transmission of the identifier.

The command is relevant if `TRIGger:A:LIN:TYPE` is set to `ERRCondition`.

Parameters:

<IdParityError> ON | OFF

*RST: OFF

TRIGger:A:LIN:SYERror <SyncError>

Triggers if synchronization caused an error.

The command is relevant if TRIGger:A:LIN:TYPE is set to ERRCondition.

Parameters:

<SyncError> ON | OFF
*RST: OFF

TRIGger:A:LIN:ICONdition <IdentifierCondition>

Sets the comparison condition for the identifier: If the pattern contains at least one X (don't care), you can trigger on values equal or not equal to the specified value. If the pattern contains only 0 and 1, you can also trigger on a range greater than or lower than the specified value.

The command is relevant if TRIGger:A:LIN:TYPE is set to ID or IDDT.

Parameters:

<IdentifierCondition> EQUal | NEQual | GTHan | LTHan
*RST: EQ

TRIGger:A:LIN:IDENtifier <Identifier>

Defines the identifier pattern.

The command is relevant if TRIGger:A:LIN:TYPE is set to ID or IDDT.

Parameters:

<Identifier> String containing binary pattern. Characters 0, 1, and X are allowed. Enter the 6 bit identifier without parity bits, not the protected identifier.

TRIGger:A:LIN:DATA <Data>

Defines the data pattern. The number of bytes in the data pattern is defined with TRIGger:A:LIN:DLENgth.

The command is relevant if TRIGger:A:LIN:TYPE is set to IDDT.

Parameters:

<Data> String containing binary pattern with max. 64 bit. Characters 0, 1, and X are allowed. Make sure to enter complete bytes.

TRIGger:A:LIN:DCONdition <DataCondition>

Sets the comparison condition for data: If the pattern contains at least one X (don't care), you can trigger on values equal or not equal to the specified value. If the pattern contains only 0 and 1, you can also trigger on a range greater than or lower than the specified value.

The command is relevant if TRIGger:A:LIN:TYPE is set to IDDT.

Parameters:
<DataCondition> EQUal | NEQual | GTHan | LTHan
*RST: EQ

TRIGger:A:LIN:DLENgth <DataLength>

Defines the length of the data pattern - the number of bytes in the pattern.

The command is relevant if `TRIGger:A:LIN:TYPE` is set to `IDDT`.

Parameters:
<DataLength> Range: 1 to 8
Increment: 1
*RST: 1
Default unit: Byte

LIN - Decode Results

BUS<b>:LIN:FCOunt?....426
BUS<b>:LIN:FRAMe<n>:DATA?....426
BUS<b>:LIN:FRAMe<n>:STATus?....427
BUS<b>:LIN:FRAMe<n>:STARt?....427
BUS<b>:LIN:FRAMe<n>:STOP?....427
BUS<b>:LIN:FRAMe<n>:CSSTate?....428
BUS<b>:LIN:FRAMe<n>:CSValue?....428
BUS<b>:LIN:FRAMe<n>:IDPValue?....428
BUS<b>:LIN:FRAMe<n>:IDSTate?....429
BUS<b>:LIN:FRAMe<n>:IDValue?....429
BUS<b>:LIN:FRAMe<n>:SYSTate?....429
BUS<b>:LIN:FRAMe<n>:SYValue?....430
BUS<b>:LIN:FRAMe<n>:VERSion?....430
BUS<b>:LIN:FRAMe<n>:BCOunt?....430
BUS<b>:LIN:FRAMe<n>:BYTE<o>:STATe?....431
BUS<b>:LIN:FRAMe<n>:BYTE<o>:VALue?....431

BUS<b>:LIN:FCOunt?

Returns the number of received frames of the active LIN bus.

Suffix:
<b> 1..4
Selects the bus.

Return values:
<FrameCount> Total number of decoded frames.

Usage: Query only

BUS<b>:LIN:FRAMe<n>:DATA?

Returns the data bytes of the specified frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<FrameData> Comma-separated list of decimal values of the data bytes.

Usage: Query only

BUS<b>:LIN:FRAMe<n>:STATus?

Suffix:
<b> 1..4
Selects the bus.

<n> *

Return values:
<FrameStatus> OK | UART | CHCKsum | PRERror | SYERror | WAKeup | INSufficient | ERR | LENer

Usage: Query only

BUS<b>:LIN:FRAMe<n>:STARt?

Returns the start time of the specified frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<StartTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:LIN:FRAMe<n>:STOP?

Returns the end time of the specified frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<StopTime> Range: depends on sample rate, record length, and time base
Increment: depends on the time base
Default unit: s

Usage: Query only

BUS<b>:LIN:FRAMe<n>:CSSTate?

Returns the checksum state of the specified frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<ChecksumState> OK | ERR | UNDF
ERR: error
UNDF: undefined

Usage: Query only

BUS<b>:LIN:FRAMe<n>:CSValue?

Returns the checksum value.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<ChecksumValue> Decimal value

Usage: Query only

BUS<b>:LIN:FRAMe<n>:IDPValue?

Returns the parity value.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<IdentifierParityValue> Decimal value

Usage: Query only

BUS<b>:LIN:FRAMe<n>:IDSTate?

Returns the identifier state of the selected frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<IdentifierState> OK | PRERror | UVAL | INSufficient
PRERror: parity error
UVAL: unexpected value
INSufficient: the frame is not completely contained in the acquisition. The decoded part of the frame is valid.

Usage: Query only

BUS<b>:LIN:FRAMe<n>:IDValue?

Returns the identifier value (address)

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:
<IdentifierValue> Decimal value

Usage: Query only

BUS<b>:LIN:FRAMe<n>:SYSTate?

Returns the state of the sync field for the specified frame.

Suffix:
<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:

<SyncFieldState> OK | ERR | UNDF
ERR: error
UNDF: undefined

Usage: Query only

BUS<b>:LIN:FRAMe<n>:SYValue?

Returns the value of the synchronization field.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:

<SyncFieldValue> Decimal value

Usage: Query only

BUS<b>:LIN:FRAMe<n>:VERSion?

Returns the version of the LIN standard for the specified frame.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:

<FrameVersion> V1X | V2X | UNK
UNK: Unknown

Usage: Query only

BUS<b>:LIN:FRAMe<n>:BCOunt?

Returns the number of data bytes in the specified frame.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

Return values:

<ByteCount> Number of words (bytes)

Usage: Query only

BUS<b>:LIN:FRAMe<n>:BYTE<o>:STATe?

Returns the state of the specified data byte.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

<o> *
Selects the byte number (1...n).

Return values:

<ByteStatus> OK | INS | UART

The byte is not completely contained in the acquisition

UART
At least one UART error occured. LIN uses UART words without parity bit.

Usage: Query only

BUS<b>:LIN:FRAMe<n>:BYTE<o>:VALue?

Returns the decimal value of the specified byte.

Suffix:

<b> 1..4
Selects the bus.

<n> *
Selects the frame (1...n).

<o> *
Selects the byte number (1...n).

Return values:

<ByteValue> Decimal value

Usage: Query only

LIN - Search

SEARch:PROTocol:LIN:CONDition....432
SEARch:PROTocol:LIN:FRAMe....432
SEARch:PROTocol:LIN:IPERror....433
SEARch:PROTocol:LIN:CHKSerror....433
SEARch:PROTocol:LIN:SYERror....433
SEARch:PROTocol:LIN:ICONdition....433
SEARch:PROTocol:LIN:IDENtifier....433

SEARch:PROTocol:LIN:DLENgth....434
SEARch:PROTocol:LIN:DCONdition....434
SEARch:PROTocol:LIN:DATA....434

SEARch:PROTocol:LIN:CONDition <SearchCondition>

Sets the event or combination of events to be searched for. Depending on the selected event, further settings are required.

Parameters:

<SearchCondition> FRAMe | ERRor | IDENtifier | IDData | IDERror

FRAMe
Search for a frame type.
Set the frame type with `SEARch:PROTocol:LIN:FRAMe`.

ERRor
Search for errors of one or more error types.
Set the error types with `SEARch:PROTocol:LIN:CHKSerror`, `SEARch:PROTocol:LIN:IPERror`, and `SEARch:PROTocol:LIN:SYERror`.

IDENtifier
Search for identifier.
Specifiy the identifier with `SEARch:PROTocol:LIN:ICONdition` and `SEARch:PROTocol:LIN:IDENtifier`.

IDData
Search for identifier and data.
Set the identifier (see IDENtifier) and the data with `SEARch:PROTocol:LIN:DLENgth`, `SEARch:PROTocol:LIN:DCONdition`, and `SEARch:PROTocol:LIN:DATA`.

IDERror
Search for errors that occur with a specified identifier. Set the identifier (see IDENtifier) and the errors to be found (see ERRor).

*RST: FRAM

SEARch:PROTocol:LIN:FRAMe <Frame>

Selects the frame type to be searched for.

The command is relevant if `SEARch:PROTocol:LIN:CONDition` is set to `FRAMe`.

Parameters:

<Frame> SOF | WAKeup

SOF: start of frame
WAKeup: Wakeup frame

*RST: SOF

SEARch:PROTocol:LIN:IPERror <IdParityError>

Searches for parity errors.

The command is relevant if `SEARch:PROTocol:LIN:CONDition` is set to `ERRor` or `IDERror`.

Parameters:

<IdParityError> ON | OFF

*RST: OFF

SEARch:PROTocol:LIN:CHKSerror <ChecksumError>

Searches for checksum errors.

The command is relevant if `SEARch:PROTocol:LIN:CONDition` is set to `ERRor` or `IDERror`.

Parameters:

<ChecksumError> ON | OFF

*RST: OFF

SEARch:PROTocol:LIN:SYERror <SyncError>

Searches for synchronization errors.

The command is relevant if `SEARch:PROTocol:LIN:CONDition` is set to `ERRor` or `IDERror`.

Parameters:

<SyncError> ON | OFF

*RST: OFF

SEARch:PROTocol:LIN:ICONdition <IdCondition>

Sets the comparison condition for the identifier: If the pattern contains at least one X (don't care), you can trigger on values equal or not equal to the specified value. If the pattern contains only 0 and 1, you can also trigger on a range greater than or lower than the specified value.

The command is relevant if `SEARch:PROTocol:LIN:CONDition` is set to `IDENtifier`, `IDData` or `IDERror`.

Parameters:

<IdCondition> EQUal | NEQual | GTHan | LTHan

*RST: EQU

SEARch:PROTocol:LIN:IDENtifier <Identifier>

Defines the identifier pattern.

The command is relevant if SEARch:PROTocol:LIN:CONDition is set to IDENtifier, IDData or IDERror.

Parameters:

<Identifier> String containing binary pattern. Characters 0, 1, and X are allowed. Enter the 6 bit identifier without parity bits, not the protected identifier.

SEARch:PROTocol:LIN:DLENgth <DataLength>

Defines the length of the data pattern - the number of bytes in the pattern.

The command is relevant if SEARch:PROTocol:LIN:CONDition is set to IDData.

Parameters:

<DataLength>
Range: 1 to 8
Increment: 1
*RST: 1
Default unit: Byte

SEARch:PROTocol:LIN:DCONdition <DataCondition>

Sets the comparison condition for data: If the pattern contains at least one X (don't care), you can trigger on values equal or not equal to the specified value. If the pattern contains only 0 and 1, you can also trigger on a range greater than or lower than the specified value.

The command is relevant if SEARch:PROTocol:LIN:CONDition is set to IDData.

Parameters:

<DataCondition> EQUal | NEQual | GTHan | LTHan
*RST: EQU

SEARch:PROTocol:LIN:DATA <Data>

Defines the data pattern. The pattern length is defined with SEARch:PROTocol:LIN:DLENgth.

The command is relevant if SEARch:PROTocol:LIN:CONDition is set to IDData.

Parameters:

<Data> String containing binary pattern with max. 64 bit. Characters 0, 1, and X are allowed. Make sure to enter complete bytes.

15.2.14 Mixed Signal Option (MSO, R&S RTM-B1)

- Digital Channels....435
- Parallel Buses....437

15.2.14.1 Digital Channels

DIGital<m>:DISPlay....435
DIGital<m>:TECHnology....435
DIGital<m>:THReshold....435
DIGital<m>:THCoupling....436
DIGital<m>:Hysteresis....436
DIGital<m>:LABel....436
DIGital<m>:POSition....436
DIGital<m>:LABel:STATe....437
DIGital<m>:SIZE....437

DIGital<m>:DISPlay <State>

Enables and displays the indicated digital channel, or disables it.

Suffix:
<m> 0..15
Number of the digital channel

Parameters:
<State> ON | OFF
*RST: OFF

DIGital<m>:TECHnology

Selects the threshold voltage for various types of integrated circuits and applies it to the channel group to which the indicated digital channel belongs.

Suffix:
<m> 0..15
Number of the digital channel.
Channel groups: 0..3; 4..7; 8..11; 12..15

Parameters:
<ThresholdMode> TTL | ECL | CMOS | MANual
TTL: 1.4 V
ECL: -1.3 V
CMOS: 2.5 V
MANual: Set a user-defined threshold value with `DIGital<m>:THReshold`
*RST: MAN

DIGital<m>:THReshold

Sets the logical threshold for the channel group to which the indicated digital channel belongs.

Suffix:
<m> 0..15
Number of the digital channel.
Channel groups: 0..3; 4..7; 8..11; 12..15

Parameters:
<ThresholdLevel> *RST: 1.4
Default unit: V

DIGital<m>:THCoupling

Applies the last defined threshold and hysteresis values to all digital channels.

Suffix:
<m> 0..15
Number of the digital channel

Parameters:
<ThresholdCoupling> ON | OFF

DIGital<m>:Hysteresis

Defines the size of the hysteresis to avoid the change of signal states due to noise. The setting applied to the channel group to which the indicated digital channel belongs.

Suffix:
<m> 0..15
Number of the digital channel.
Channel groups: 0..3; 4..7; 8..11; 12..15

Parameters:
<Hysteresis> MAXimum | ROBust | NORMal

DIGital<m>:LABel <Label>

Defines a label for the indicated digital channel.

Suffix:
<m> 0..15
Number of the digital channel

Parameters:
<Label> String value
String parameter

Example: `DIGital4:LABel "Data"`
Defines the label "Data" dor digital channel D4.

DIGital<m>:POSition <Position>

Sets the vertical position of the indicated vertical channel.

Suffix:
<m> 0..15
Number of the digital channel

Parameters:
<Position> Vertical position in divisions
Default unit: div

DIGital<m>:LABel:STATe

Displays or hides the label of the indicated digital channel.

Suffix:
<m> 0..15
Number of the digital channel

Parameters:
<State> ON | OFF
*RST: OFF

DIGital<m>:SIZE <Size>

Sets the size of the indicated vertical channel.

Suffix:
<m> 0..15
Number of the digital channel

Parameters:
<Size> SMALl | MEDium | LARGe
*RST: SMAL

15.2.14.2 Parallel Buses

- Parallel Bus - Configuration....437
- Parallel Clocked Bus - Configuration....438
- Parallel Buses - Decode Results....439

Parallel Bus - Configuration

BUS<b>:PARallel:WIDTh <BusWidth>

Sets the number of lines to be analyzed.

Suffix:
<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<BusWidth> Maximum number is the number of input channels.

Range: 1 to 16
Increment: 1
*RST: 4
Default unit: Bit

Parallel Clocked Bus - Configuration

BUS<b>:CPARallel:WIDTh....438
BUS<b>:CPARallel:CLOCK:SLOPe....438
BUS<b>:CPARallel:CS:POLarity....438

BUS<b>:CPARallel:WIDTh <BusWidth>

Sets the number of lines to be analyzed. D0 and D1 are reserved for chip select and clock, all other digital channels can be used for data.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<BusWidth> Range: 1 to 14
Increment: 1
*RST: 4
Default unit: Bit

BUS<b>:CPARallel:CLOCK:SLOPe <ClockSlope>

Selects if the data is sampled on the rising or falling slope of the clock, or on both edges (EITHer). The clock slope marks the begin of a new bit

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<ClockSlope> POSitive | NEGative | EITHer

BUS<b>:CPARallel:CS:POLarity <Polarity>

Selects wether the chip select signal is high active (high = 1) or low active (low = 1).

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Parameters:

<Polarity> POSitive | NEGative

POSitive = high active
NEGative = low active

Parallel Buses - Decode Results

The commands to query results of decoded parallel clocked and unclocked buses are similar and described together in this chapter..

BUS<b>:PARallel:FCOunt?....439
BUS<b>:CPARallel:FCOunt?....439
BUS<b>:PARallel:FRAMe<n>:DATA?....439
BUS<b>:CPARallel:FRAMe<n>:DATA?....439
BUS<b>:PARallel:FRAMe<n>:STATe?....440
BUS<b>:CPARallel:FRAMe<n>:STATe?....440
BUS<b>:PARallel:FRAMe<n>:STARt?....440
BUS<b>:CPARallel:FRAMe<n>:STARt?....440
BUS<b>:PARallel:FRAMe<n>:STOP?....440
BUS<b>:CPARallel:FRAMe<n>:STOP?....440

BUS<b>:PARallel:FCOunt?
BUS<b>:CPARallel:FCOunt?

Returns the number of decoded frames.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

Return values:

<FrameCount> Total number of decoded frames.

Usage: Query only

BUS<b>:PARallel:FRAMe<n>:DATA?
BUS<b>:CPARallel:FRAMe<n>:DATA?

Returns the data words of the specified frame.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

Return values:

<FrameData> List of decimal values of data words

Usage: Query only

BUS<b>:PARallel:FRAMe<n>:STATe?
BUS<b>:CPARallel:FRAMe<n>:STATe?

Returns the overall state of the specified frame.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

Return values:

<FrameStatus> OK | ERRor | INSufficient

Usage: Query only

BUS<b>:PARallel:FRAMe<n>:STARt?
BUS<b>:CPARallel:FRAMe<n>:STARt?

Returns the start time of the specified frame.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

Return values:

<StartTime> Default unit: s

Usage: Query only

BUS<b>:PARallel:FRAMe<n>:STOP?
BUS<b>:CPARallel:FRAMe<n>:STOP?

Returns the end time of the specified frame.

Suffix:

<b> 1..4
Selects the bus.
Note: SPI/SSPI and UART protocols occupy two bus lines.

<n> *
Selects the frame.

Return values:

<StopTime> Default unit: s

Usage: Query only

15.2.15 Data and File Management

This chapter describes commands on how to print and save screenshots, and how to manage measurement settings and data..

- Screenshots....441
- Saving and Loading Data: MMEMory Commands....443

15.2.15.1 Screenshots

This chapter describes remote commands used to print and save screenshots.

HCOPy:DESTination....441
MMEMory:NAME....441
HCOPy[:IMMediate]....442
HCOPy:LANGuage....442
HCOPy:PAGE:SIZE....442
HCOPy:PAGE:ORIentation....442
HCOPy:COLor:SCHeme....442
SYSTem:COMMunicate:PRINter:SELect....443
SYSTem:COMMunicate:PRINter:ENUMerate:FIRSt?....443
SYSTem:COMMunicate:PRINter:ENUMerate[:NEXT]?....443

HCOPy:DESTination <Medium>

Defines whether the screenshot is saved or printed.

Parameters:

<Medium> MMEM | SYST:COMM:PRIN

String parameter

MMEM
Saves the screenshot to a file. Specify the file name and location with `MMEMory:NAME`.

SYST:COMM:PRIN
Prints on the printer specified with `SYSTem:COMMunicate:PRINter:SELect`. The printer must be specified before the `HCOPy:DESTination` is sent.

*RST: MMEM

Example: `HCOP:DEST "MMEM"`

chapter 15.3.3.1, "Saving Screenshots to File", on page 461

MMEMory:NAME <FileName>

Defines the file name to store an image of the display with `HCOPy[:IMMediate]`.

Parameters:

<FileName> String parameter

Example:

chapter 15.3.3.1, "Saving Screenshots to File", on page 461

HCOPy[:IMMediate]

Prints an image of the display to the printer or saves an image to a file or the clipboard, depending on the `HCOPy:DESTination` setting.

Before starting the printout, make sure that:

- The printer is defined by `SYSTem:COMMunicate:PRINter:SELect`.
- The path for storage is defined correctly by `MMEMory:CDIRectory`
- The file name for storage is defined by `MMEMory:NAME`.

Example: chapter 15.3.3.1, "Saving Screenshots to File", on page 461

Usage: Event

HCOPy:LANGuage <Format>

Defines the format of the printed or saved screenshot.

Parameters:

<Format> GDI | BMP | PNG

GDI
For output on printer

BMP | PNG
File formats for saved screenshots

*RST: PNG

Example: chapter 15.3.3.1, "Saving Screenshots to File", on page 461

HCOPy:PAGE:SIZE <Size>

Defines the page size to be used.

Parameters:

<Size> A4 | A5 | B5 | B6 | EXECutive

HCOPy:PAGE:ORIentation <Orientation>

Defines the page orientation.

Parameters:

<Orientation> LANDscape | PORTrait

HCOPy:COLor:SCHeme <ColorScheme>

Defines the color mode for saved and printed screenshots.

Parameters:

<ColorScheme> COLor | GRAYscale | INVerted

INVerted inverts the colors of the output, i.e. a dark waveform is printed on a white background.

*RST: COLor

Example: chapter 15.3.3.1, "Saving Screenshots to File", on page 461

SYSTem:COMMunicate:PRINter:SELect <PrinterName>

Selects a configured printer.

Parameters:

<PrinterName> String parameter

Enter the string as it is returned with `SYSTem:COMMunicate:PRINter:ENUMerate:FIRSt?` or `SYSTem:COMMunicate:PRINter:ENUMerate[:NEXT]?`.

SYSTem:COMMunicate:PRINter:ENUMerate:FIRSt?

Queries the name of the first printer in the list of printers. The names of other installed printers can be queried with the `SYSTem:COMMunicate:PRINter:ENUMerate[:NEXT]?` command.

Return values:

<PrinterName> String parameter

If no printer is configured an empty string is returned.

Usage: Query only

SYSTem:COMMunicate:PRINter:ENUMerate[:NEXT]?

Queries the name of the next printer installed. The `SYSTem:COMMunicate:PRINter:ENUMerate:FIRSt?` command should be sent previously to return to the beginning of the printer list and query the name of the first printer.

Return values:

<PrinterName> String parameter

After all available printer names have been returned, an empty string enclosed by quotation marks (") is returned for the next query. Further queries are answered by a query error.

Usage: Query only

15.2.15.2 Saving and Loading Data: MMEMory Commands

The Mass MEMomory subsystem provides commands to access the storage media and to save and reload instrument settings and data.

The R&S RTM has three storage devices indicated as drives:

- /INT: internal storage with default directories for each data type
- /USB_FRONT: USB connector on the front panel
- /USB_REAR: USB connector on the rear panel

Common computer and network drives like `C:`, `D:`, `\\server\share` are not available.

Name conventions

The names of files and directories have to meet the following rules:

- Only the 8.3 format with ASCI characters is supported.
- No special characters are allowed.
- Use / (slash) instead of \ (backslash).

MMEMory:DRIVes?....444
MMEMory:MSIS....444
MMEMory:CDIRectory....445
MMEMory:MDIRectory....445
MMEMory:RDIRectory....445
MMEMory:DCATalog?....446
MMEMory:DCATalog:LENGth?....446
MMEMory:CATalog?....447
MMEMory:CATalog:LENGth?....447
MMEMory:COPY....448
MMEMory:MOVE....448
MMEMory:DELete....448
MMEMory:DATA....449
MMEMory:STORe:STATe....449
MMEMory:LOAD:STATe....449

MMEMory:DRIVes?

Returns the storage devices available on the R&S RTM.

Return values:

<Drive> List of strings, for example, ""/INT"","/USB_FRONT"","/USB_REAR""

/INT: internal storage
/USB_FRONT: USB connector on the front panel
/USB_REAR: USB connector on the rear panel

Usage: Query only

MMEMory:MSIS [<MassStorageIS>]

Changes the storage device (drive).

Parameters:

<MassStorageIS> One of the available drives: /INT, /USB_FRONT, or /USB_REAR

Example: `MMEM:MSIS '/USB_FRONT'`
Sets the USB flash drive connected to the front panel as storage device to be used.

MMEMory:CDIRectory [<DirectoryName>]

Specifies the current directory for file access.

Setting parameters:
<DirectoryName> String parameter to specify the directory, including the storage device.

Example: `MMEM:CDIR "/USB_FRONT/DATA"`

Example: chapter 15.3.3.2, "Saving, Copying, and Loading Setup Data", on page 461

MMEMory:MDIRectory <DirectoryName>

Creates a new directory with the specified name.

Setting parameters:
<DirectoryName> String parameter

Absolute path including the storage device, or relative to the current directory.

Example: Create directory DATA on the front USB flash device, with absolute path:
`MMEM:MDIR "/USB_FRONT/DATA"`

Example: Create directory JANUARY in the DATA directory, with relative path:
`MMEM:CDIR "/USB_FRONT/DATA/"`
`MMEM:MDIR "JANUARY"`

Usage: Setting only

MMEMory:RDIRectory <DirectoryName>

Deletes the specified directory.

Note: All subdirectories and all files in the specified directory and in the subdirectories will be deleted!

You cannot delete the current directory or a superior directory. In this case, the instrument returns an execution error.

Setting parameters:
<DirectoryName> String parameter, absolute path or relative to the current directory

Example: `MMEM:RDIR "/INT/TEST"`
Deletes the directory TEST in the internal storage device, and all files and subdirectories in the directory.

Usage: Setting only

MMEMory:DCATalog? <PathName>

Returns the subdirectories of the specified directory. The result corresponds to the number of strings returned by the `MMEMory:DCATalog:LENgth?` command.

Query parameters:

<PathName> String parameter

Specifies the directory.

Return values:

<FileEntry> String parameter

List of subdirectory strings separated by commas. If the specified directory does not have any subdirectory, the current and the parent directories are returned (`".,,0",".,,,0"`)

Example: Query for directories with absolute path:

```
MMEM:DCAT? "/USB_FRONT/*"
received ".,,0",",,,0","DATA,,0","DATA_NEW,,
0","SCREENSHOTS,,0"
MMEM:DCAT:LENG? "/USB_FRONT/*"
received 5
```

Example: Query for directories in the current directory:

```
MMEM:CDIR "/USB_FRONT/DATA/"
MMEM:DCAT? "*"
received ".,,0",",,,0","JANUARY,,
0","FEBRUARY,,0"
MMEM:DCAT:LENG? "*"
received 4
```

Example: Query with filter:

```
MMEM:DCAT? "/USB_FRONT/DA*"
received "DATA,,0","DATA_NEW,,0"
MMEM:DCAT:LENG? "/USB_FRONT/DA*"
received 2
```

Usage: Query only

MMEMory:DCATalog:LENGth? <PathName>

Returns the number of directories in specified directory. The result corresponds to the number of strings returned by the `MMEMory:DCATalog?` command.

Query parameters:

<PathName> String parameter

Specifies the directory.

Return values:

<FileEntryCount> Number of directories.

Example: see `MMEMory:DCATalog?`

Usage: Query only

MMEMory:CATalog? <PathName>[,<Format>]

Returns the a list of files contained in the specified directory. The result corresponds to the number of files returned by the `MMEMory:CATalog:LENgth?` command.

Query parameters:

<PathName> String parameter

Specifies the directory. A filter can be used to list, for example, only files of a given file type.

<Format> ALL | WTIMe

ALL: Extended result including file, date, time and attributes
WTIMe: Result including file, date, time

Return values:

<UsedMemory> Total amount of storage currently used in the directory, in bytes.

<FreeMemory> Total amount of storage available in the directory, in bytes.

<FileEntry> String parameter

All files of the directory are listed with their file name, format and size in bytes.

Example: Query for files in the DATA directory, with absolute path:

```
MMEM:CAT? "/USB_FRONT/DATA/*.*"
received: 511104,8633856,"MONDAY.TXT,,
8","TUESDAY.CSV,,8"
```

Example: Query for TXT files in the DATA directory, with relative path:

```
MMEM:CDIR "/USB_FRONT/DATA"'
MMEM:CAT? "*.TXT"
received: 511104,8633856,"MONDAY.TXT,,8"
MMEM:CAT:LENGTH? "*.TXT"
received 1
```

Example: chapter 15.3.3.2, "Saving, Copying, and Loading Setup Data", on page 461

Usage: Query only

MMEMory:CATalog:LENGth? <PathName>

Returns the number of files in the specified directory. The result corresponds to the number of files returned by the `MMEMory:CATalog?` command.

Query parameters:

<PathName> String parameter

Directory to be queried, absolute or relative path

Return values:
<Count> Number of files.

Example: see `MMEMory:CATalog?`

Usage: Query only

MMEMory:COPY <FileSource>,<FileDestination>

Copies data to another directory on the same or different storage device. The file name can be changed, too.

Setting parameters:
<FileSource> String parameter
Name and path of the file to be copied

<FileDestination> String parameter
Name and path of the new file. If the file already exists, it is overwritten without notice.

Example:
```
MMEM:COPY "/INT/SETTINGS/SET001.SET",
"/USB_FRONT/SETTINGS/TESTSET1.SET"
```

Example: chapter 15.3.3.2, "Saving, Copying, and Loading Setup Data", on page 461

Usage: Setting only

MMEMory:MOVE <FileSource>,<FileDestination>

Moves an existing file to a new location.

Setting parameters:
<FileSource> String parameter
Path and name of the file to be moved

<FileDestination> String parameter
Path and name of the new file

Example:
```
MMEM:MOVE "/INT/SETTINGS/SET001.SET",
"/USB_FRONT/SETTINGS/SET001.SET"
```

Usage: Setting only

MMEMory:DELete <FileSource>

Removes a file from the specified directory.

Setting parameters:
<FileSource> String parameter
File name and path of the file to be removed. If the path is omitted, the specified file will be deleted in the current directory. Filters are not allowed.

Example: chapter 15.3.3.2, "Saving, Copying, and Loading Setup Data", on page 461

Usage: Setting only

MMEMory:DATA <FileName>,<Data>

Writes data to the specified file in the current directory `MMEMory:CDIRectory`, or reads the data.

Parameters:

<Data> 488.2 block data

The block begins with character '#'. The next digit is the length of the length information, followed by this given number of digits providing the number of bytes in the binary data attached.

Parameters for setting and query:

<FileName> String parameter containing the file name

Example:
```
MMEM:DATA "abc.txt", #216This is the file
```
#2: the length infomation has two digits
16: the binary data has 16 bytes.
```
MMEM:DATA? "abc.txt"
received: This is the file
```

Example: chapter 15.3.3.2, "Saving, Copying, and Loading Setup Data", on page 461

MMEMory:STORe:STATe <StateNumber>,<FileName>

Saves the current device settings to the specified file in the current directory.

Setting parameters:

<StateNumber> Range: 1 to 1
Increment: 0
*RST: 1

<FileName> String parameter

File name, with or without file extension

Example:
```
MMEM:CDIR "/USB_FRONT/DATA"'
MMEM:STOR:STAT 1,"MORNING.SET"
```

Example: chapter 15.3.3.2, "Saving, Copying, and Loading Setup Data", on page 461

Usage: Setting only

MMEMory:LOAD:STATe <StateNumber>,<FileName>

Loads the device settings from the specified file in the current directory.

Setting parameters:

<StateNumber> Range: 1 to 1
Increment: 0
*RST: 1

<FileName> String parameter
File name, with or without file extension

Example:
```
MMEM:CDIR "/USB_FRONT/DATA"'
MMEM:LOAD:STAT 1,"MORNING"
```

Example: chapter 15.3.3.2, "Saving, Copying, and Loading Setup Data", on page 461

Usage: Setting only

15.2.16 General Instrument Setup

DISPlay:LANGuage....450
TRIGger:OUT:MODE....450
TRIGger:OUT:PLENgth....451
TRIGger:OUT:POLarity....451
SYSTem:NAME....451
SYSTem:DATE....451
SYSTem:TIME....451
SYSTem:BEEPer:CONTrol:STATe....452
SYSTem:BEEPer:ERRor:STATe....452
SYSTem:BEEPer:TRIG:STATe....452
SYSTem:BEEPer[:IMMediate]....452
SYSTem:SET....452
SYSTem:ERRor:[NEXT]?....453
SYSTem:ERRor:ALL?....453
SYST:PRESet....453

DISPlay:LANGuage <Language>

Sets the language in which the softkey labels, help and other screen information can be displayed.

Parameters:

<Language> ENGLish | GERMan | FRENch | SPANishRUSSian | SCHinese | TCHinese | JAPanese | ENGLish | GERMan | FRENch | SPANish | RUSSian | SCHinese | TCHinese | JAPanese | KOREan

Supported languages are listed in the "Specifications" data sheet.

*RST: Reset does not change the language

TRIGger:OUT:MODE <OutputMode>

Defines wether and when a trigger out pulse is generated: never, on trigger event, or on mask violation.

Parameters:

<OutputMode> OFF | TRIGger | MASK
*RST: OFF

TRIGger:OUT:PLENgth <PulseLength>

Defines the pulse width of the trigger out pulse.

Parameters:

<PulseLength> *RST: 1E-6
Default unit: s

TRIGger:OUT:POLarity <Polarity>

Sets the polarity of the trigger out pulse.

Parameters:

<Polarity> POSitive | NEGative
*RST: POS

SYSTem:NAME

Defines an instrument name.

Parameters:

<Name> String with max. 20 characters

SYSTem:DATE <Year>,<Month>,<Day>

Specifies the internal date for the instrument.

Parameters:

<Year> Increment: 1
Default unit: a

<Month> Range: 1 to 12
Increment: 1

<Day> Range: 1 to 31
Increment: 1
Default unit: d

Usage: SCPI confirmed

SYSTem:TIME <Hour>,<Minute>,<Second>

Specifies the internal time for the instrument.

Parameters:

<Hour>	Range:	0 to 23
	Increment:	1
	Default unit:	h
<Minute>	Range:	0 to 59
	Increment:	1
	Default unit:	min
<Second>	Range:	0 to 59
	Increment:	1
	Default unit:	s

Usage: SCPI confirmed

SYSTem:BEEPer:CONTrol:STATe

Enables or diables a sound for general control events, e.g. reaching the rotary encoder end or changing the measuring mode in the "Automeasure" menu.

Parameters:

<ControlBeep> ON | OFF

SYSTem:BEEPer:ERRor:STATe

Enables or disables the beep if an error occurs.

Parameters:

<ErrorBeep> ON | OFF

SYSTem:BEEPer:TRIG:STATe

Enables or disables the beep if a trigger occurs.

Parameters:

<TriggerBeep> ON | OFF

SYSTem:BEEPer[:IMMediate]

Generates an immediate beep.

Usage: Event

SYSTem:SET <Setup>

Defines or queries the device settings that can be saved and load manually with FILE > "Device Settings".

Parameters:

<Setup> 488.2 block data

Usage: SCPI confirmed

SYSTem:ERRor:[NEXT]?

Queries the error/event queue for the oldest item and removes it from the queue. The response consists of an error number and a short description of the error.

Positive error numbers are instrument-dependent. Negative error numbers are reserved by the SCPI standard.

Return values:

<Error> Error/event_number,"Error/event_description>[;Device-dependent info]"
If the queue is empty, the response is `0,"No error"`

Usage: Query only
SCPI confirmed

SYSTem:ERRor:ALL?

Queries the error/event queue for all unread items and removes them from the queue. The response is a comma separated list of error number and a short description of the error in FIFO order.

Positive error numbers are instrument-dependent. Negative error numbers are reserved by the SCPI standard.

Return values:

<Error> List of: Error/event_number,"Error/event_description>[;Device-dependent info]"
If the queue is empty, the response is `0,"No error"`

Usage: Query only
SCPI confirmed

SYST:PRESet

Resets the instrument to the default state, has the same effect as *RST.

Usage: Event

15.2.17 Status Reporting

15.2.17.1 STATus:OPERation Register

The commands of the `STATus:OPERation` subsystem control the status reporting structures of the STATus:OPERation register:

See also:

- chapter 15.1.6.1, "Structure of a SCPI Status Register", on page 262
- "STATus:OPERation Register" on page 267

The following commands are available:

STATus:OPERation:CONDition?....454
STATus:OPERation:ENABle....454
STATus:OPERation:NTRansition....454
STATus:OPERation:PTRansition....454
STATus:OPERation[:EVENt]?....454

STATus:OPERation:CONDition?

Returns the of the CONDition part of the operational status register.

Return values:

<Condition> Condition bits in decimal representation. ALIGnment (bit 0) , SELFtest (bit 1) , AUToset (bit 2), WTRigger (bit 3).

Range: 1 to 65535
Increment: 1

Usage: Query only

STATus:OPERation:ENABle <Enable>

Parameters:

<Enable> Range: 1 to 65535
Increment: 1

STATus:OPERation:NTRansition <NegativeTransition>

Parameters:

<NegativeTransition> Range: 1 to 65535
Increment: 1

STATus:OPERation:PTRansition <PositiveTransition>

Parameters:

<PositiveTransition> Range: 1 to 65535
Increment: 1

STATus:OPERation[:EVENt]?

Return values:

<Event> Range: 1 to 65535
Increment: 1

Usage: Query only

15.2.17.2 STATus:QUEStionable Registers

The commands of the `STATus:QUEStionable` subsystem control the status reporting structures of the STATus:QUEStionable registers:

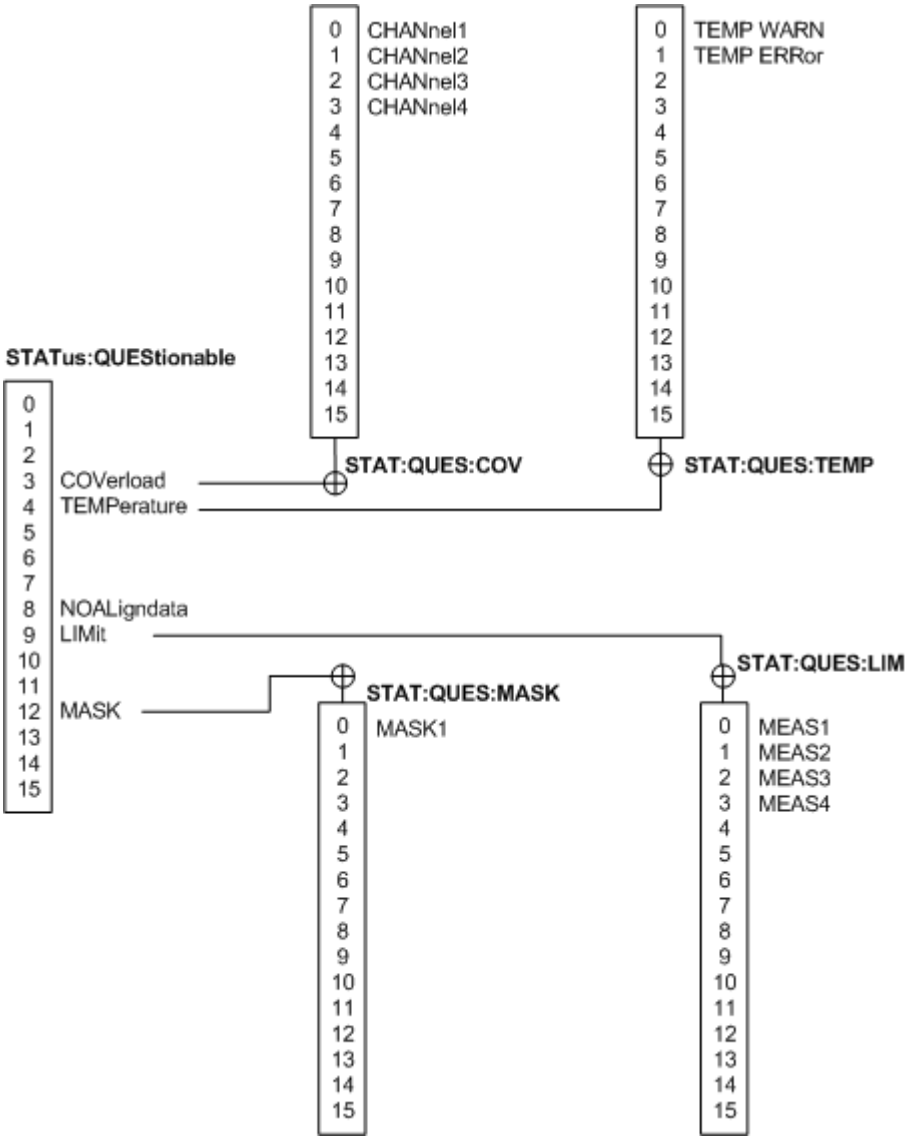

Fig. 15-4: Structure of the STATus:QUEStionable register

See also:

- chapter 15.1.6.1, "Structure of a SCPI Status Register", on page 262
- "STATus:QUEStionable Register" on page 267

The following commands are available:

STATus:PRESet....456
STATus:QUEStionable:CONDition?....456
STATus:QUEStionable:COVerload:CONDition?....456
STATus:QUEStionable:LIMit:CONDition?....456

STATus:QUEStionable:MASK:CONDition?....456
STATus:QUEStionable:ENABle....456
STATus:QUEStionable:COVerload:ENABle....456
STATus:QUEStionable:LIMit:ENABle....456
STATus:QUEStionable:MASK:ENABle....456
STATus:QUEStionable[:EVENt]?....457
STATus:QUEStionable:COVerload[:EVENt]?....457
STATus:QUEStionable:LIMit[:EVENt]?....457
STATus:QUEStionable:MASK[:EVENt]?....457
STATus:QUEStionable:NTRansition....457
STATus:QUEStionable:COVerload:NTRansition....457
STATus:QUEStionable:LIMit:NTRansition....457
STATus:QUEStionable:MASK:NTRansition....457
STATus:QUEStionable:PTRansition....457
STATus:QUEStionable:COVerload:PTRansition....457
STATus:QUEStionable:LIMit:PTRansition....457
STATus:QUEStionable:MASK:PTRansition....457

STATus:PRESet

Resets all STATUS:QUESTIONALBLE registers.

Usage: Event

STATus:QUEStionable:CONDition?
STATus:QUEStionable:COVerload:CONDition?
STATus:QUEStionable:LIMit:CONDition?
STATus:QUEStionable:MASK:CONDition?

Returns the contents of the CONDition part of the status register to check for questionable instrument or measurement states. Reading the CONDition registers does not delete the contents.

Return values:

<Condition> Condition bits in decimal representation
Range: 1 to 65535
Increment: 1

Usage: Query only

STATus:QUEStionable:ENABle <Enable>
STATus:QUEStionable:COVerload:ENABle <Enable>
STATus:QUEStionable:LIMit:ENABle <Enable>
STATus:QUEStionable:MASK:ENABle <Enable>

Sets the enable mask that allows true conditions in the EVENt part to be reported in the summary bit. If a bit is set to 1 in the enable part and its associated event bit transitions to true, a positive transition occurs in the summary bit and is reported to the next higher level.

Parameters:

<Enable> Bit mask in decimal representation

Range: 1 to 65535
Increment: 1

Example: `STATus:QUEStionable:MASK:ENABle 24`
Set bits no. 3 and 4 of the STATus:QUEStionable:MASK:ENABle register part: *24 = 8 + 16 = 2^3 + 2^4*

STATus:QUEStionable[:EVENt]?
STATus:QUEStionable:COVerload[:EVENt]?
STATus:QUEStionable:LIMit[:EVENt]?
STATus:QUEStionable:MASK[:EVENt]?

Returns the contents of the EVENt part of the status register to check whether an event has occurred since the last reading. Reading an EVENt register deletes its contents.

Return values:

<Event> Event bits in decimal representation

Range: 1 to 65535
Increment: 1

Usage: Query only

STATus:QUEStionable:NTRansition <NegativeTransition>
STATus:QUEStionable:COVerload:NTRansition <NegativeTransition>
STATus:QUEStionable:LIMit:NTRansition <NegativeTransition>
STATus:QUEStionable:MASK:NTRansition <NegativeTransition>

Sets the negative transition filter. If a bit is set, a 1 to 0 transition in the corresponding bit of the condition register causes a 1 to be written in the corresponding bit of the event register.

Parameters:

<NegativeTransition> Bit mask in decimal representation

Range: 1 to 65535
Increment: 1

Example: `STATus:QUEStionable:MASK:NTRansition 24`
Set bits no. 3 and 4 of the STATus:QUEStionable:MASK:NTRansition register part: *24 = 8 + 16 = 2^3 + 2^4*

STATus:QUEStionable:PTRansition <PositiveTransition>
STATus:QUEStionable:COVerload:PTRansition <PositiveTransition>
STATus:QUEStionable:LIMit:PTRansition <PositiveTransition>
STATus:QUEStionable:MASK:PTRansition <PositiveTransition>

Sets the positive transition filter. If a bit is set, a 0 to 1 transition in the corresponding bit of the condition register causes a 1 to be written in the corresponding bit of the event register.

Parameters:

<PositiveTransition> Bit mask in decimal representation

Range: 1 to 65535
Increment: 1

Example: `STATus:QUEStionable:MASK:PTRansition 24`
Set bits no. 3 and 4 of the STATus:QUEStionable:MASK:PTRansition register part: *24 = 8 + 16 = 2^3 + 2^4*

15.3 Programming Examples

15.3.1 Data Export

15.3.1.1 Reading Waveform Data from Memory

Set data format and sample range, read channel header and data.

Command description in chapter 15.2.3, "General Remote Settings and Queries", on page 277 and chapter 15.2.4.5, "Waveform Data", on page 293.

```
* Connected to: TCPIP0::192.168.1.1::inst0::INSTR
SYST:ERR?
<-- 0,"No error"
*IDN?
<-- Rohde&Schwarz,RTM1052,1305.0008K52/101489,04.502

*RST
CHAN:TYPE HRES              // Set high resolution mode (16 bit data)
ACQ:WRAT MSAM               // Set maximum waveform rate
TIM:SCAL 1E-7               // Set time base
FORM REAL                   // Set REAL data format
FORM:BORD LSBF              // Set little endian byte order
CHAN:DATA:POIN DMAX         // Set sample range to memory data in displayed time range
SING;*OPC?                  // Start single acquisition
<--  1
CHAN:DATA:HEAD?             // Read header
<--  -4.9980E-07,5.0000E-07,5000,1    // Xstart, Xstop, record length in samples
CHAN:DATA?                  // Read channel data
<--  #520000>??[>??[>??[>??[>??[>??...   // Binary block data,
                                         // 4-byte floating point number/sample
```

15.3.1.2 Reading Waveform Data in Unsigned Integer Format

Read the channel header, the waveform conversion data, set the UINT binary data format and read the channel data.

Command description in: chapter 15.2.3, "General Remote Settings and Queries", on page 277.

```
*RST
TIM:SCAL 1E-7
CHAN:DATA:POIN DMAX       // Set data range
SING;*OPC?
<--  1
CHAN:DATA:HEAD?           // Read header
<--  -4.9980E-07,5.0000E-07,5000,1    // Xstart, Xstop, record length in samples
CHAN:DATA:YRES?           // Read vertical resolution
<--  8
CHAN:DATA:YOR?            // Read voltage value for binary value 0
<--  -2.549999943E-2
CHAN:DATA:XOR?            // Read time of the first sample
<--  -4.998000058E-7
CHAN:DATA:XINC?           // Read time between two adjacent samples
<--  2.000000023E-10
FORM UINT,8;FORM?         // Set data format to unsigned integer, 8 bit
<--  UINT,8
CHAN:DATA:YINC?           // Read voltage value per bit
<--  1.999999949E-4
CHAN:DATA?                // Read channel data
<--  128,125,120...       // 5000 bytes total
FORM UINT,16;FORM?        // Change data format to unsigned integer, 16 bit
<--  UINT,16
CHAN:DATA:YINC?           // Read voltage value per bit
<--  7.812499803E-7
CHAN:DATA?                // Read channel data
<--  32768,32000,30720... // 10000 bytes total
```

Note the following correlations:

- The number of received data values matches the number of samples indicated in the header.
- The time of the first sample (XORigin) matches the start time Xstart indicated in the header.
- The Y-increment adjusts to the data length defined in the data format (8 or 16 bit).

Data conversion

Definition: the sample numbers start with *0* and end with *record length - 1*.

Sample time

$t_n = n * xIncrement + xOrigin$

First sample: $t_0 = -4.998000058E-7$ (= Xstart)

Last sample: $t_{4999} = 4999 * 2E^{-10} - 4.998E^{-7} = 5.0\ E^{-7}$ (= Xstop)

Sample value

$Y_n = yOrigin + (yIncrement * byteValue_n)$

The format `UINT,8` has the data range 0 to 255. The voltage value for byte value 128 is:

$Y_n = -2.55E^{-2} + (2E^{-4} * 128) = 0.0001$

The center of the display at position 0 div always has the byte value 127.5. The corresponding voltage value is:

$Y_n = -2.55E^{-2} + (2E^{-4} * 127.5) = 0$

8-bit and 16-bit data

At the end of the above example, the 8-bit waveform is read as 16-bit data, for example, *0xFF* is read *0xFF00*, or *0x1A* is read *0x1A00*. The *yOrigin* value is the same in both cases, but the *yIncrement* differs.

	8-bit data	16-bit data	Result
$yIncrement * byteValue_n$	$2e^{-4} * 128$	$7{,}8125E^{-7} * 32768$	0,0256 V
	$2e^{-4} * 125$	$7{,}8125E^{-7} * 32000$	0,025 V

In the reverse case, if a 16-bit waveform is read with 8-bit data format, data precision may be reduced. Data values ar truncated, and only the more significiant bits remain. For example, the 16-bit data *0xabcd* is read *0xab* in 8-bit format, and *cd* is lost.

15.3.2 Search

15.3.2.1 Searching for a Pulse of Specified Width

Search for positive pulses with pulse width 12 ± 10 µs (2 µs to 22 µs).

Command description in: chapter 15.2.12, "Search", on page 358.

```
SEAR:STAT ON                // Turn on search
SEAR:COND WIDTH             // Select search condition
SEAR:SOUR CH2               // Configure search source
SEAR:TRIG:WIDT:POL POS      // Configure search parameters: Polarity
SEAR:TRIG:WIDT:RANG WITH    // Configure search parameters: Condition = within
SEAR:TRIG:WIDT:WIDT 12e-6   // Configure search parameters: Pulse width
SEAR:TRIG:WIDT:DELT 10e-6   // Configure search parameters: +/- delta
SEAR:RESD:SHOW ON           // Show result table
SEAR:RCO?                   // Get number of search events found
<--  1.400E+01
SEAR:RES:ALL?               // Get all search results
<--  1,5.201200e-06,0,WIDTH,POSITIVE,1.220160e-05,2,4.120040e-05,0,WIDTH,
POSITIVE,3.076800e-06,3,4.732480e-05,0,WIDTH,POSITIVE,9.127200e-06,4,
6.499960e-05,0,WIDTH,POSITIVE,1.835160e-05,5,8.634920e-05,0,WIDTH,POSITIVE,
```

```
3.052000e-06,6,1.293984e-04,0,WIDTH,POSITIVE,9.176800e-06,7,1.477228e-04,0,
WIDTH,POSITIVE,3.052000e-06,8,1.623224e-04,0,WIDTH,POSITIVE,3.102000e-06,9,
1.684724e-04,0,WIDTH,POSITIVE,1.215160e-05,10,1.953216e-04,0,WIDTH,POSITIVE,
3.027200e-06,11,2.044716e-04,0,WIDTH,POSITIVE,6.052000e-06,12,2.252212e-04,0,
WIDTH,POSITIVE,3.052000e-06,13,2.435456e-04,0,WIDTH,POSITIVE,3.027200e-06,14,
2.496456e-04,0,WIDTH,POSITIVE,6.702000e-06
```

15.3.3 Data and File Management

15.3.3.1 Saving Screenshots to File

Save two display images in png format to the `PIX` folder on a USB flash drive that is connected to the front panel. One screenshot is colored and the other is grayscaled. Finally, the data of the gray screenshot is read for further user on the control computer.

Command description in: chapter 15.2.15.1, "Screenshots", on page 441.

```
*RST
MMEM:CDIR "/USB_FRONT"
MMEM:MDIR "/USB_FRONT/PIX"
MMEM:CDIR "/USB_FRONT/PIX/"

HCOP:DEST "MMEM"
HCOP:LANG PNG
HCOP:COL:SCH COL
MMEM:NAME "COLORED"
HCOP:IMM
HCOP:COL:SCH GRAY
MMEM:NAME "GRAY"
HCOP:IMM

MMEM:CAT? "*.PNG"
MMEM:DATA? "GRAY.PNG"
```

15.3.3.2 Saving, Copying, and Loading Setup Data

Save instrument settings to a file on internal storage device, duplicate this file and save it to a USB stick attached to the front panel. Finally, there are three setup files on the internal storage `/INT/SETTINGS`, and one file on the USB flash device.

Command description in: chapter 15.2.15.2, "Saving and Loading Data: MMEMory Commands", on page 443.

```
CHAN1:STAT ON                       // Turn channel 1 on
CHAN2:STAT ON                       // Turn channel 2 on
TIM:ZOOM:STAT ON                    // Show zoom diagram
MMEM:CDIR "/INT/SETTINGS"           // Set storage device and directory
MMEM:STOR:STAT 1,"ZOOM_A.SET"       // Save settings to internal storage
MMEM:CAT? "*.SET"                   // Check
```

```
<--  332112,8633856,"ZOOM_A.SET,,2759"
MMEM:COPY "ZOOM_A.SET","ZOOM_B.SET" // Copy file
MMEM:CAT? "*.SET"                   // Check
<--  332112,8633856,"ZOOM_A.SET,,2759","ZOOM_B.SET,,2759"
MMEM:COPY "/INT/SETTINGS/ZOOM_B.SET","/USB_FRONT/ZOOM_B.SET"
                                    // Save copied file to USB stick
MMEM:CDIR "/USB_FRONT"              // Check
MMEM:CAT? "*.SET"
<--  4890624,-641765376,"ZOOM_B.SET,,2759"
MMEM:COPY "/USB_FRONT/ZOOM_B.SET","/USB_FRONT/ZOOM_USB.SET"
                                    // Duplicate file on USB stick
MMEM:CAT? "*.SET"                   // Check
<--  4890624,-641765376,"ZOOM_B.SET,,2759","ZOOM_USB.SET,,2759"
MMEM:DEL "ZOOM_B.SET"               // Delete original file
MMEM:CAT? "*.SET"                   // Check
<--  4886528,-641765376,"ZOOM_USB.SET,,2759"
MMEM:COPY "/USB_FRONT/ZOOM_USB.SET","/INT/SETTINGS/"
                                    // Copy new file to the instrument
MMEM:CDIR "/INT/SETTINGS"           // Check
MMEM:CAT? "*.SET"
<--  332112,8633856,"ZOOM_A.SET,,2759","ZOOM_B.SET,,2759","ZOOM_USB.SET,,2759"
*RST;*OPC?
<--  1
MMEM:CDIR "/INT/SETTINGS"
MMEM:LOAD:STAT 1,"ZOOM_USB.SET"     // Load settings
```

List of Commands

*CAL?....274
*CLS....274
*ESE....275
*ESR?....275
*IDN?....275
*OPC....275
*OPT?....275
*PSC....276
*RST....276
*SRE....276
*STB?....276
*TRG....276
*TST?....277
*WAI....277
ACQuire:AVERage:COUNt....285
ACQuire:FILTer:FREQuency....287
ACQuire:INTerpolate....285
ACQuire:MODE....285
ACQuire:NSINgle:COUNt....282
ACQuire:POINts:ARATe?....288
ACQuire:SRATe?....288
ACQuire:WRATe....286
AUToscale....284
BUS<b>:CAN:BITRate....407
BUS<b>:CAN:DATA:SOURce....406
BUS<b>:CAN:FCOunt?....411
BUS<b>:CAN:FRAMe<n>:ACKState?....413
BUS<b>:CAN:FRAMe<n>:ACKValue?....414
BUS<b>:CAN:FRAMe<n>:BCOunt?....416
BUS<b>:CAN:FRAMe<n>:BSEPosition?....416
BUS<b>:CAN:FRAMe<n>:BYTE<o>:STATe?....417
BUS<b>:CAN:FRAMe<n>:BYTE<o>:VALue?....417
BUS<b>:CAN:FRAMe<n>:CSSTate?....414
BUS<b>:CAN:FRAMe<n>:CSValue?....414
BUS<b>:CAN:FRAMe<n>:DATA?....413
BUS<b>:CAN:FRAMe<n>:DLCState?....414
BUS<b>:CAN:FRAMe<n>:DLCValue?....415
BUS<b>:CAN:FRAMe<n>:IDSTate?....415
BUS<b>:CAN:FRAMe<n>:IDTYpe?....415
BUS<b>:CAN:FRAMe<n>:IDValue?....416
BUS<b>:CAN:FRAMe<n>:STARt?....412
BUS<b>:CAN:FRAMe<n>:STATus?....412
BUS<b>:CAN:FRAMe<n>:STOP?....413
BUS<b>:CAN:FRAMe<n>:TYPE?....411
BUS<b>:CAN:SAMPlepoint....406

BUS<b>:CAN:TYPE....406
BUS<b>:CPARallel:CLOCK:SLOPe....438
BUS<b>:CPARallel:CS:POLarity....438
BUS<b>:CPARallel:FCOunt?....439
BUS<b>:CPARallel:FRAMe<n>:DATA?....439
BUS<b>:CPARallel:FRAMe<n>:STARt?....440
BUS<b>:CPARallel:FRAMe<n>:STATe?....440
BUS<b>:CPARallel:FRAMe<n>:STOP?....440
BUS<b>:CPARallel:WIDTh....438
BUS<b>:DSIGnals....375
BUS<b>:DSIZe....375
BUS<b>:FORMat....375
BUS<b>:I2C:CLOCk:SOURce....389
BUS<b>:I2C:DATA:SOURce....389
BUS<b>:I2C:FCOunt?....392
BUS<b>:I2C:FRAMe<n>:AACCess?....394
BUS<b>:I2C:FRAMe<n>:ACCess?....394
BUS<b>:I2C:FRAMe<n>:ACOMplete?....395
BUS<b>:I2C:FRAMe<n>:ADBStart?....395
BUS<b>:I2C:FRAMe<n>:ADDRess?....395
BUS<b>:I2C:FRAMe<n>:ADEVice?....396
BUS<b>:I2C:FRAMe<n>:AMODe?....396
BUS<b>:I2C:FRAMe<n>:ASTart?....396
BUS<b>:I2C:FRAMe<n>:BCOunt?....397
BUS<b>:I2C:FRAMe<n>:BYTE<o>:ACCess?....397
BUS<b>:I2C:FRAMe<n>:BYTE<o>:ACKStart?....397
BUS<b>:I2C:FRAMe<n>:BYTE<o>:COMPlete?....398
BUS<b>:I2C:FRAMe<n>:BYTE<o>:STARt?....398
BUS<b>:I2C:FRAMe<n>:BYTE<o>:VALue?....398
BUS<b>:I2C:FRAMe<n>:DATA?....392
BUS<b>:I2C:FRAMe<n>:STARt?....393
BUS<b>:I2C:FRAMe<n>:STATus?....393
BUS<b>:I2C:FRAMe<n>:STOP?....394
BUS<b>:LIN:BITRate....423
BUS<b>:LIN:DATA:SOURce....422
BUS<b>:LIN:FCOunt?....426
BUS<b>:LIN:FRAMe<n>:BCOunt?....430
BUS<b>:LIN:FRAMe<n>:BYTE<o>:STATe?....431
BUS<b>:LIN:FRAMe<n>:BYTE<o>:VALue?....431
BUS<b>:LIN:FRAMe<n>:CSSTate?....428
BUS<b>:LIN:FRAMe<n>:CSValue?....428
BUS<b>:LIN:FRAMe<n>:DATA?....426
BUS<b>:LIN:FRAMe<n>:IDPValue?....428
BUS<b>:LIN:FRAMe<n>:IDSTate?....429
BUS<b>:LIN:FRAMe<n>:IDValue?....429
BUS<b>:LIN:FRAMe<n>:STARt?....427
BUS<b>:LIN:FRAMe<n>:STATus?....427
BUS<b>:LIN:FRAMe<n>:STOP?....427

BUS<b>:LIN:FRAMe<n>:SYSTate?....429
BUS<b>:LIN:FRAMe<n>:SYValue?....430
BUS<b>:LIN:FRAMe<n>:VERSion?....430
BUS<b>:LIN:POLarity....422
BUS<b>:LIN:STANdard....422
BUS<b>:LIST:SAVE....376
BUS<b>:LIST?....376
BUS<b>:PARallel:FCOunt?....439
BUS<b>:PARallel:FRAMe<n>:DATA?....439
BUS<b>:PARallel:FRAMe<n>:STARt?....440
BUS<b>:PARallel:FRAMe<n>:STATe?....440
BUS<b>:PARallel:FRAMe<n>:STOP?....440
BUS<b>:PARallel:WIDTh....437
BUS<b>:POSition....376
BUS<b>:RESult....376
BUS<b>:SPI:BORDer....379
BUS<b>:SPI:CLOCk:POLarity....378
BUS<b>:SPI:CLOCk:SOURce....378
BUS<b>:SPI:CS:POLarity....377
BUS<b>:SPI:CS:SOURce....377
BUS<b>:SPI:DATA:POLarity....379
BUS<b>:SPI:DATA:SOURce....378
BUS<b>:SPI:FCOunt?....381
BUS<b>:SPI:FRAME<n>:DATA:MISO?....383
BUS<b>:SPI:FRAME<n>:DATA:MOSI?....383
BUS<b>:SPI:FRAME<n>:STARt?....382
BUS<b>:SPI:FRAME<n>:STATus?....382
BUS<b>:SPI:FRAME<n>:STOP?....382
BUS<b>:SPI:FRAME<n>:WCOunt?....383
BUS<b>:SPI:FRAME<n>:WORD<o>:MISO?....385
BUS<b>:SPI:FRAME<n>:WORD<o>:MOSI?....385
BUS<b>:SPI:FRAME<n>:WORD<o>:STARt?....384
BUS<b>:SPI:FRAME<n>:WORD<o>:STOP?....384
BUS<b>:SPI:SSIZe....379
BUS<b>:SSPI:BITime....387
BUS<b>:SSPI:BORDer....387
BUS<b>:SSPI:CLOCk:POLarity....386
BUS<b>:SSPI:CLOCk:SOURce....386
BUS<b>:SSPI:DATA:POLarity....387
BUS<b>:SSPI:DATA:SOURce....386
BUS<b>:SSPI:SSIZe....388
BUS<b>:STATe....374
BUS<b>:TYPE....375
BUS<b>:UART:BAUDrate....401
BUS<b>:UART:BITime....402
BUS<b>:UART:DATA:POLarity....400
BUS<b>:UART:DATA:SOURce....399
BUS<b>:UART:PARity....401

BUS<b>:UART:POLarity....400
BUS<b>:UART:RX:FCOunt?....404
BUS<b>:UART:RX:FRAMe<n>:WCOunt?....404
BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STARt?....405
BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STATe?....404
BUS<b>:UART:RX:FRAMe<n>:WORD<o>:STOP?....405
BUS<b>:UART:RX:FRAMe<n>:WORD<o>:VALue?....405
BUS<b>:UART:SBIT....401
BUS<b>:UART:SSIZe....400
CALCulate:MATH<m>:ARIThmetics....349
CALCulate:MATH<m>:DATA:HEADer?....348
CALCulate:MATH<m>:DATA:XINCrement?....280
CALCulate:MATH<m>:DATA:XORigin?....279
CALCulate:MATH<m>:DATA:YINCrement?....280
CALCulate:MATH<m>:DATA:YORigin?....280
CALCulate:MATH<m>:DATA:YRESolution?....281
CALCulate:MATH<m>:DATA?....347
CALCulate:MATH<m>:FFT:AVERage:COUNt....350
CALCulate:MATH<m>:FFT:BANDwidth[:RESolution]:ADJusted?....351
CALCulate:MATH<m>:FFT:BANDwidth[:RESolution]:AUTO....351
CALCulate:MATH<m>:FFT:BANDwidth[:RESolution]:RATio....351
CALCulate:MATH<m>:FFT:BANDwidth[:RESolution][:VALue]....352
CALCulate:MATH<m>:FFT:CFRequency....352
CALCulate:MATH<m>:FFT:FULLspan....352
CALCulate:MATH<m>:FFT:MAGNitude:SCALe....350
CALCulate:MATH<m>:FFT:SPAN....352
CALCulate:MATH<m>:FFT:SRATe?....354
CALCulate:MATH<m>:FFT:STARt....353
CALCulate:MATH<m>:FFT:STOP....353
CALCulate:MATH<m>:FFT:TIME:POSition....354
CALCulate:MATH<m>:FFT:TIME:RANGe....353
CALCulate:MATH<m>:FFT:WINDow:TYPE....349
CALCulate:MATH<m>:POSition....346
CALCulate:MATH<m>:SCALe....346
CALCulate:MATH<m>:STATe....345
CALCulate:MATH<m>[:EXPRession][:DEFine]....346
CHANnel<m>:ARIThmetics....287
CHANnel<m>:BANDwidth....290
CHANnel<m>:COUPling....289
CHANnel<m>:DATA:ENVelope:HEADer?....294
CHANnel<m>:DATA:ENVelope:XINCrement?....280
CHANnel<m>:DATA:ENVelope:XORigin?....279
CHANnel<m>:DATA:ENVelope:YINCrement?....280
CHANnel<m>:DATA:ENVelope:YORigin?....280
CHANnel<m>:DATA:ENVelope:YRESolution?....281
CHANnel<m>:DATA:ENVelope?....294
CHANnel<m>:DATA:HEADer?....294
CHANnel<m>:DATA:POINts....295

CHANnel<m>:DATA:XINCrement?....280
CHANnel<m>:DATA:XORigin?....279
CHANnel<m>:DATA:YINCrement?....280
CHANnel<m>:DATA:YORigin?....280
CHANnel<m>:DATA:YRESolution?....281
CHANnel<m>:DATA?....293
CHANnel<m>:LABel....292
CHANnel<m>:LABel:STATe....292
CHANnel<m>:OFFSet....290
CHANnel<m>:OVERload....291
CHANnel<m>:POLarity....291
CHANnel<m>:POSition....290
CHANnel<m>:RANGe....289
CHANnel<m>:SCALe....289
CHANnel<m>:SKEW....291
CHANnel<m>:STATe....288
CHANnel<m>:THReshold....292
CHANnel<m>:THReshold:FINDlevel....379
CHANnel<m>:THReshold:FINDlevel....388
CHANnel<m>:THReshold:FINDlevel....389
CHANnel<m>:THReshold:FINDlevel....402
CHANnel<m>:THReshold:FINDlevel....407
CHANnel<m>:THReshold:FINDlevel....423
CHANnel<m>:TYPE....286
CURSor<m>:AOFF....327
CURSor<m>:FUNCtion....328
CURSor<m>:RESult?....332
CURSor<m>:SNPeak....331
CURSor<m>:SOURce....327
CURSor<m>:SPPeak....331
CURSor<m>:SSCReen....331
CURSor<m>:STATe....327
CURSor<m>:SWAVe....331
CURSor<m>:TRACking:SCALe[:STATe]....331
CURSor<m>:TRACking[:STATe]....330
CURSor<m>:X1Position....330
CURSor<m>:X2Position....330
CURSor<m>:X3Position....330
CURSor<m>:XCOupling....330
CURSor<m>:XDELta:INVerse?....332
CURSor<m>:XDELta[:VALue]?....332
CURSor<m>:XRATio[:VALue]?....333
CURSor<m>:Y1Position....330
CURSor<m>:Y2Position....330
CURSor<m>:Y3Position....330
CURSor<m>:YCOupling....330
CURSor<m>:YDELta:SLOPe?....333
CURSor<m>:YDELta[:VALue]?....333

CURSor<m>:YRATio:UNIT....334
CURSor<m>:YRATio[:VALue]?....334
CURsor<m>:XRATio:UNIT....333
DIGital<m>:DISPlay....435
DIGital<m>:Hysteresis....436
DIGital<m>:LABel....436
DIGital<m>:LABel:STATe....437
DIGital<m>:POSition....436
DIGital<m>:SIZE....437
DIGital<m>:TECHnology....435
DIGital<m>:THCoupling....436
DIGital<m>:THReshold....435
DISPlay:GRID:STYLe....319
DISPlay:INTensity:BACKlight....317
DISPlay:INTensity:GRID....317
DISPlay:INTensity:WAVeform....317
DISPlay:LANGuage....450
DISPlay:MODE....314
DISPlay:PALette....314
DISPlay:PERSistence:CLEar....319
DISPlay:PERSistence:INFinite....318
DISPlay:PERSistence:STATe....318
DISPlay:PERSistence:TIME....318
DISPlay:PERSistence:TIME:AUTO....318
DISPlay:STYLe....319
DISPlay:VSCReen:ENABle....319
DISPlay:VSCReen:POSition....320
DISPlay:XY:XSOurce....315
DISPlay:XY:Y1Source....315
DISPlay:XY:Y2Source....316
DISPlay:XY:ZMODe....316
DISPlay:XY:ZSOurce....316
DISPlay:XY:ZTHReshold....316
FORMat:BORDer....279
FORMat[:DATA]....278
HCOPy:COLor:SCHeme....442
HCOPy:DESTination....441
HCOPy:LANGuage....442
HCOPy:PAGE:ORIentation....442
HCOPy:PAGE:SIZE....442
HCOPy[:IMMediate]....442
MASK:ACTion:PRINt:EVENt:COUNt....358
MASK:ACTion:PRINt:EVENt:MODE....357
MASK:ACTion:SCRSave:EVENt:COUNt....358
MASK:ACTion:SCRSave:EVENt:MODE....357
MASK:ACTion:SOUNd:EVENt:COUNt....358
MASK:ACTion:SOUNd:EVENt:MODE....357
MASK:ACTion:STOP:EVENt:COUNt....358

MASK:ACTion:STOP:EVENt:MODE....357
MASK:ACTion:WFMSave:EVENt:COUNt....358
MASK:ACTion:WFMSave:EVENt:MODE....357
MASK:CHCopy....355
MASK:COUNt?....357
MASK:LOAD....355
MASK:RESet:COUNter....357
MASK:SAVE....355
MASK:SOURce....355
MASK:STATe....355
MASK:TEST....355
MASK:VCOunt?....357
MASK:XWIDth....356
MASK:YPOSition....356
MASK:YSCale....356
MASK:YWIDth....356
MEASurement<m>:ALL[:STATe]....335
MEASurement<m>:AOFF....335
MEASurement<m>:AON....335
MEASurement<m>:ARESult?....335
MEASurement<m>:CATegory?....340
MEASurement<m>:DELay:SLOPe....339
MEASurement<m>:MAIN....336
MEASurement<m>:RESult:AVG?....343
MEASurement<m>:RESult:NPEak?....344
MEASurement<m>:RESult:PPEak?....344
MEASurement<m>:RESult:STDDev?....343
MEASurement<m>:RESult:WFMCount?....344
MEASurement<m>:RESult[:ACTual]?....340
MEASurement<m>:SOURce....338
MEASurement<m>:STATistics:RESet....343
MEASurement<m>:STATistics:VALue:ALL?....344
MEASurement<m>:STATistics:VALue<n>?....345
MEASurement<m>:STATistics:WEIGht....342
MEASurement<m>:STATistics[:ENABle]....342
MEASurement<m>[:ENABle]....336
MMEMory:CATalog:LENGth?....447
MMEMory:CATalog?....447
MMEMory:CDIRectory....445
MMEMory:COPY....448
MMEMory:DATA....449
MMEMory:DCATalog:LENGth?....446
MMEMory:DCATalog?....446
MMEMory:DELete....448
MMEMory:DRIVes?....444
MMEMory:LOAD:STATe....449
MMEMory:MDIRectory....445
MMEMory:MOVE....448

MMEMory:MSIS....444
MMEMory:NAME....441
MMEMory:RDIRectory....445
MMEMory:STORe:STATe....449
PROBe<m>:ID:BUILd?....300
PROBe<m>:ID:PARTnumber?....300
PROBe<m>:ID:PRDate?....301
PROBe<m>:ID:SRNumber?....301
PROBe<m>:ID:SWVersion?....301
PROBe<m>:SETup:ATTenuation:MANual....297
PROBe<m>:SETup:ATTenuation:UNIT....297
PROBe<m>:SETup:ATTenuation[:AUTO]?....297
PROBe<m>:SETup:BANDwidth?....297
PROBe<m>:SETup:CAPacitance?....298
PROBe<m>:SETup:DCOFfset?....298
PROBe<m>:SETup:IMPedance?....298
PROBe<m>:SETup:MODE....299
PROBe<m>:SETup:NAME?....299
PROBe<m>:SETup:OFFSwitch....299
PROBe<m>:SETup:TYPE?....299
PROBe<m>:SETup:UOFFset....300
REFCurve<m>:DATA:HEADer?....325
REFCurve<m>:DATA:XINCrement?....280
REFCurve<m>:DATA:XORigin?....279
REFCurve<m>:DATA:YINCrement?....280
REFCurve<m>:DATA:YORigin?....280
REFCurve<m>:DATA:YRESolution?....281
REFCurve<m>:DATA?....325
REFCurve<m>:HORizontal:POSition....324
REFCurve<m>:HORizontal:SCALe....324
REFCurve<m>:LOAD....324
REFCurve<m>:LOAD:STATe....324
REFCurve<m>:SAVE....323
REFCurve<m>:SOURce....322
REFCurve<m>:SOURce:CATalog?....323
REFCurve<m>:STATe....322
REFCurve<m>:UPDate....323
REFCurve<m>:VERTical:POSition....325
REFCurve<m>:VERTical:SCALe....325
REFLevel:RELative:LOWer....341
REFLevel:RELative:MIDDle....342
REFLevel:RELative:MODE....341
REFLevel:RELative:UPPer....341
RUN....281
RUNContinous....282
RUNSingle....282
SEARch:CONDition....359
SEARch:GATE:ABSolute:START....361

SEARch:GATE:ABSolute:STOP....361
SEARch:GATE:MODE....361
SEARch:MEASure:LEVel:PEAK:MAGNitude....364
SEARch:MEASure:PEAK:POLarity....364
SEARch:PROTocol:CAN:ACKerror....419
SEARch:PROTocol:CAN:BITSterror....419
SEARch:PROTocol:CAN:CONDition....418
SEARch:PROTocol:CAN:CRCerror....419
SEARch:PROTocol:CAN:DATA....421
SEARch:PROTocol:CAN:DCONdition....421
SEARch:PROTocol:CAN:DLENgth....421
SEARch:PROTocol:CAN:FORMerror....420
SEARch:PROTocol:CAN:FRAMe....418
SEARch:PROTocol:CAN:FTYPe....420
SEARch:PROTocol:CAN:ICONdition....420
SEARch:PROTocol:CAN:IDENtifier....420
SEARch:PROTocol:CAN:ITYPe....420
SEARch:PROTocol:LIN:CHKSerror....433
SEARch:PROTocol:LIN:CONDition....432
SEARch:PROTocol:LIN:DATA....434
SEARch:PROTocol:LIN:DCONdition....434
SEARch:PROTocol:LIN:DLENgth....434
SEARch:PROTocol:LIN:FRAMe....432
SEARch:PROTocol:LIN:ICONdition....433
SEARch:PROTocol:LIN:IDENtifier....433
SEARch:PROTocol:LIN:IPERror....433
SEARch:PROTocol:LIN:SYERror....433
SEARch:RCOunt?....374
SEARch:RESDiagram:SHOW....372
SEARch:RESult:ALL?....373
SEARch:RESult<n>?....373
SEARch:SOURce....361
SEARch:STATe....359
SEARch:TRIGger:DATatoclock:CEDGe....369
SEARch:TRIGger:DATatoclock:CLEVel....369
SEARch:TRIGger:DATatoclock:CLEVel:DELTa....369
SEARch:TRIGger:DATatoclock:CSOurce....368
SEARch:TRIGger:DATatoclock:DLEVel....369
SEARch:TRIGger:DATatoclock:DLEVel:DELTa....369
SEARch:TRIGger:DATatoclock:HTIMe....369
SEARch:TRIGger:DATatoclock:STIMe....370
SEARch:TRIGger:EDGE:LEVel....362
SEARch:TRIGger:EDGE:LEVel:DELTa....362
SEARch:TRIGger:EDGE:SLOPe....362
SEARch:TRIGger:LEVel:RISetime:LOWer....365
SEARch:TRIGger:LEVel:RISetime:UPPer....365
SEARch:TRIGger:LEVel:RUNT:LOWer....367
SEARch:TRIGger:LEVel:RUNT:UPPer....367

SEARch:TRIGger:PATTern:FUNCtion....370
SEARch:TRIGger:PATTern:LEVel<n>....371
SEARch:TRIGger:PATTern:LEVel<n>:DELTa....371
SEARch:TRIGger:PATTern:SOURce....370
SEARch:TRIGger:PATTern:WIDTh:DELTa....372
SEARch:TRIGger:PATTern:WIDTh:RANGe....371
SEARch:TRIGger:PATTern:WIDTh[:WIDTh]....372
SEARch:TRIGger:RISetime:DELTa....366
SEARch:TRIGger:RISetime:RANGe....365
SEARch:TRIGger:RISetime:SLOPe....365
SEARch:TRIGger:RISetime:TIME....366
SEARch:TRIGger:RUNT:DELTa....368
SEARch:TRIGger:RUNT:POLarity....367
SEARch:TRIGger:RUNT:RANGe....367
SEARch:TRIGger:RUNT:WIDTh....368
SEARch:TRIGger:WIDTh:DELTa....364
SEARch:TRIGger:WIDTh:LEVel....363
SEARch:TRIGger:WIDTh:LEVel:DELTa....363
SEARch:TRIGger:WIDTh:POLarity....362
SEARch:TRIGger:WIDTh:RANGe....363
SEARch:TRIGger:WIDTh:WIDTh....364
SINGle....282
STATus:OPERation:CONDition?....454
STATus:OPERation:ENABle....454
STATus:OPERation:NTRansition....454
STATus:OPERation:PTRansition....454
STATus:OPERation[:EVENt]?....454
STATus:PRESet....456
STATus:QUEStionable:CONDition?....456
STATus:QUEStionable:COVerload:CONDition?....456
STATus:QUEStionable:COVerload:ENABle....456
STATus:QUEStionable:COVerload:NTRansition....457
STATus:QUEStionable:COVerload:PTRansition....457
STATus:QUEStionable:COVerload[:EVENt]?....457
STATus:QUEStionable:ENABle....456
STATus:QUEStionable:LIMit:CONDition?....456
STATus:QUEStionable:LIMit:ENABle....456
STATus:QUEStionable:LIMit:NTRansition....457
STATus:QUEStionable:LIMit:PTRansition....457
STATus:QUEStionable:LIMit[:EVENt]?....457
STATus:QUEStionable:MASK:CONDition?....456
STATus:QUEStionable:MASK:ENABle....456
STATus:QUEStionable:MASK:NTRansition....457
STATus:QUEStionable:MASK:PTRansition....457
STATus:QUEStionable:MASK[:EVENt]?....457
STATus:QUEStionable:NTRansition....457
STATus:QUEStionable:PTRansition....457
STATus:QUEStionable[:EVENt]?....457

STOP....282
SYST:PRESet....453
SYSTem:BEEPer:CONTrol:STATe....452
SYSTem:BEEPer:ERRor:STATe....452
SYSTem:BEEPer:TRIG:STATe....452
SYSTem:BEEPer[:IMMediate]....452
SYSTem:COMMunicate:PRINter:ENUMerate:FIRSt?....443
SYSTem:COMMunicate:PRINter:ENUMerate[:NEXT]?....443
SYSTem:COMMunicate:PRINter:SELect....443
SYSTem:DATE....451
SYSTem:ERRor:ALL?....453
SYSTem:ERRor:[NEXT]?....453
SYSTem:NAME....451
SYSTem:SET....452
SYSTem:TIME....451
TIMebase:ACQTime....283
TIMebase:DIVisions?....283
TIMebase:POSition....284
TIMebase:RANGe....283
TIMebase:RATime?....283
TIMebase:REFerence....284
TIMebase:ROLL:ENABle....287
TIMebase:SCALe....283
TIMebase:ZOOM:POSition....321
TIMebase:ZOOM:SCALe....320
TIMebase:ZOOM:STATe....320
TIMebase:ZOOM:TIME....320
TRIGger:A:CAN:ACKerror....410
TRIGger:A:CAN:BITSterror....410
TRIGger:A:CAN:CRCerror....410
TRIGger:A:CAN:DATA....410
TRIGger:A:CAN:DCONdition....409
TRIGger:A:CAN:DLC....409
TRIGger:A:CAN:FORMerror....410
TRIGger:A:CAN:FTYPe....408
TRIGger:A:CAN:ICONdition....409
TRIGger:A:CAN:IDENtifier....409
TRIGger:A:CAN:ITYPe....408
TRIGger:A:CAN:TYPE....407
TRIGger:A:EDGE:COUPling....305
TRIGger:A:EDGE:FILTer:LPASs....305
TRIGger:A:EDGE:FILTer:NREJect....305
TRIGger:A:EDGE:SLOPe....304
TRIGger:A:FINDlevel....302
TRIGger:A:HOLDoff:MODE....304
TRIGger:A:HOLDoff:TIME....304
TRIGger:A:HYSTeresis....304
TRIGger:A:I2C:ACCess....390

TRIGger:A:I2C:ADDRess....391
TRIGger:A:I2C:AMODe....390
TRIGger:A:I2C:MODE....390
TRIGger:A:I2C:PATTern....391
TRIGger:A:I2C:PLENgth....391
TRIGger:A:I2C:POFFset....392
TRIGger:A:LEVel<n>:RISetime:LOWer....311
TRIGger:A:LEVel<n>:RISetime:UPPer....311
TRIGger:A:LEVel<n>[:VALue]....302
TRIGger:A:LIN:CHKSerror....424
TRIGger:A:LIN:DATA....425
TRIGger:A:LIN:DCONdition....425
TRIGger:A:LIN:DLENgth....426
TRIGger:A:LIN:ICONdition....425
TRIGger:A:LIN:IDENtifier....425
TRIGger:A:LIN:IPERror....424
TRIGger:A:LIN:SYERror....424
TRIGger:A:LIN:TYPE....423
TRIGger:A:MODE....302
TRIGger:A:PATTern:CONDition....309
TRIGger:A:PATTern:FUNCtion....309
TRIGger:A:PATTern:MODE....309
TRIGger:A:PATTern:SOURce....308
TRIGger:A:PATTern:WIDTh:DELTa....310
TRIGger:A:PATTern:WIDTh:RANGe....310
TRIGger:A:PATTern:WIDTh[:WIDTh]....310
TRIGger:A:RISetime:DELTa....312
TRIGger:A:RISetime:RANGe....311
TRIGger:A:RISetime:SLOPe....311
TRIGger:A:RISetime:TIME....311
TRIGger:A:SOURce....303
TRIGger:A:SOURce:UART....402
TRIGger:A:SPI:MODE....380
TRIGger:A:SPI:PATTern....380
TRIGger:A:SPI:PLENgth....381
TRIGger:A:SPI:POFFset....381
TRIGger:A:TV:FIELd....307
TRIGger:A:TV:LINE....308
TRIGger:A:TV:POLarity....307
TRIGger:A:TV:STANdard....307
TRIGger:A:TYPE....303
TRIGger:A:UART:MODE....402
TRIGger:A:UART:PATTern....403
TRIGger:A:UART:PLENgth....403
TRIGger:A:UART:POFFset....404
TRIGger:A:WIDTh:DELTa....306
TRIGger:A:WIDTh:POLarity....305
TRIGger:A:WIDTh:RANGe....306

TRIGger:A:WIDTh:WIDTh....306
TRIGger:B:DELay....313
TRIGger:B:EDGE:SLOPe....312
TRIGger:B:ENABle....312
TRIGger:B:EVENt:COUNt....313
TRIGger:B:FINDlevel....313
TRIGger:B:HYSTeresis....314
TRIGger:B:LEVel....312
TRIGger:B:MODE....313
TRIGger:B:SOURce....312
TRIGger:EXTern:COUPling....303
TRIGger:OUT:MODE....450
TRIGger:OUT:PLENgth....451
TRIGger:OUT:POLarity....451
TSTamp:ACLear....321
TSTamp:CLEar....321
TSTamp:NEXT....321
TSTamp:PREVious....321
TSTamp:SET....321

Index

Symbols

*OPC ... 260
*OPC? ... 260
*RST ... 273
*WAI ... 260

A

Acquisition
  Limited number ... 39
  Modes ... 14
  set number of a. ... 25
  Start and stop ... 39
  Time ... 15
Acquisition modes ... 14
Actions
  Mask violation ... 130
Active probe
  differential ... 18
  Micro Button ... 33
  overview ... 18
  ProbeMeter ... 33
  Settings ... 33
ADC sample rate ... 12
ADC samples ... 12
Alignment
  internal ... 239
Amplitude ... 87
Asynchronuous commands ... 259
Attenuation, probe ... 32
Automatic measurements ... 87
  Remote control ... 335
  Settings ... 94
Auxiliary cursors
  displaying ... 55
  Setting ... 60
Average ... 24

B

Backlight (intensity) ... 58
Bandwidth ... 30
  instrument ... 12
  probe ... 12
Base level ... 87
BIN ... 228
Bits
  Bit lines display ... 150
Boolean parameters ... 256
Brightness ... 55
B-Trigger ... 42
Burst width ... 78, 87
Bus
  Display ... 150
Buses
  Label ... 151
  Node labels ... 151
Bus Type ... 150
Bus Width ... 212

C

CAN ... 185
  Protocol settings ... 185
  Search settings ... 194
  Trigger settings ... 186
Case-sensitivity
  SCPI ... 252
Center
  softkey ... 119
Center frequency
  remote ... 352
Change directory
  Remote ... 445
  softkey ... 222
Channel
  Keys ... 28
  Label ... 29
  Menu ... 29
  name label ... 34
Channel cursors
  displaying ... 55
Channel Cursors ... 60
Clear Persist. ... 59
Clear status
  remote ... 274
Clock SCL (I²C) ... 167
Colon ... 257
Color mode
  printing ... 216
  softkey ... 231
Colors, temperature ... 59
Comma ... 257
Commands
  colon ... 257
  comma ... 257
  command line structure ... 257
  common ... 249
  double dagger ... 257
  GBIP, addressed ... 250
  GBIP, universal ... 250
  instrument control ... 249
  overlapping ... 259
  question mark ... 257
  quotation mark ... 257
  SCPI compliant ... 249
  sequential ... 259
  structure ... 251
  syntax elements ... 257
  white space ... 257
Command sequence
  recommendation ... 273
  remote ... 277
Comment
  softkey ... 220
Common commands
  syntax ... 251
CONDition ... 262
Configuration
  Protocol settings menu ... 150
Constant
  softkey ... 108

Controls
Position / Offset (vertical) ... 28
Position (horizontal) ... 23
Scale (horizontal) ... 23
Scale (vertical) ... 29
Copy Channel ... 129
Count ... 78, 87
Coupling ... 11, 30
Cursor ... 84
Trigger source ... 44
Create directory
remote ... 445
softkey ... 222
Crest factor ... 78, 87
Crosshairs
displaying ... 55
CSV ... 123, 227
Cursor
Activating ... 83
configuring ... 81
FFT ... 78
measurements ... 78
measurements on FFT ... 115
measurement type ... 78
positioning ... 82
Positioning ... 85
remote ... 327
Remote control ... 326
Set To Screen ... 84
Set to Wave ... 84
Source ... 83
Track Scaling ... 84
Cursor measurements
Settings ... 82

D

Data2Clock
Search ... 142
Data SDA (I²C) ... 167
Date ... 236
DCL ... 250
Decimal Point
softkey ... 108
Decimation ... 14
Decimation Mode ... 24
Decode ... 150
Decoding format ... 150
DEF ... 255
Defaults
Cursor display ... 61
Default values
remote ... 276
Delay measurement ... 87, 97
Deskew ... 31
Destination
softkey ... 223
Device settings
import/export ... 218
Device Settings ... 225
Menu ... 226
saving ... 225
Saving and loading ... 225
softkey ... 224
Device-specific commands ... 249
DHCP ... 243
interface setting ... 237
Differential probe ... 18
Digital channels ... 208
Label ... 211
Vertical position ... 211
Vertical scale ... 211
Digital signals ... 208
Digitization threshold ... 31
Directory name
defining ... 218
Display
configuring ... 54
Data format ... 150
Menu ... 57
Display Mode ... 58
Dots Only ... 59
Double dagger ... 257
DOWN ... 255
Duty cycle ... 78, 87

E

Edge
Search ... 137
Edge trigger ... 43
Edit Constant
softkey ... 108
Edit Equations
softkey ... 103
ENABle ... 262
Enable registers
remote ... 276
Envelope ... 24
Eq. Set Label
softkey ... 109
Equation
editing ... 99
label ... 109
softkey ... 102, 103
Equation Label
softkey ... 109
Equation set
editing ... 100
Equation Set
label ... 109
Equation sets
import/export ... 218
Import/Export ... 232
loading ... 100
saving ... 100
Equivalent-time sampling ... 26
Error queues
recommendations ... 273
ESE (event status enable register) ... 266
ESR ... 264
ESR (event status register) ... 266
EVENt ... 262
Events
Search ... 147
Event status enable register
remote ... 275
Event status enable register (ESE) ... 266
Event status register
remote ... 275
Event status register (ESR) ... 266
Exporting ... 222
device settings ... 218
equation sets ... 218

masks ... 218
reference ... 218

F

Fall time ... 87
FFT
activating ... 111
Center ... 119
configuring ... 112, 115, 118
cursor measurements ... 78, 115
deactivating ... 111, 121
displaying ... 110
general setup ... 111
key ... 116
Main Time Base ... 70, 120
menu ... 115
mode (remote) ... 349
No. of Averages ... 117
Position ... 120
Span ... 119
starting ... 115
waveform arithmetic ... 116
Window ... 117
Y-Position ... 120
Y-Scale ... 119, 120
Y-Scaling ... 118
YT-Window ... 119
FFT off
softkey ... 121
FFT-Setup
softkey ... 118
File formats
BIN ... 228
CSV (masks) ... 123
CSV (waveforms) ... 227
masks ... 123
MSK ... 123
TRF ... 227
TXT (masks) ... 124
TXT (waveforms) ... 228
Waveforms ... 227
File name
defining ... 218
softkey ... 220
Filter on channel signal ... 24
Find level
Channel threshold ... 31
FORCE ... 39
Format
softkey ... 230, 231
Waveforms ... 227
Formats
masks ... 123
Frame Table ... 150
Frequency ... 87

G

Gain, vertical ... 11
Gate
search ... 137
Search ... 146
GET ... 250
GPIB
address ... 243
characteristics ... 242
interface ... 236
interface messages ... 250
remote control interface ... 242
Grid ... 61
displaying ... 55
intensity ... 59
GTL ... 250

H

Hold Off ... 42
Horizontal position ... 15
Host name ... 247
Hysteresis of trigger level ... 44, 53

I

Identification
remote ... 275
IEEE488
interface ... 236
IFC ... 250
Import/Export
Equation sets ... 232
Masks ... 232
References ... 232
Remote ... 448
softkey ... 222, 223
Importing ... 222
device settings ... 218
equation sets ... 218
reference ... 218
INF ... 255
Information on instrument ... 237
Intensity ... 55
Settings ... 58
Interface messages ... 249
Interfaces
Activating ... 236
Deactivating ... 236
for remote control ... 241
GPIB ... 236, 242
IEEE488 ... 236
LAN ... 236
parameters ... 237
Setting ... 236
USB ... 242
Interrupt ... 270
Inverse Brightn. ... 59
Invert signal amplitude ... 31
IP address ... 247
changing ... 243
I²C ... 165
basics ... 165
Configuration ... 167
Protocol settings ... 167
Triggering ... 168
Trigger settings ... 169

K

Keys
Acquisition ... 23
CH N ... 28
Display ... 57
FFT ... 116
NEXT ... 73

PREV 73
PRINT 224
Setup (instrument) 234
SIGNAL OFF 28
ZOOM 69

L

Label
Bus 151
Digital channels 211
Label List 151
Label lists 151
LAN
Configuration 243
interface 236, 242
IP address 247
parameter setup 243
remote control interface 242
resource string 247
VXI protocol 242
Language 236
LEVEL 40
LIN 197
Protocol settings 198
Search settings 205
Trigger settings 199
Lines 61
LLO 250
Load
softkey 77
Loading
Device settings 225
equation sets 100
references 75
Load Mask 130
Load Settings
softkey 77
Low-pass filter 24

M

Main Time Base
softkey 70, 120
Malfunctions
reacting 273
Markers 73
Go to next 73
Go to previous 73
Masks
Actions 130
copy 122
Creating 125, 129
creating CSV file 123
definition 122
export/import 122
import/export 218
Import/Export 232
Loading 127, 130
Menu 128
results 122
save and load 122
Saving 125
Testing 127, 128
test results 122
Masks Test Off 131
MATH
menu 101
Mathematics
configuring 98
equation sets 100
FFT 115
menu 101
Math waveforms
displaying 98
MAX 255
Mean 78
Mean Cycle 87
Mean Value 87
Meas. Place 95
Meas. Type 83, 95
automatic measurement (remote) 336
cursor measurement 78
Measure 95
remote 336
Measurement
Activating 95
activating (remote) 336
Measurements
Amplitude 87
Base level 87
Burst width 78
Count 78, 87
Crest factor 78, 87
deactivating 97
Delay 87, 97
Duty cycle 78, 87
Fall time 87
Frequency 87
Mean 78
Mean Cycle 87
Mean value 87
Peak 78, 87
Period 87
Phase 97
Pulse width 87
Ratio X 78
Ratio Y 78
reference levels 97
Rise time 78, 87
RMS 78
RMS Cycle 87
RMS value 87
Time 78
Top level 87
Trigger frequency (A- and B-trigger) 87
Trigger period (A- and B-trigger) 87
V-Marker 78
Voltage 78
Measurement types 87
Memory depth 25
Memory usage 227
Menu Off
softkey 235
Menus
Acquisition 23
Auto Measure 94
Cursor 82
Setup (instrument) 234
Zoom 69
Messages
instrument responses 249
Micro button 18

Micro Button
Settings ... 33
MIN ... 255
Mnemonics ... 251
optional ... 253
MODE ... 39
MSK ... 123
MSO
Parallel bus configuration ... 212

N

NAN ... 255
New Mask ... 129
NEXT ... 73
Next peak ... 85
NINF ... 255
No. of Averages
softkey ... 117
NTRansition ... 262
Numeric values
special ... 255
Nx Single ... 25

O

Offset ... 28
Operand 1
softkey ... 107
Operand 2
softkey ... 108
Operation complete
remote ... 275
Operator
softkey ... 103
Option identification
remote ... 275
Options ... 238
Output buffer ... 264
Overlapping
preventing ... 260
Overlapping commands ... 259

P

Paper format ... 216
Parallel buses ... 208
Configuration ... 212
Parameters
block data ... 257
boolean ... 256
interfaces ... 237
SCPI ... 254
special numeric values ... 255
string ... 256
text ... 256
units ... 255
Passive probe
attenuation ... 32
overview ... 17
Settings ... 32
Pattern
Search ... 144
Pause
Mask test ... 129
Peak ... 78, 87
Search ... 139
Peak detection ... 24
Period ... 87
Persist. Time ... 59
Persistence ... 55, 59
remote ... 318
Persistence time
remote ... 318
Phase measurement ... 97
Position
Digital channels ... 211
Horizontal ... 15, 23
softkey ... 120
Vertical ... 11, 28
PPC ... 250
PPU ... 250
Prefix
softkey ... 108
PREV ... 73
Prev. peak ... 84
Print ... 130
softkey ... 232
Printer
communication ... 217
settings ... 238
Printing
screenshots ... 232
Print Key
softkey ... 224
PRINT key ... 223
Configuring ... 224
ProbeMeter ... 18, 33
Probes
active ... 18
adjusting ... 239
differential ... 18
passive ... 17
Programming examples ... 458
Protocol
VXI ... 242
Protocols
CAN ... 185
CAN configuration settings ... 185
CAN search settings ... 194
CAN trigger settings ... 186
Display configuration ... 150
I²C ... 165
I²C configuration settings ... 167
I²C trigger settings ... 169
Label list ... 151
LIN ... 197
LIN configuration settings ... 198
LIN search settings ... 205
LIN trigger settings ... 199
Parallel bus configuration ... 212
SPI/SSPI ... 155
SPI/SSPI configuration settings ... 157
SPI/SSPI trigger settings ... 160
Symbolic ID ... 151
UART/RS-232 ... 175
UART configuration settings ... 177
UART trigger settings ... 180
PTRansition ... 262
Pulse width ... 87

Q

Queries ... 249, 258
  Status ... 271
Question mark ... 257, 258
Quick measurement
  deactivating (remote) ... 335
Quick measurements
  remote control ... 334
Quotation mark ... 257

R

Ratio X ... 78
Ratio Y ... 78
Real time sampling ... 26
Recommendations
  remote control programming ... 272
Record length ... 12, 25
REF
  key ... 76
Reference ... 74
  displaying ... 74
  softkey ... 76, 77
Reference Level
  Remote control ... 341
Reference levels ... 97
References
  import/export ... 218
  Import/Export ... 232
  loading ... 75
  menu ... 76
  saving ... 75
Registers ... 264
Remote control
  Automatic measurements ... 335
  basics ... 241
  Cursor measurements ... 326
  GPIB address ... 243
  interfaces ... 241
  Programming examples ... 458
  protocols ... 241
  quick measurements ... 334
  Reference Level ... 341
  starting ... 248
  Statistical measurements ... 342
Remove directory
  remote ... 445
  softkey ... 222
Remove file
  remote ... 448
  softkey ... 221
Reset values
  remote ... 276
Resolution ... 11, 12
Resource string
  LAN ... 247
Results
  mask testing ... 122
  Search ... 147
Reticle ... 61
Rise/Fall Time
  Search ... 139
Rise time ... 78, 87
RMS ... 78
RMS Cycle ... 87
RMS Value ... 87
Roll mode ... 26
RS232
  basics ... 175
RUN CONT ... 39
RUN Nx SINGLE ... 39
Runt
  Search ... 141

S

Sample Mode ... 26
Sample modes ... 14
Sample rate ... 12, 25
Samples ... 12
Save
  menu ... 220
  Remote ... 449
  softkey ... 221
Save/Recall
  references ... 76
Save (masks) ... 130
Saving
  data to a file ... 223
  Device settings ... 225
  equation sets ... 100
  file name ... 220
  references ... 75
  Screenshots ... 230
  Waveforms ... 227
Scale
  Digital channels ... 211
  horizontal ... 23
  vertical ... 29
  Vertical ... 11
SCPI
  parameters ... 254
  syntax ... 251
  version ... 241
SCPI compliant commands ... 249
Screen & Setup (softkey) ... 225
Screenshot ... 130
Screenshots ... 230
  printing ... 225, 232
  saving ... 224, 225
  Saving ... 230
  softkey ... 224, 225, 231
SDC ... 250
Search
  CAN ... 194
  Data2Clock ... 142
  Edge ... 137
  Events ... 147
  gate ... 137
  Gate ... 146
  LIN ... 205
  Pattern ... 144
  Peak ... 139
  Results ... 147
  Rise/Fall Time ... 139
  Runt ... 141
  Types ... 136
  Width ... 138
Self-alignment ... 239, 274
Selftest
  remote ... 277
Sequential commands ... 259
Service request (SRQ) ... 265, 270

Service request enable
remote ... 276
Service request enable register (SRE) ... 265
SET CLEAR ... 73
Setting commands ... 249
Settings
Instrument ... 226
Instrument (default) ... 227
Set To Screen ... 84
Set to Wave ... 84
Setup
menu (instrument setup) ... 234
SETUP (trigger) ... 40
Setup & Label ... 226
SIGNAL OFF ... 28
Slope
Edge trigger ... 43
SLOPE ... 40
Smoothed waveform ... 24
Softkeys
1kHz ... 239
1MHz ... 239
Active (SSPI) ... 157
Attenuation factor ... 32
Automatic ... 240
Bandwidth ... 30
Change directory ... 222
Color mode ... 216, 231
Command Set (printer) ... 217
Comment ... 220
Constant ... 108
Control Beep ... 238
Coupling ... 30
Create directory ... 222
Data ... 230
Date & Time ... 236
Day ... 236
Decimal Point ... 108
Decimation Mode ... 24
Default ... 237
Default sett. ... 227
Deskew ... 31
Destination ... 223
Device Information ... 237
Device Name ... 240
Device Settings ... 224, 226
DHCP ... 237
Edit Constant ... 108
Edit Equations ... 103
Eq. Set Label ... 109
Equation ... 102, 103
Equation Label ... 109
Error Beep ... 238
Execute ... 237, 238
File name ... 220
Firmware ... 237
Format ... 230, 231
Hour ... 236
Hysteresis A/B ... 44, 53
IEEE488 ... 236
Import/Export ... 222, 223
Interface ... 236, 238
Invert ... 31
LAN ... 236
LED Intensity ... 240
Load ... 221
Main Time Base ... 70, 120
Meas.Type (cursor) ... 78
Memory usage ... 227
Menu Off ... 235
Minute ... 236
Month ... 236
Offset ... 28
Operand 1 ... 107
Operand 2 ... 108
Operator ... 103
Paper format ... 216
Parameter ... 237
Prefix ... 108
Print ... 232
Printer ... 238
Print Key ... 224
Probe ... 31
Probe Adjust ... 239
Remove directory ... 222
Remove file ... 221
Save ... 221
Screen & Setup ... 225
Screenshots ... 224, 225, 231
Secure Erase ... 240
Self Alignment ... 239
Setup & Label ... 226
Slope (Clock SSPI) ... 158
Sound ... 238
Source ... 223
Source (SPI, SSPI) ... 157
Source X ... 64
Source Y1 ... 64
Source Y2 ... 65
Source Z ... 65
Storage ... 222
Termination ... 30
Threshold ... 31, 66
Time Reference ... 235
Trigger Beep ... 238
Trigger Offset ... 70, 121
Trigger On ... 53
Unit ... 102, 109
Unit (probe) ... 33
Update ... 237
Upgrade ... 238
USB ... 236
Value ... 108
Visible ... 102
Waveform ... 230
Waveforms ... 224, 229
X-CH1 Y-CH2 ... 65
X-CH2 Y-CH1 ... 65
XYZ Setup ... 64
Year ... 236
Y-Scale ... 29
Z ... 65
Z-Intensity ... 65
Z Setup ... 65
Sound ... 130
Sounds
setting ... 238
Source
Automatic measurements ... 96
Cursor ... 83
softkey ... 76, 223
Trigger ... 42
SOURCE (trigger) ... 40

Span
remote ... 352
softkey ... 119
SPD ... 250
SPE ... 250
Special characters
SCPI ... 254
SPI/SSPI ... 155
Configuration ... 156
Configuration settings ... 157
Trigger ... 159
SPI/SSPI protocols
Trigger settings ... 160
SPI protocol
basics ... 155
SRE ... 264
SRE (service request enable register) ... 265
SRQ (service request) ... 265, 270
SSPI protocol
basics ... 155
Statistic
Settings ... 96
Statistical measurements
Remote control ... 342
Status
Queries ... 271
Status byte
remote ... 274, 276
Status registers ... 264
CONDition ... 262
ENABle ... 262
EVENt ... 262
model ... 262
NTRansition ... 262
parts ... 262
PTRansition ... 262
STATus:OPERation ... 267
Status reporting system
Common commands ... 274
Status reports ... 261
application ... 270
STB ... 264
Stop ... 130
Storage
configuring ... 218
device ... 218
directory ... 218
file name ... 218
Front USB ... 217
Internal ... 217
Rear USB ... 217
softkey ... 222
Storing
waveforms, traces ... 229
Stretch Y (masks) ... 129
Suffixes ... 253
Symbolic ID ... 151
Syntax elements
SCPI ... 257

T

Temperature Colors ... 59
Termination ... 11, 30
Test (masks) ... 128
Test results
masks ... 122
Threshold
Protocols ... 148
Time ... 78, 236
Time base ... 15, 70, 120
Time diagram ... 58
Time reference ... 15
Time Reference ... 235
Time scale ... 15
Timestamps ... 73
Top level ... 87
Track Scaling (cursor) ... 84
TRF ... 227
Trigger
Auto/normal ... 39
Edge trigger, slope ... 40
Force ... 39
Hold off ... 42
Level ... 40
level (remote) ... 302
Mode ... 39
offset ... 70, 121
position ... 70, 121
Setup ... 40
Source ... 40, 42
Type ... 41
UART ... 179
Trigger event
displaying ... 55
remote ... 276
Showing ... 60
Trigger frequency (A- and B-trigger) ... 87
Trigger hysteresis
Showing ... 61
Trigger Level ... 42
Trigger mode
remote ... 302
Trigger offset ... 15, 23
Trigger Offset
softkey ... 70, 121
Trigger period (A- and B-trigger) ... 87
Trogger
Edge ... 43
Width ... 45
TXT ... 124, 228

U

UART
basics ... 175
Configuration ... 176
Protocol settings ... 177
Trigger ... 179
Trigger settings ... 180
UART/RS-232 ... 175
Undersampling ... 12
Unit
softkey ... 102, 109
Units ... 255
UP ... 255
Update
softkey ... 77
Updates
firmware ... 237
interfaces ... 238
USB
remote control interface ... 242

V

Value
softkey ... 108
Vertical
Position ... 11
Resolution ... 11
Scale ... 11
Vertical settings ... 29
Vertical system ... 11
VISA Address String ... 247
Visible
softkey ... 102
softkey (remote) ... 345
V-Marker ... 78
Voltage ... 78
VXI protocol ... 242

W

Wait
remote ... 277
Waveform
Action on mask violation ... 130
Arithmetic ... 14
Waveform (Intensity) ... 58
Waveform Arithmetic ... 24
Waveform rate ... 25
Waveforms
File formats ... 227
Save and load ... 227
saving ... 224, 230
Saving to USB flash device ... 229
softkey ... 224
switch off ... 28
Waveform samples ... 12
Wfm. Arithmetic
FFT ... 116
softkey ... 116
White space ... 257
Width
Search ... 138
Width trigger ... 45
Width X (masks) ... 130
Width Y (masks) ... 129
Window
softkey ... 117
Window type
remote ... 349

X

XY-diagram ... 61
Activate ... 58
configuring ... 62
XYZ Setup ... 58

Y

Y(t)-Setup
softkey ... 120
Y-Position
softkey ... 120
Y-Position (masks) ... 129
Y-Scale
softkey ... 119
Y-Scaling
softkey ... 118
YT-Window
softkey ... 119

Z

Zoom
Main Time Base ... 70, 120
menu ... 69
Zoom Off
softkey ... 71
Zoom Time
softkey ... 70
Zoom Time Base
softkey ... 70